

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120723\
 Data File : PS025043.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 07 Dec 2023 21:36
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 07 23:30:53 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	6.355	6.770	1237.8E6	398.7E6	553.118	550.257
Target Compounds						
1) T Dalapon	0.000	2.562	0	3361178	N.D.	2.930
2) T 3,5-DICHL...	5.696	0.000	4148778	0	1.227	N.D. #
3) T 4-Nitroph...	6.197	0.000	7790055	0	5.290	N.D. #
5) T DICAMBA	0.000	6.971	0	4629638	N.D.	1.494
6) T MCPP	6.678	7.081f	6235379	571172	<MDL	<MDL #
8) T DICHLORPROP	0.000	7.556	0	5041353	N.D.	6.409
9) T 2,4-D	7.245	7.770f	37300885	602532	12.281	<MDL #
12) T 2,4,5-T	0.000	8.978	0	1043971	N.D.	<MDL
13) T 2,4-DB	0.000	9.471	0	1042194	N.D.	1.883
15) T Picloram	9.678	10.762	12827377	8765194	<MDL	1.339 #
16) T DCPA	0.000	10.762	0	8765194	N.D.	1.617



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120723\
Data File : PS025043.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 07 Dec 2023 21:36
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 07 23:30:53 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

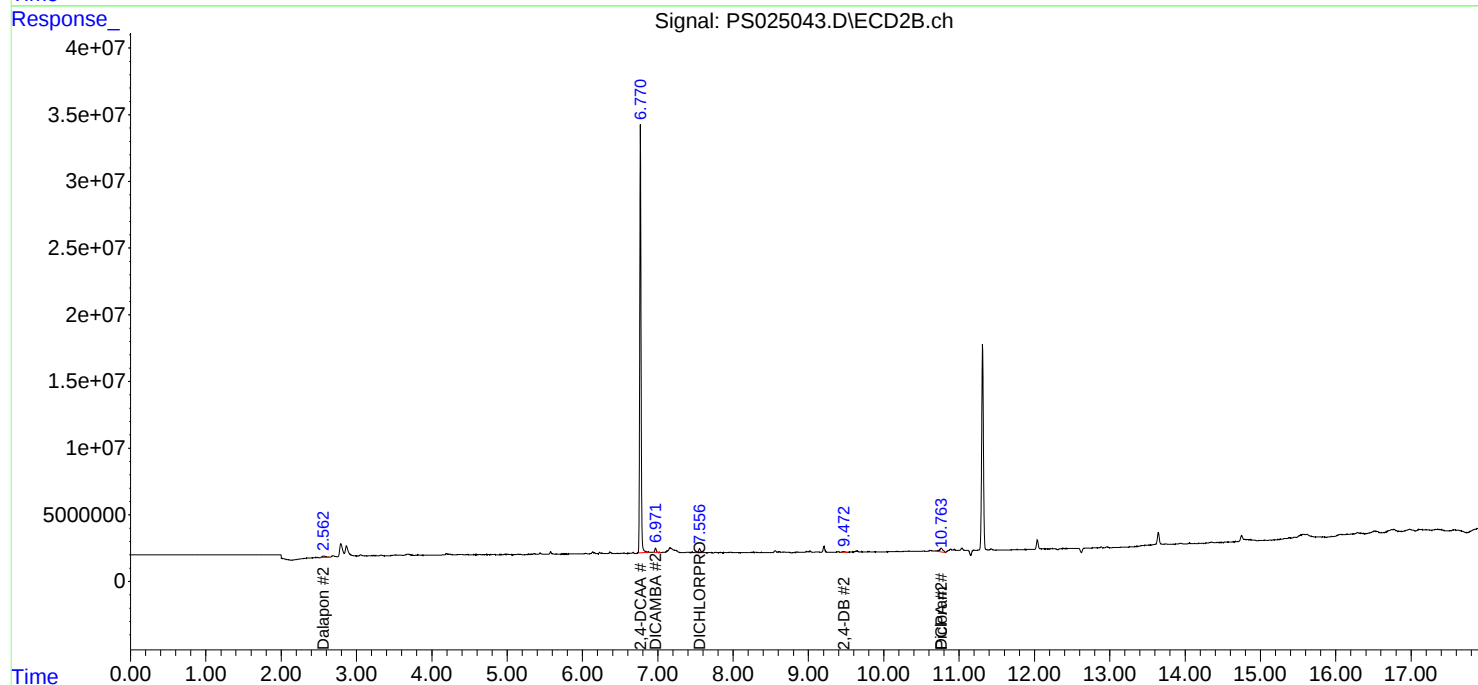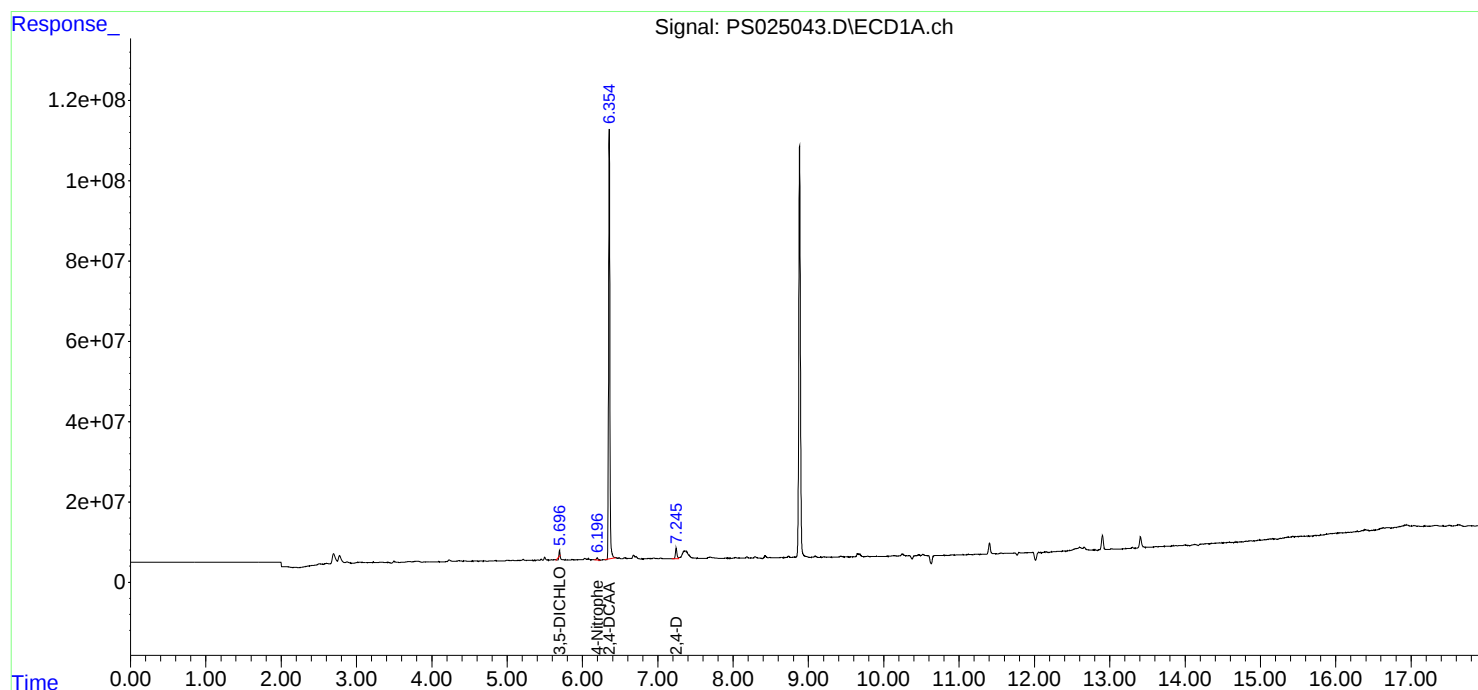


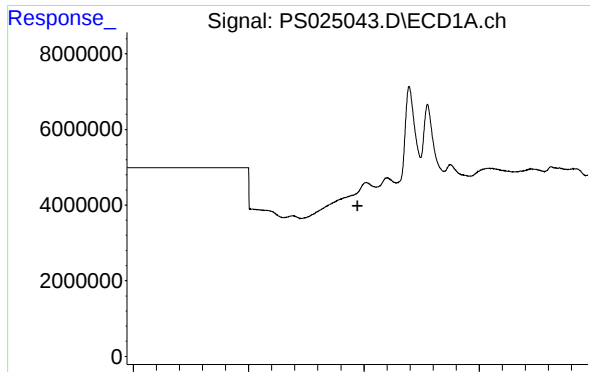

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.472 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

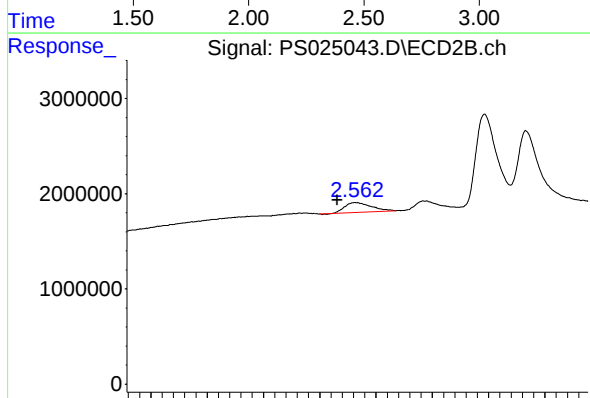


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: 0.031 min
Response: 3361178
Conc: 2.93 ng/ml

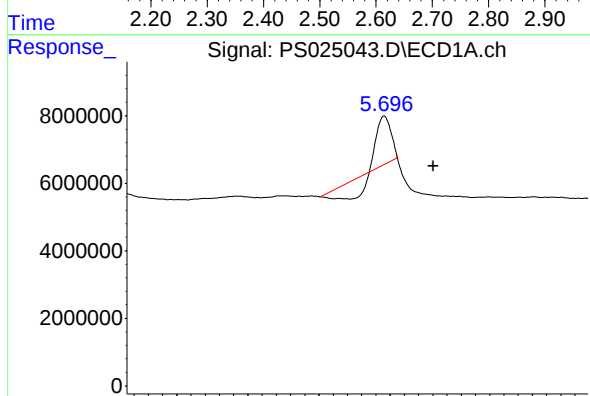


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 5.696 min
Delta R.T.: -0.034 min
Response: 4148778
Conc: 1.23 ng/ml

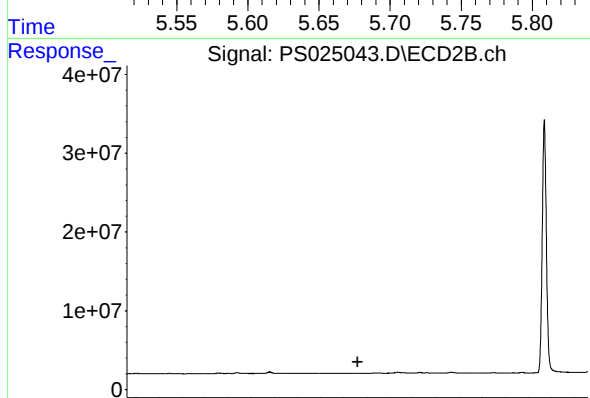

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 0.000 min
Exp R.T.: 5.960 min
Response: 0
Conc: N.D.

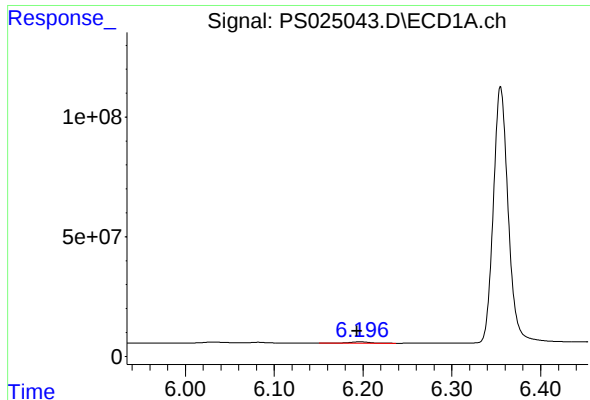

#3 4-Nitrophenol


R.T.: 6.197 min
Delta R.T.: 0.004 min
Response: 7790055
Conc: 5.29 ng/ml

Instrument :
ECD_S
ClientSampleId :

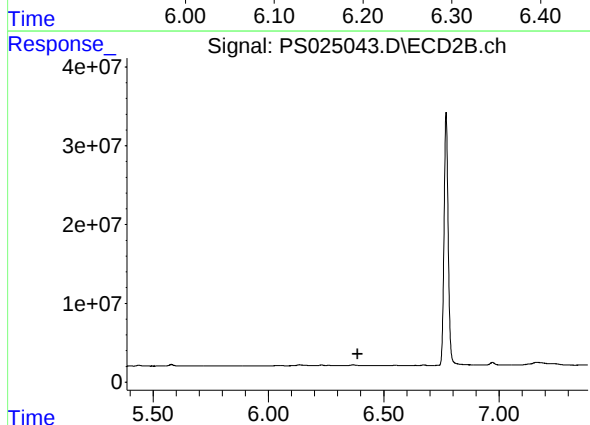


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

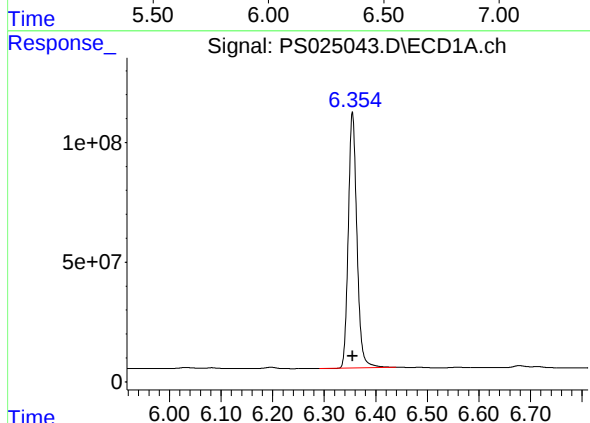


#4 2,4-DCAA

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 1237790947
Conc: 553.12 ng/ml

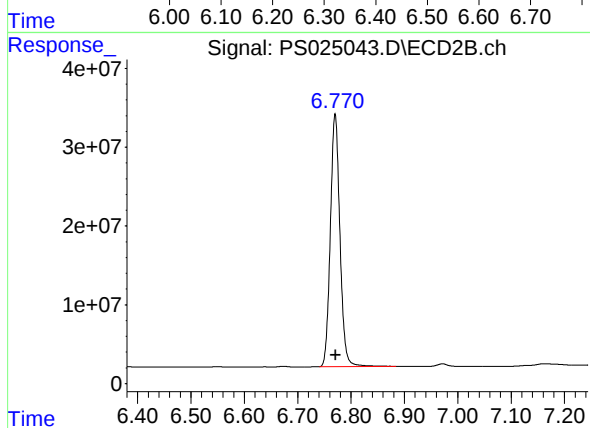

#4 2,4-DCAA


R.T.: 6.770 min
Delta R.T.: -0.001 min
Response: 398691430
Conc: 550.26 ng/ml

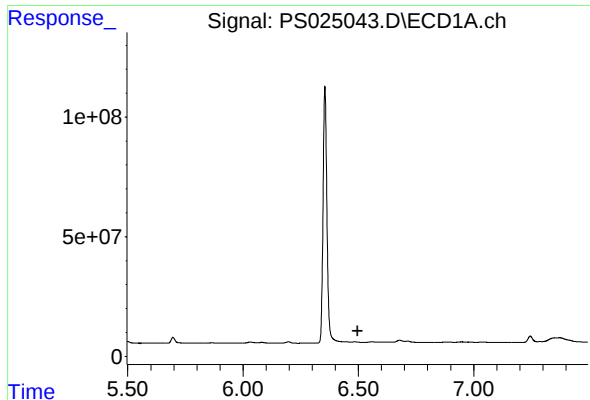

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 6.496 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

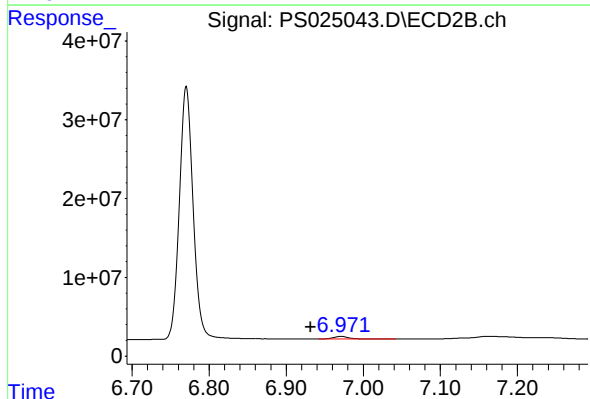


#5 DICAMBA

R.T.: 6.971 min
Delta R.T.: 0.040 min
Response: 4629638
Conc: 1.49 ng/ml

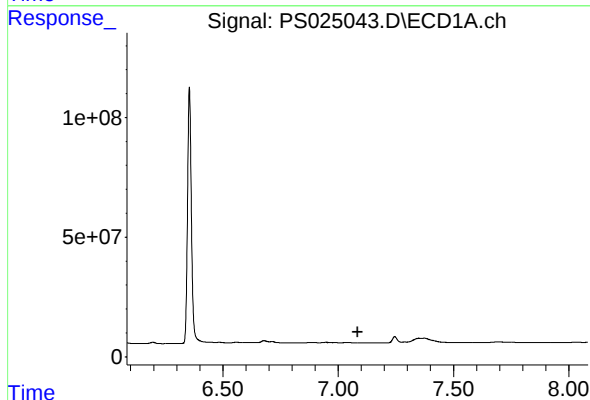


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

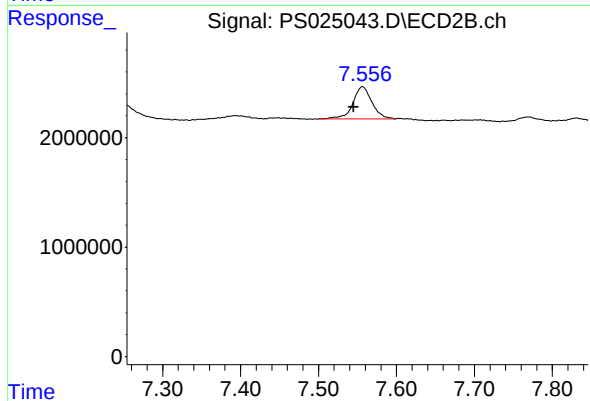

#8 DICHLORPROP


R.T.: 7.556 min
Delta R.T.: 0.011 min
Response: 5041353
Conc: 6.41 ng/ml

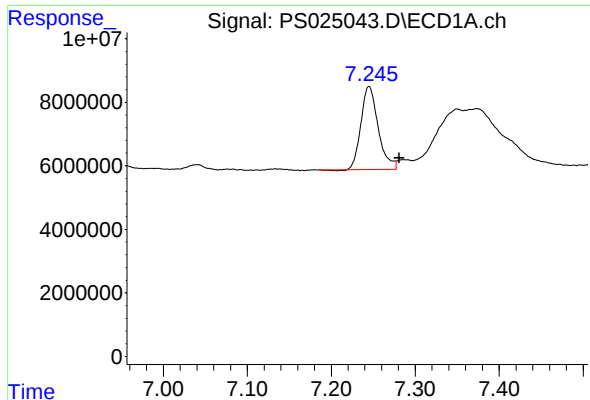

#9 2,4-D


R.T.: 7.245 min
Delta R.T.: -0.036 min
Response: 37300885
Conc: 12.28 ng/ml

Instrument :
ECD_S
ClientSampleId :

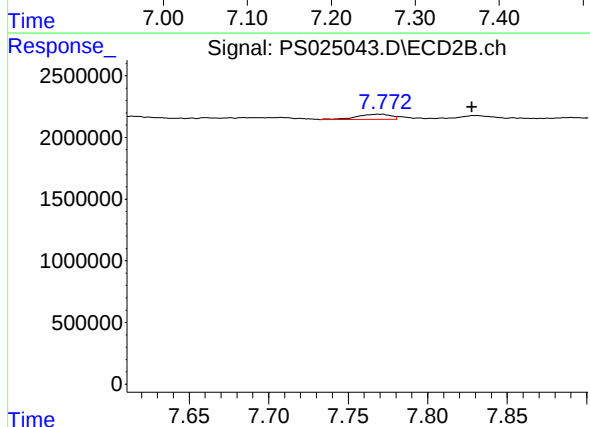


#9 2,4-D

R.T.: 7.770 min
Delta R.T.: -0.058 min
Response: 602532
Conc: N.D.

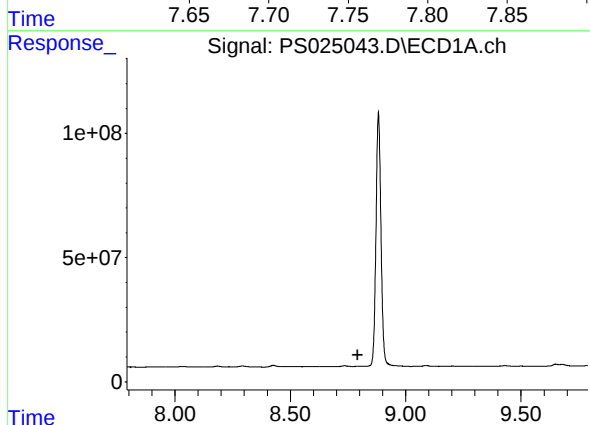


#13 2,4-DB

R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

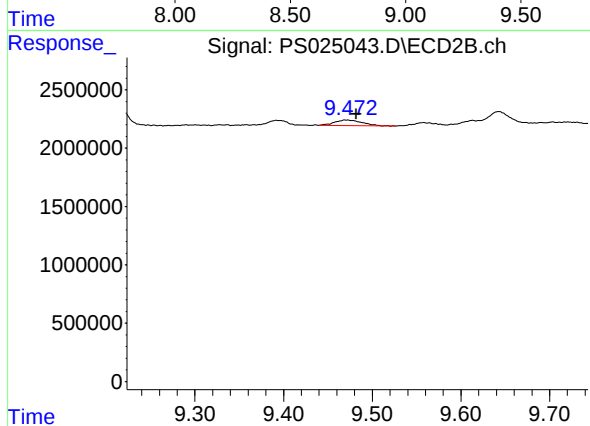

#13 2,4-DB


R.T.: 9.471 min
Delta R.T.: -0.011 min
Response: 1042194
Conc: 1.88 ng/ml

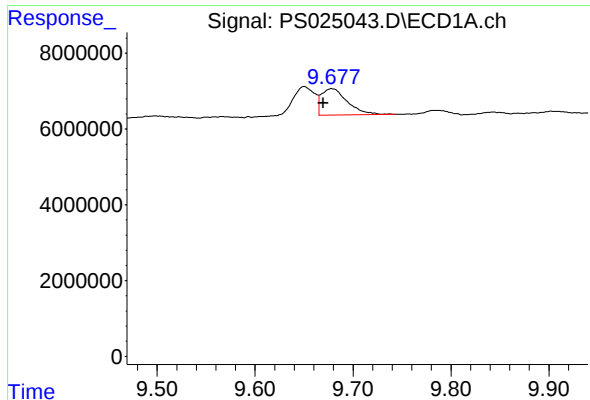

#15 Picloram


R.T.: 9.678 min
Delta R.T.: 0.009 min
Response: 12827377
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

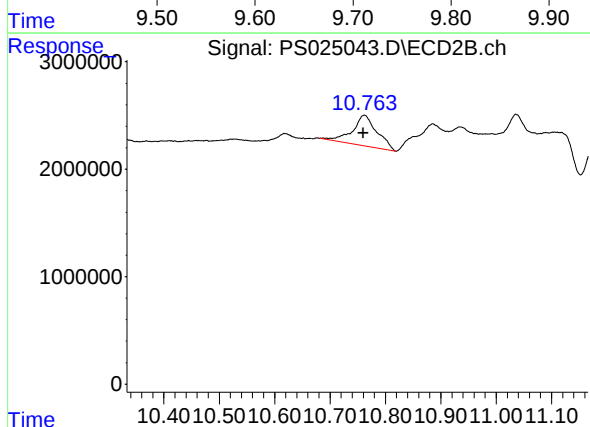


#15 Picloram

R.T.: 10.762 min
Delta R.T.: 0.002 min
Response: 8765194
Conc: 1.34 ng/ml

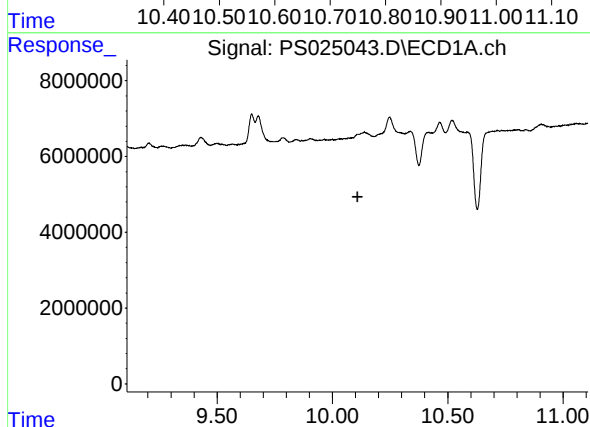

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

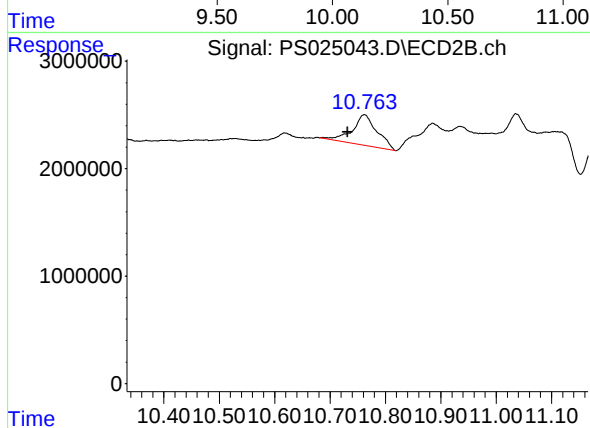

#16 DCPA

R.T.: 10.762 min
Delta R.T.: 0.031 min
Response: 8765194
Conc: 1.62 ng/ml