

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120821\
 Data File : PS017571.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 08 Dec 2021 08:58
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 08 16:20:41 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.157	0.000	3548712	0	2.257	N.D. #
Target Compounds							
5) T	DICAMBA	7.337	0.000	10621489	0	1.740	N.D. #
7) T	MCPA	7.609f	0.000	4373161	0	<MDL	N.D. #
8) T	DICHLORPROP	8.031	0.000	3867525	0	2.519	N.D. #
9) T	2,4-D	8.278	0.000	23104336	0	12.365	N.D. #
10) T	Pentachlo...	8.561	8.223	24425707	9596892	1.157	1.143
11) T	2,4,5-TP ...	9.113	8.586	17445184	6653365	2.093	1.877
12) T	2,4,5-T	9.409	8.971	26000737	7527503	3.078	2.264 #
14) T	DINOSEB	11.094	0.000	17380285	0	2.791	N.D. #
15) T	Picloram	10.948	10.788	66360905	18821023	5.443	4.313
16) T	DCPA	11.362	10.719	26424312	10510328	2.474	2.385



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120821\
Data File : PS017571.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 08 Dec 2021 08:58
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 08 16:20:41 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

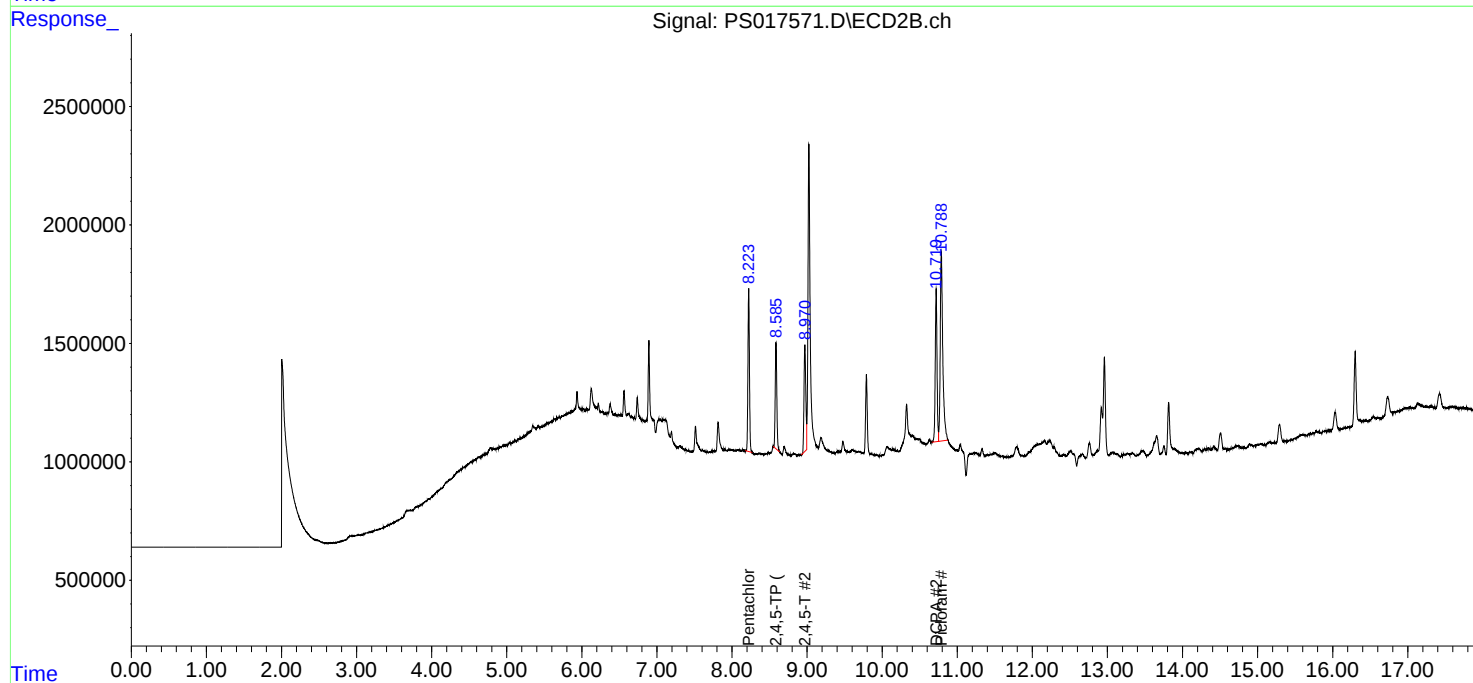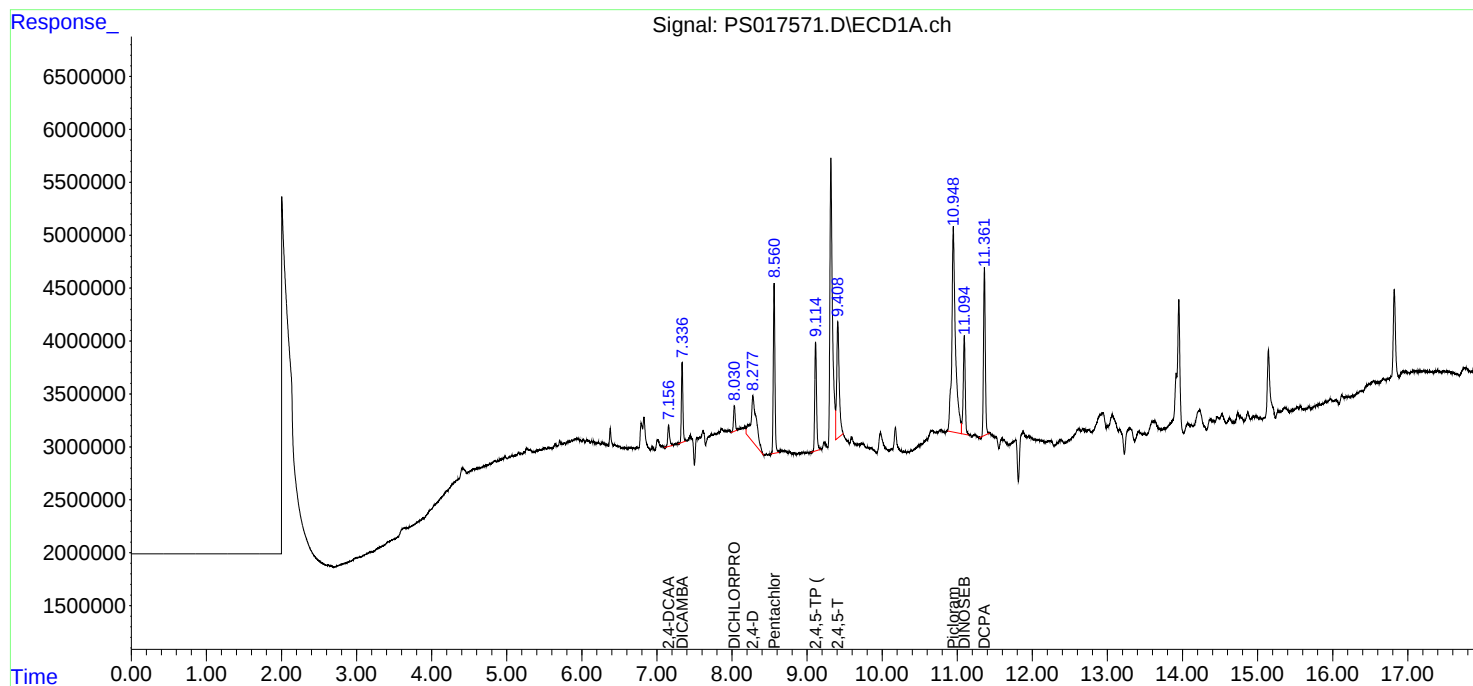


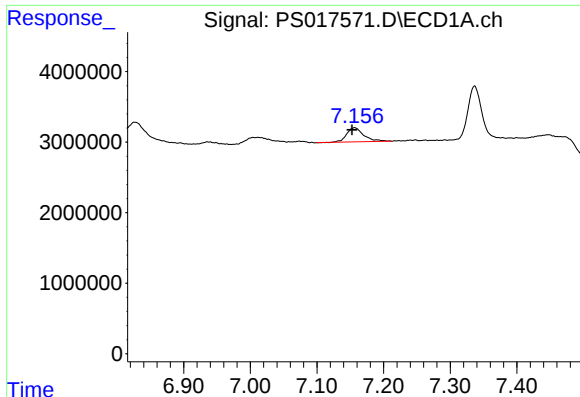

#4 2,4-DCAA


R.T.: 7.157 min
Delta R.T.: 0.004 min
Response: 3548712
Conc: 2.26 ng/ml

Instrument :
ECD_S
ClientSampleId :

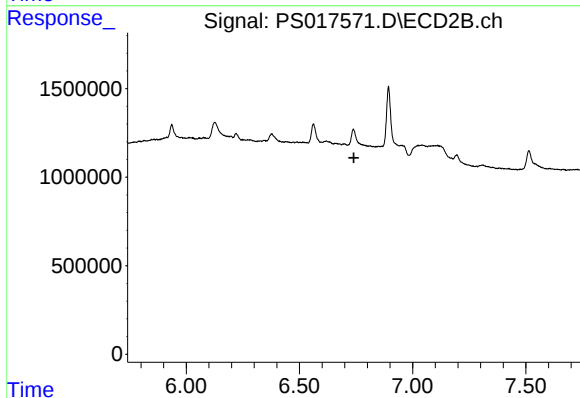


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.740 min
Response: 0
Conc: N.D.

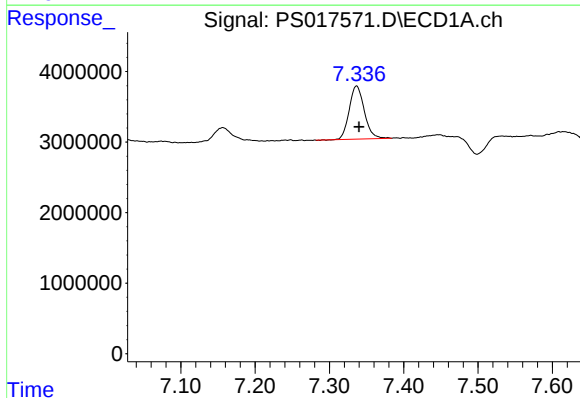


#5 DICAMBA

R.T.: 7.337 min
Delta R.T.: -0.003 min
Response: 10621489
Conc: 1.74 ng/ml

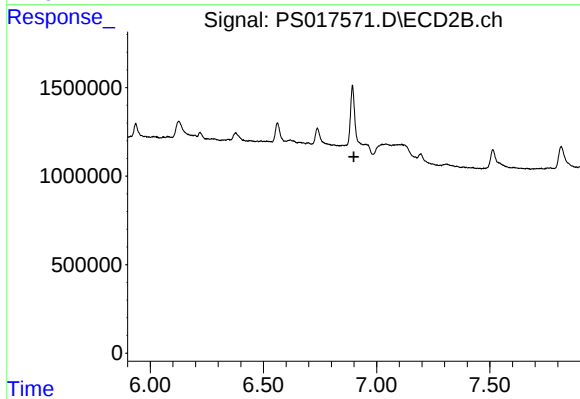

#5 DICAMBA


R.T.: 0.000 min
Exp R.T. : 6.900 min
Response: 0
Conc: N.D.

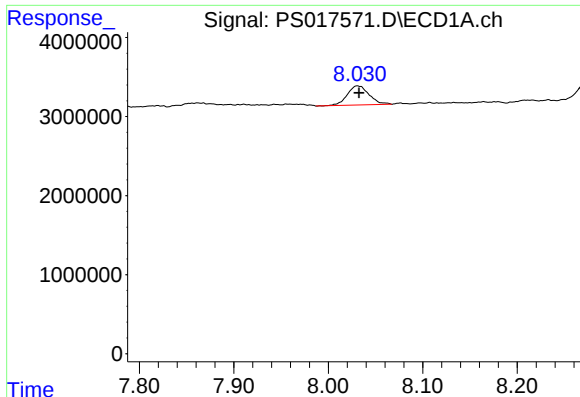

#8 DICHLORPROP


R.T.: 8.031 min
Delta R.T.: -0.002 min
Response: 3867525
Conc: 2.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

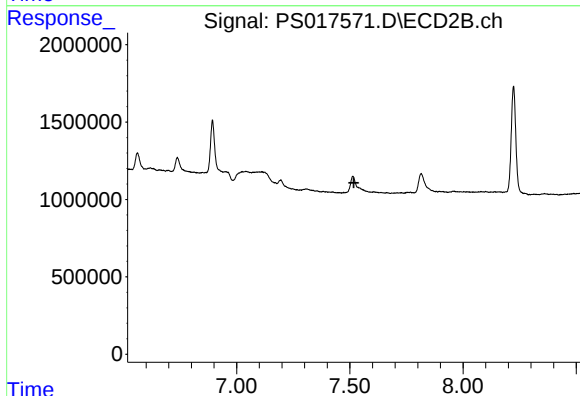


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.518 min
Response: 0
Conc: N.D.

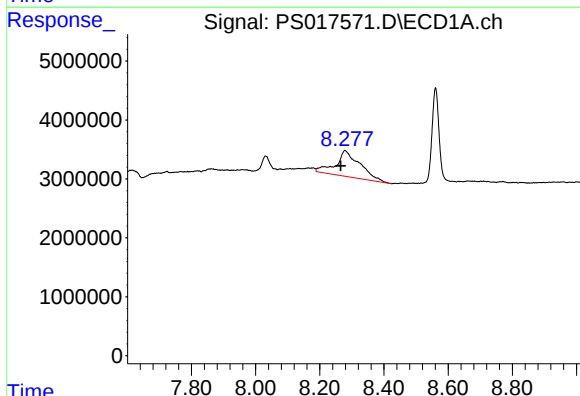


#9 2,4-D

R.T.: 8.278 min
Delta R.T.: 0.013 min
Response: 23104336
Conc: 12.36 ng/ml

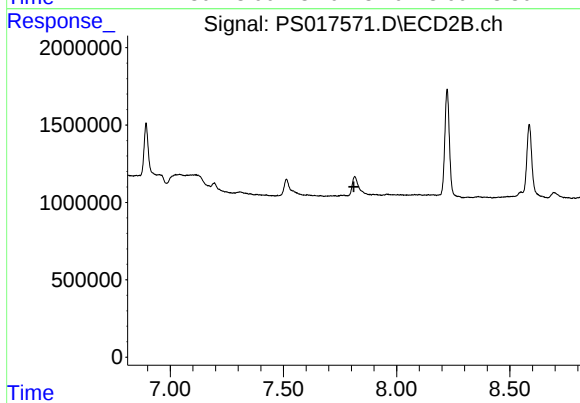

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.811 min
Response: 0
Conc: N.D.

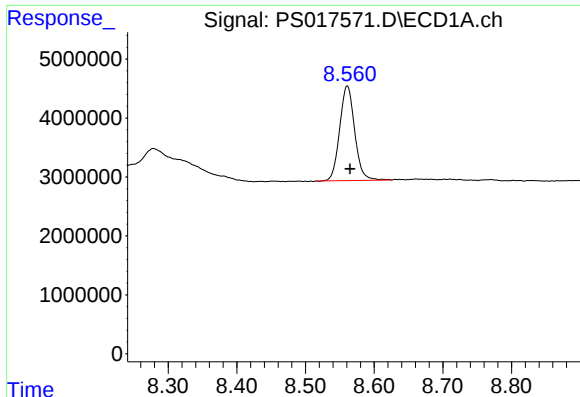

#10 Pentachlorophenol


R.T.: 8.561 min
Delta R.T.: -0.004 min
Response: 24425707
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :

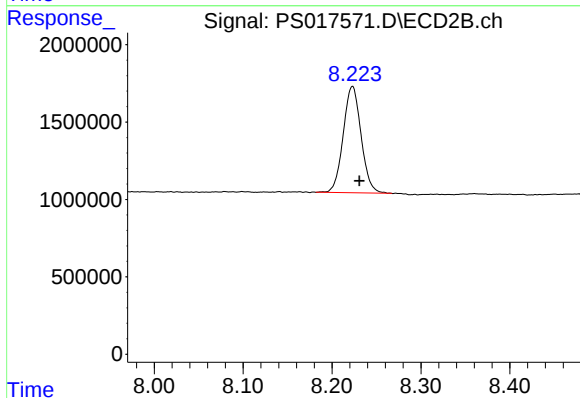


#10 Pentachlorophenol

R.T.: 8.223 min
Delta R.T.: -0.008 min
Response: 9596892
Conc: 1.14 ng/ml

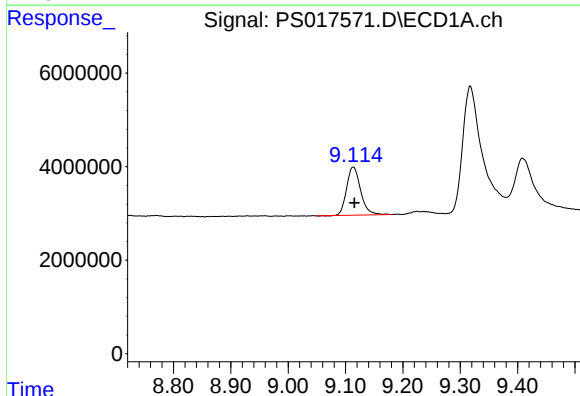


#11 2,4,5-TP (SILVEX)

R.T.: 9.113 min
Delta R.T.: -0.002 min
Response: 17445184
Conc: 2.09 ng/ml

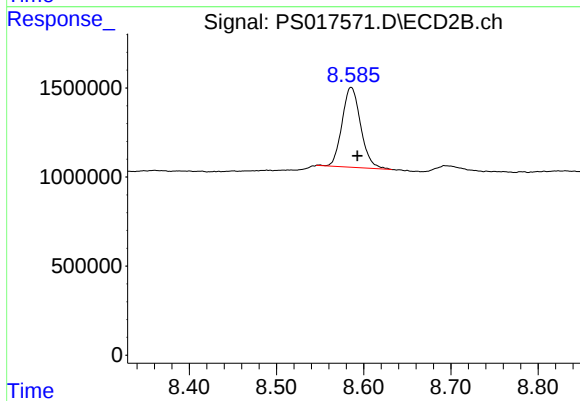

#11 2,4,5-TP (SILVEX)


R.T.: 8.586 min
Delta R.T.: -0.007 min
Response: 6653365
Conc: 1.88 ng/ml

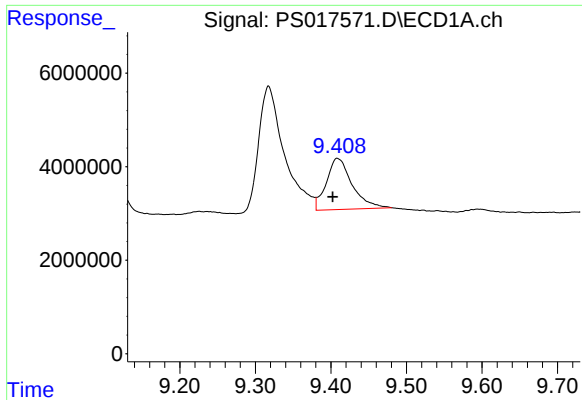

#12 2,4,5-T


R.T.: 9.409 min
Delta R.T.: 0.006 min
Response: 26000737
Conc: 3.08 ng/ml

Instrument :
ECD_S
ClientSampleId :

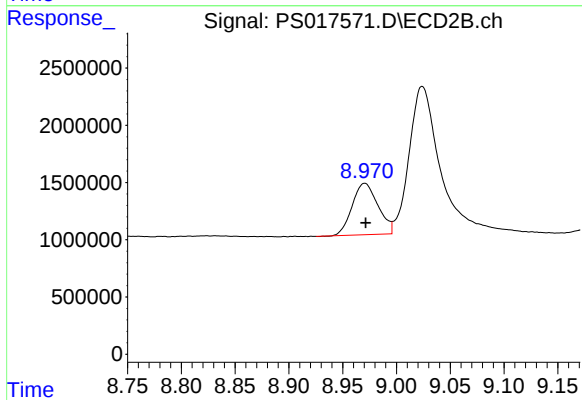


#12 2,4,5-T

R.T.: 8.971 min
Delta R.T.: 0.000 min
Response: 7527503
Conc: 2.26 ng/ml

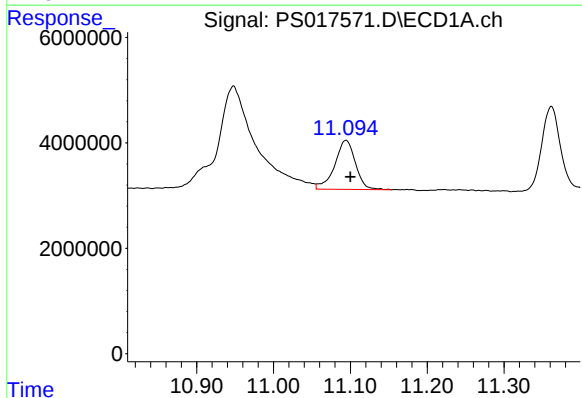


#14 DINOSEB

R.T.: 11.094 min
Delta R.T.: -0.006 min
Response: 17380285
Conc: 2.79 ng/ml

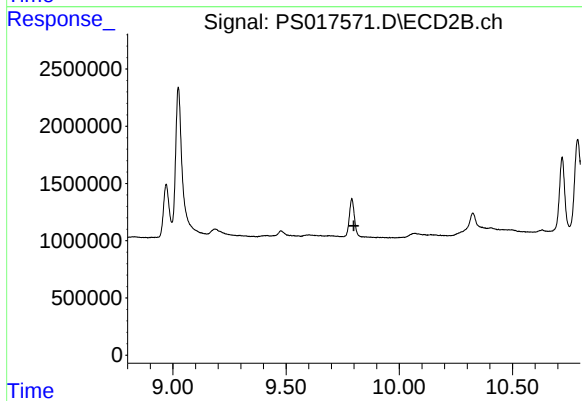

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 9.799 min
Response: 0
Conc: N.D.

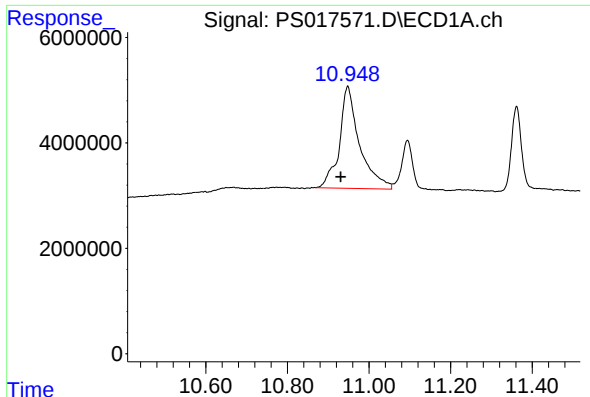

#15 Picloram


R.T.: 10.948 min
Delta R.T.: 0.018 min
Response: 66360905
Conc: 5.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

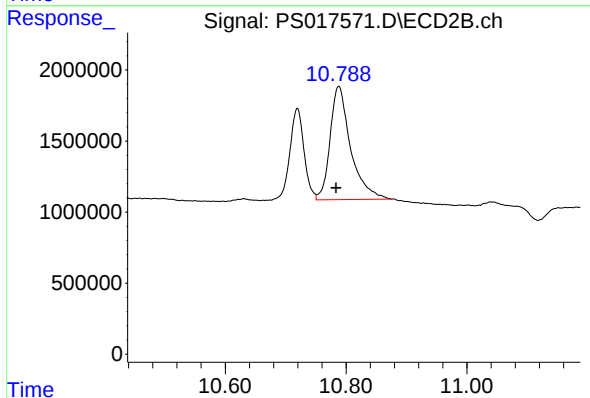


#15 Picloram

R.T.: 10.788 min
Delta R.T.: 0.005 min
Response: 18821023
Conc: 4.31 ng/ml

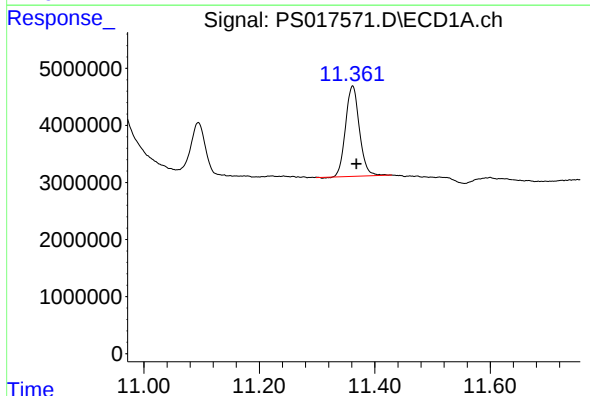

#16 DCPA

R.T.: 11.362 min
Delta R.T.: -0.006 min
Response: 26424312
Conc: 2.47 ng/ml

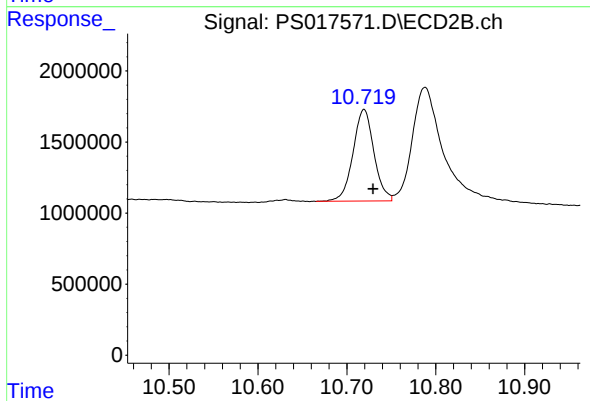

#16 DCPA

R.T.: 10.719 min
Delta R.T.: -0.010 min
Response: 10510328
Conc: 2.39 ng/ml