

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
 Data File : PS007953.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2019 10:22
 Operator : SM\AJ
 Sample : PB125285BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB125285BL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 12:09:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.429	5.154	494.9E6	295.3E6	316.334	380.613
Target Compounds							
1) T	Dalapon	1.991	1.711	130.7E6	191.7E6	64.106	161.377 #
2) T	3,5-DICHL...	0.000	4.489	0	50400006	N.D.	48.701
5) T	DICAMBA	5.516	0.000	70625443	0	12.413	N.D. #
7) T	MCPA	5.891	5.522	33687838	28637222	5.648	8.987 #
9) T	2,4-D	6.475	6.057	73671118	13090134	45.793	14.814 #
10) T	Pentachlo...	0.000	6.366	0	42804645	N.D.	3.921
11) T	2,4,5-TP ...	0.000	6.756	0	26933810	N.D.	6.280
15) T	Picloram	0.000	8.921	0	28567408	N.D.	4.625



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
Data File : PS007953.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2019 10:22
Operator : SM\AJ
Sample : PB125285BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
PB125285BL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 12:09:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

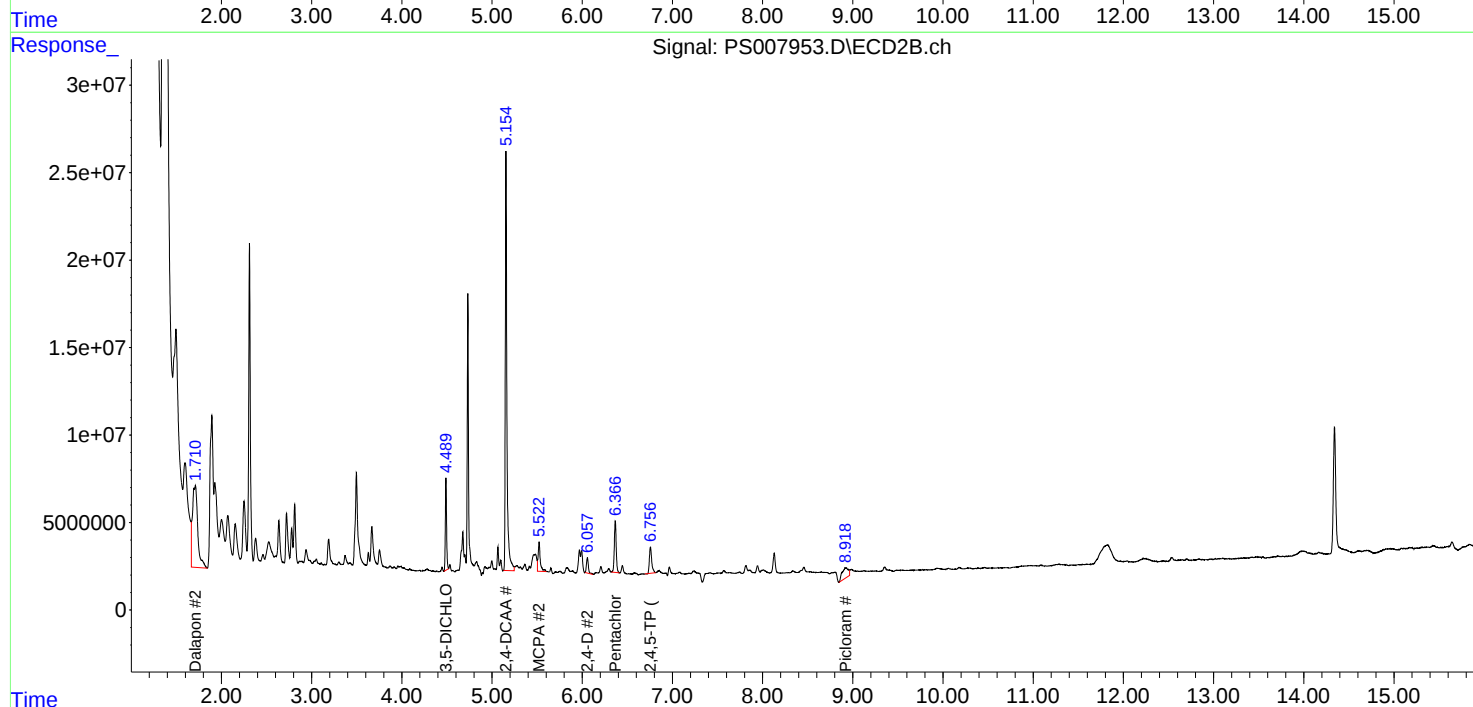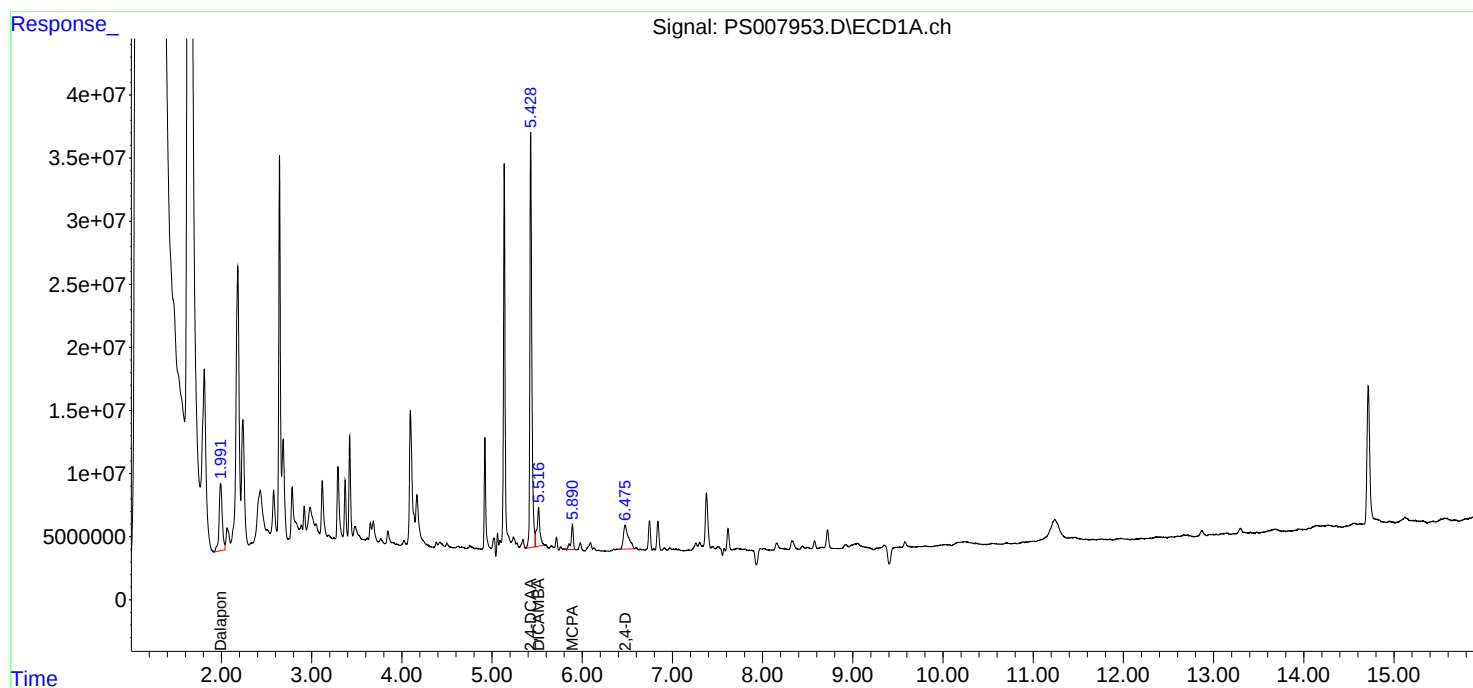


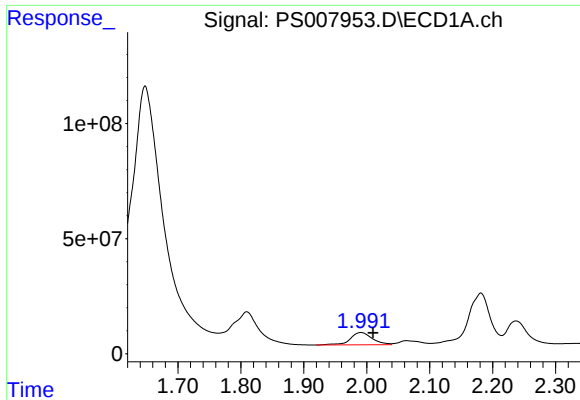

#1 Dalapon


R.T.: 1.991 min
Delta R.T.: -0.019 min
Response: 130732602
Conc: 64.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125285BL

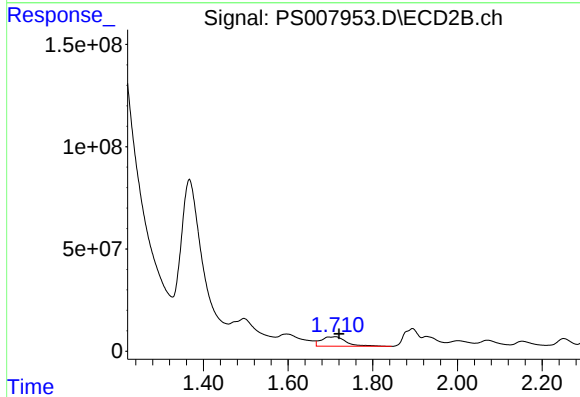


#1 Dalapon

R.T.: 1.711 min
Delta R.T.: -0.009 min
Response: 191682742
Conc: 161.38 ng/ml

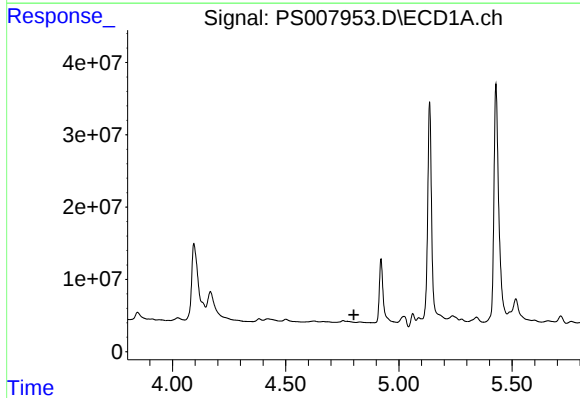


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

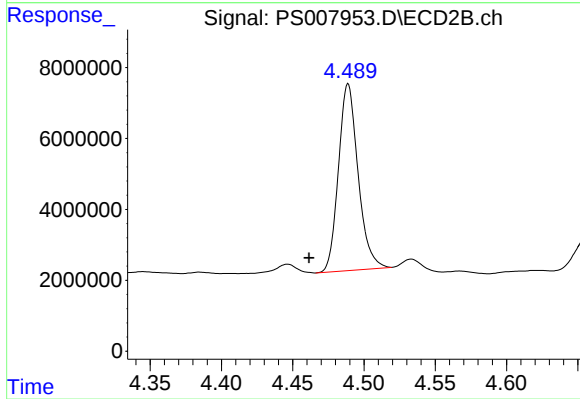

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.489 min
Delta R.T.: 0.028 min
Response: 50400006
Conc: 48.70 ng/ml

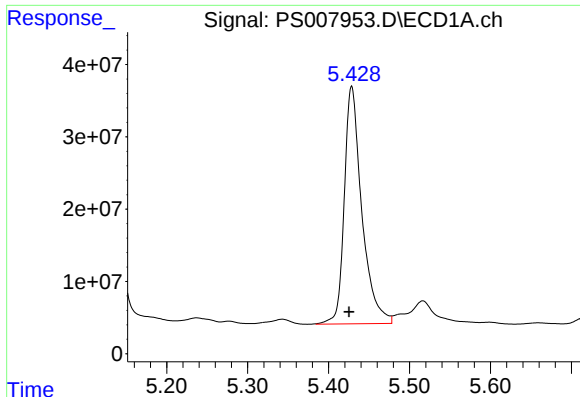

#4 2,4-DCAA


R.T.: 5.429 min
Delta R.T.: 0.004 min
Response: 494852237
Conc: 316.33 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB125285BL

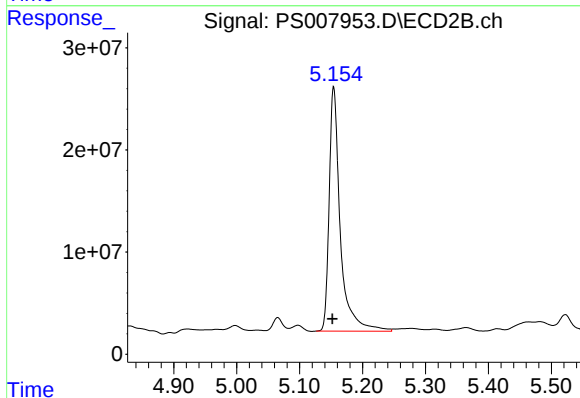


#4 2,4-DCAA

R.T.: 5.154 min
Delta R.T.: 0.003 min
Response: 295324241
Conc: 380.61 ng/ml

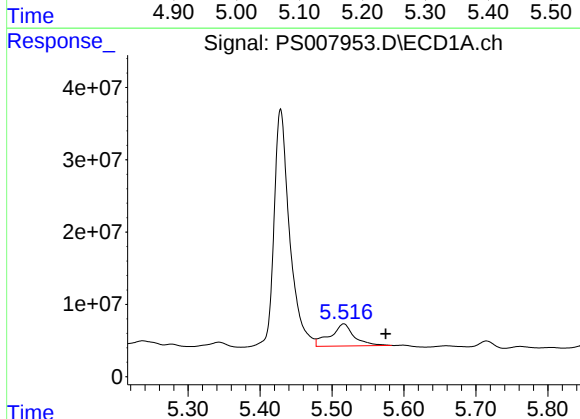


#5 DICAMBA

R.T.: 5.516 min
Delta R.T.: -0.059 min
Response: 70625443
Conc: 12.41 ng/ml

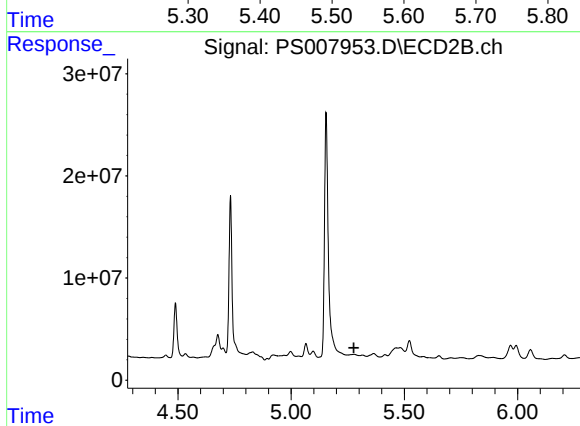

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

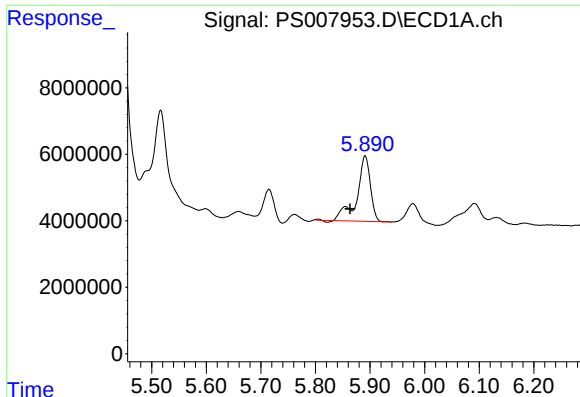

#7 MCPA


R.T.: 5.891 min
Delta R.T.: 0.027 min
Response: 33687838
Conc: 5.65 ug/ml

Instrument :
ECD_S
ClientSampleId :
PB125285BL

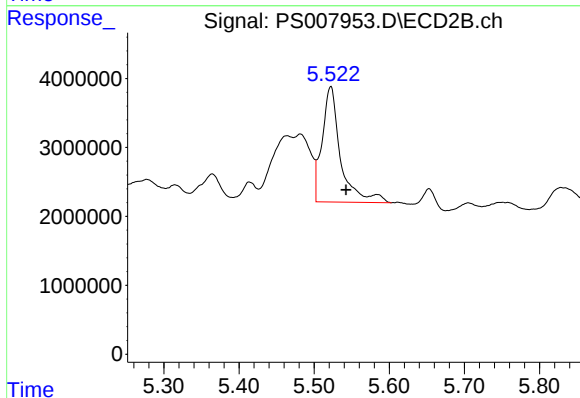


#7 MCPA

R.T.: 5.522 min
Delta R.T.: -0.021 min
Response: 28637222
Conc: 8.99 ug/ml

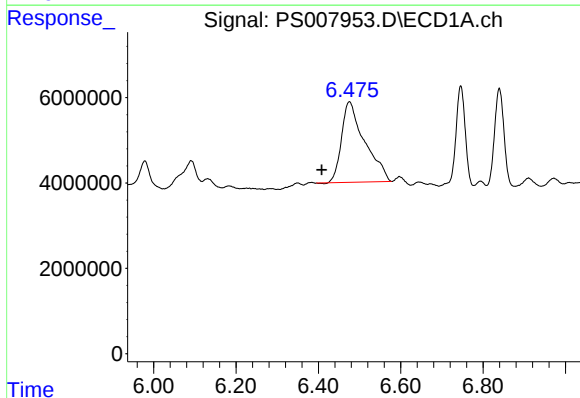


#9 2,4-D

R.T.: 6.475 min
Delta R.T.: 0.067 min
Response: 73671118
Conc: 45.79 ng/ml

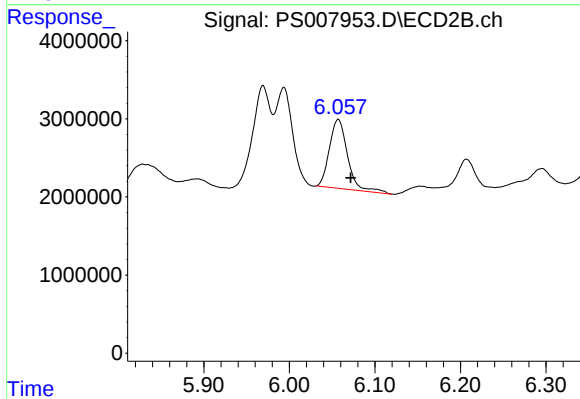

#9 2,4-D


R.T.: 6.057 min
Delta R.T.: -0.015 min
Response: 13090134
Conc: 14.81 ng/ml

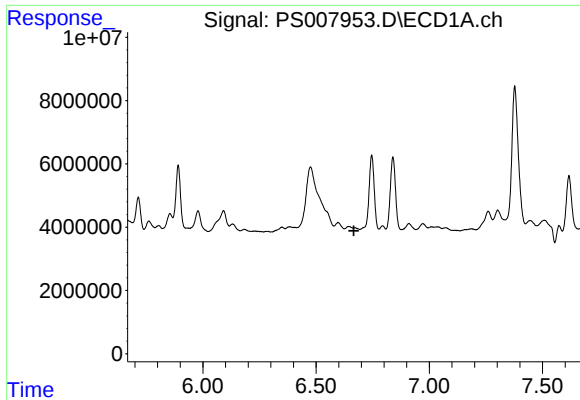

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125285BL

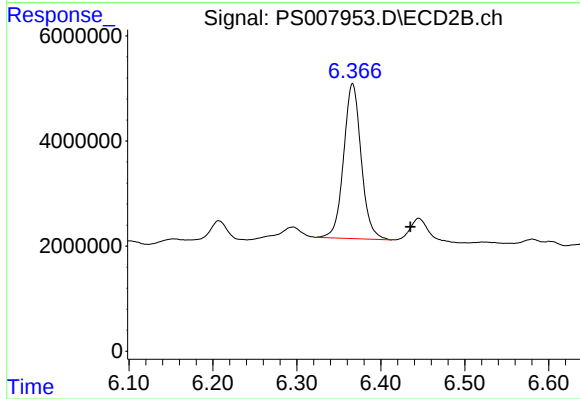


#10 Pentachlorophenol

R.T.: 6.366 min
Delta R.T.: -0.069 min
Response: 42804645
Conc: 3.92 ng/ml

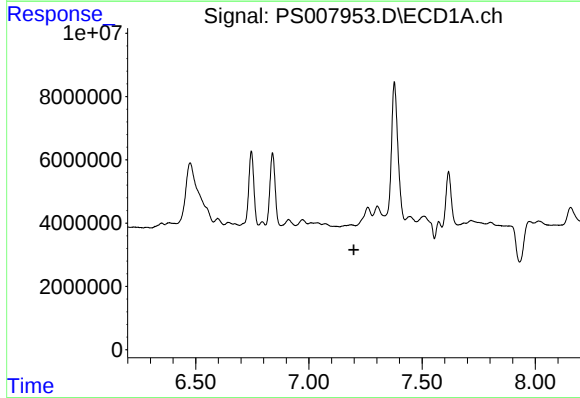


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

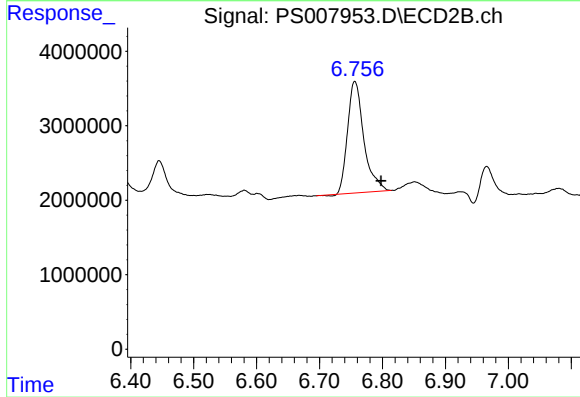

#11 2,4,5-TP (SILVEX)


R.T.: 6.756 min
Delta R.T.: -0.042 min
Response: 26933810
Conc: 6.28 ng/ml

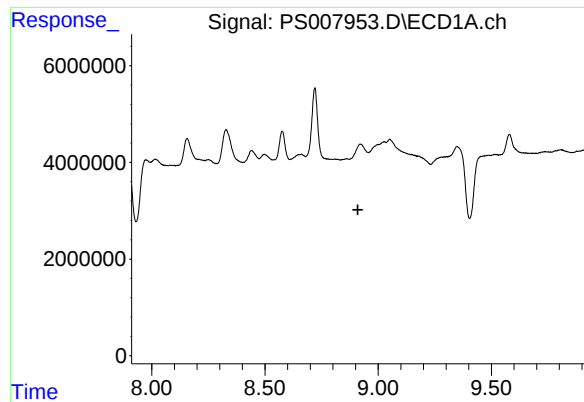

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB125285BL

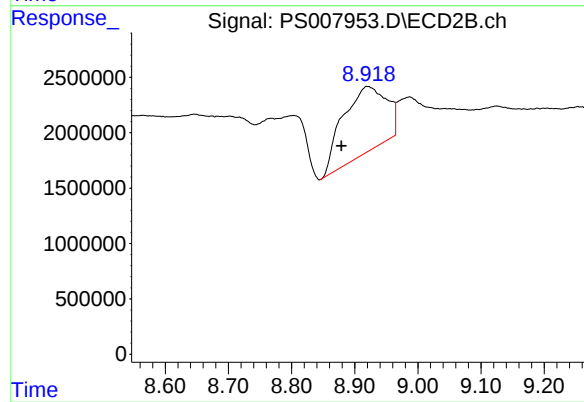

#15 Picloram

R.T.: 8.921 min
Delta R.T.: 0.041 min
Response: 28567408
Conc: 4.63 ng/ml