

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
 Data File : PS007976.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2019 18:56
 Operator : SM\AJ
 Sample : K6119-04
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SB-6-(7-9)

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:32:34 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.440	5.169	242.2E6	111.1E6	154.817	143.179
Target Compounds							
1) T	Dalapon	2.005	0.000	74480402	0	36.522	N.D. #
2) T	3,5-DICHL...	0.000	4.448	0	7653308	N.D.	7.395
5) T	DICAMBA	5.532	0.000	60159646	0	10.574	N.D. #
7) T	MCPA	5.906	5.537	26898702	27142318	4.510	8.518 #
8) T	DICHLORPROP	0.000	5.827	0	9617959	N.D.	13.417
9) T	2,4-D	0.000	6.072	0	6894117	N.D.	7.802
10) T	Pentachlo...	0.000	6.381	0	59180523	N.D.	5.421
11) T	2,4,5-TP ...	0.000	6.766	0	43791622	N.D.	10.211
14) T	DINOSEB	0.000	7.958	0	19638947	N.D.	6.003
15) T	Picloram	0.000	8.914	0	16520883	N.D.	2.675



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
Data File : PS007976.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2019 18:56
Operator : SM\AJ
Sample : K6119-04
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SB-6-(7-9)

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:32:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

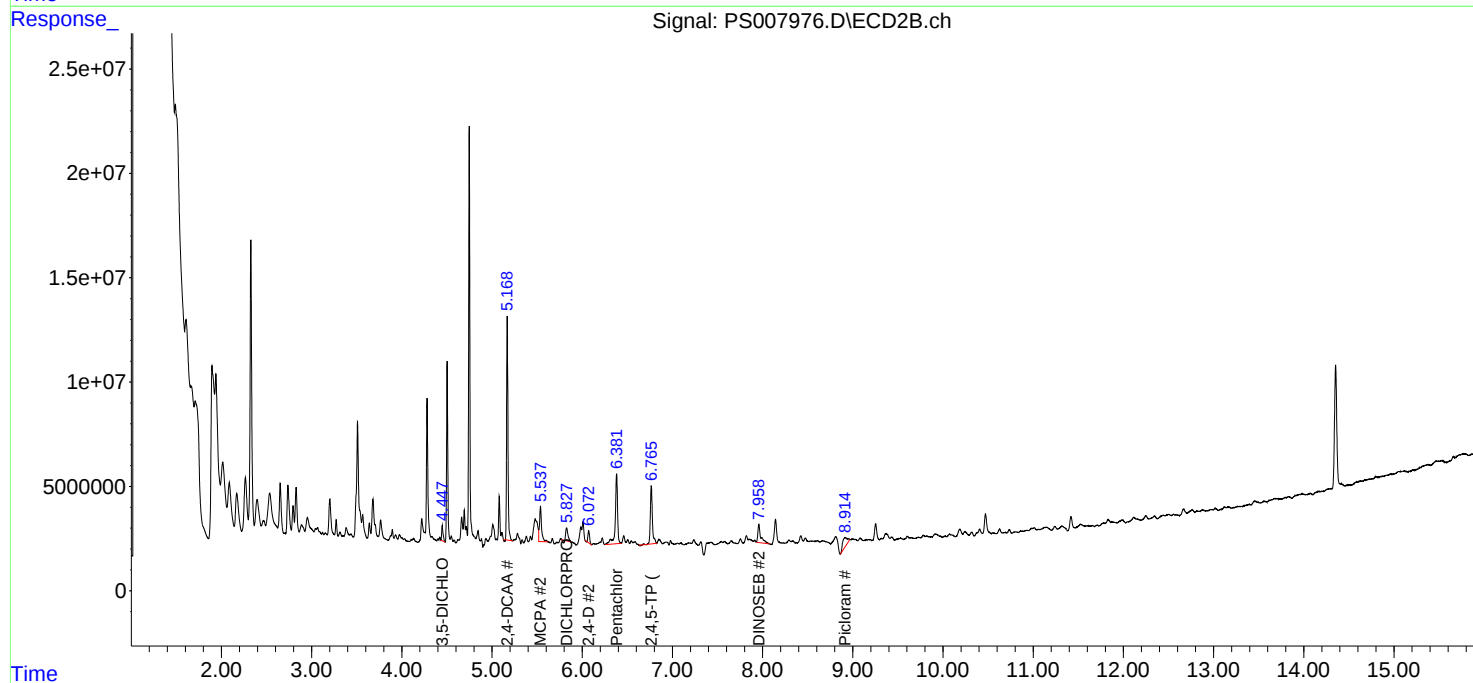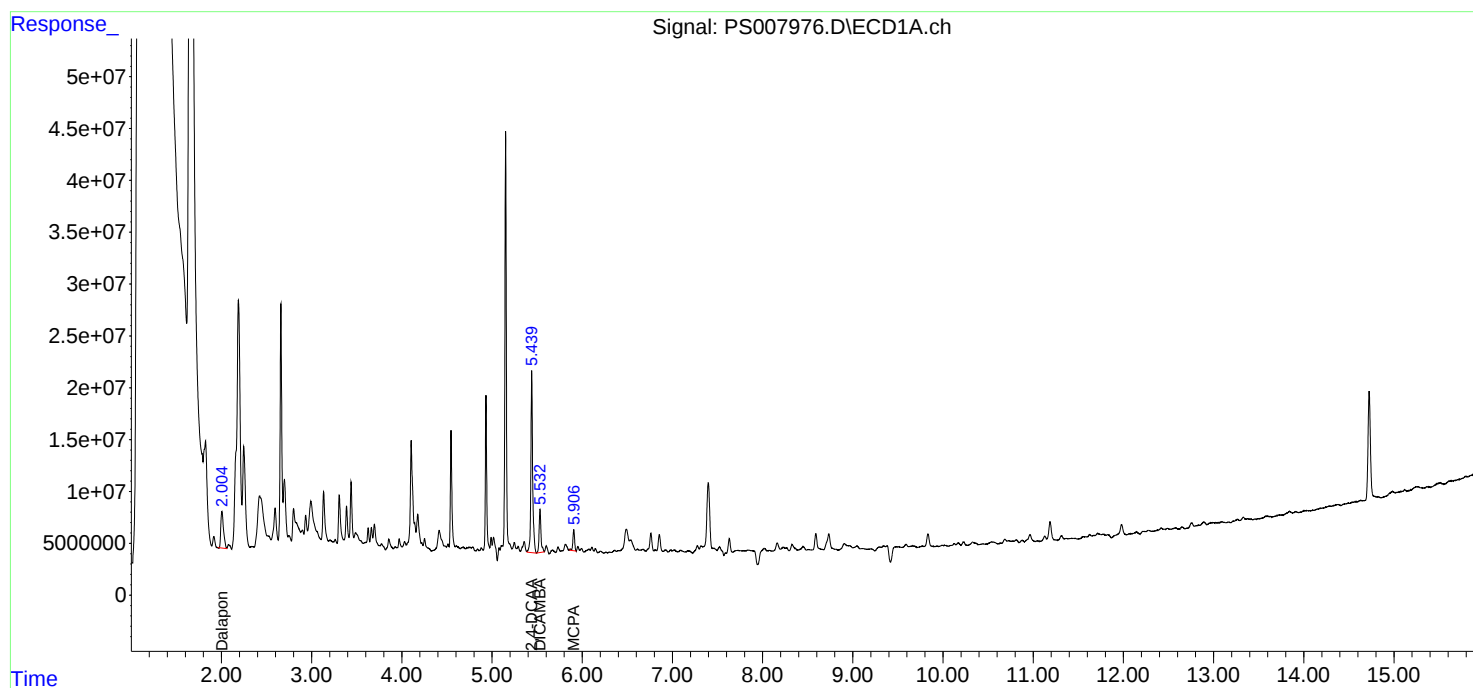


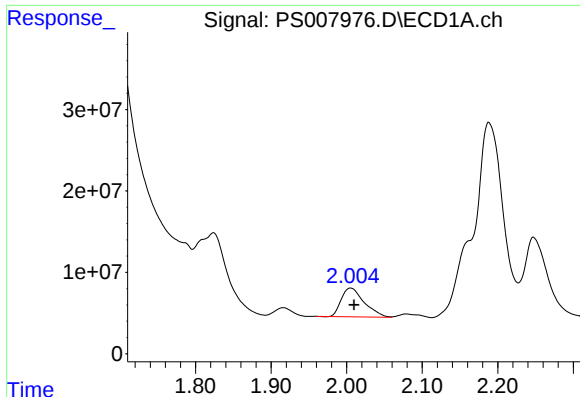

#1 Dalapon


R.T.: 2.005 min
Delta R.T.: -0.005 min
Response: 74480402
Conc: 36.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6-(7-9)

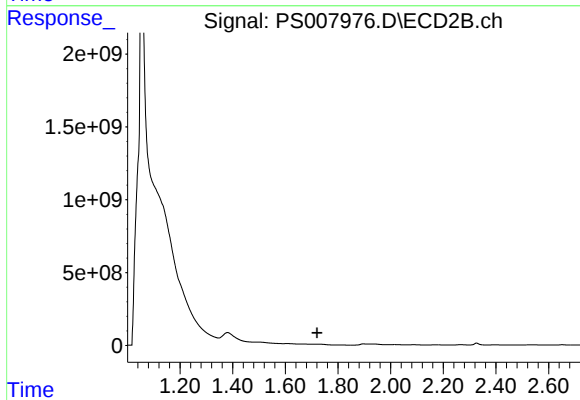


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 1.721 min
Response: 0
Conc: N.D.

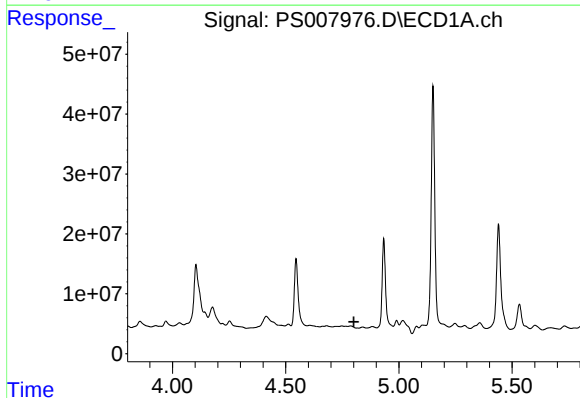


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

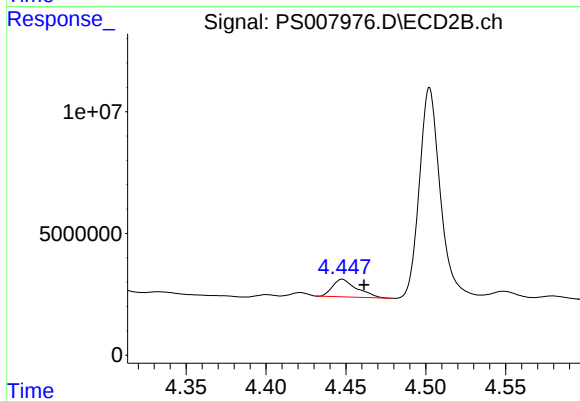

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.448 min
Delta R.T.: -0.013 min
Response: 7653308
Conc: 7.40 ng/ml

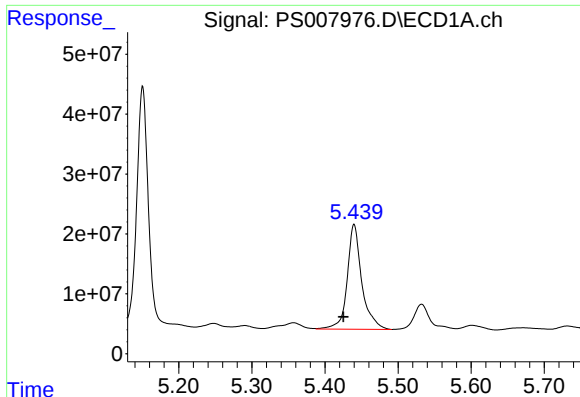

#4 2,4-DCAA


R.T.: 5.440 min
Delta R.T.: 0.015 min
Response: 242185987
Conc: 154.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6-(7-9)

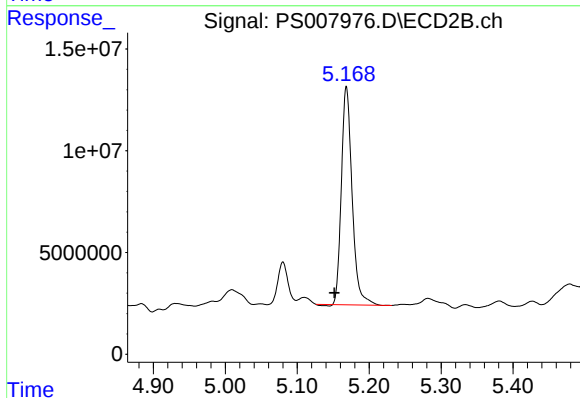


#4 2,4-DCAA

R.T.: 5.169 min
Delta R.T.: 0.017 min
Response: 111094945
Conc: 143.18 ng/ml

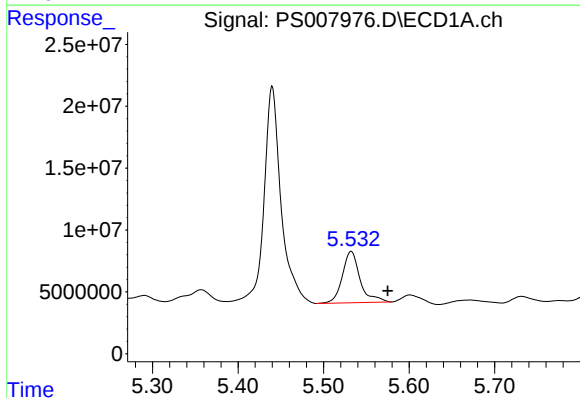


#5 DICAMBA

R.T.: 5.532 min
Delta R.T.: -0.043 min
Response: 60159646
Conc: 10.57 ng/ml

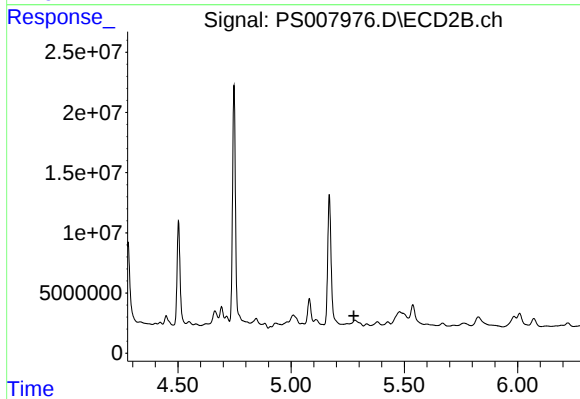

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 5.277 min
Response: 0
Conc: N.D.

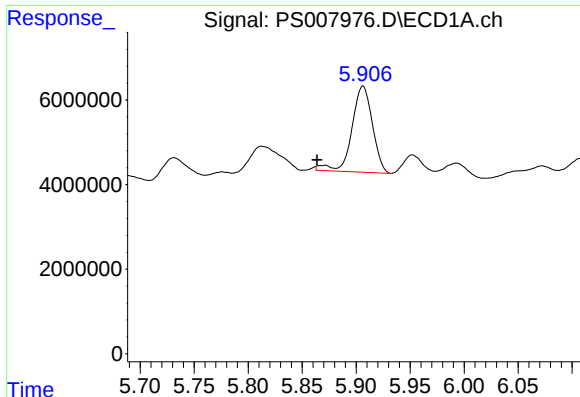

#7 MCPA


R.T.: 5.906 min
Delta R.T.: 0.042 min
Response: 26898702
Conc: 4.51 ug/ml

Instrument :
ECD_S
ClientSampleId :
SB-6-(7-9)

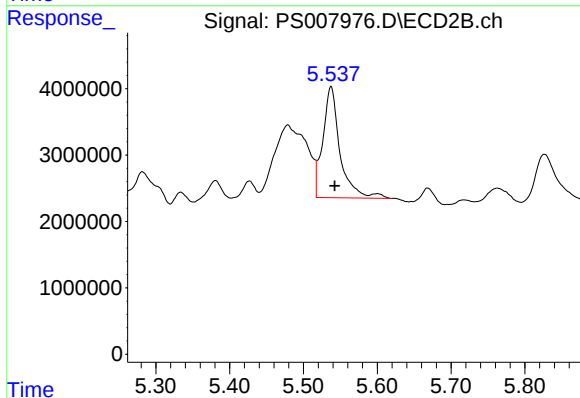


#7 MCPA

R.T.: 5.537 min
Delta R.T.: -0.005 min
Response: 27142318
Conc: 8.52 ug/ml

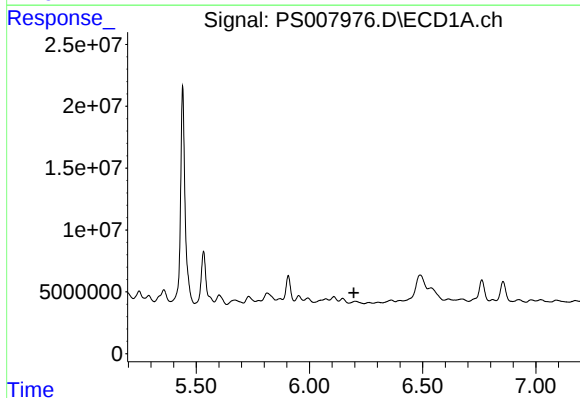


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

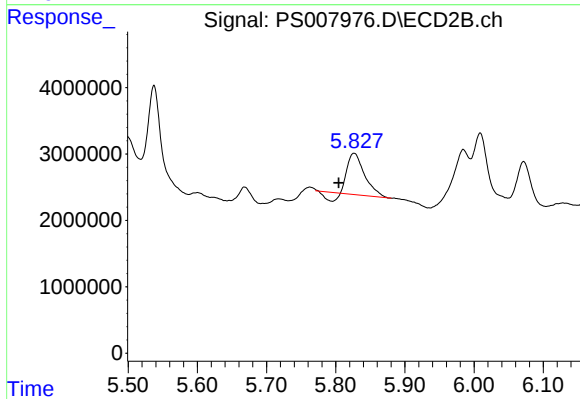

#8 DICHLORPROP


R.T.: 5.827 min
Delta R.T.: 0.022 min
Response: 9617959
Conc: 13.42 ng/ml

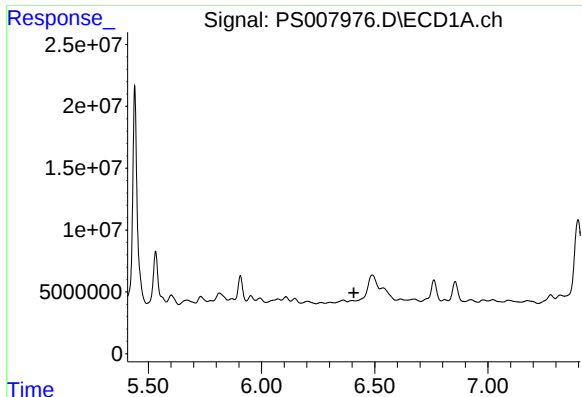

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SB-6-(7-9)

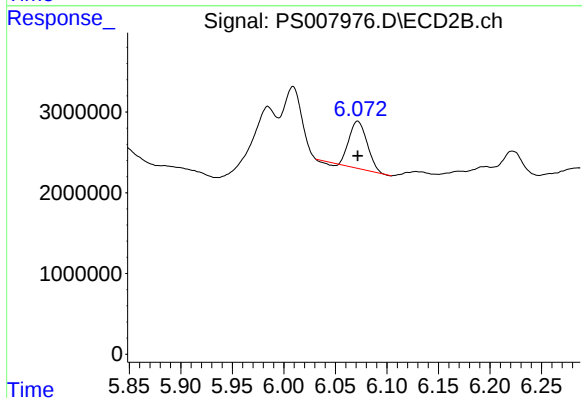


#9 2,4-D

R.T.: 6.072 min
Delta R.T.: 0.000 min
Response: 6894117
Conc: 7.80 ng/ml

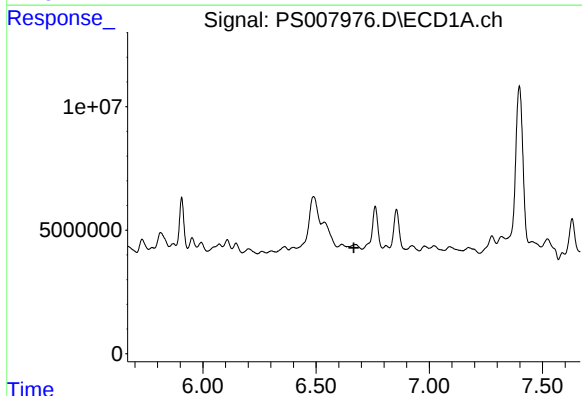


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

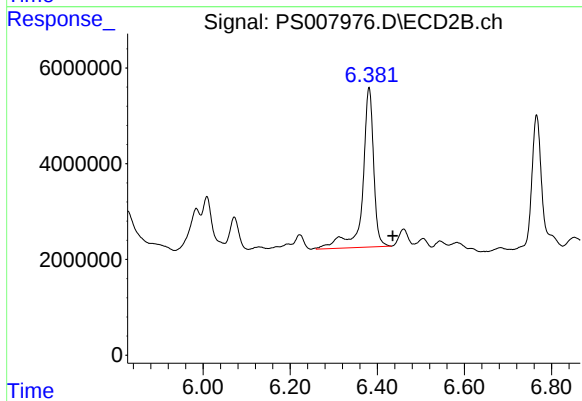

#10 Pentachlorophenol


R.T.: 6.381 min
Delta R.T.: -0.054 min
Response: 59180523
Conc: 5.42 ng/ml

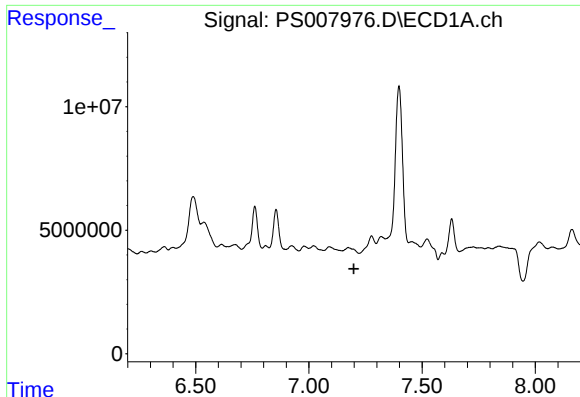

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SB-6-(7-9)

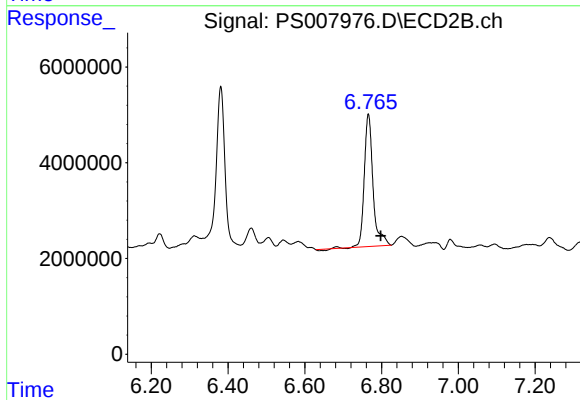


#11 2,4,5-TP (SILVEX)

R.T.: 6.766 min
Delta R.T.: -0.032 min
Response: 43791622
Conc: 10.21 ng/ml

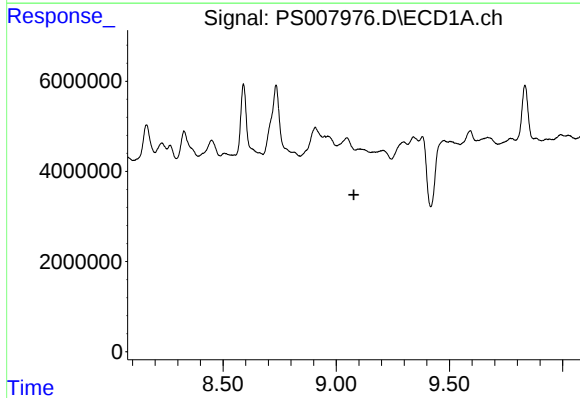


#14 DINOSEB

R.T.: 0.000 min
Exp R.T.: 9.078 min
Response: 0
Conc: N.D.

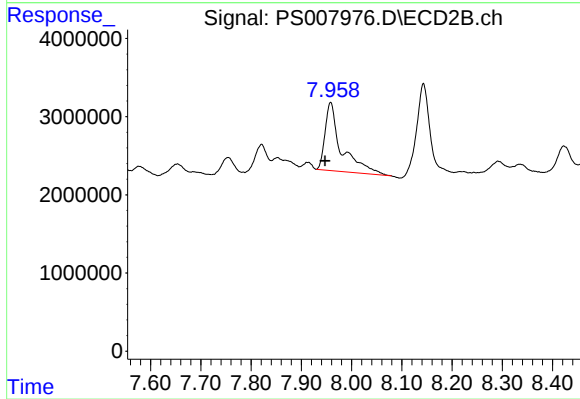

#14 DINOSEB


R.T.: 7.958 min
Delta R.T.: 0.011 min
Response: 19638947
Conc: 6.00 ng/ml

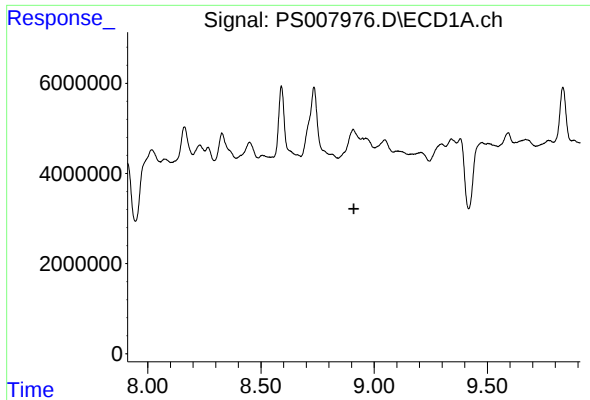

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SB-6-(7-9)

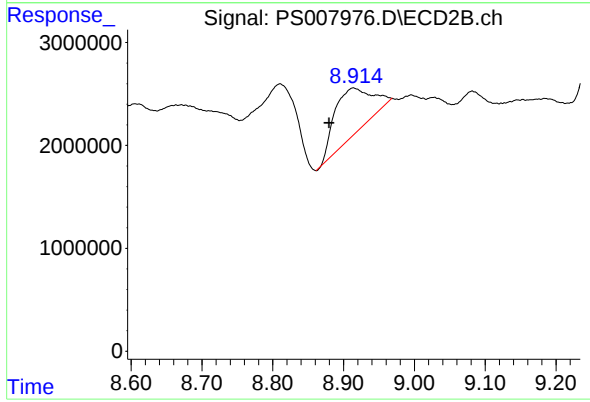

#15 Picloram

R.T.: 8.914 min
Delta R.T.: 0.035 min
Response: 16520883
Conc: 2.67 ng/ml