

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
 Data File : PS007977.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2019 19:18
 Operator : SM\AJ
 Sample : K6119-05
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:32:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.421	5.150	498.5E6	238.3E6	318.683	307.140
Target Compounds							
1) T	Dalapon	1.987	1.691	102.2E6	428.1E6	50.092	360.414 #
2) T	3,5-DICHL...	0.000	4.485	0	20164638	N.D.	19.485
3) T	4-Nitroph...	5.228	0.000	31777974	0	41.809	N.D. #
5) T	DICAMBA	5.514	0.000	52976486	0	9.311	N.D. #
7) T	MCPA	5.889	5.519	29949489	28602893	5.022	8.976 #
8) T	DICHLORPROP	0.000	5.809	0	7081348	N.D.	9.879
9) T	2,4-D	6.471	6.054	100.0E6	8486138	62.169	9.604 #
11) T	2,4,5-TP ...	0.000	6.749	0	9845294	N.D.	2.296



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
Data File : PS007977.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2019 19:18
Operator : SM\AJ
Sample : K6119-05
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:32:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

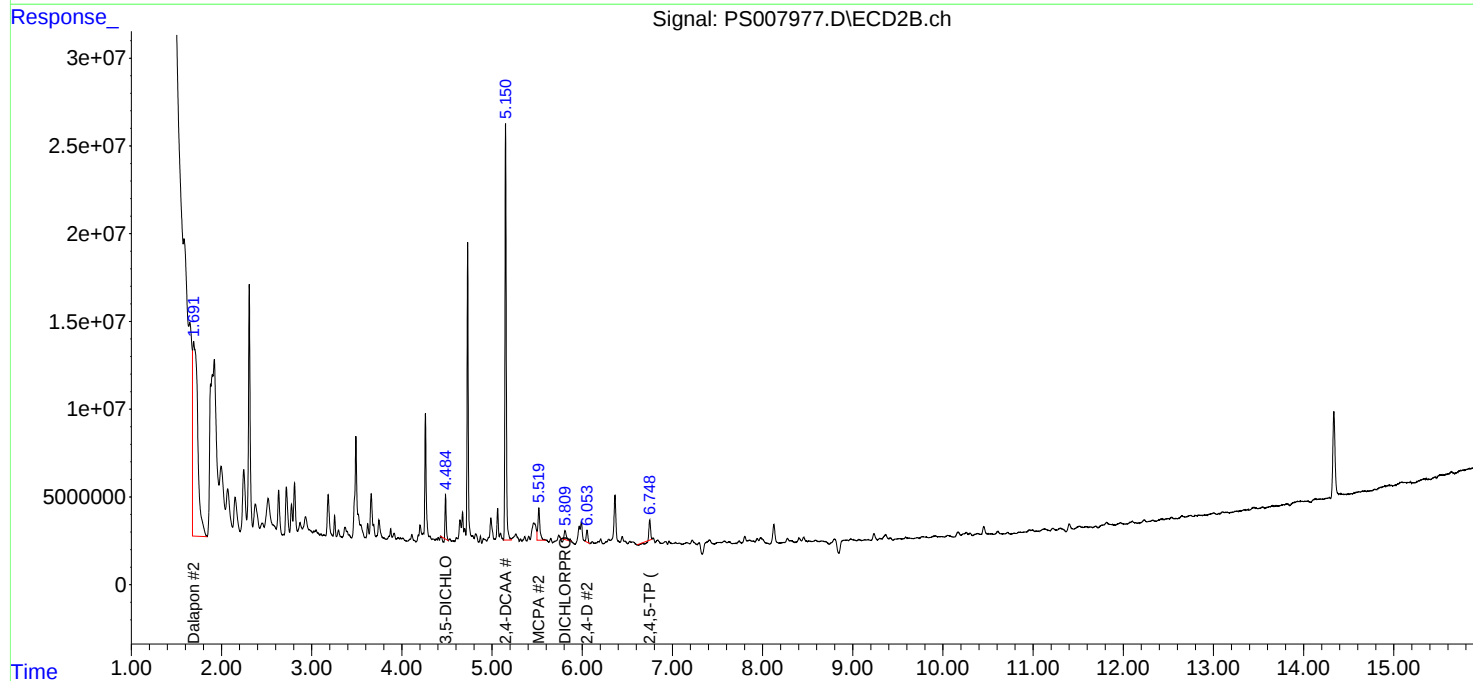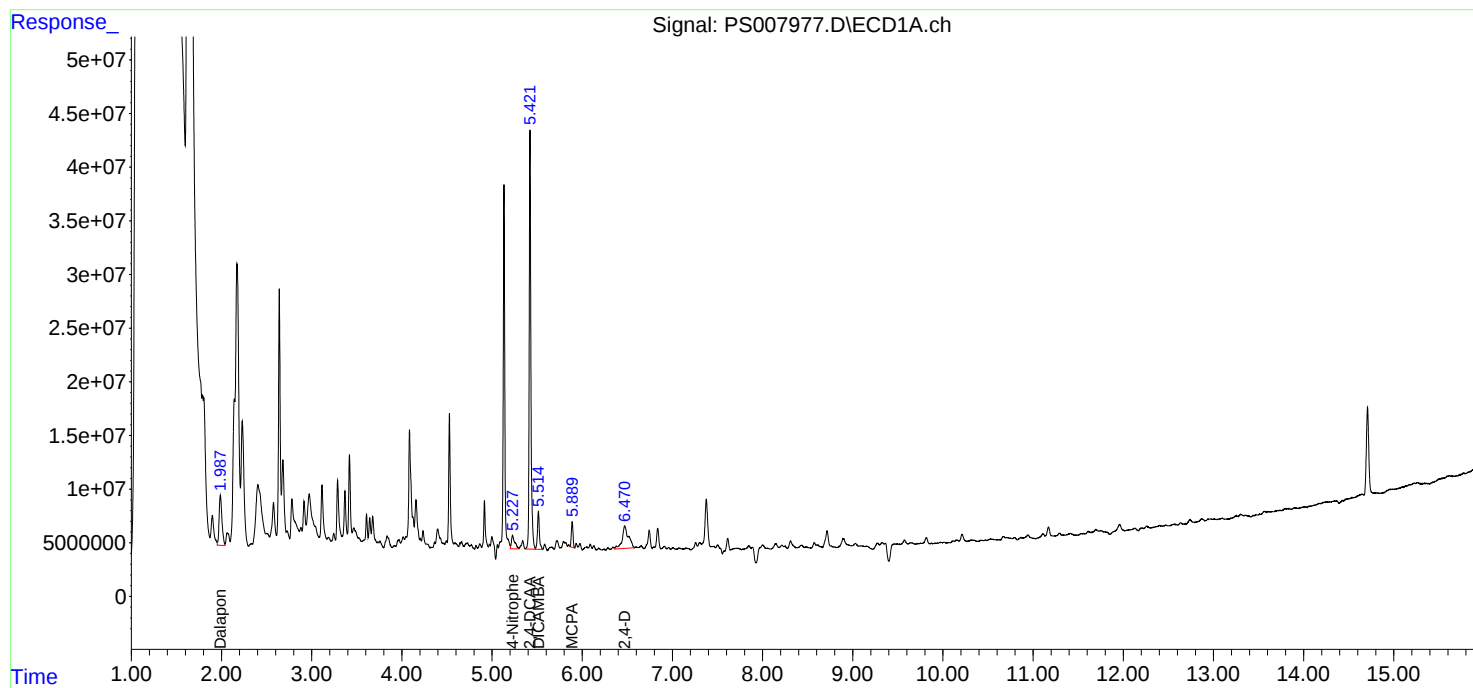


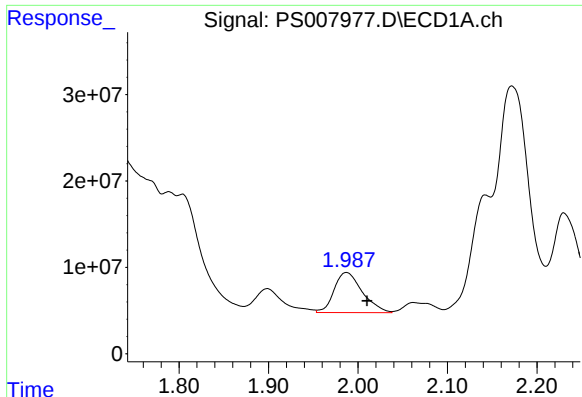

#1 Dalapon


R.T.: 1.987 min
Delta R.T.: -0.023 min
Response: 102153780
Conc: 50.09 ng/ml

Instrument :
ECD_S
ClientSampleId :

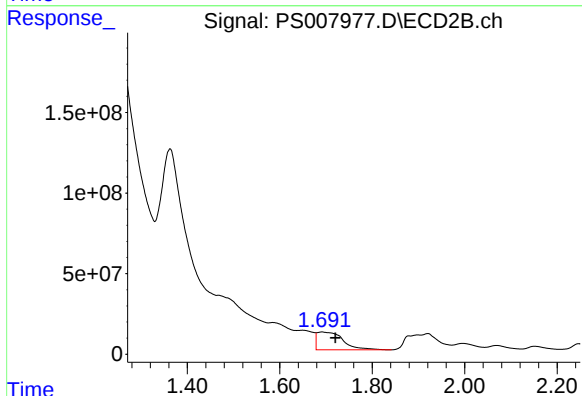


#1 Dalapon

R.T.: 1.691 min
Delta R.T.: -0.029 min
Response: 428096544
Conc: 360.41 ng/ml

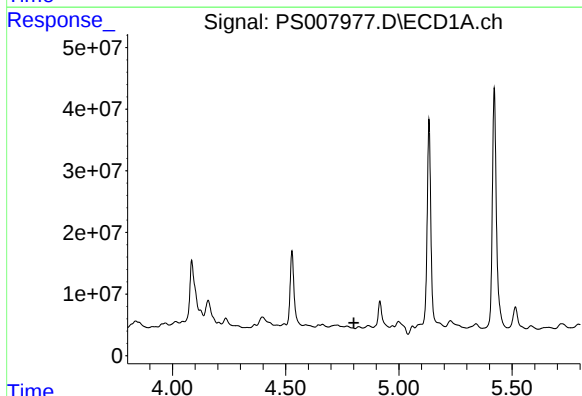


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

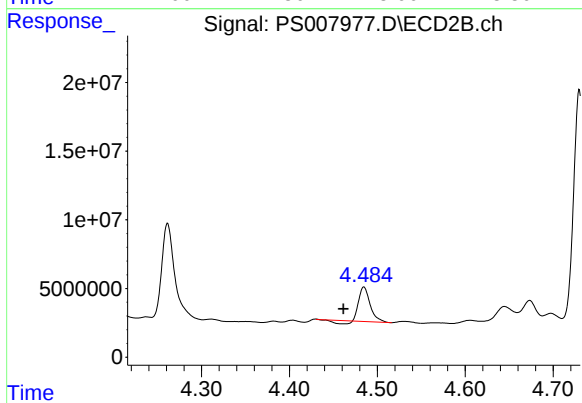

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.485 min
Delta R.T.: 0.024 min
Response: 20164638
Conc: 19.49 ng/ml

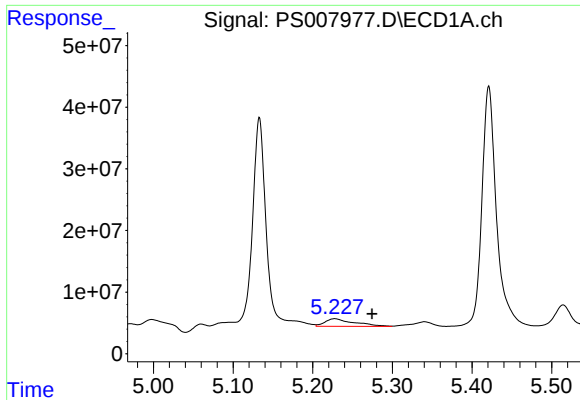

#3 4-Nitrophenol


R.T.: 5.228 min
Delta R.T.: -0.047 min
Response: 31777974
Conc: 41.81 ng/ml

Instrument :
ECD_S
ClientSampleId :

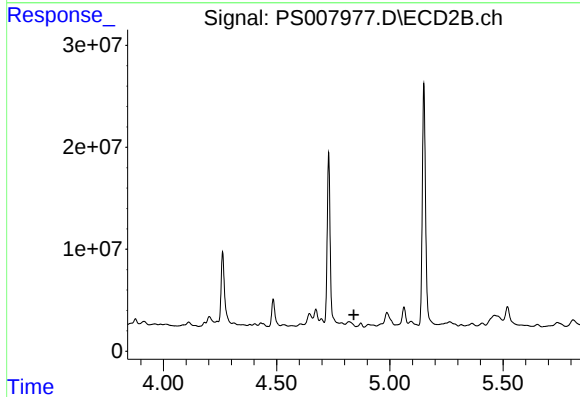


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 4.841 min
Response: 0
Conc: N.D.

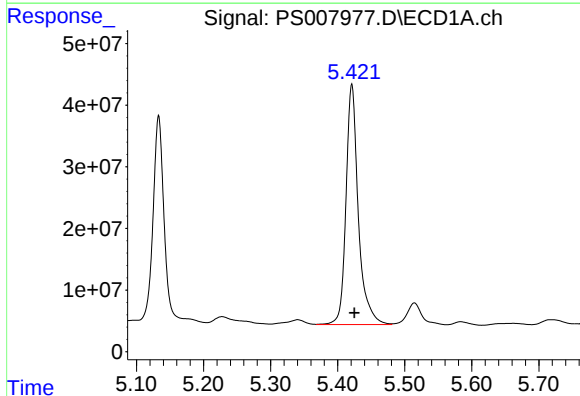


#4 2,4-DCAA

R.T.: 5.421 min
Delta R.T.: -0.004 min
Response: 498526475
Conc: 318.68 ng/ml

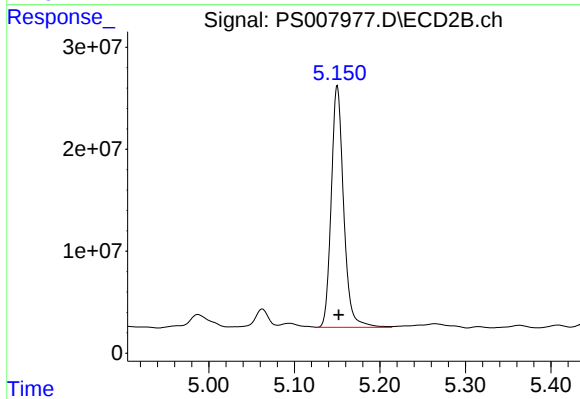

#4 2,4-DCAA


R.T.: 5.150 min
Delta R.T.: -0.002 min
Response: 238315564
Conc: 307.14 ng/ml

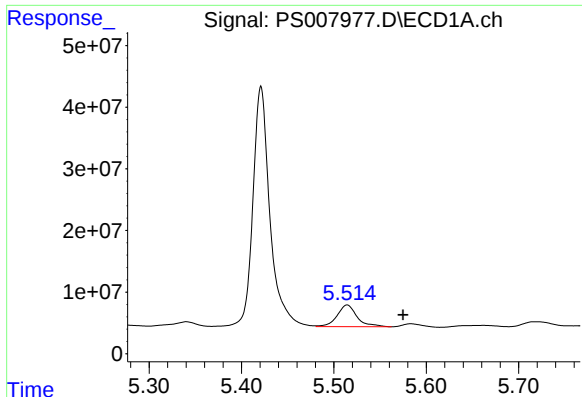

#5 DICAMBA


R.T.: 5.514 min
Delta R.T.: -0.060 min
Response: 52976486
Conc: 9.31 ng/ml

Instrument :
ECD_S
ClientSampleId :

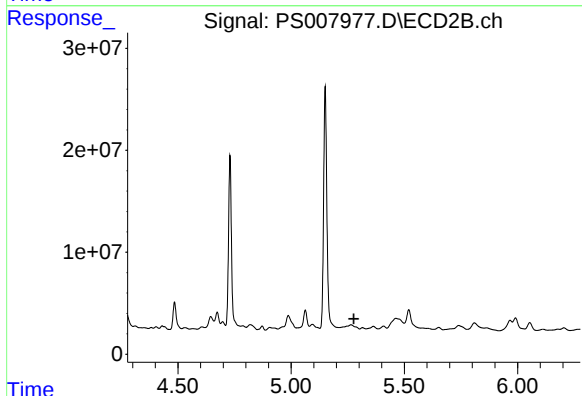


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

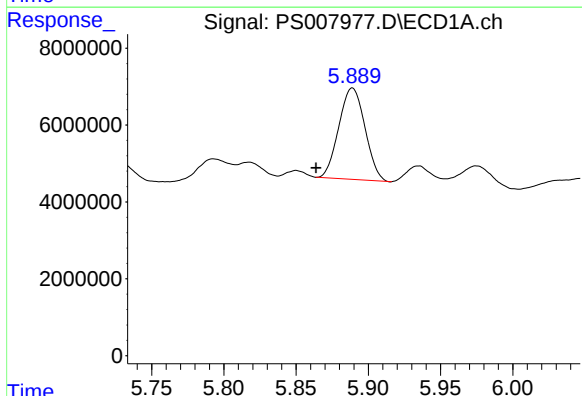


#7 MCPA

R.T.: 5.889 min
Delta R.T.: 0.025 min
Response: 29949489
Conc: 5.02 ug/ml

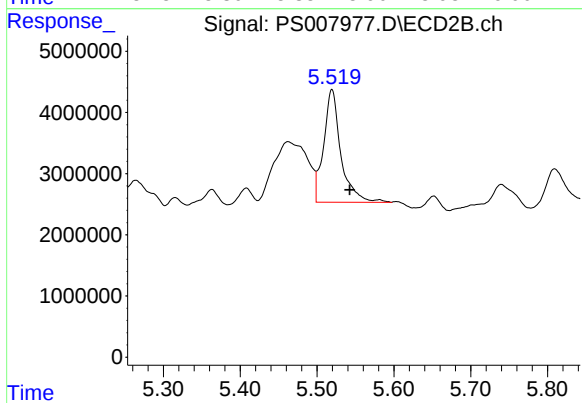

#7 MCPA


R.T.: 5.519 min
Delta R.T.: -0.023 min
Response: 28602893
Conc: 8.98 ug/ml

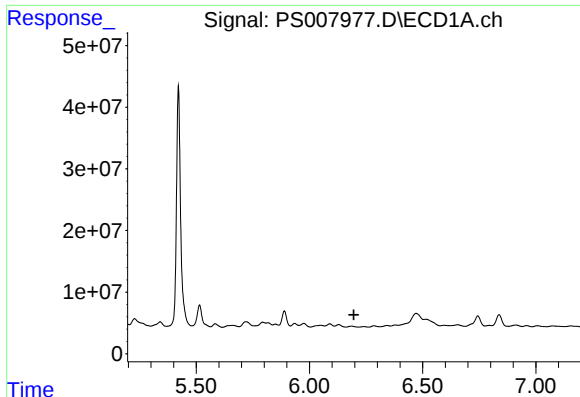

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

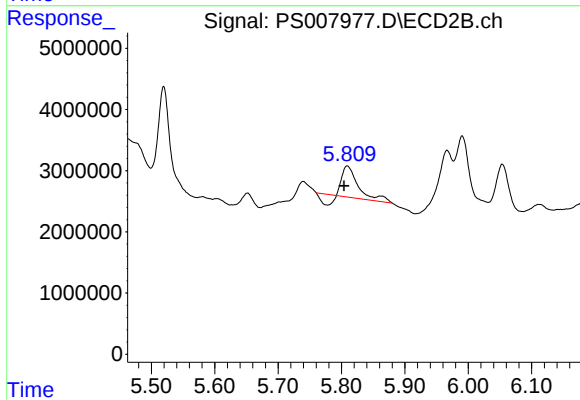


#8 DICHLORPROP

R.T.: 5.809 min
Delta R.T.: 0.005 min
Response: 7081348
Conc: 9.88 ng/ml

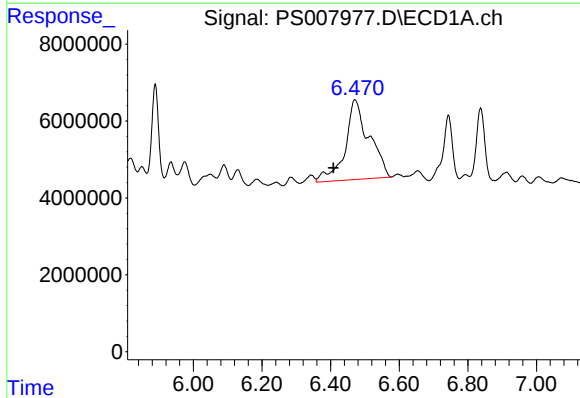


#9 2,4-D

R.T.: 6.471 min
Delta R.T.: 0.063 min
Response: 100017111
Conc: 62.17 ng/ml

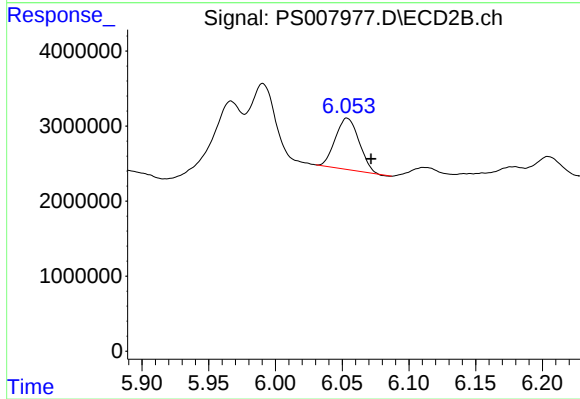

#9 2,4-D


R.T.: 6.054 min
Delta R.T.: -0.018 min
Response: 8486138
Conc: 9.60 ng/ml

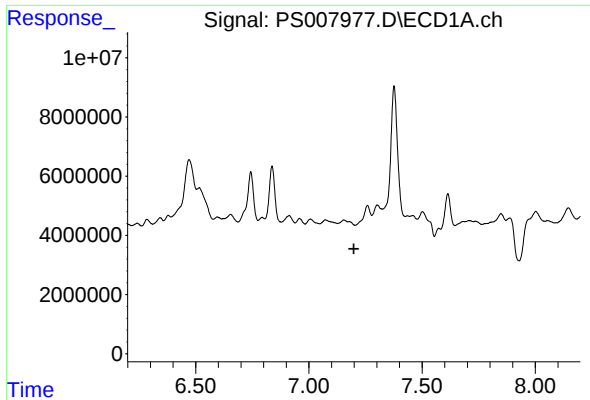

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

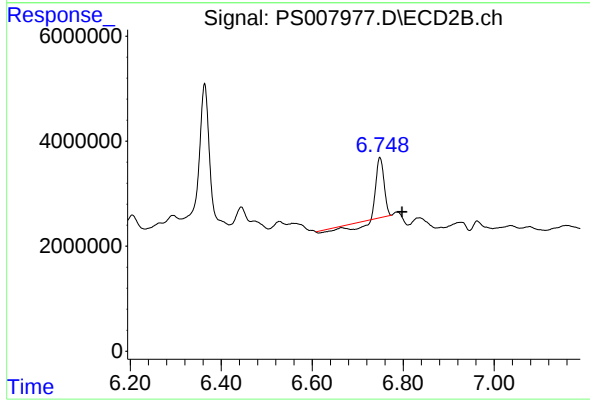

#11 2,4,5-TP (SILVEX)

R.T.: 6.749 min
Delta R.T.: -0.049 min
Response: 9845294
Conc: 2.30 ng/ml