

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
 Data File : PS007970.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2019 16:45
 Operator : SM\AJ
 Sample : K6174-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SOLID-COMP

Manual Integrations
 APPROVED

Ankita
 12/10/2019 10:26:48 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 17:03:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.444	5.174	718.6E6	358.5E6	459.381	462.066m

Target Compounds

 (f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
Data File : PS007970.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2019 16:45
Operator : SM\AJ
Sample : K6174-01
Misc :
ALS Vial : 20 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SOLID-COMP


Manual Integrations
APPROVED

Ankita
12/10/2019 10:26:48 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 17:03:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

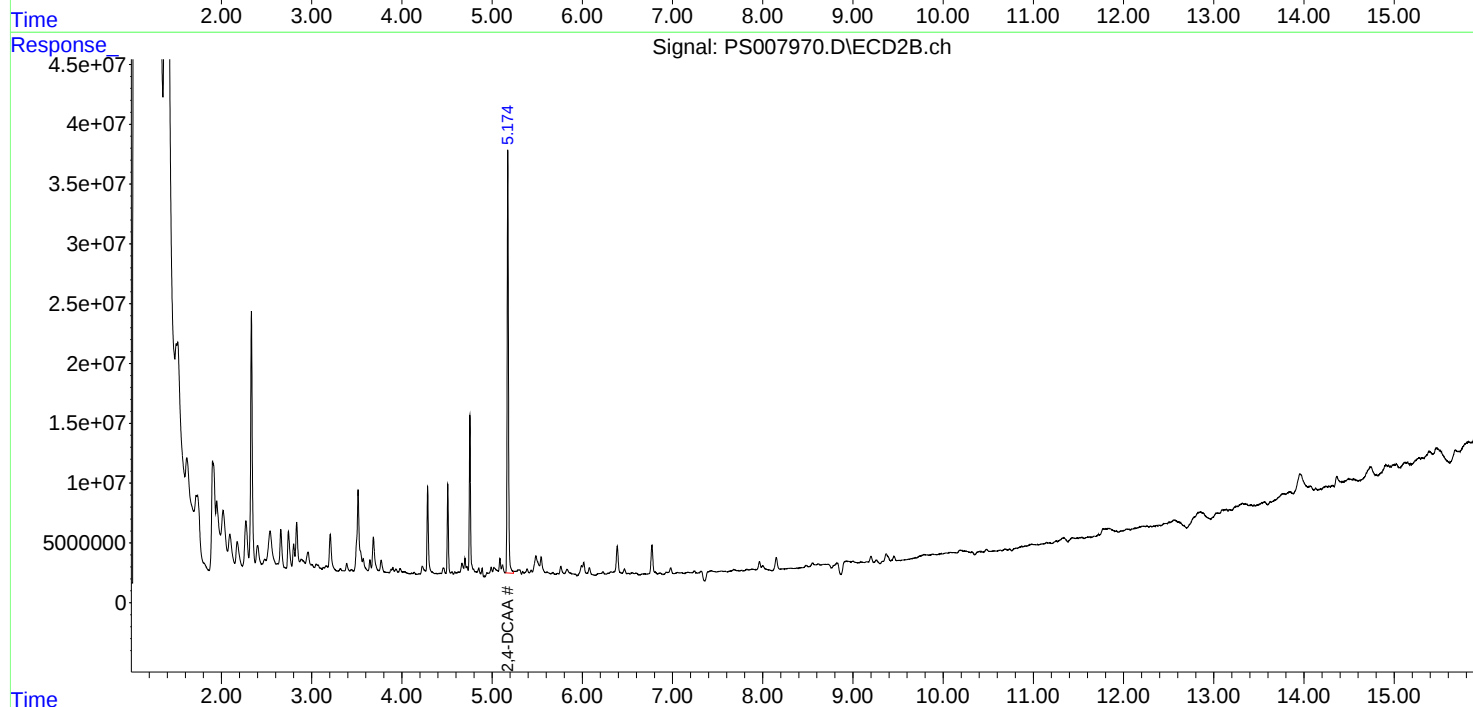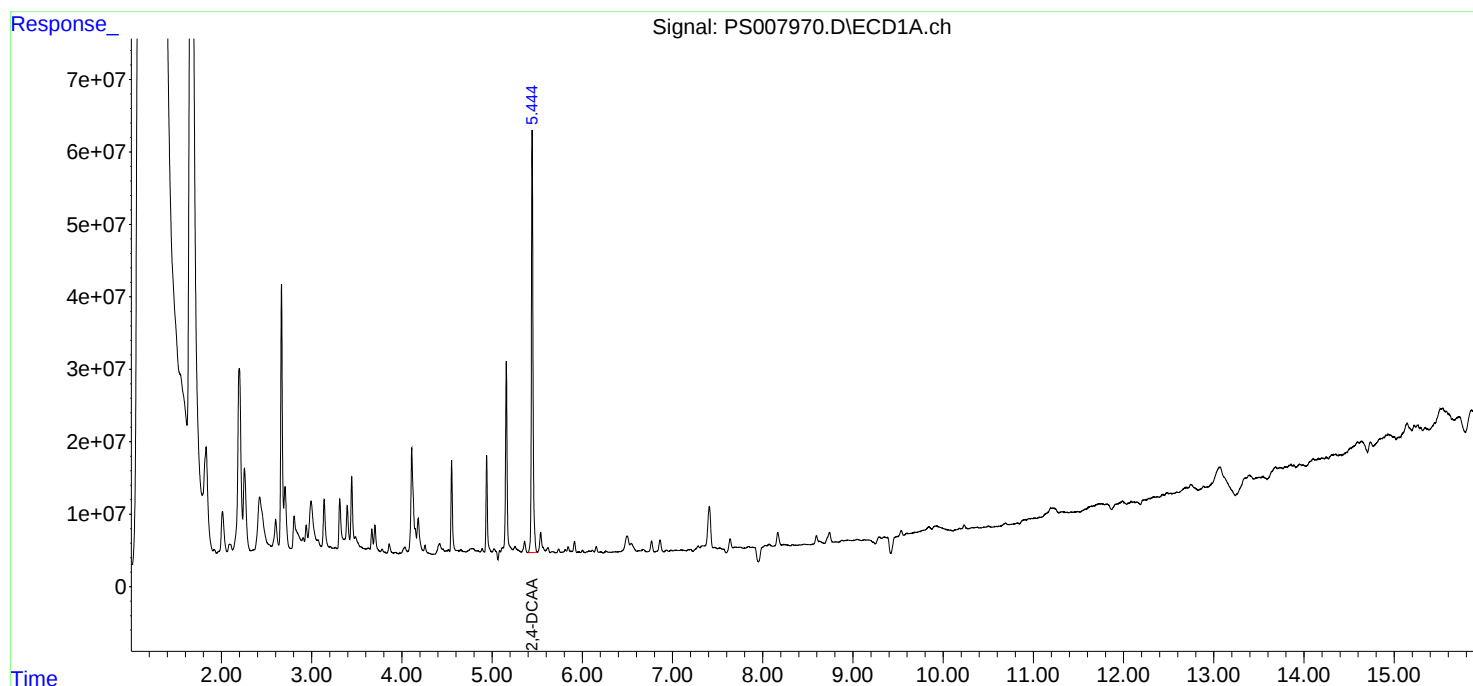

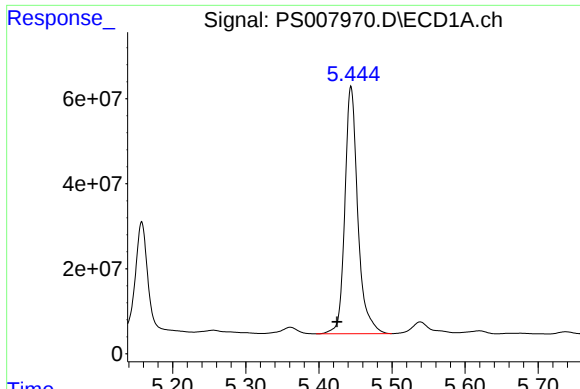


#4 2,4-DCAA

R.T.: 5.444 min
Delta R.T.: 0.019 min
Response: 718625307
Conc: 459.38 ng/ml

Instrument :
ECD_S
ClientSampleId :
SOLID-COMP

Manual Integrations
APPROVED

Ankita
12/10/2019 10:26:48 AM

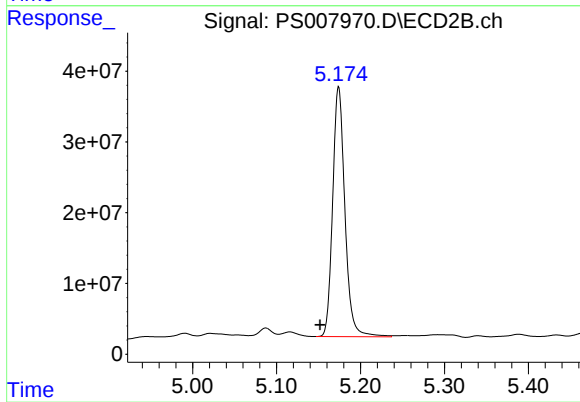

#4 2,4-DCAA

R.T.: 5.174 min
Delta R.T.: 0.022 min
Response: 358525276
Conc: 462.07 ng/ml m