

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
 Data File : PS007973.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2019 17:50
 Operator : SM\AJ
 Sample : K6119-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SB-6-(1-3)

Manual Integrations
 APPROVED

Ankita
 12/10/2019 10:26:54 AM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 00:31:41 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	5.420	5.151	679.7E6	146.8E6	434.522	189.191m#

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120919\
Data File : PS007973.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2019 17:50
Operator : SM\AJ
Sample : K6119-03
Misc :
ALS Vial : 23 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
SB-6-(1-3)


Manual Integrations
APPROVED

Ankita
12/10/2019 10:26:54 AM

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 00:31:41 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

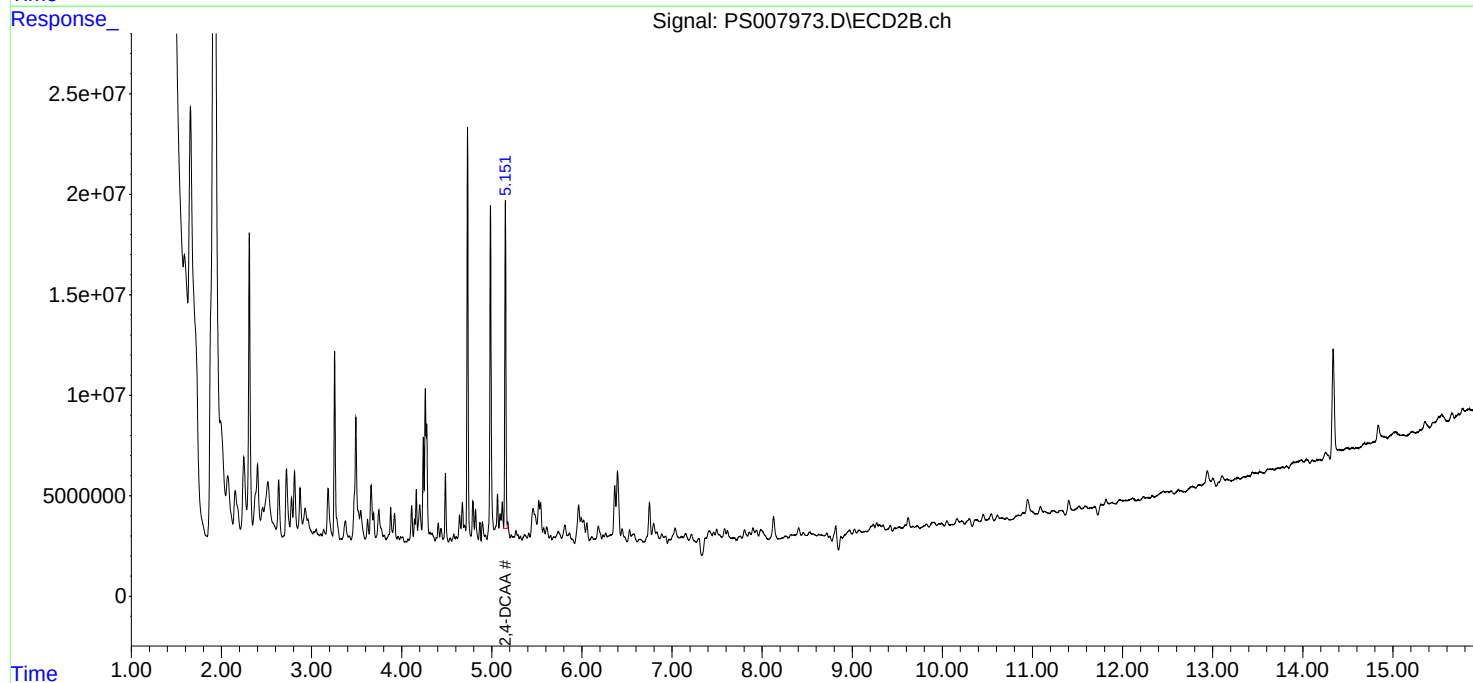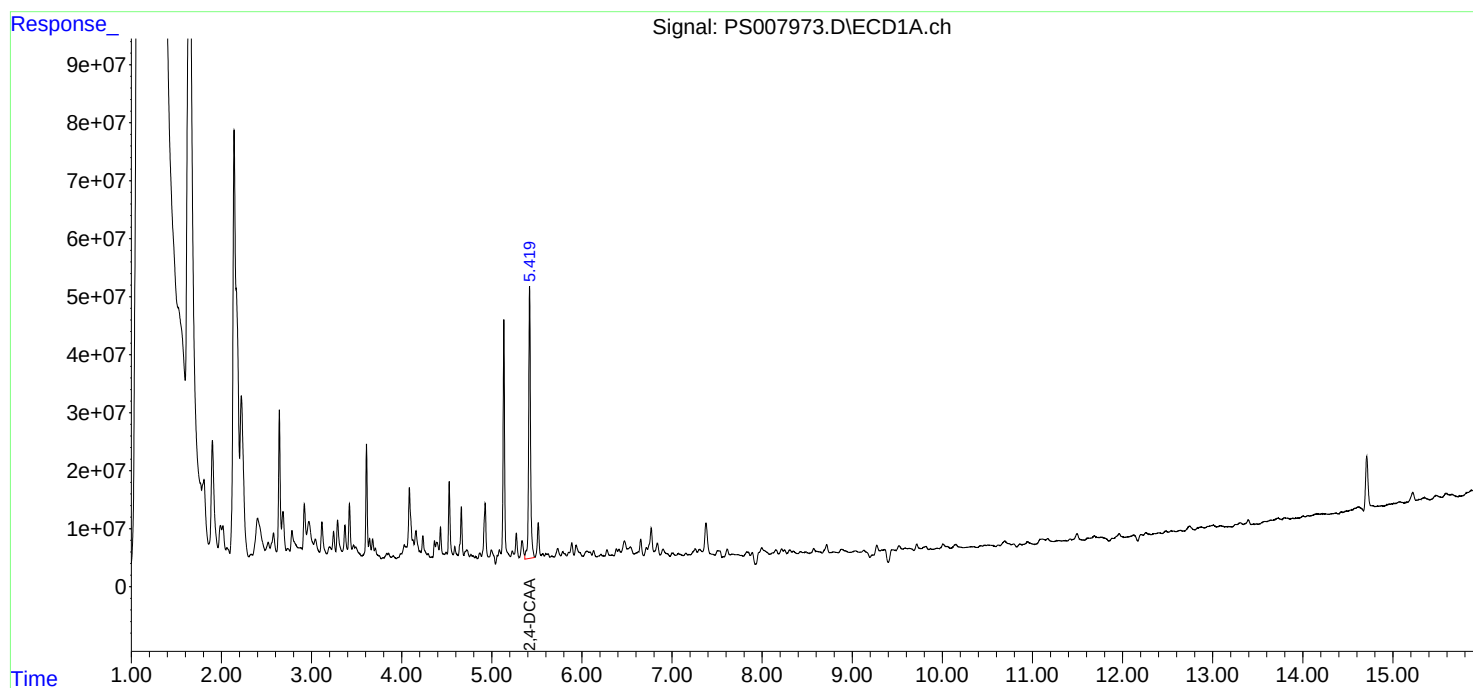

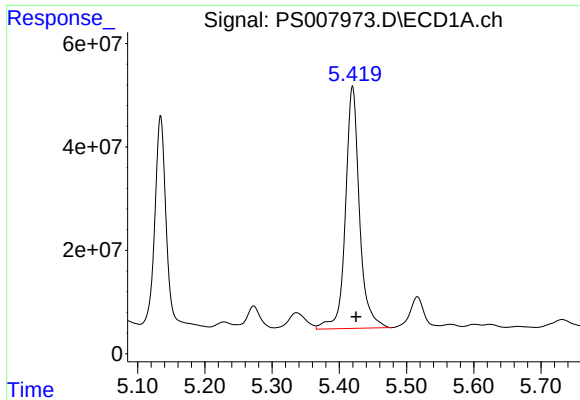


#4 2,4-DCAA

R.T.: 5.420 min
Delta R.T.: -0.005 min
Response: 679736640
Conc: 434.52 ng/ml

Instrument :
ECD_S
ClientSampleId :
SB-6-(1-3)

Manual Integrations
APPROVED

Ankita
12/10/2019 10:26:54 AM

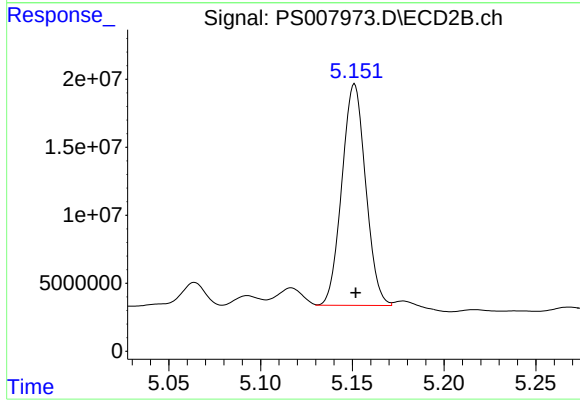

#4 2,4-DCAA

R.T.: 5.151 min
Delta R.T.: -0.001 min
Response: 146796880
Conc: 189.19 ng/ml m