

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120920\
 Data File : PS013421.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 08:36
 Operator : DD\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 03:43:39 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

2) T	3,5-DICHL...	6.474f	0.000	69457658	0	54.192	N.D.	#
15) T	Picloram	10.973	11.058f	106.2E6	10619829	15.419	3.050	#



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120920\
Data File : PS013421.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 08:36
Operator : DD\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 03:43:39 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

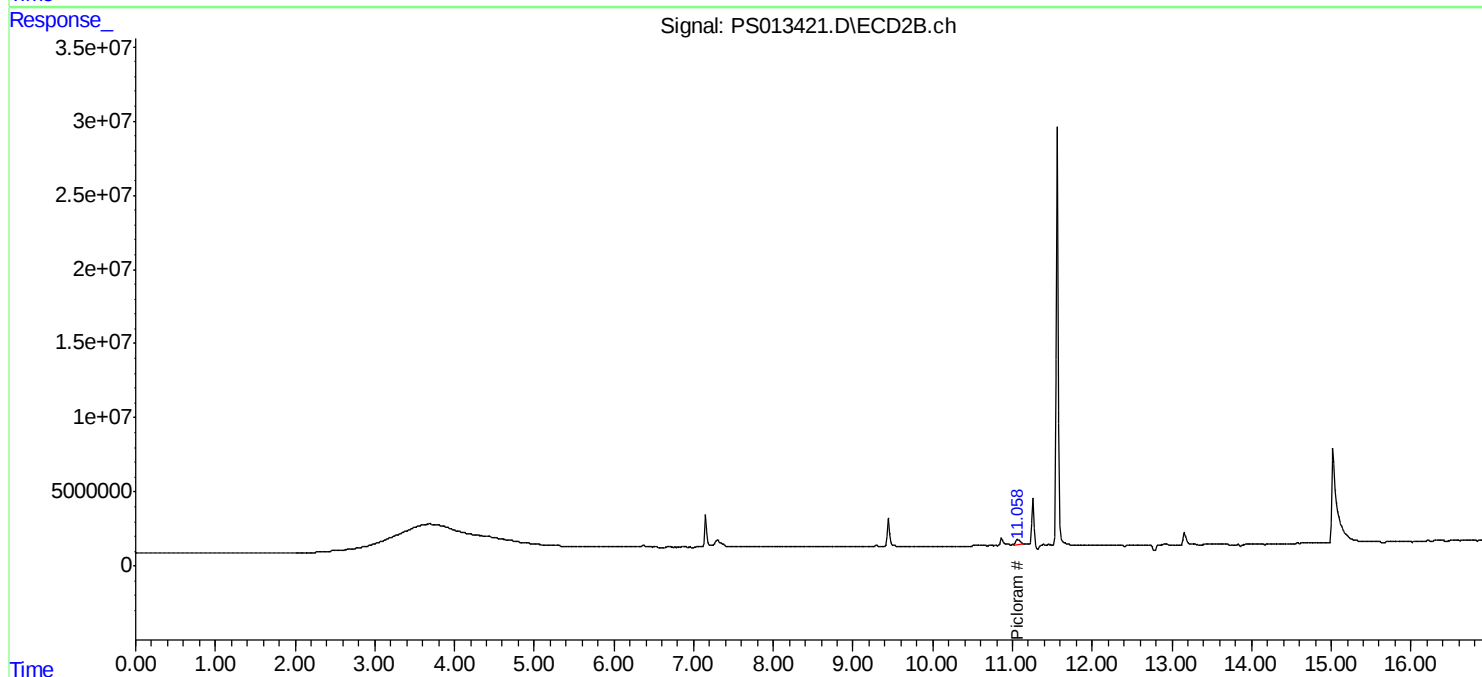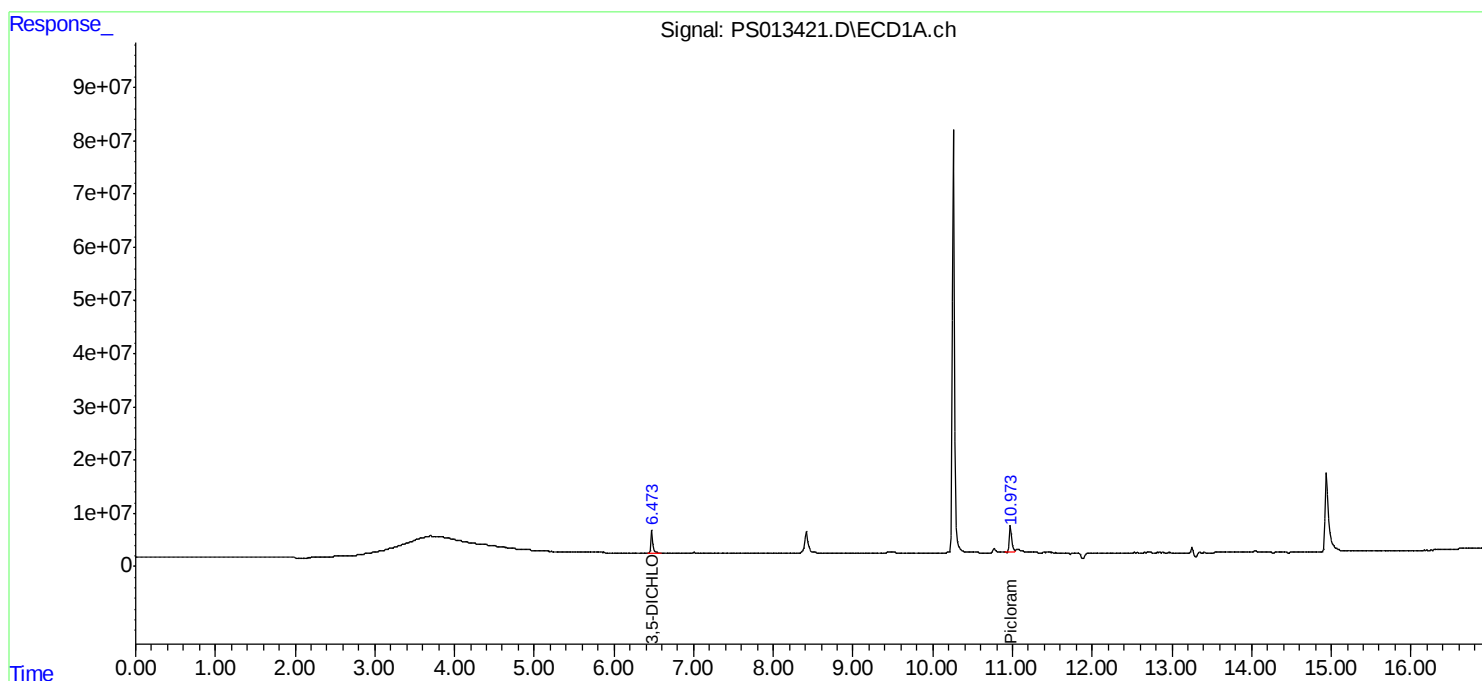


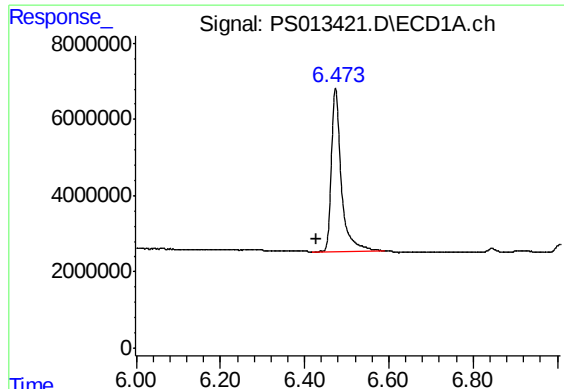

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.474 min
Delta R.T.: 0.046 min
Response: 69457658
Conc: 54.19 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

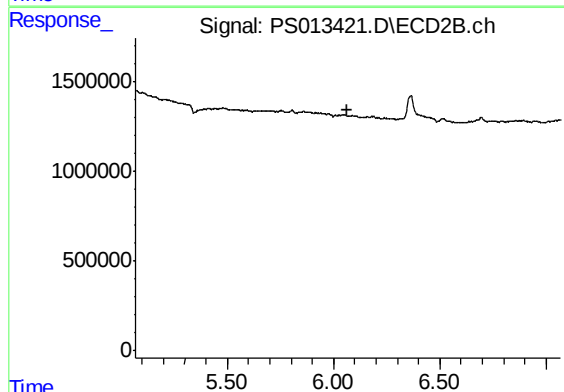


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.068 min
Response: 0
Conc: N.D.

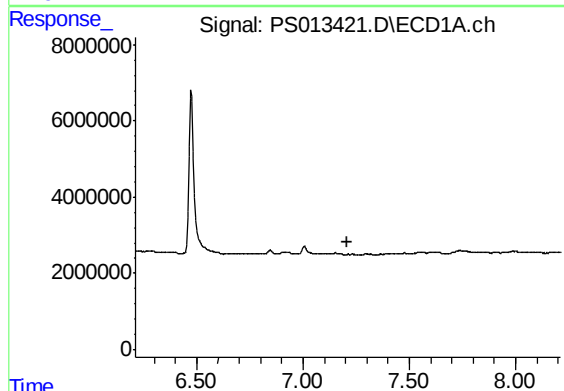


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.211 min
Response: 0
Conc: N.D.

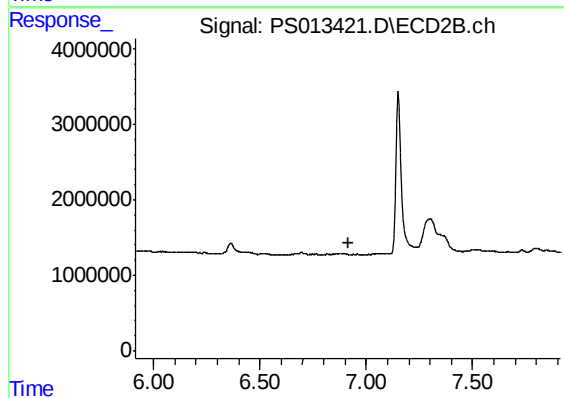

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.914 min
Response: 0
Conc: N.D.

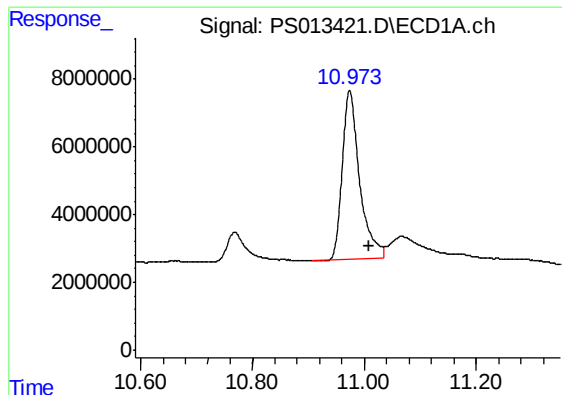

#15 Picloram

R.T.: 10.973 min
Delta R.T.: -0.035 min
Response: 106203174
Conc: 15.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

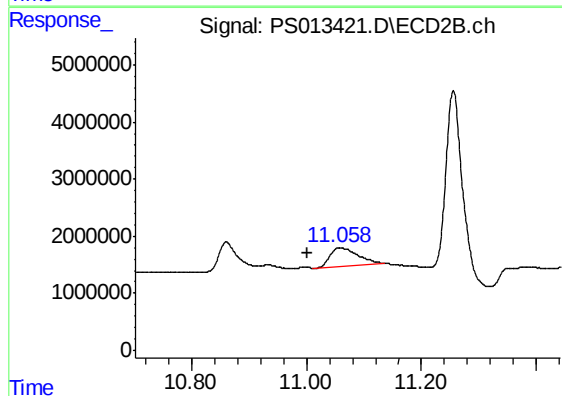

#15 Picloram

R.T.: 11.058 min
Delta R.T.: 0.057 min
Response: 10619829
Conc: 3.05 ng/ml