

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120920\
 Data File : PS013442.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2020 19:51
 Operator : DD\AJ
 Sample : PB133505TB
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PB133505TB

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 05:04:07 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.212	6.915	238.9E6	120.4E6	256.563	306.037
Target Compounds							
1) T	Dalapon	2.993	2.589	45230086	21975075	42.106	41.815
2) T	3,5-DICHL...	0.000	6.095	0	45956188	N.D.	73.960
3) T	4-Nitroph...	7.100f	0.000	5719147	0	12.693	N.D. #
5) T	DICAMBA	7.387	7.047	9669110	4750429	2.618	2.827
7) T	MCPA	7.709	0.000	81056240	0	20.738	N.D. #
8) T	DICHLORPROP	0.000	7.743	0	22008847	N.D.	49.246
10) T	Pentachlo...	8.685f	0.000	11082699	0	<MDL	N.D. #
11) T	2,4,5-TP ...	0.000	8.759	0	22646361	N.D.	9.646
12) T	2,4,5-T	9.400f	0.000	36881542	0	6.671	N.D. #
15) T	Picloram	10.977	0.000	5418171	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120920\
Data File : PS013442.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2020 19:51
Operator : DD\AJ
Sample : PB133505TB
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
PB133505TB

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 05:04:07 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

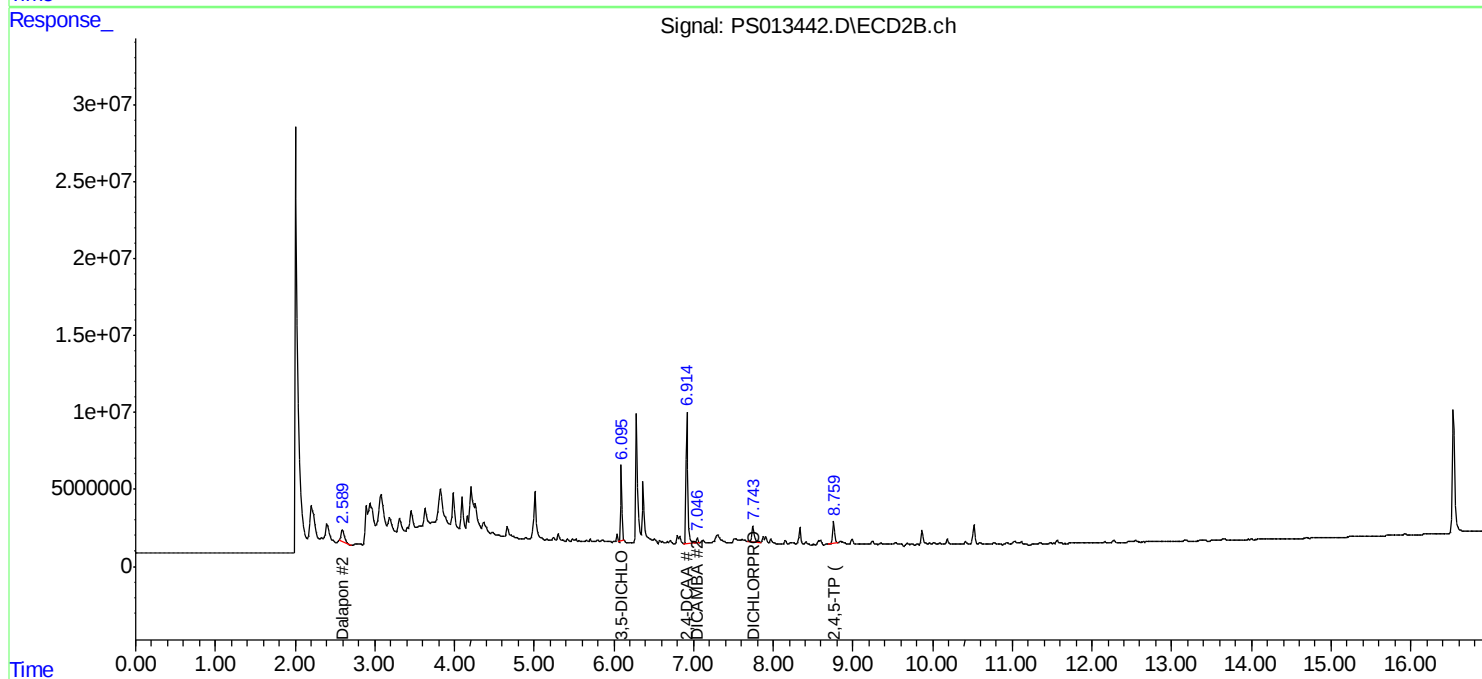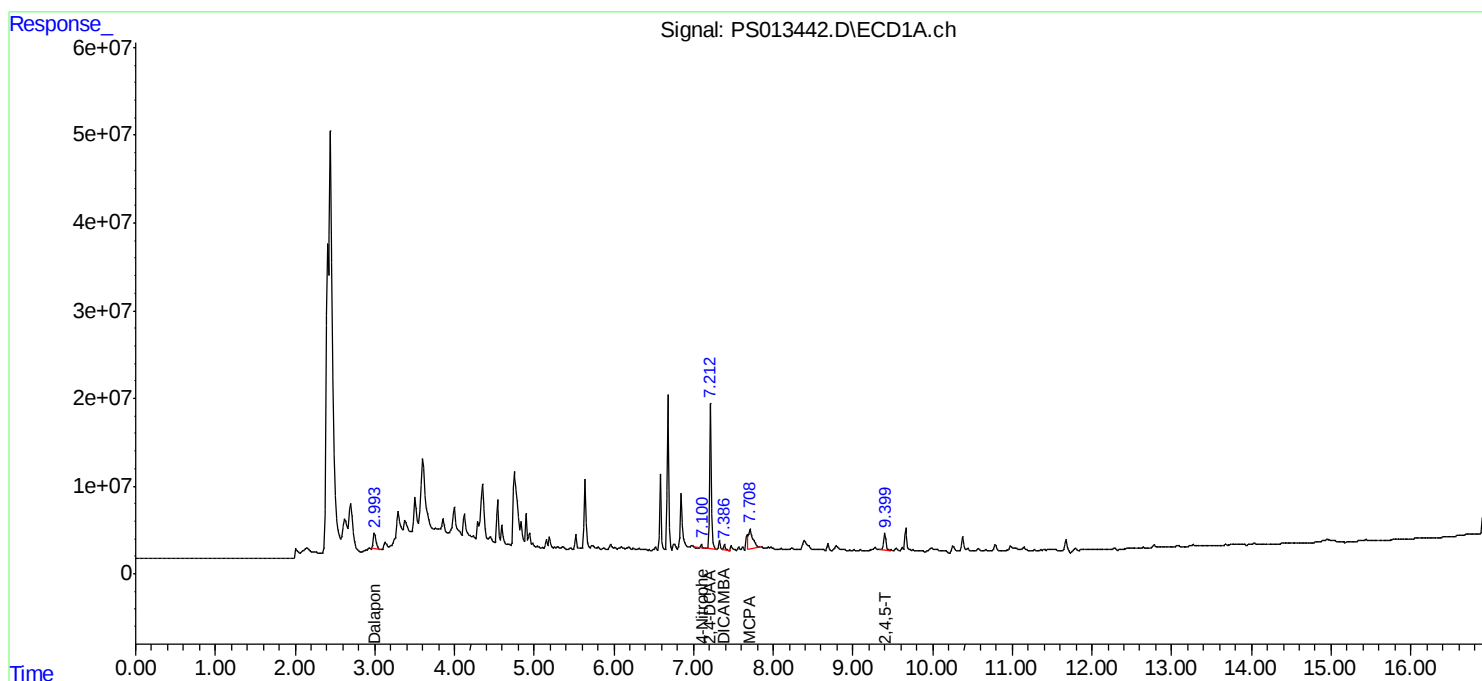


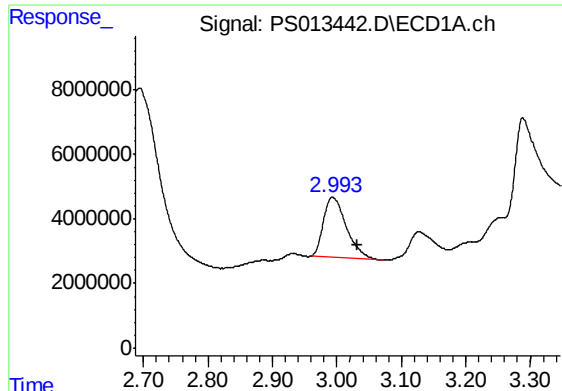

#1 Dalapon


R.T.: 2.993 min
Delta R.T.: -0.038 min
Response: 45230086
Conc: 42.11 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB133505TB

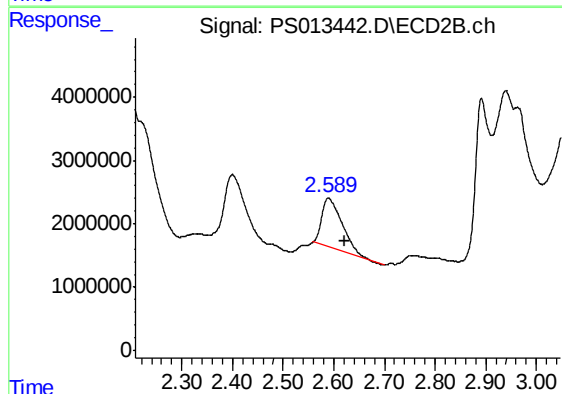


#1 Dalapon

R.T.: 2.589 min
Delta R.T.: -0.033 min
Response: 21975075
Conc: 41.82 ng/ml

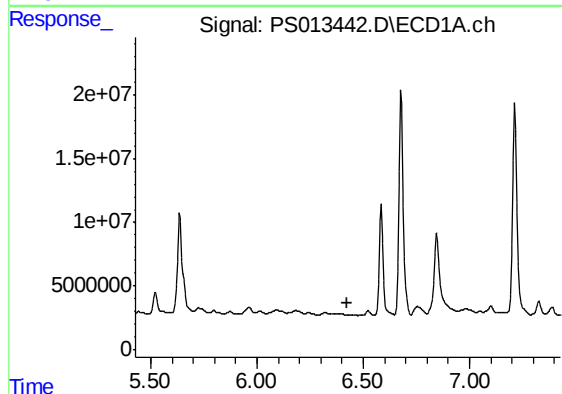


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

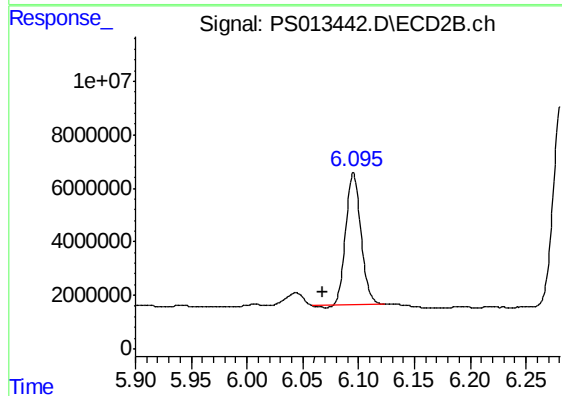

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 45956188
Conc: 73.96 ng/ml

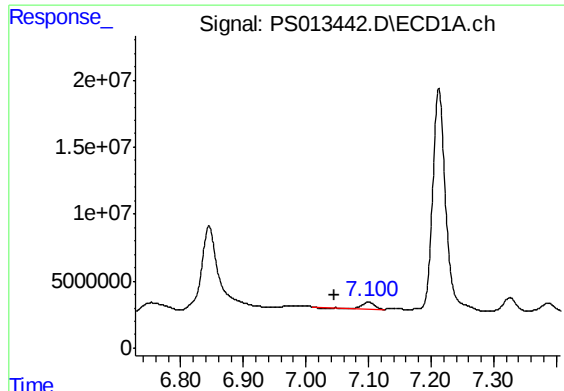

#3 4-Nitrophenol


R.T.: 7.100 min
Delta R.T.: 0.054 min
Response: 5719147
Conc: 12.69 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB133505TB

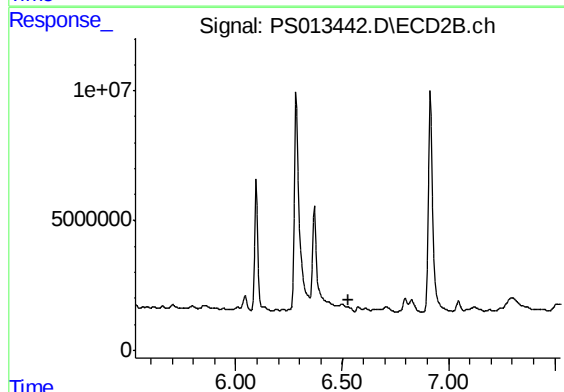


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.527 min
Response: 0
Conc: N.D.

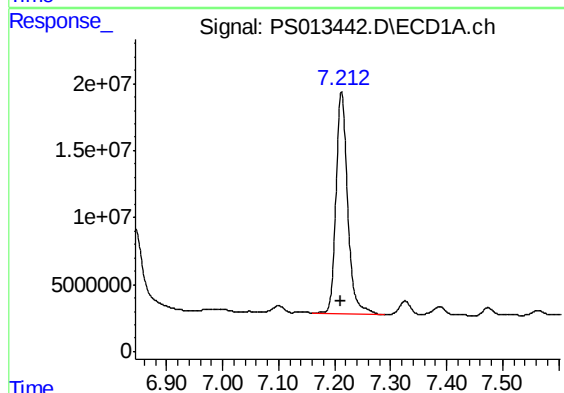


#4 2,4-DCAA

R.T.: 7.212 min
Delta R.T.: 0.002 min
Response: 238875006
Conc: 256.56 ng/ml

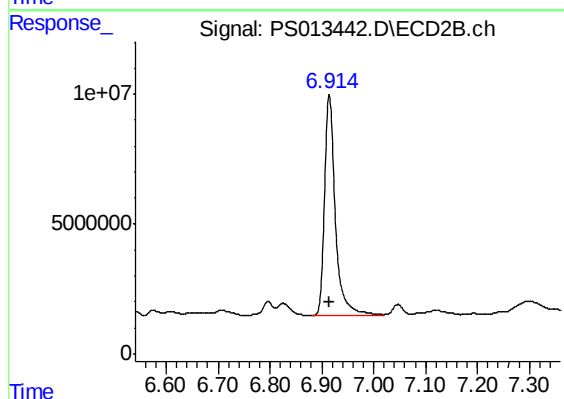

#4 2,4-DCAA


R.T.: 6.915 min
Delta R.T.: 0.000 min
Response: 120383110
Conc: 306.04 ng/ml

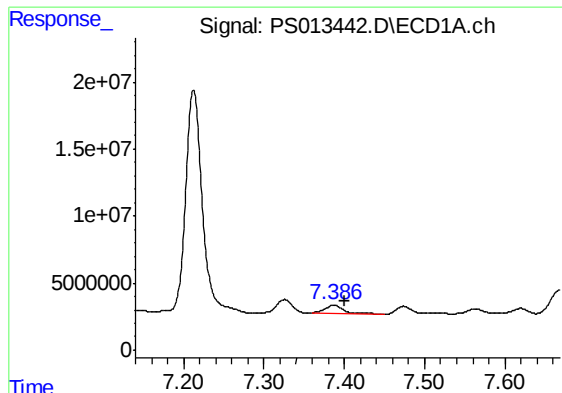

#5 DICAMBA


R.T.: 7.387 min
Delta R.T.: -0.014 min
Response: 9669110
Conc: 2.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB133505TB

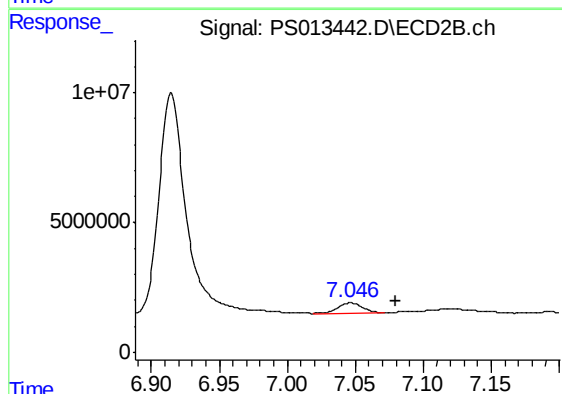


#5 DICAMBA

R.T.: 7.047 min
Delta R.T.: -0.034 min
Response: 4750429
Conc: 2.83 ng/ml

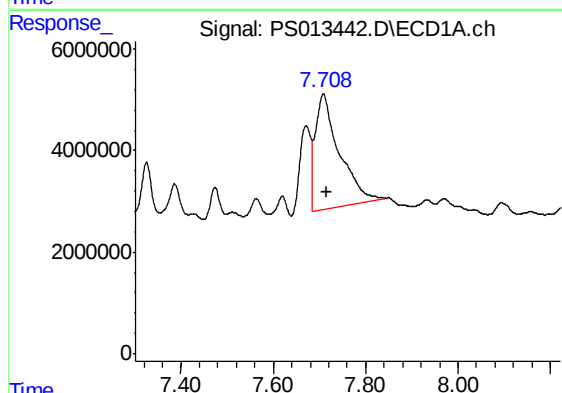


#7 MCPA

R.T.: 7.709 min
Delta R.T.: -0.008 min
Response: 81056240
Conc: 20.74 ug/ml

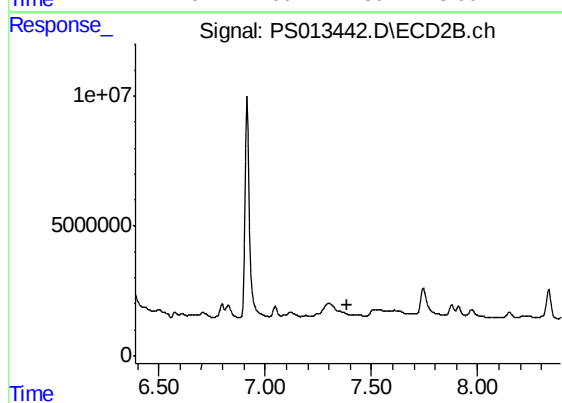

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

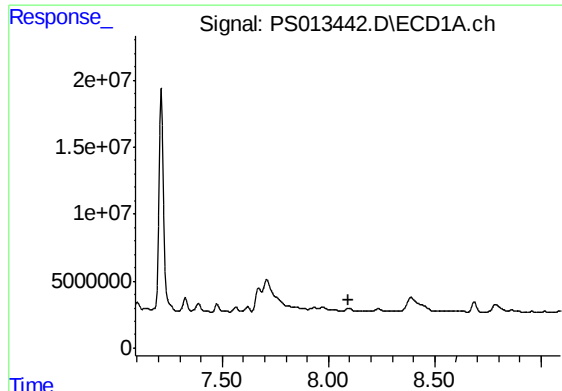

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 8.092 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
PB133505TB

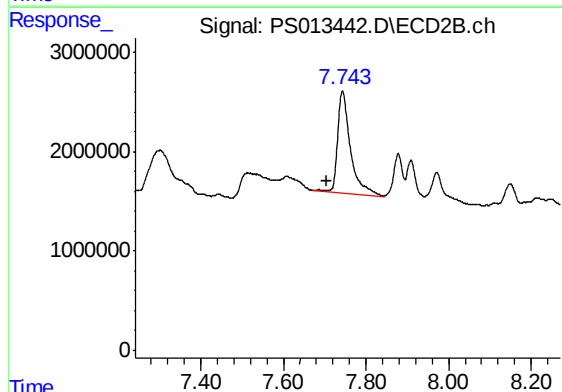


#8 DICHLORPROP

R.T.: 7.743 min
Delta R.T.: 0.038 min
Response: 22008847
Conc: 49.25 ng/ml

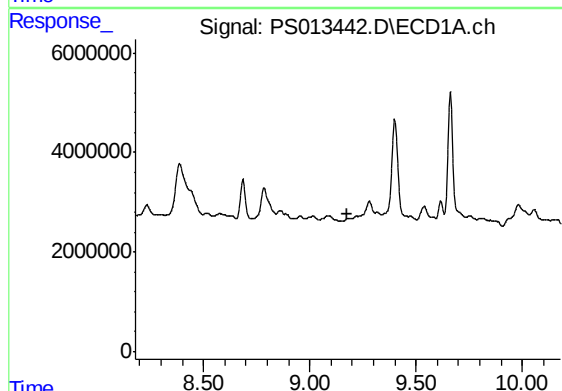


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 9.179 min
Response: 0
Conc: N.D.

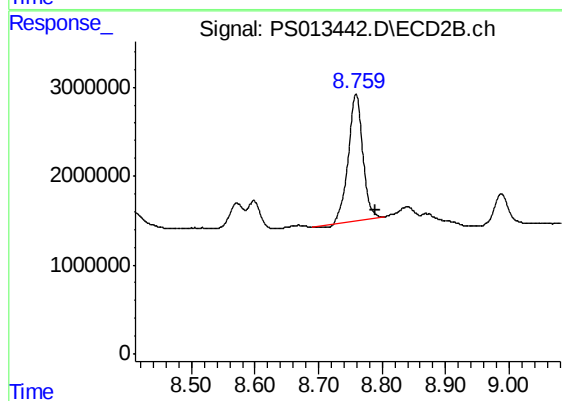

#11 2,4,5-TP (SILVEX)


R.T.: 8.759 min
Delta R.T.: -0.030 min
Response: 22646361
Conc: 9.65 ng/ml

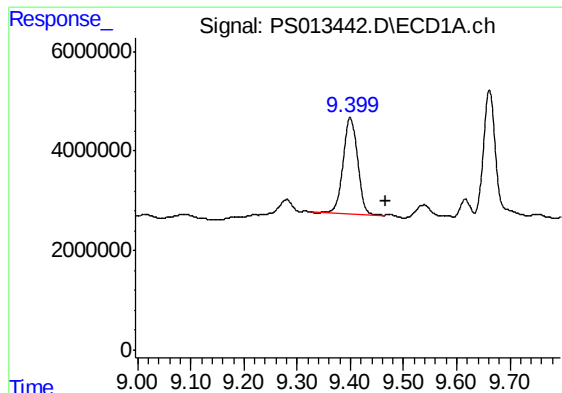

#12 2,4,5-T

R.T.: 9.400 min
Delta R.T.: -0.067 min
Response: 36881542
Conc: 6.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
PB133505TB

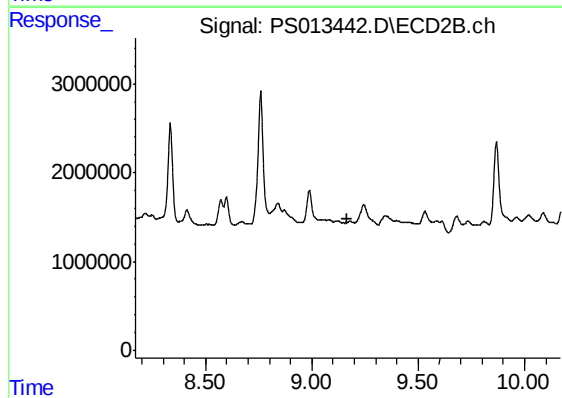

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.