

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120920\
 Data File : PS013456.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2020 01:13
 Operator : DD\AJ
 Sample : L4983-13
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR2-A-D-COMP

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 05:08:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 03 02:59:27 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.213	6.914	314.7E6	155.8E6	338.008	396.055
Target Compounds							
1) T	Dalapon	2.992	2.592	76242246	89581405	70.976	170.459 #
2) T	3,5-DICHL...	0.000	6.095	0	44461774	N.D.	71.555
5) T	DICAMBA	7.388	7.047	8717567	5720340	2.361	3.404 #
7) T	MCPA	7.713	0.000	171.5E6	0	43.875	N.D. #
8) T	DICHLORPROP	0.000	7.746f	0	9972428	N.D.	22.314
10) T	Pentachlo...	8.684f	0.000	16140482	0	1.204	N.D. #
11) T	2,4,5-TP ...	0.000	8.760	0	23200115	N.D.	9.882
12) T	2,4,5-T	9.403f	0.000	29329945	0	5.305	N.D. #
14) T	DINOSEB	11.146	0.000	13550464	0	3.197	N.D. #
15) T	Picloram	10.978	0.000	11145608	0	1.618	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120920\
Data File : PS013456.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2020 01:13
Operator : DD\AJ
Sample : L4983-13
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampled :
TR2-A-D-COMP

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 05:08:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120220.M
Quant Title : 8080.M
QLast Update : Thu Dec 03 02:59:27 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

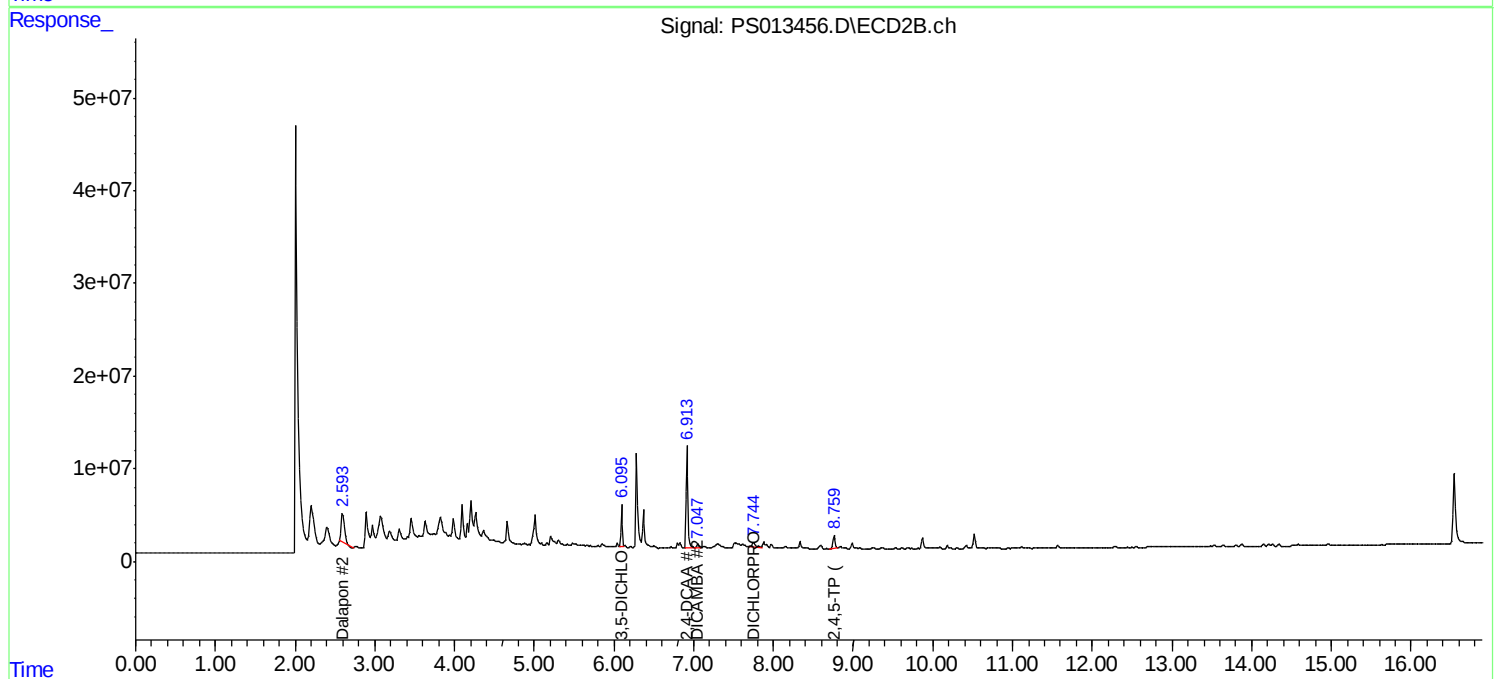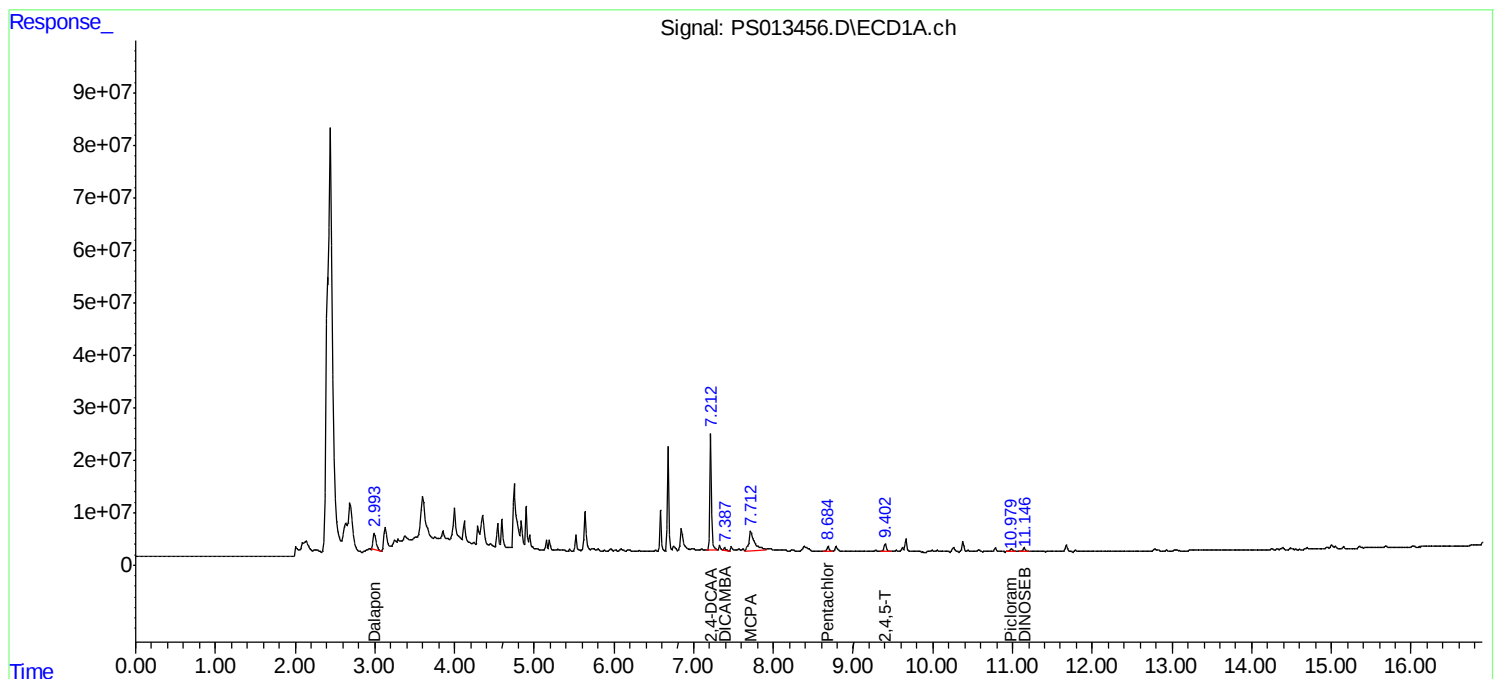


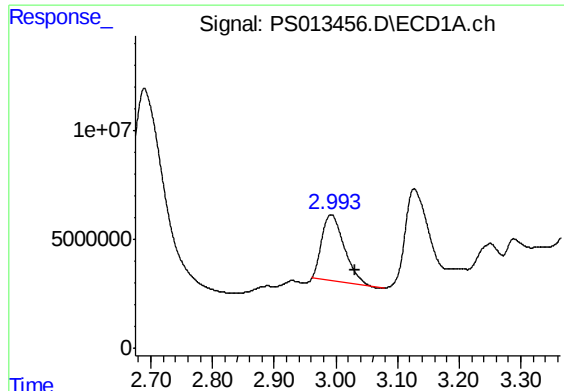

#1 Dalapon


R.T.: 2.992 min
Delta R.T.: -0.039 min
Response: 76242246
Conc: 70.98 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR2-A-D-COMP

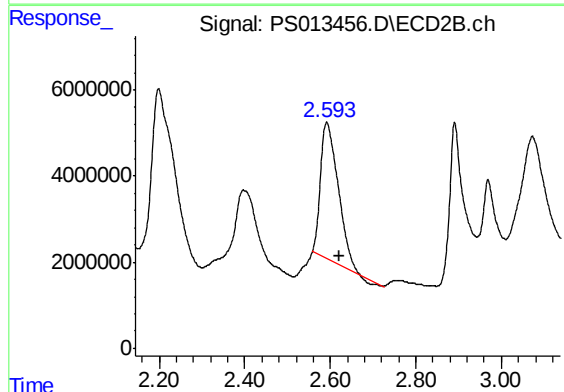


#1 Dalapon

R.T.: 2.592 min
Delta R.T.: -0.030 min
Response: 89581405
Conc: 170.46 ng/ml

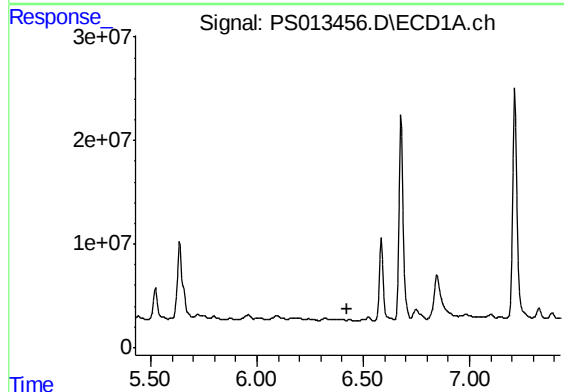


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 6.428 min
Response: 0
Conc: N.D.

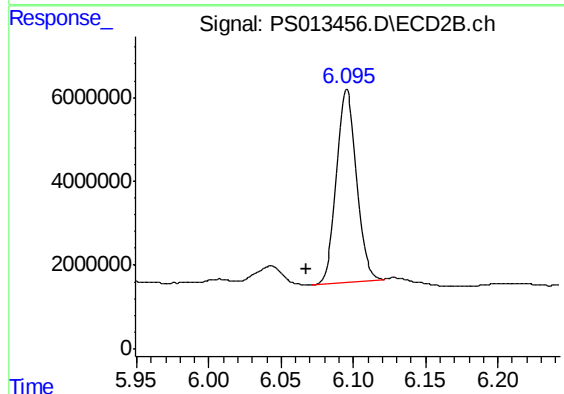

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.095 min
Delta R.T.: 0.028 min
Response: 44461774
Conc: 71.55 ng/ml

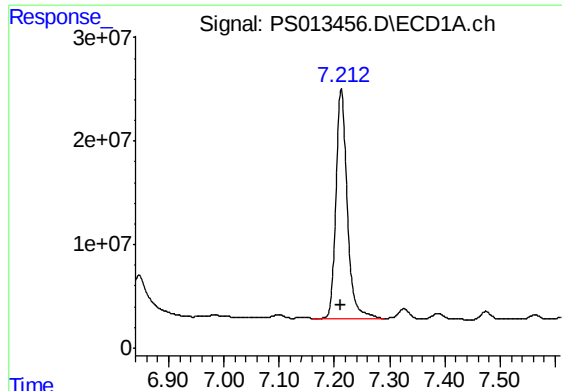

#4 2,4-DCAA


R.T.: 7.213 min
Delta R.T.: 0.002 min
Response: 314705854
Conc: 338.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR2-A-D-COMP

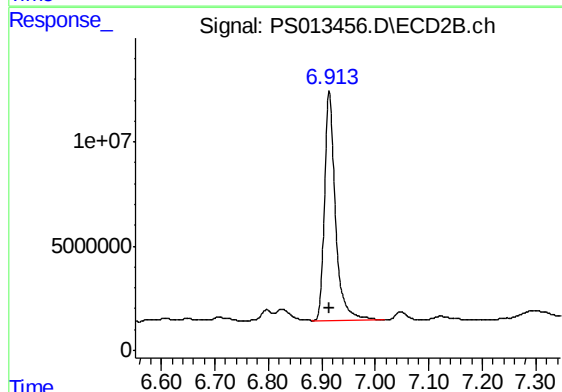


#4 2,4-DCAA

R.T.: 6.914 min
Delta R.T.: 0.000 min
Response: 155792592
Conc: 396.05 ng/ml

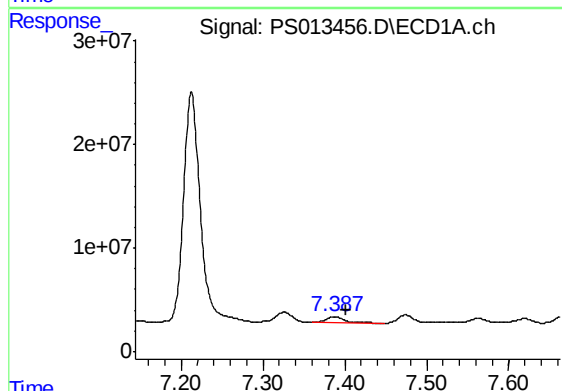


#5 DICAMBA

R.T.: 7.388 min
Delta R.T.: -0.013 min
Response: 8717567
Conc: 2.36 ng/ml

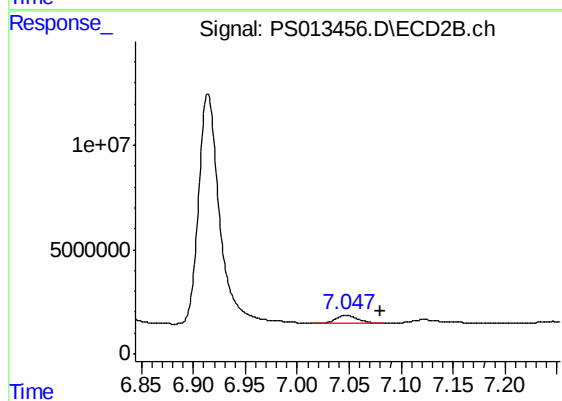

#5 DICAMBA


R.T.: 7.047 min
Delta R.T.: -0.033 min
Response: 5720340
Conc: 3.40 ng/ml

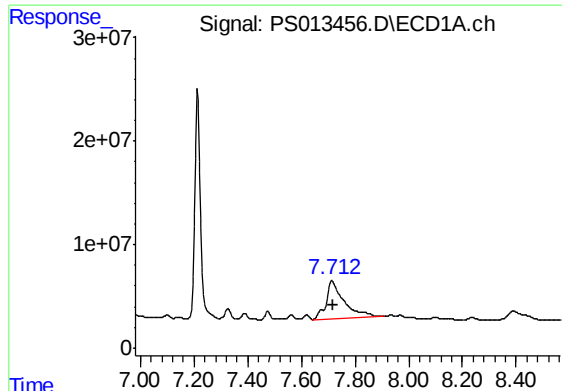

#7 MCPA


R.T.: 7.713 min
Delta R.T.: -0.004 min
Response: 171488057
Conc: 43.87 ug/ml

Instrument :
ECD_S
ClientSampleId :
TR2-A-D-COMP

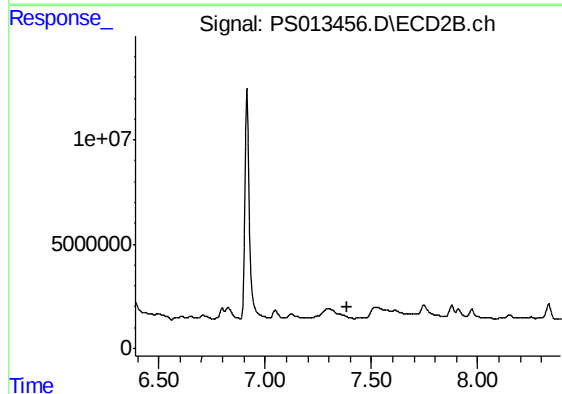


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 7.389 min
Response: 0
Conc: N.D.

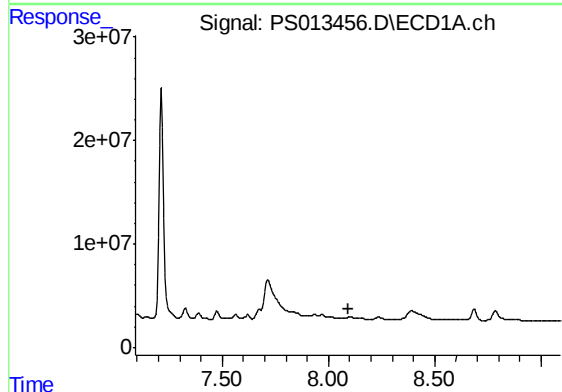


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.092 min
Response: 0
Conc: N.D.

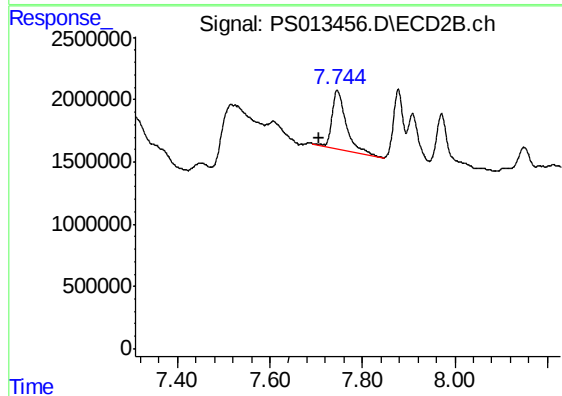

#8 DICHLORPROP


R.T.: 7.746 min
Delta R.T.: 0.041 min
Response: 9972428
Conc: 22.31 ng/ml

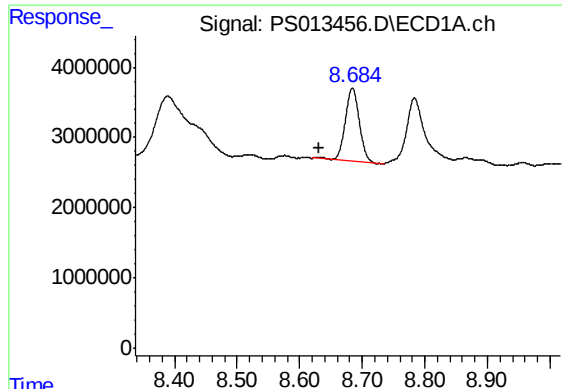

#10 Pentachlorophenol


R.T.: 8.684 min
Delta R.T.: 0.054 min
Response: 16140482
Conc: 1.20 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR2-A-D-COMP

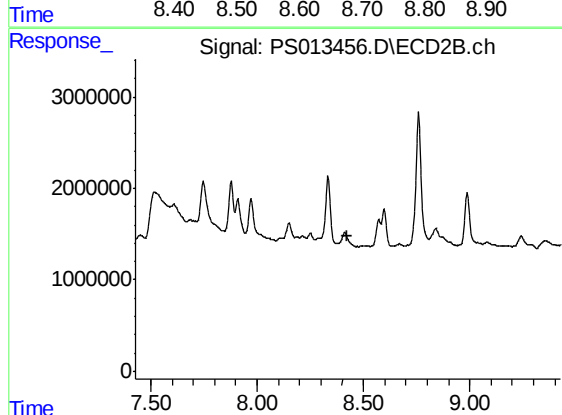


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 8.427 min
Response: 0
Conc: N.D.

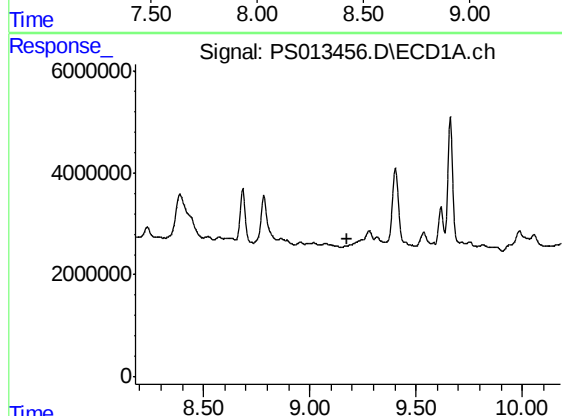


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 9.179 min
Response: 0
Conc: N.D.

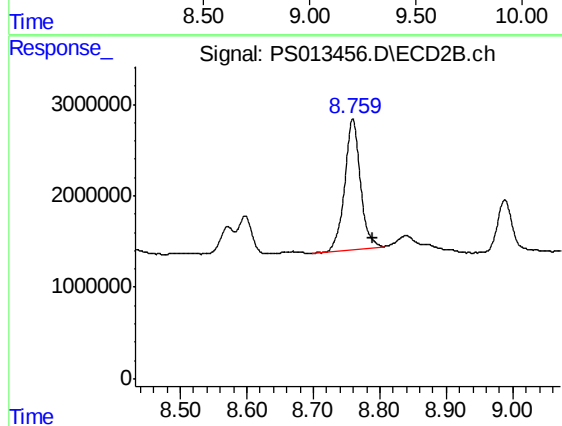

#11 2,4,5-TP (SILVEX)


R.T.: 8.760 min
Delta R.T.: -0.029 min
Response: 23200115
Conc: 9.88 ng/ml

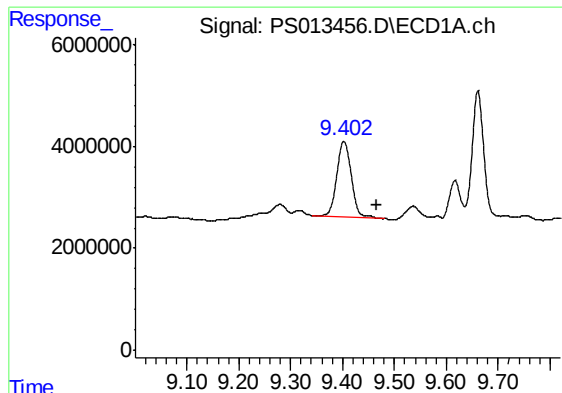

#12 2,4,5-T


R.T.: 9.403 min
Delta R.T.: -0.064 min
Response: 29329945
Conc: 5.30 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR2-A-D-COMP

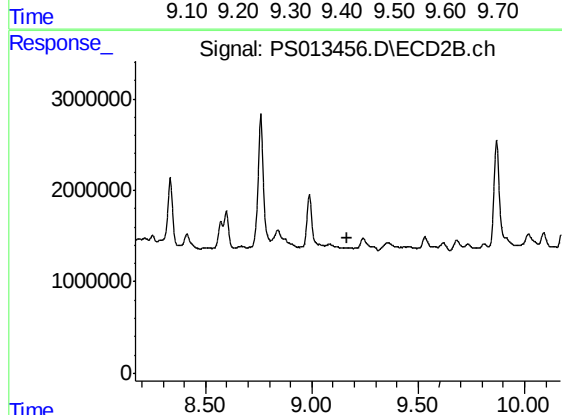


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T. : 9.170 min
Response: 0
Conc: N.D.

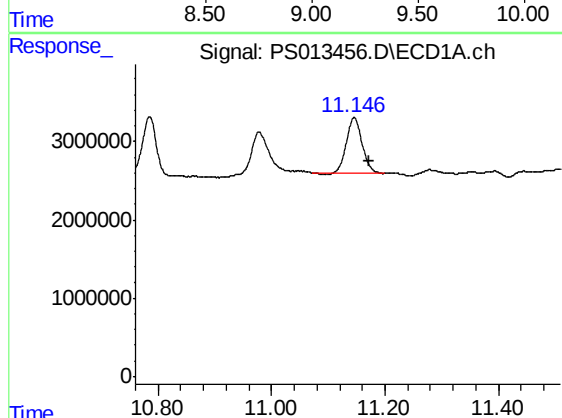


#14 DINOSEB

R.T.: 11.146 min
Delta R.T.: -0.026 min
Response: 13550464
Conc: 3.20 ng/ml

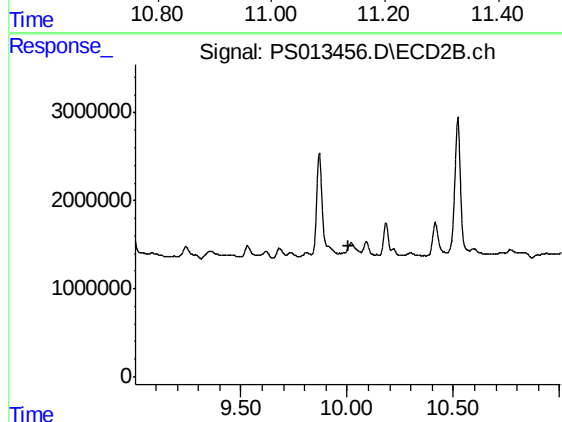

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 10.004 min
Response: 0
Conc: N.D.

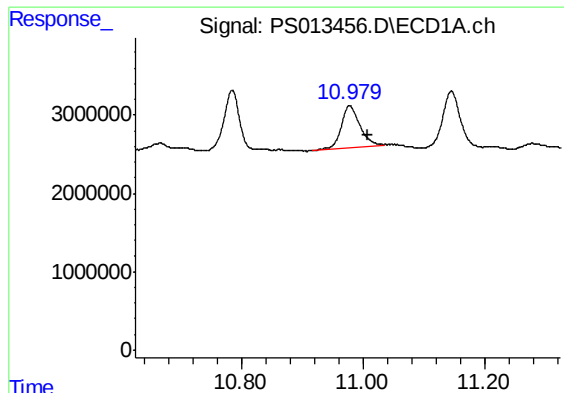

#15 Picloram

R.T.: 10.978 min
Delta R.T.: -0.031 min
Response: 11145608
Conc: 1.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR2-A-D-COMP

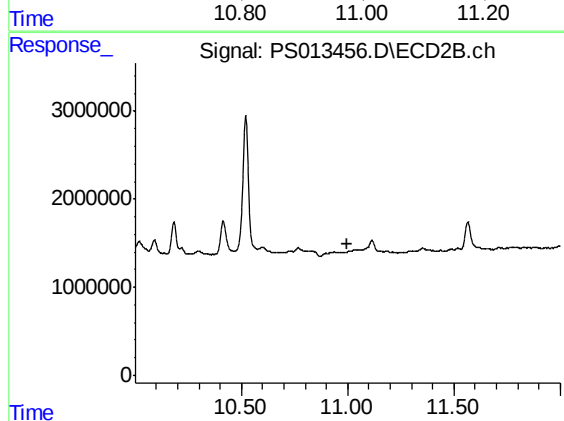

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 11.001 min
Response: 0
Conc: N.D.