

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120921\
 Data File : PS017592.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2021 08:59
 Operator : AJ\MA
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 14:51:48 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.154	0.000	4986006	0	3.171	N.D. #
Target Compounds							
5) T	DICAMBA	7.336	6.894	15762223	7258656	2.582	2.792
8) T	DICHLORPROP	8.031	0.000	5065318	0	3.299	N.D. #
9) T	2,4-D	8.276	0.000	16989111	0	9.092	N.D. #
10) T	Pentachlo...	8.561	8.224	30383972	12321693	1.439	1.468
11) T	2,4,5-TP ...	9.113	8.586	27275061	8569935	3.273	2.417 #
12) T	2,4,5-T	9.408	8.971	22744110	7724618	2.692	2.323
14) T	DINOSEB	11.094	9.791	21967946	7420811	3.528	3.147
15) T	Picloram	10.948	10.719f	10519205	12010591	<MDL	2.752 #
16) T	DCPA	11.362	10.719	30926939	12010591	2.896	2.726



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120921\
Data File : PS017592.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2021 08:59
Operator : AJ\MA
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 14:51:48 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

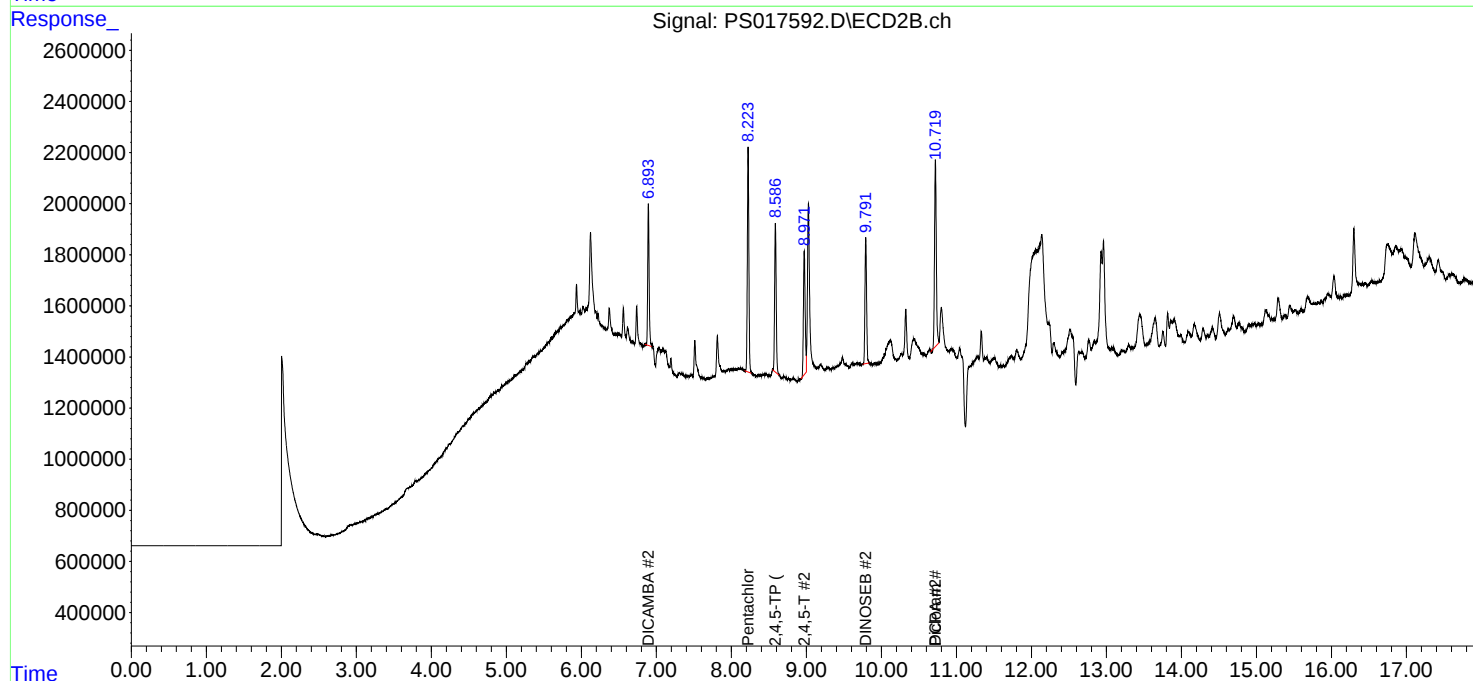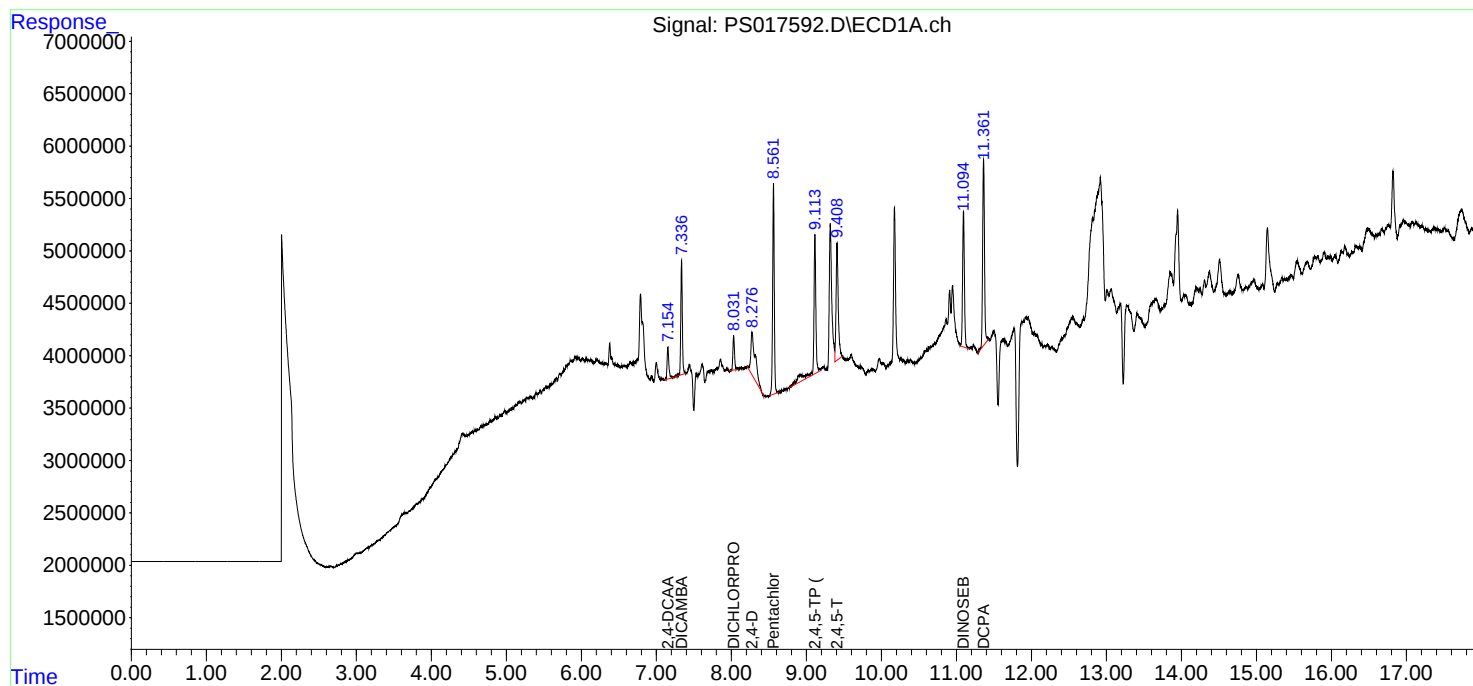


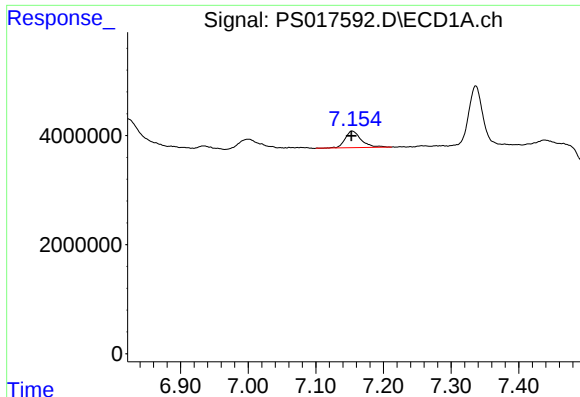

#4 2,4-DCAA


R.T.: 7.154 min
Delta R.T.: 0.001 min
Response: 4986006
Conc: 3.17 ng/ml

Instrument :
ECD_S
ClientSampleId :

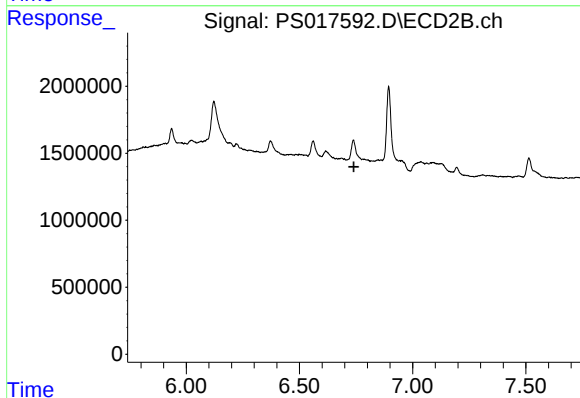


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.740 min
Response: 0
Conc: N.D.

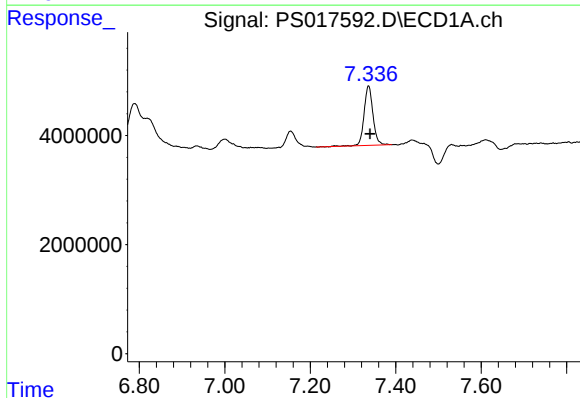


#5 DICAMBA

R.T.: 7.336 min
Delta R.T.: -0.003 min
Response: 15762223
Conc: 2.58 ng/ml

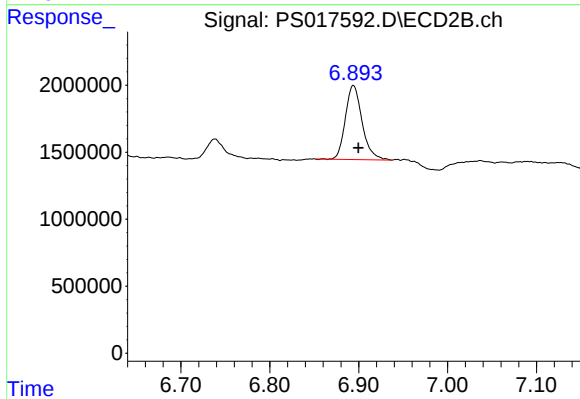

#5 DICAMBA


R.T.: 6.894 min
Delta R.T.: -0.006 min
Response: 7258656
Conc: 2.79 ng/ml

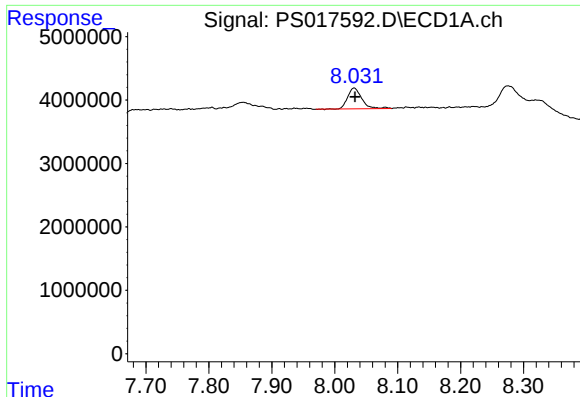

#8 DICHLORPROP


R.T.: 8.031 min
Delta R.T.: -0.002 min
Response: 5065318
Conc: 3.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

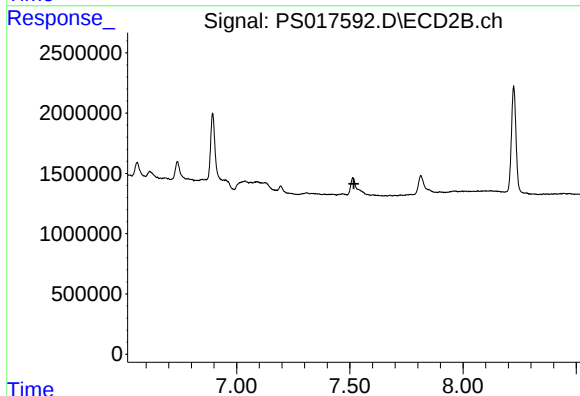


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 7.518 min
Response: 0
Conc: N.D.

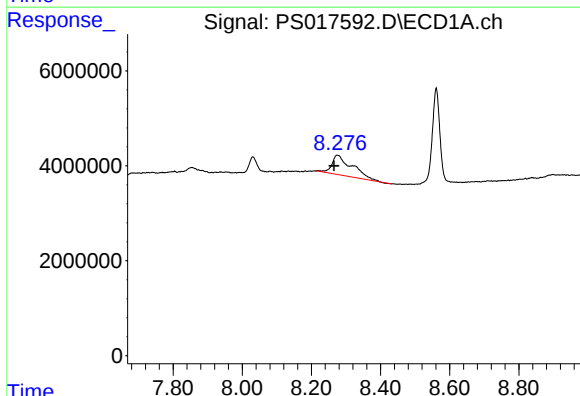


#9 2,4-D

R.T.: 8.276 min
Delta R.T.: 0.010 min
Response: 16989111
Conc: 9.09 ng/ml

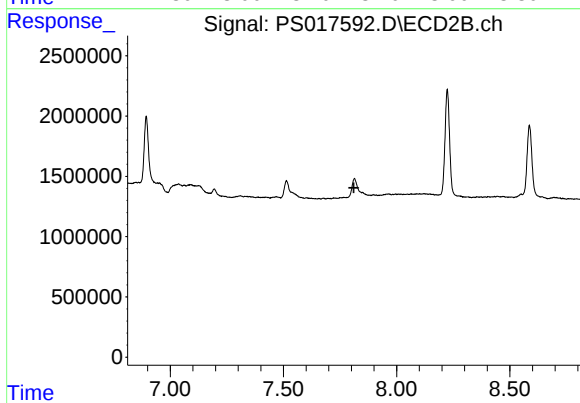

#9 2,4-D


R.T.: 0.000 min
Exp R.T. : 7.811 min
Response: 0
Conc: N.D.

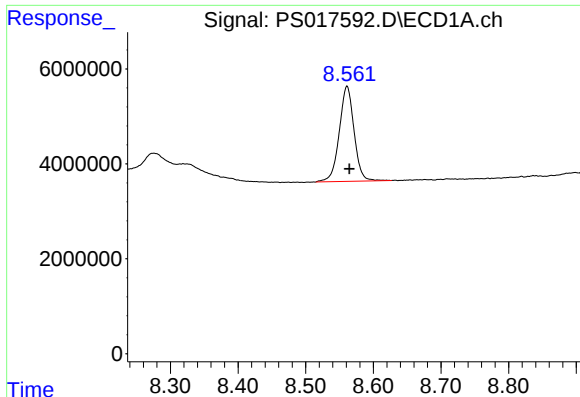

#10 Pentachlorophenol


R.T.: 8.561 min
Delta R.T.: -0.004 min
Response: 30383972
Conc: 1.44 ng/ml

Instrument :
ECD_S
ClientSampleId :

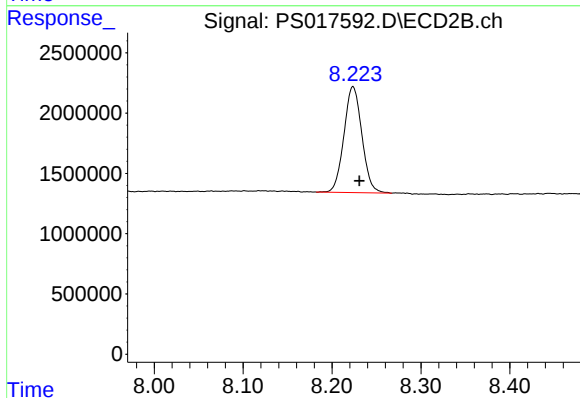


#10 Pentachlorophenol

R.T.: 8.224 min
Delta R.T.: -0.007 min
Response: 12321693
Conc: 1.47 ng/ml

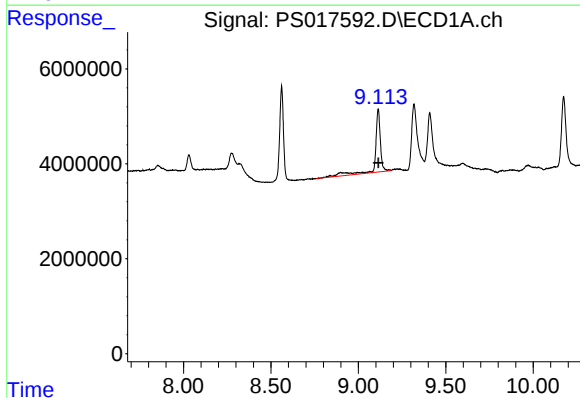


#11 2,4,5-TP (SILVEX)

R.T.: 9.113 min
Delta R.T.: -0.002 min
Response: 27275061
Conc: 3.27 ng/ml

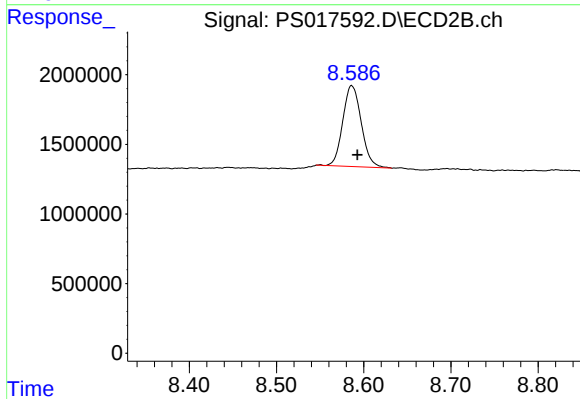

#11 2,4,5-TP (SILVEX)


R.T.: 8.586 min
Delta R.T.: -0.007 min
Response: 8569935
Conc: 2.42 ng/ml

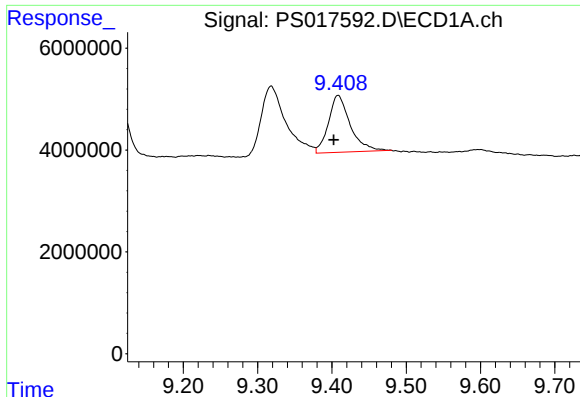

#12 2,4,5-T


R.T.: 9.408 min
Delta R.T.: 0.006 min
Response: 22744110
Conc: 2.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

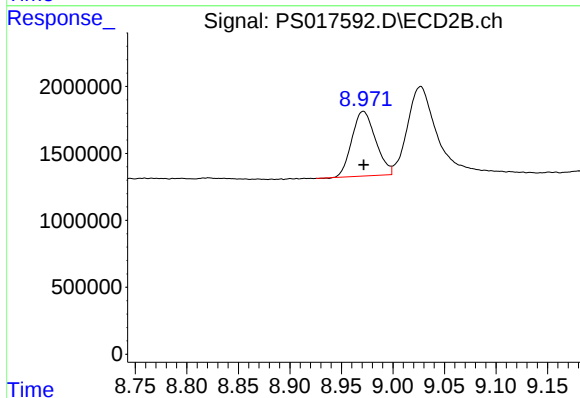


#12 2,4,5-T

R.T.: 8.971 min
Delta R.T.: 0.000 min
Response: 7724618
Conc: 2.32 ng/ml

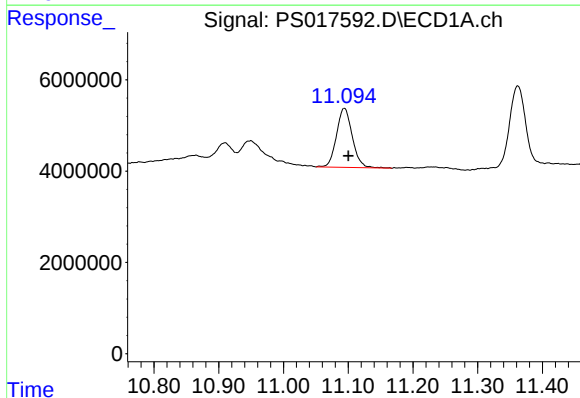


#14 DINOSEB

R.T.: 11.094 min
Delta R.T.: -0.006 min
Response: 21967946
Conc: 3.53 ng/ml

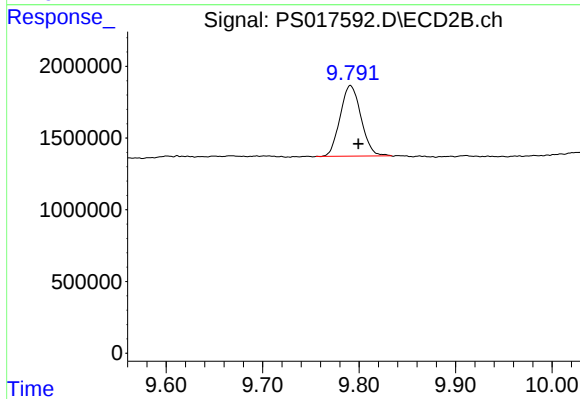

#14 DINOSEB


R.T.: 9.791 min
Delta R.T.: -0.008 min
Response: 7420811
Conc: 3.15 ng/ml

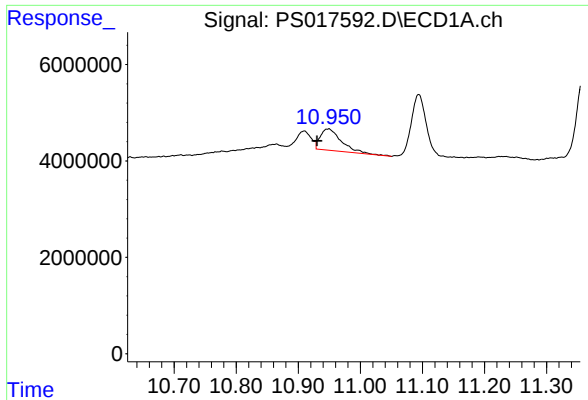

#15 Picloram


R.T.: 10.948 min
Delta R.T.: 0.018 min
Response: 10519205
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

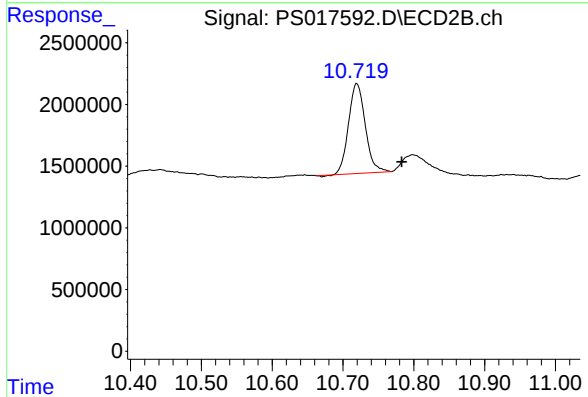


#15 Picloram

R.T.: 10.719 min
Delta R.T.: -0.064 min
Response: 12010591
Conc: 2.75 ng/ml

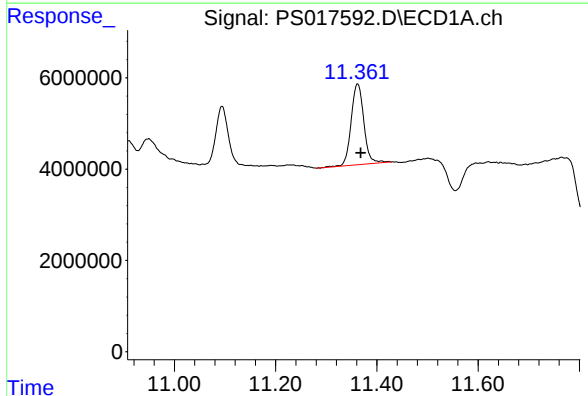

#16 DCPA

R.T.: 11.362 min
Delta R.T.: -0.006 min
Response: 30926939
Conc: 2.90 ng/ml

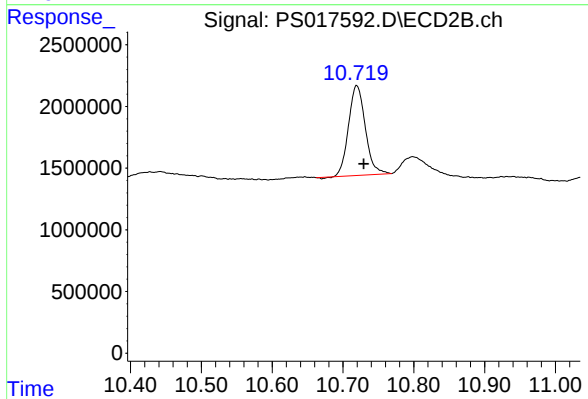

#16 DCPA

R.T.: 10.719 min
Delta R.T.: -0.010 min
Response: 12010591
Conc: 2.73 ng/ml