

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120921\
 Data File : PS017603.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2021 14:30
 Operator : AJ\MA
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 21:02:19 2021
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
 Quant Title : 8080.M
 QLast Update : Fri Nov 19 21:46:29 2021
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.145	6.737	709.6E6	286.7E6	451.356	483.830
Target Compounds							
7) T	MCPA	7.599f	0.000	9282390	0	1.416	N.D. #
9) T	2,4-D	8.324f	0.000	42222370	0	22.596	N.D. #
15) T	Picloram	10.888f	0.000	7453022	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120921\
Data File : PS017603.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2021 14:30
Operator : AJ\MA
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 21:02:19 2021
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS111821.M
Quant Title : 8080.M
QLast Update : Fri Nov 19 21:46:29 2021
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

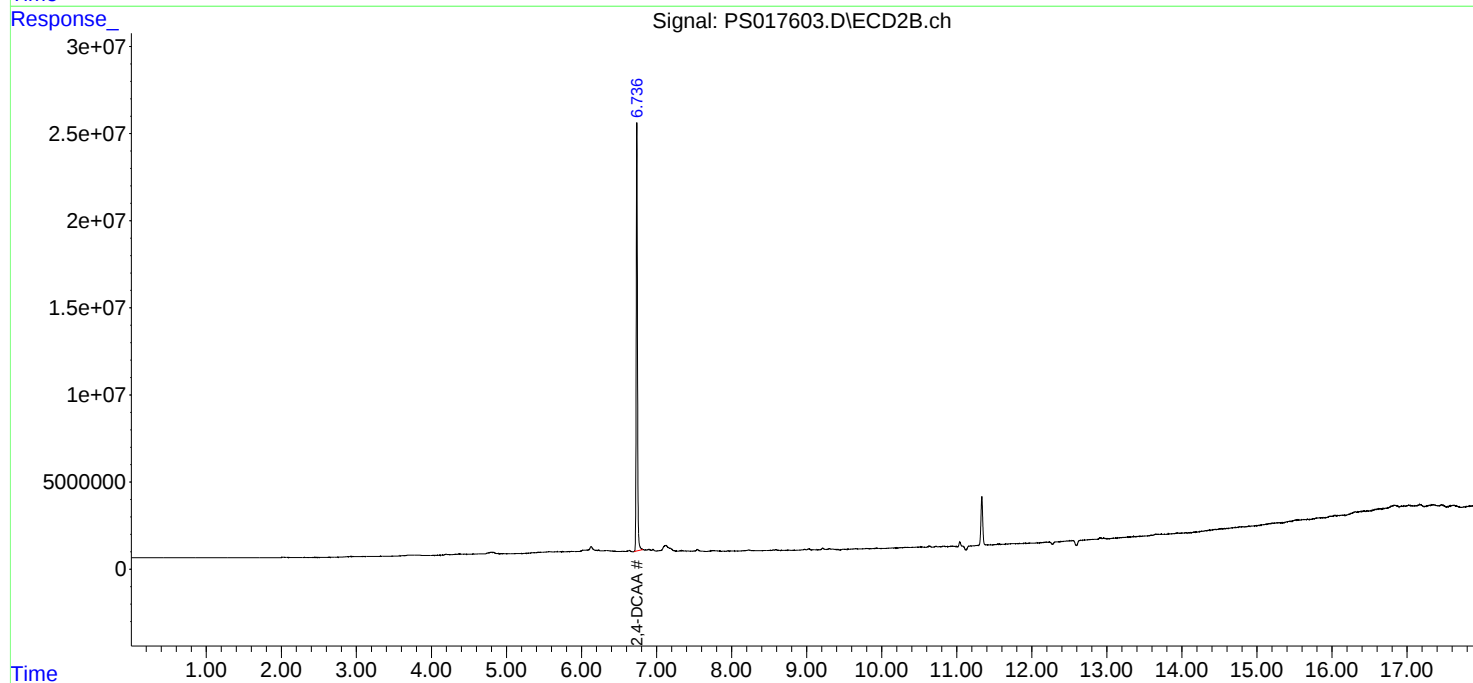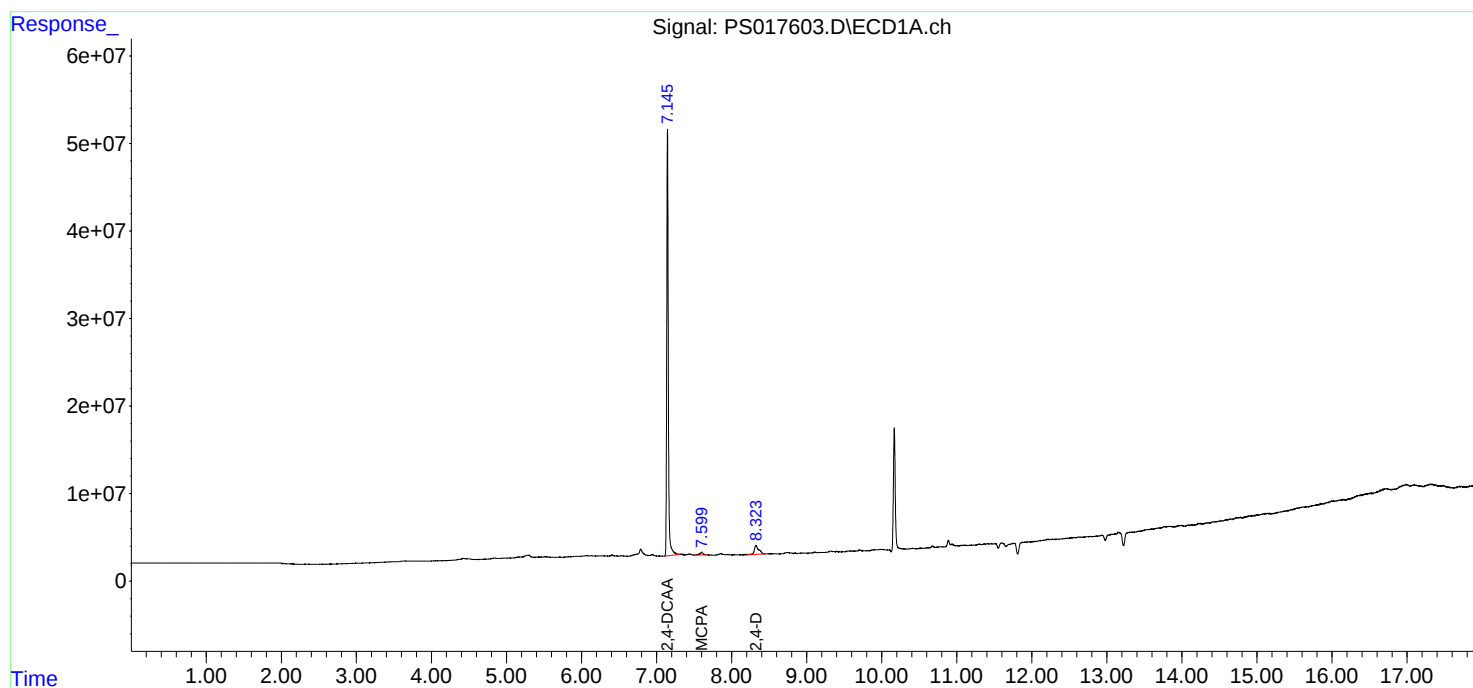


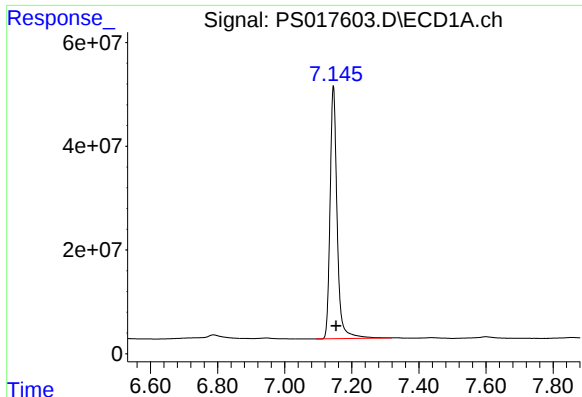

#4 2,4-DCAA


R.T.: 7.145 min
Delta R.T.: -0.008 min
Response: 709618693
Conc: 451.36 ng/ml

Instrument :
ECD_S
ClientSampleId :

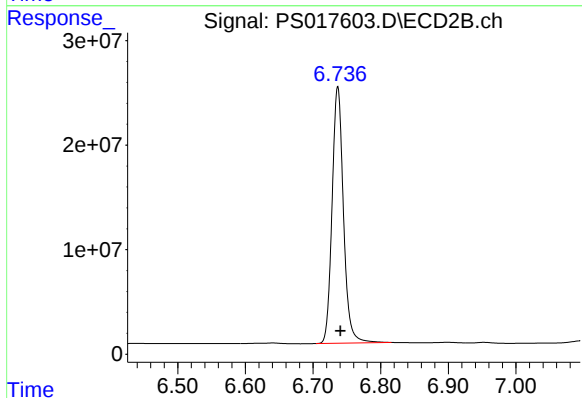


#4 2,4-DCAA

R.T.: 6.737 min
Delta R.T.: -0.004 min
Response: 286707129
Conc: 483.83 ng/ml

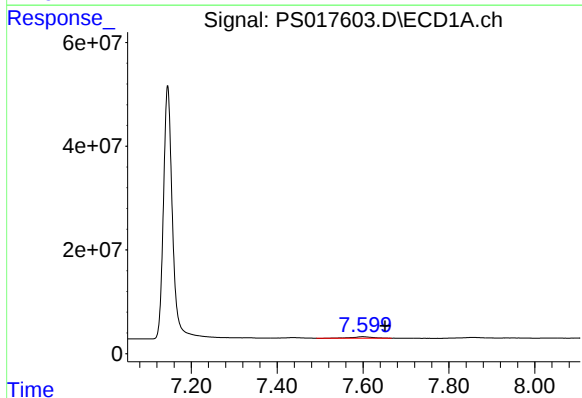


#7 MCPA

R.T.: 7.599 min
Delta R.T.: -0.052 min
Response: 9282390
Conc: 1.42 ug/ml

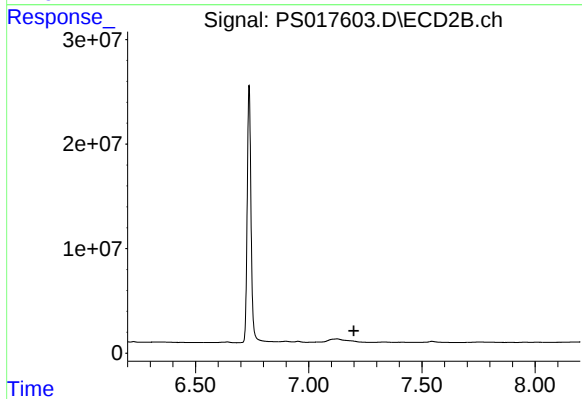

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 7.200 min
Response: 0
Conc: N.D.

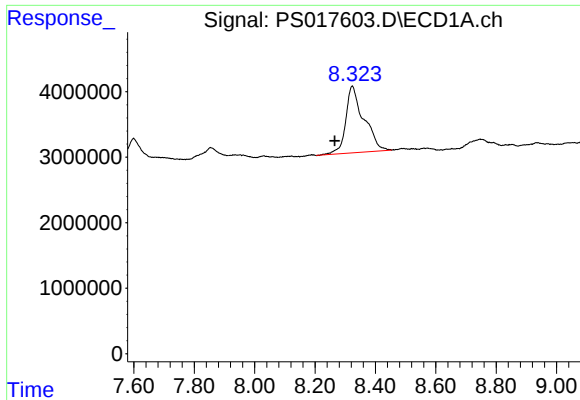

#9 2,4-D

R.T.: 8.324 min
Delta R.T.: 0.058 min
Response: 42222370
Conc: 22.60 ng/ml

Instrument :
ECD_S
ClientSampleId :

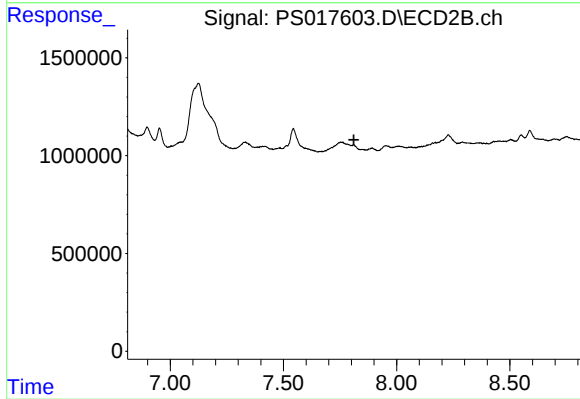

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.811 min
Response: 0
Conc: N.D.