

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120922\
 Data File : PS021403.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2022 08:30
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 11:50:46 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.383	0.000	1533576	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.513	0.000	1297899	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.737	0.000	1610915	0	<MDL	N.D. #
3) T	4-Nitroph...	6.215	0.000	5009247	0	2.786	N.D. #
5) T	DICAMBA	6.524	6.976	591028	1151342	<MDL	<MDL #
6) T	MCP	6.648	0.000	52142	0	<MDL	N.D. #
7) T	MCPA	6.784	0.000	423490	0	<MDL	N.D. #
8) T	DICHLORPROP	7.128	7.622	641638	1579486	<MDL	<MDL #
9) T	2,4-D	7.337	7.897	10710161	1074466	2.803	<MDL #
10) T	Pentachlo...	7.555	8.318	1714133	2530451	<MDL	<MDL #
11) T	2,4,5-TP ...	8.089	8.682	4596221	1204125	<MDL	<MDL #
12) T	2,4,5-T	8.355	9.060	6756346	1598290	<MDL	<MDL #
13) T	2,4-DB	8.862	0.000	998077	0	<MDL	N.D. #
14) T	DINOSEB	9.904	9.890	1843694	803602	<MDL	<MDL #
15) T	Picloram	9.764	10.873	114.2E6	94128407	3.986	5.788 #
16) T	DCPA	10.179	10.816	2373354	21463662	<MDL	1.582 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120922\
Data File : PS021403.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2022 08:30
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 11:50:46 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

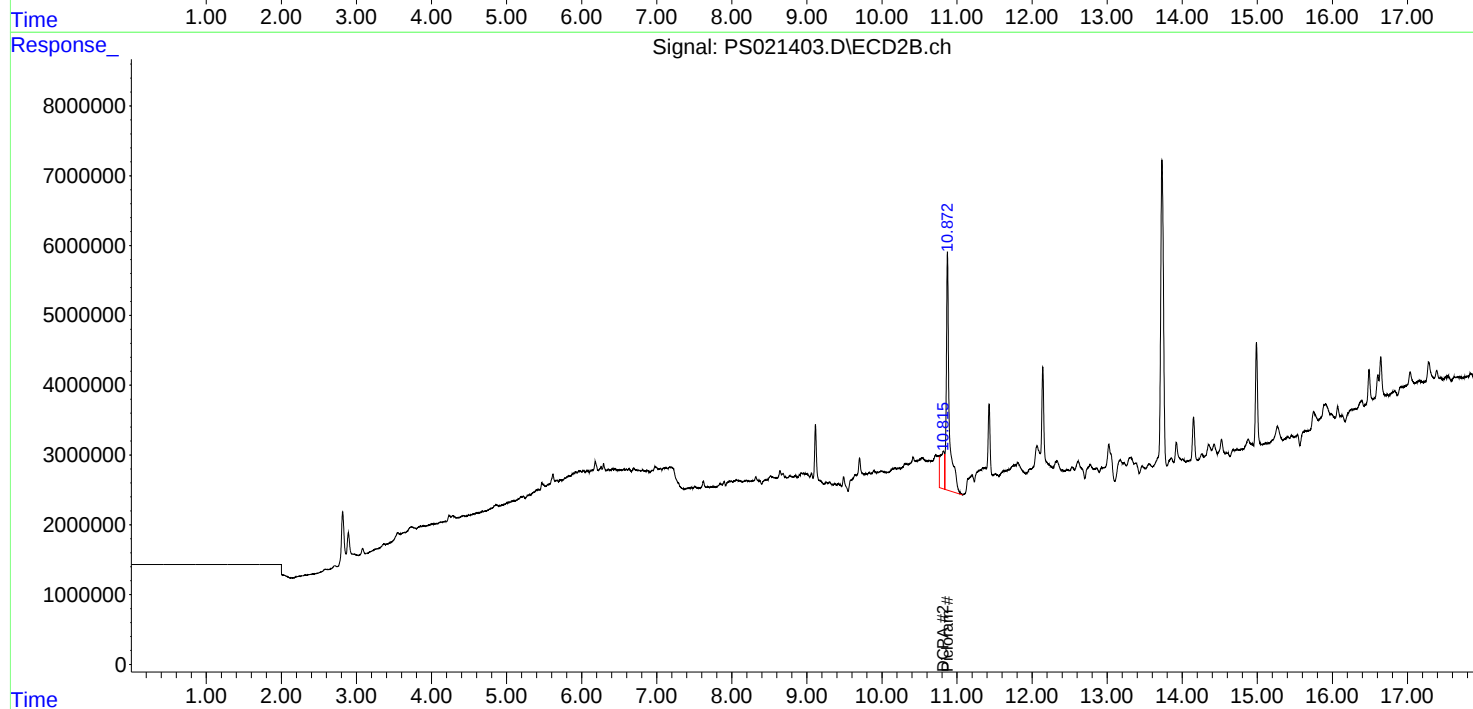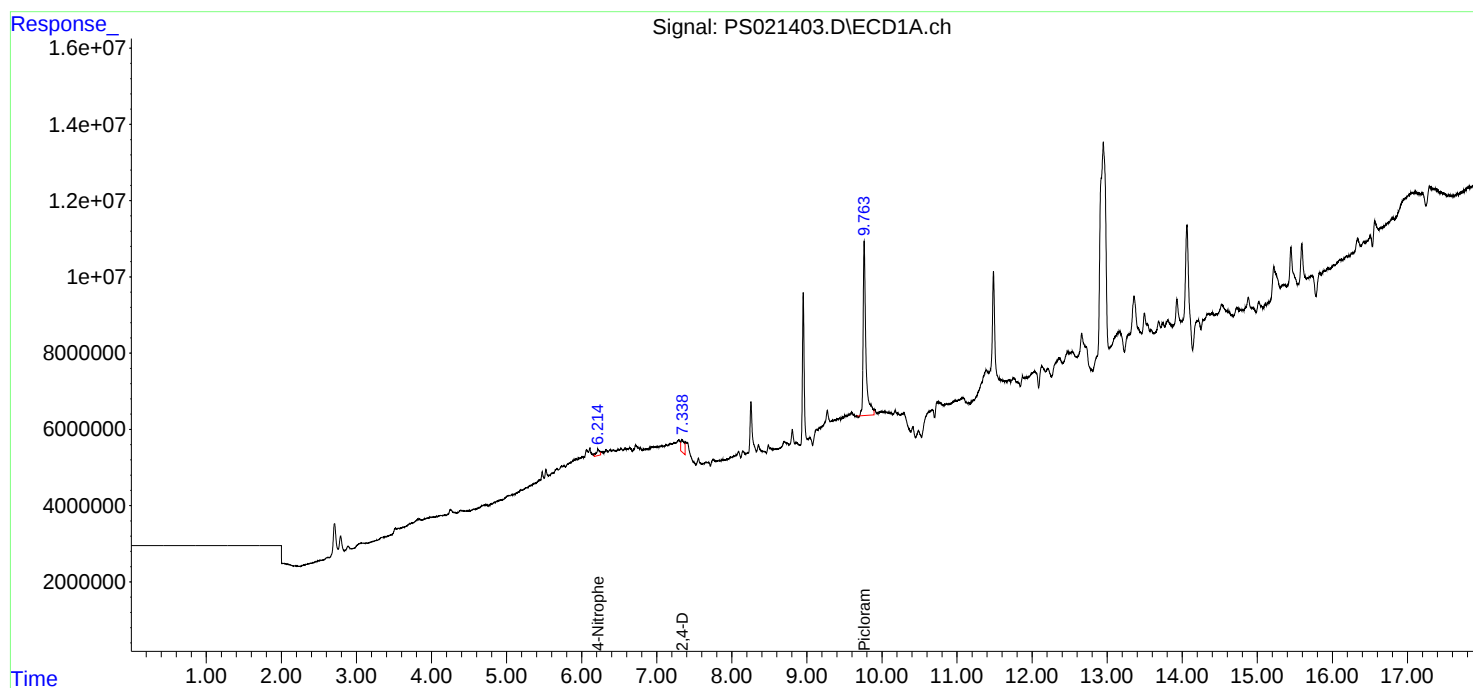


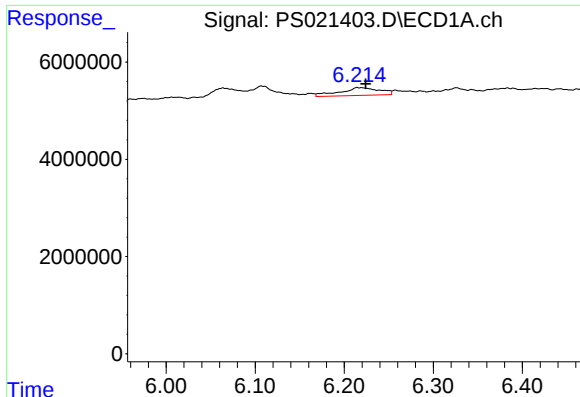

#3 4-Nitrophenol


R.T.: 6.215 min
Delta R.T.: -0.010 min
Response: 5009247
Conc: 2.79 ng/ml

Instrument :
ECD_S
ClientSampleId :

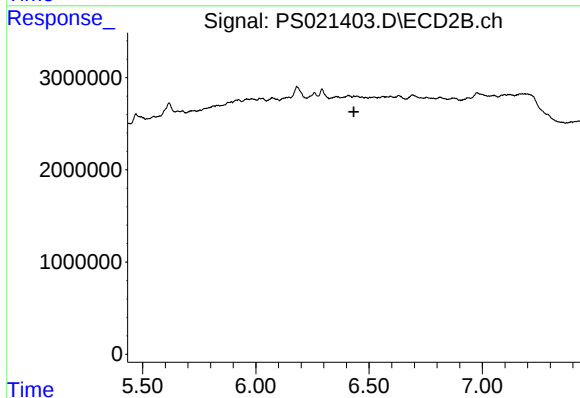


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

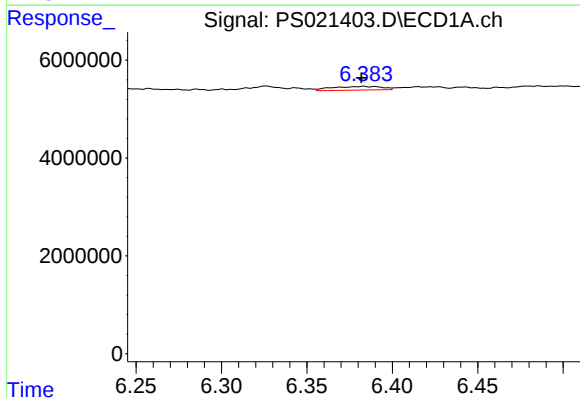


#4 2,4-DCAA

R.T.: 6.383 min
Delta R.T.: 0.001 min
Response: 1533576
Conc: N.D.

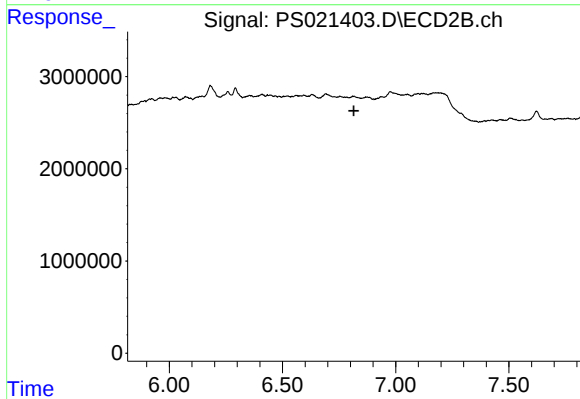

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.816 min
Response: 0
Conc: N.D.

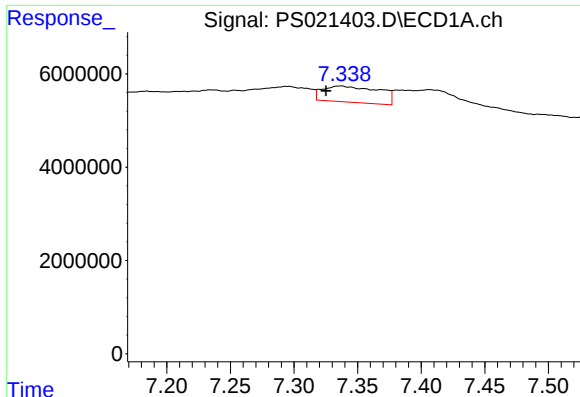

#9 2,4-D


R.T.: 7.337 min
Delta R.T.: 0.012 min
Response: 10710161
Conc: 2.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

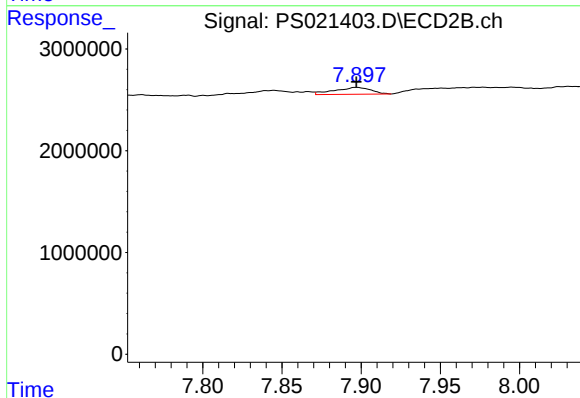


#9 2,4-D

R.T.: 7.897 min
Delta R.T.: 0.000 min
Response: 1074466
Conc: N.D.

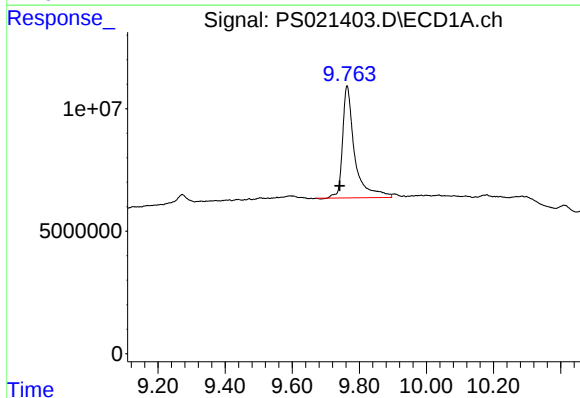


#15 Picloram

R.T.: 9.764 min
Delta R.T.: 0.021 min
Response: 114153323
Conc: 3.99 ng/ml

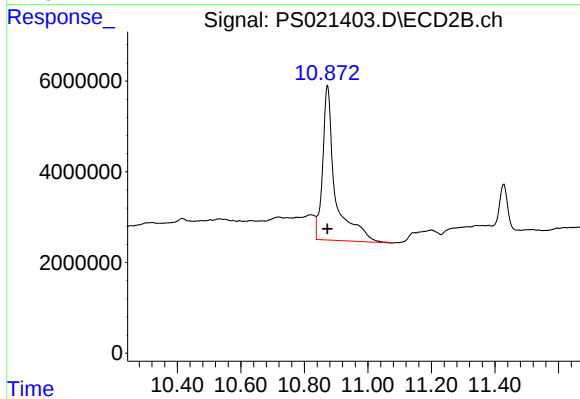

#15 Picloram


R.T.: 10.873 min
Delta R.T.: 0.000 min
Response: 94128407
Conc: 5.79 ng/ml

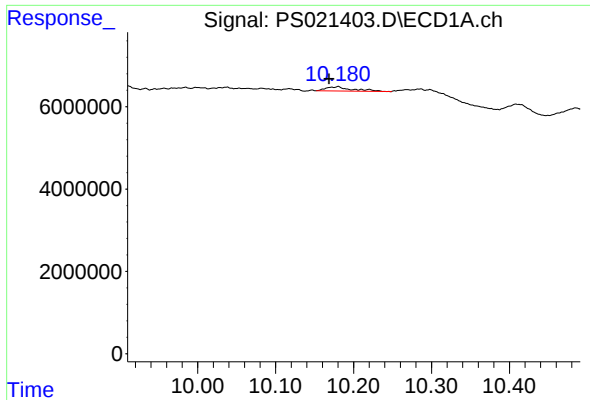

#16 DCPA

R.T.: 10.179 min
Delta R.T.: 0.010 min
Response: 2373354
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

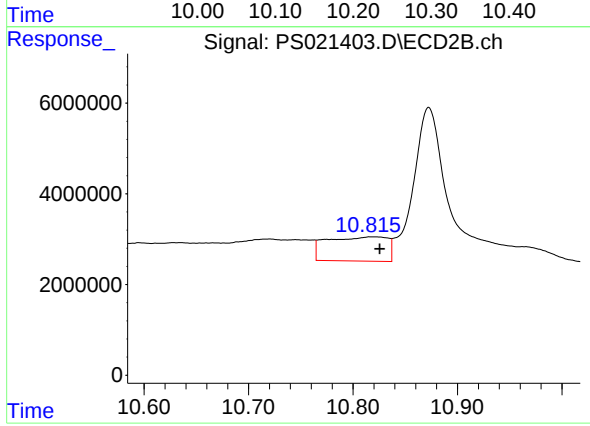

#16 DCPA

R.T.: 10.816 min
Delta R.T.: -0.009 min
Response: 21463662
Conc: 1.58 ng/ml