

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120922\
 Data File : PS021404.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2022 08:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 09 11:51:02 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.380	6.812	1382.5E6	931.2E6	475.839	540.170
Target Compounds							
1) T	Dalapon	2.532f	0.000	280191	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.729	0.000	8171294	0	2.056	N.D. #
3) T	4-Nitroph...	6.223	0.000	7022994	0	3.906	N.D. #
5) T	DICAMBA	0.000	7.032f	0	8251221	N.D.	1.080
6) T	MCP	0.000	7.032f	0	8251221	N.D.	1.402
7) T	MCPA	6.761	0.000	6354578	0	<MDL	N.D. #
8) T	DICHLORPROP	7.132	7.639	246503	4806672	<MDL	2.440 #
9) T	2,4-D	7.311	0.000	6158035	0	1.612	N.D. #
10) T	Pentachlo...	7.547	0.000	1616854	0	<MDL	N.D. #
11) T	2,4,5-TP ...	8.088	8.651	4058596	2165915	<MDL	<MDL #
12) T	2,4,5-T	8.370	9.078	6503199	2330139	<MDL	<MDL #
13) T	2,4-DB	8.833	9.640f	3540653	1070798	<MDL	<MDL #
15) T	Picloram	9.726	10.890	16809790	34957109	<MDL	2.150 #
16) T	DCPA	10.167	10.823	1687756	1301429	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120922\
Data File : PS021404.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2022 08:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 09 11:51:02 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

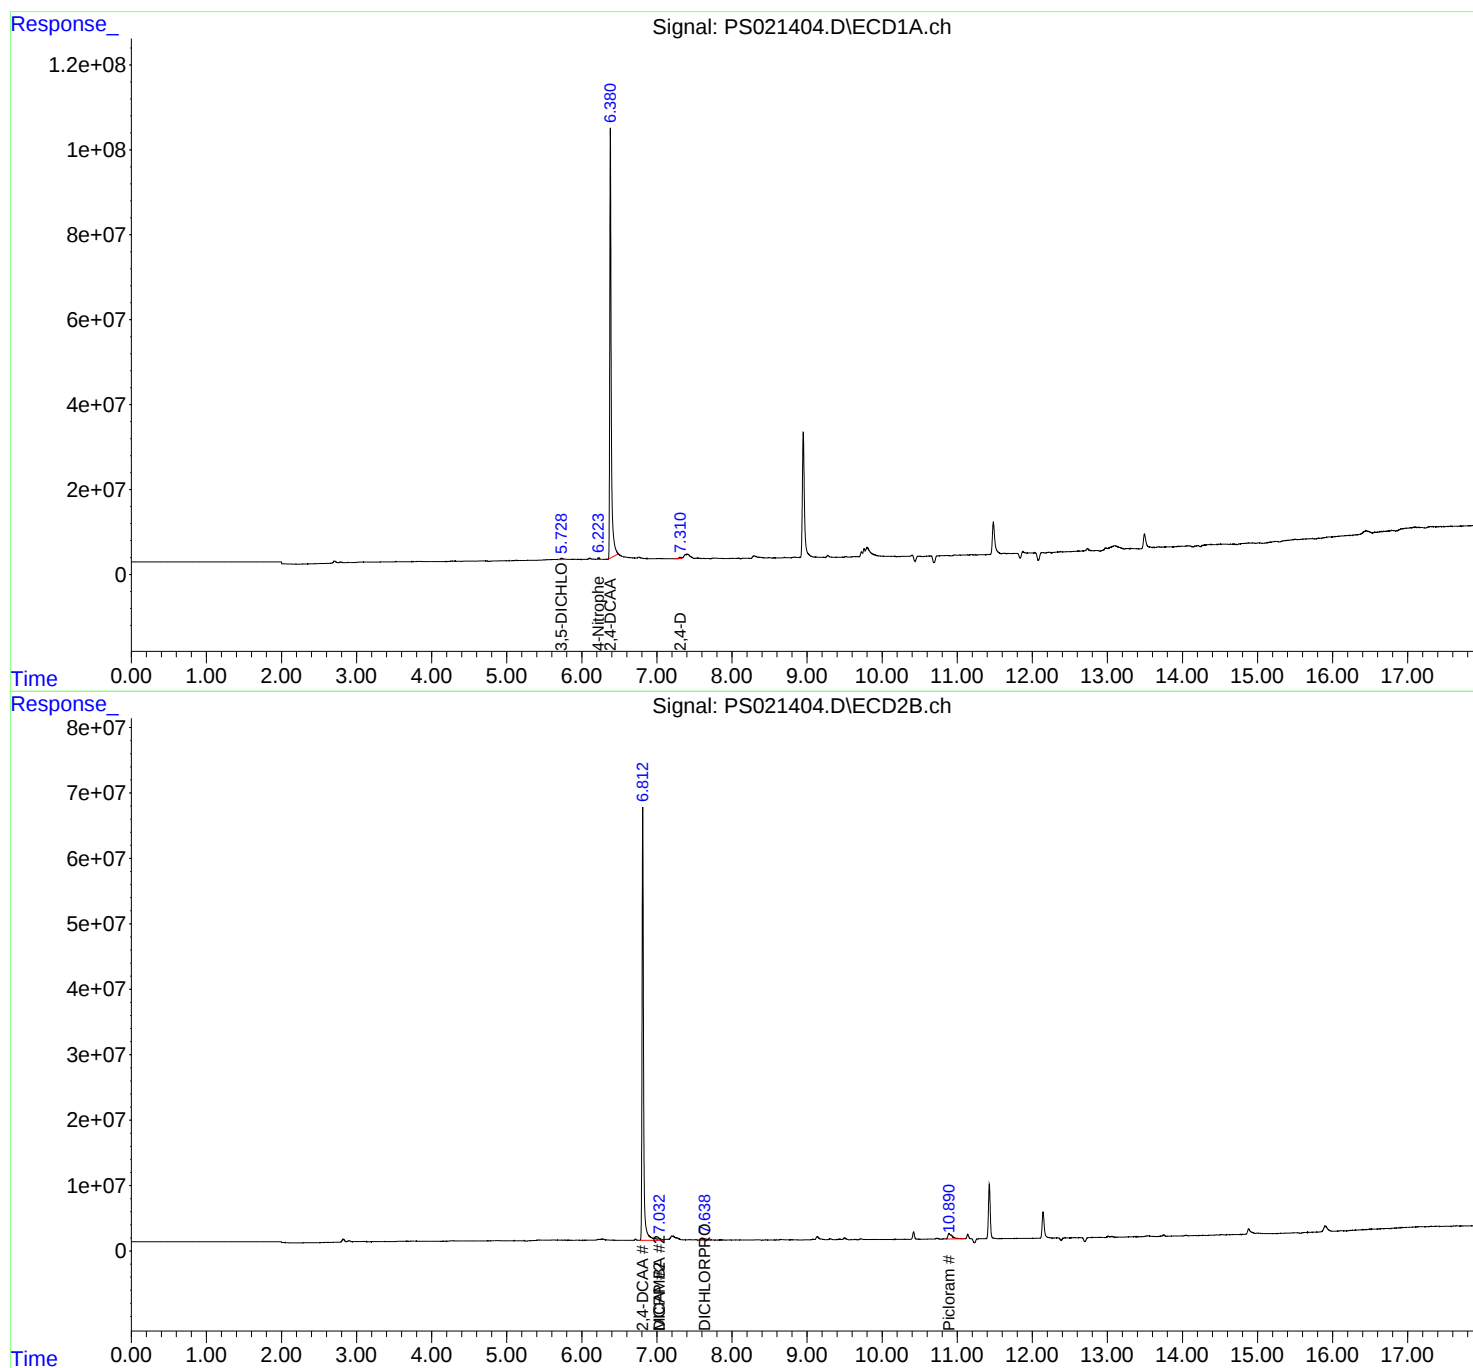


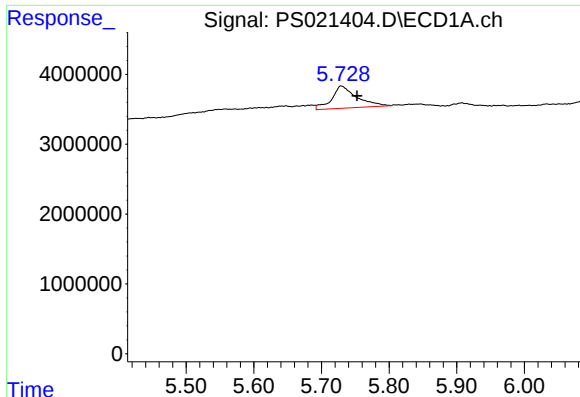

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.729 min
Delta R.T.: -0.023 min
Response: 8171294
Conc: 2.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

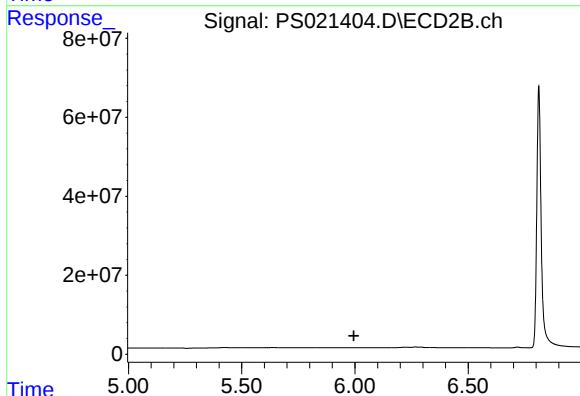


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

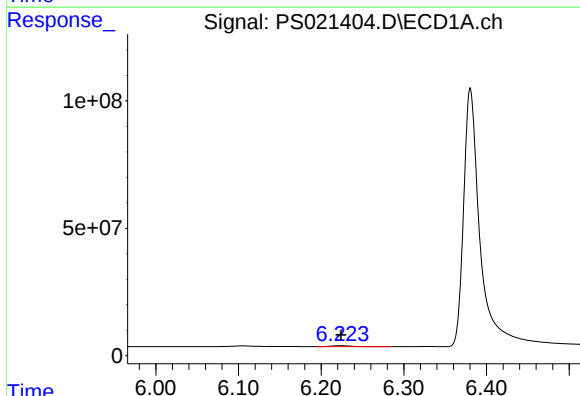


#3 4-Nitrophenol

R.T.: 6.223 min
Delta R.T.: 0.000 min
Response: 7022994
Conc: 3.91 ng/ml

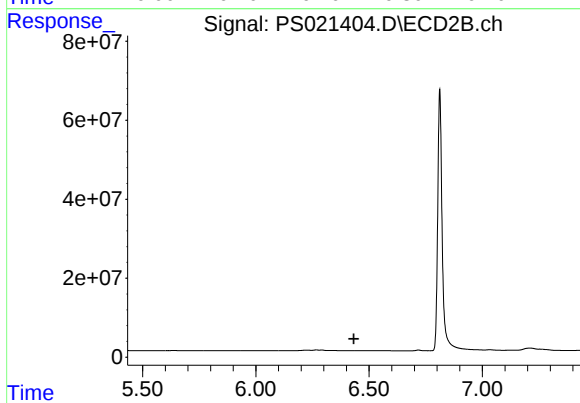

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

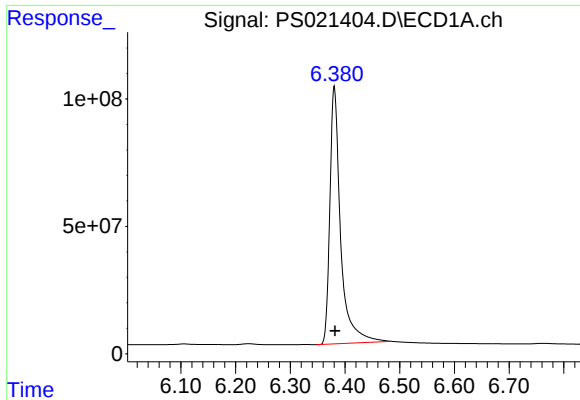

#4 2,4-DCAA


R.T.: 6.380 min
Delta R.T.: -0.001 min
Response: 1382546458
Conc: 475.84 ng/ml

Instrument :
ECD_S
ClientSampleId :

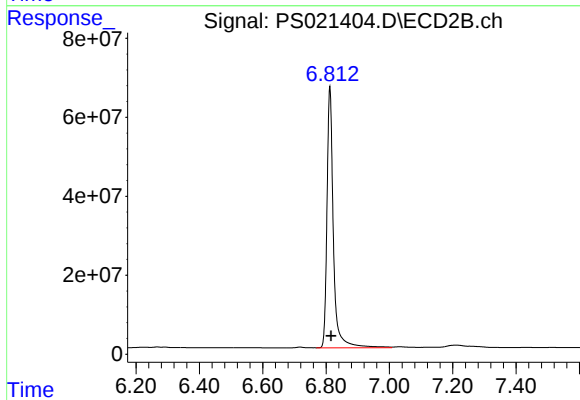


#4 2,4-DCAA

R.T.: 6.812 min
Delta R.T.: -0.003 min
Response: 931249010
Conc: 540.17 ng/ml

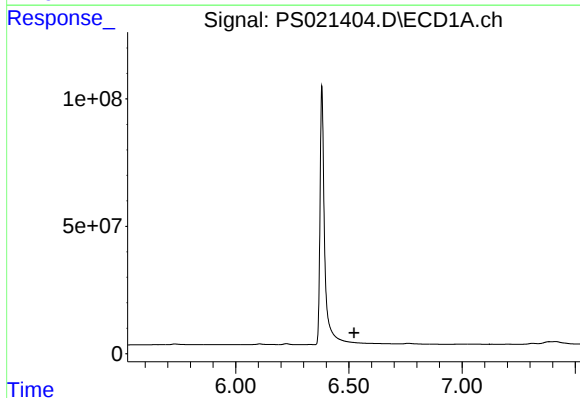


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

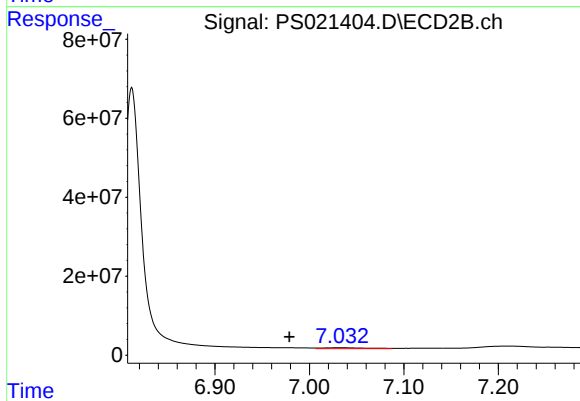

#5 DICAMBA


R.T.: 7.032 min
Delta R.T.: 0.054 min
Response: 8251221
Conc: 1.08 ng/ml

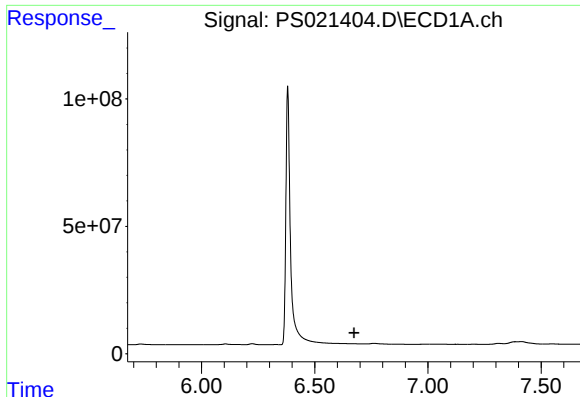

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

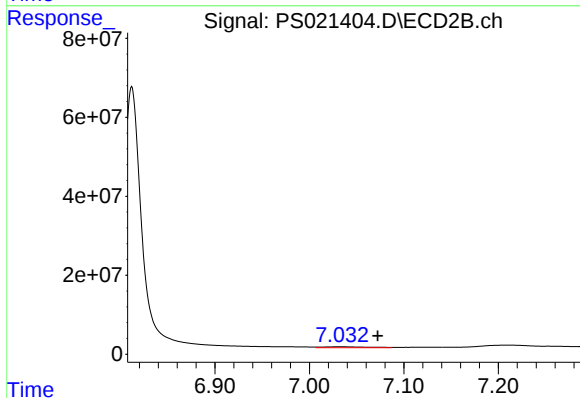


#6 MCP

R.T.: 7.032 min
Delta R.T.: -0.040 min
Response: 8251221
Conc: 1.40 ug/ml

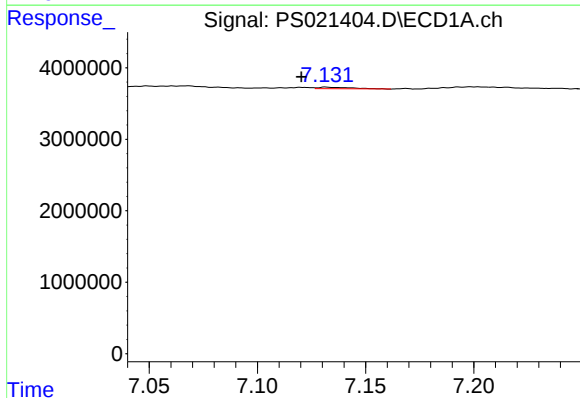


#8 DICHLORPROP

R.T.: 7.132 min
Delta R.T.: 0.012 min
Response: 246503
Conc: N.D.

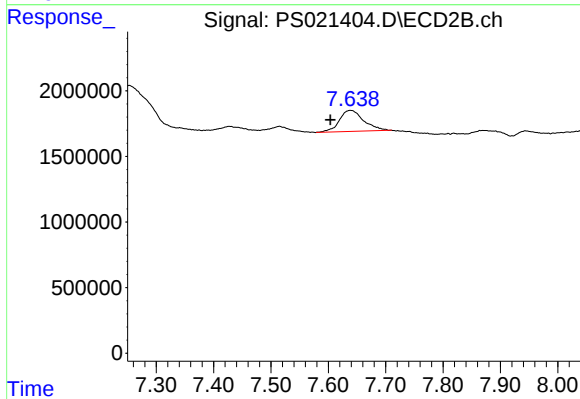

#8 DICHLORPROP


R.T.: 7.639 min
Delta R.T.: 0.035 min
Response: 4806672
Conc: 2.44 ng/ml

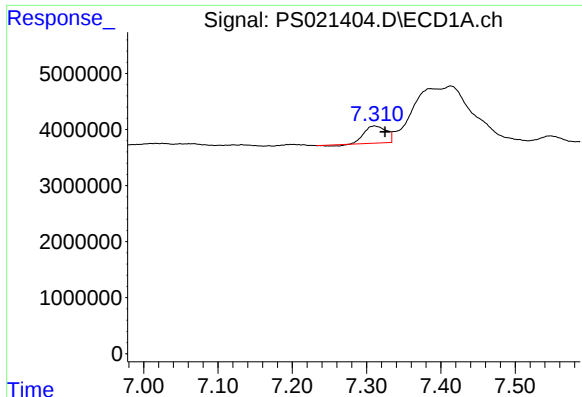

#9 2,4-D


R.T.: 7.311 min
Delta R.T.: -0.015 min
Response: 6158035
Conc: 1.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

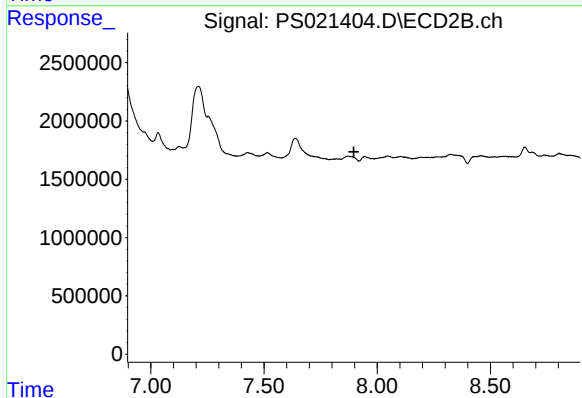


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.897 min
Response: 0
Conc: N.D.

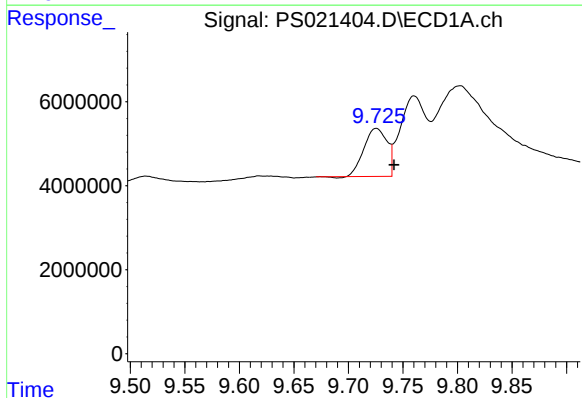

#15 Picloram

R.T.: 9.726 min
Delta R.T.: -0.017 min
Response: 16809790
Conc: N.D.

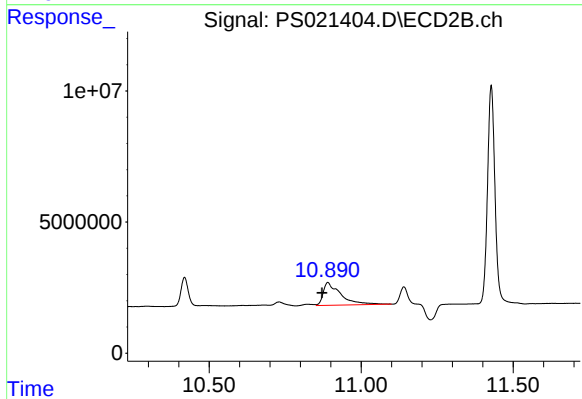

#15 Picloram

R.T.: 10.890 min
Delta R.T.: 0.018 min
Response: 34957109
Conc: 2.15 ng/ml