

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120922\
 Data File : PS021419.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2022 18:20
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 04:32:50 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.379	6.811	1423.3E6	944.3E6	489.858	547.762
Target Compounds							
1) T	Dalapon	2.531f	0.000	552200	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.727	0.000	11666090	0	2.935	N.D. #
3) T	4-Nitroph...	6.220	0.000	7500727	0	4.171	N.D. #
5) T	DICAMBA	0.000	6.975	0	6186439	N.D.	<MDL
6) T	MCPD	0.000	7.031f	0	6038377	N.D.	1.026
7) T	MCPA	6.752f	0.000	10951362	0	<MDL	N.D. #
8) T	DICHLORPROP	7.131	7.637	1059160	9210299	<MDL	4.676 #
9) T	2,4-D	7.303	0.000	8605756	0	2.252	N.D. #
10) T	Pentachlo...	7.552	8.321	3014186	4823975	<MDL	<MDL #
11) T	2,4,5-TP ...	8.087	8.686	6654692	2479015	<MDL	<MDL #
12) T	2,4,5-T	8.369	9.073	12223824	5541610	<MDL	<MDL #
13) T	2,4-DB	8.873	9.583	2023172	2173097	<MDL	1.512 #
14) T	DINOSEB	9.901	9.895	6112509	2024159	<MDL	<MDL #
15) T	Picloram	9.758	10.863	32470746	4268606	1.134	<MDL #
16) T	DCPA	10.167	10.821	4978773	11958575	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120922\
Data File : PS021419.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2022 18:20
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 04:32:50 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

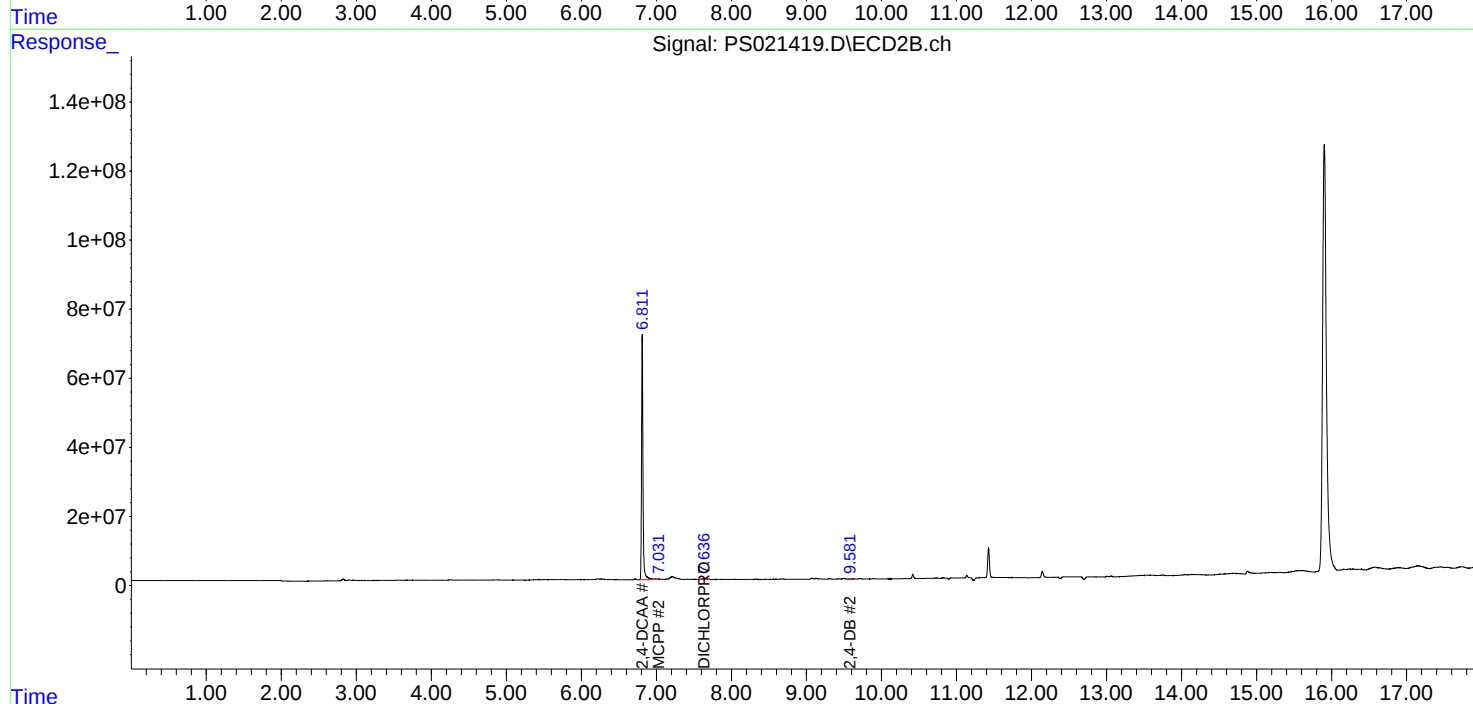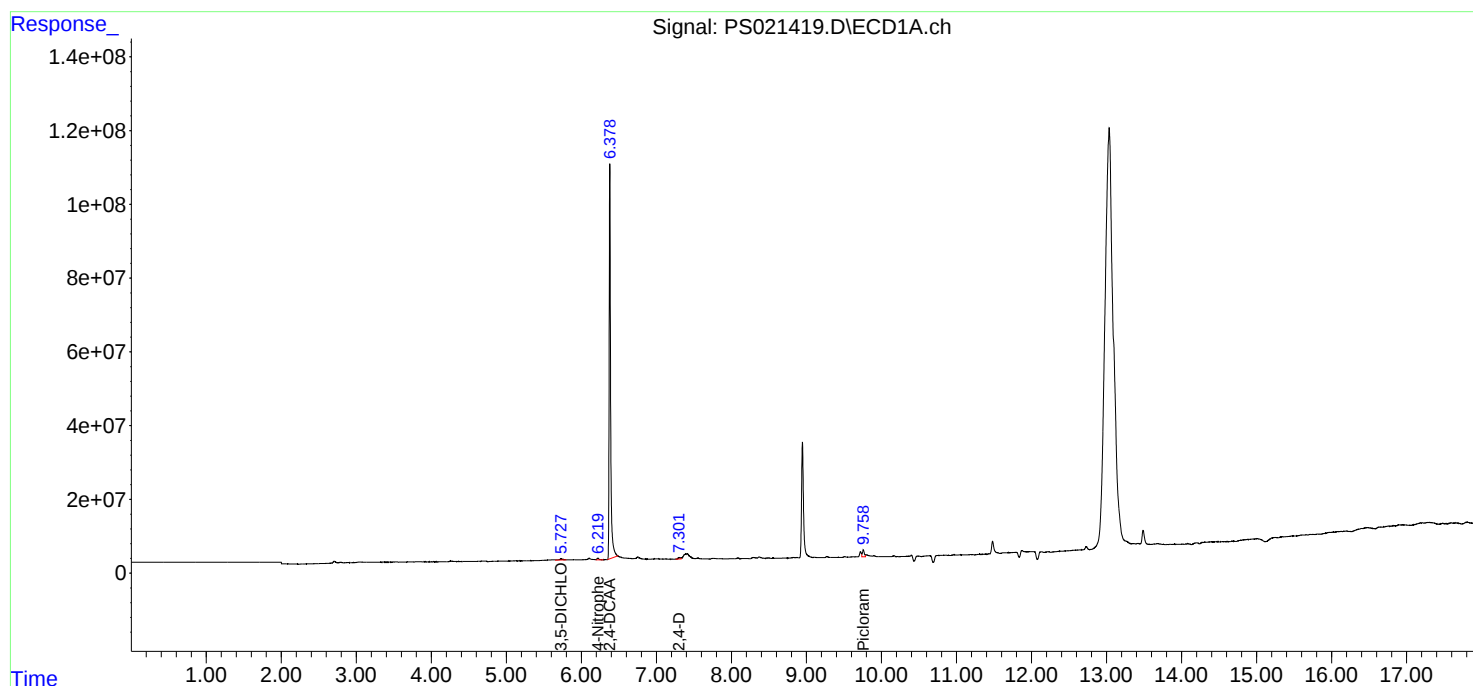


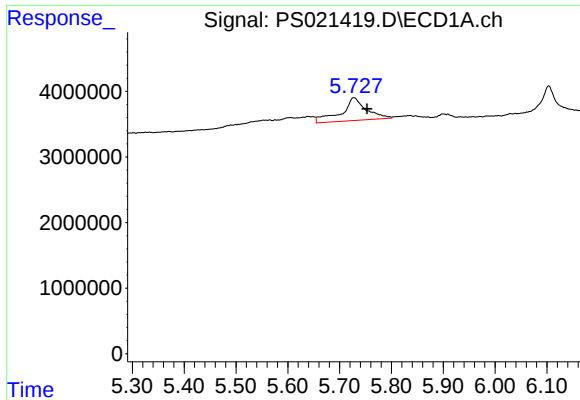

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.727 min
Delta R.T.: -0.025 min
Response: 11666090
Conc: 2.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

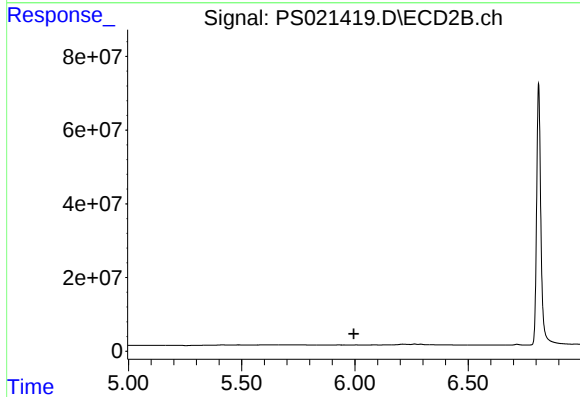


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

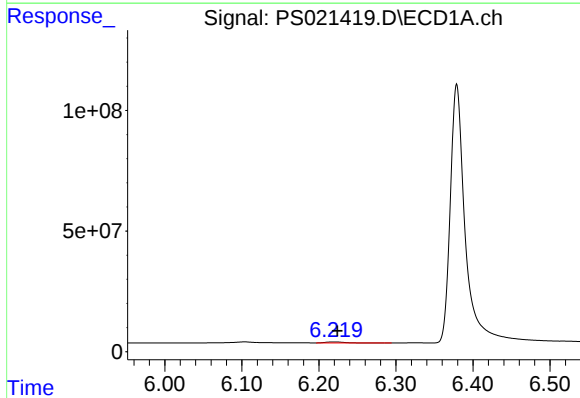


#3 4-Nitrophenol

R.T.: 6.220 min
Delta R.T.: -0.005 min
Response: 7500727
Conc: 4.17 ng/ml

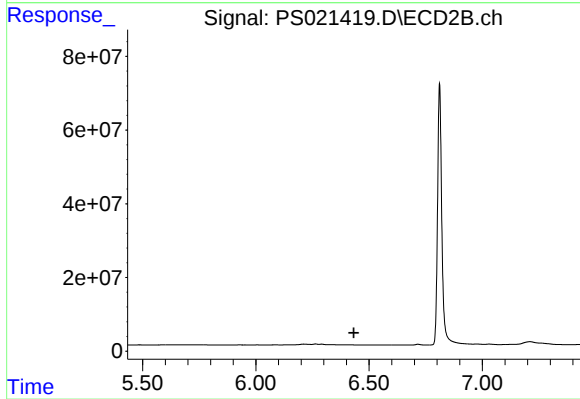

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

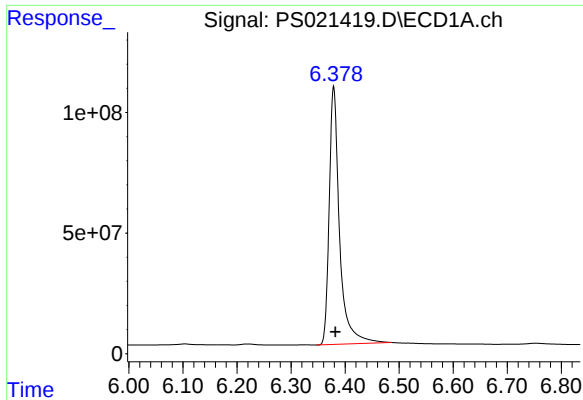

#4 2,4-DCAA


R.T.: 6.379 min
Delta R.T.: -0.003 min
Response: 1423279296
Conc: 489.86 ng/ml

Instrument :
ECD_S
ClientSampleId :

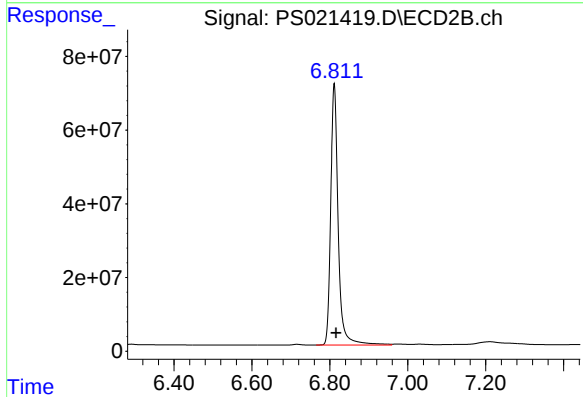


#4 2,4-DCAA

R.T.: 6.811 min
Delta R.T.: -0.004 min
Response: 944338035
Conc: 547.76 ng/ml

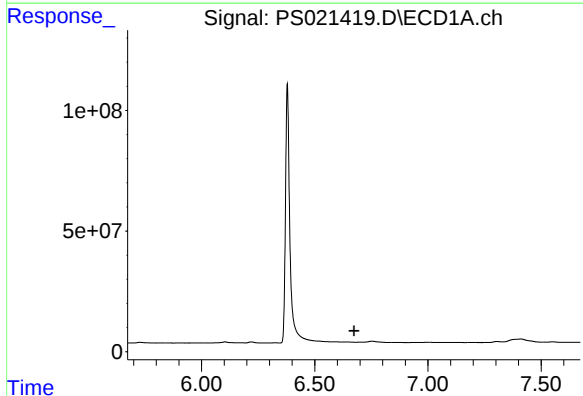


#6 MCP

R.T.: 0.000 min
Exp R.T. : 6.673 min
Response: 0
Conc: N.D.

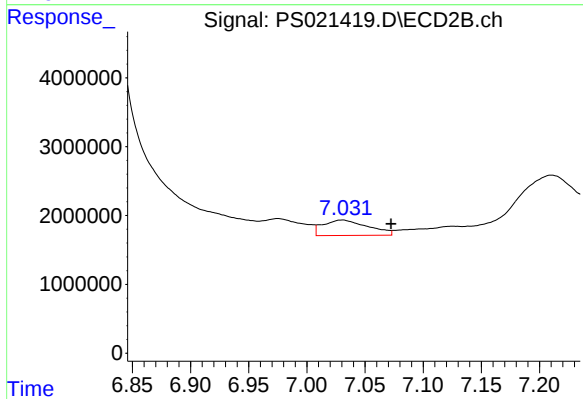

#6 MCP


R.T.: 7.031 min
Delta R.T.: -0.042 min
Response: 6038377
Conc: 1.03 ug/ml

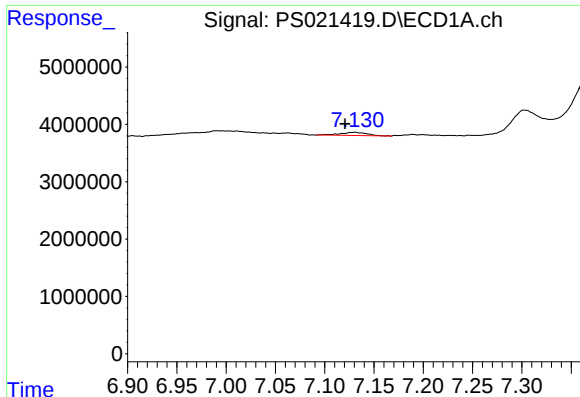

#8 DICHLORPROP


R.T.: 7.131 min
Delta R.T.: 0.010 min
Response: 1059160
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

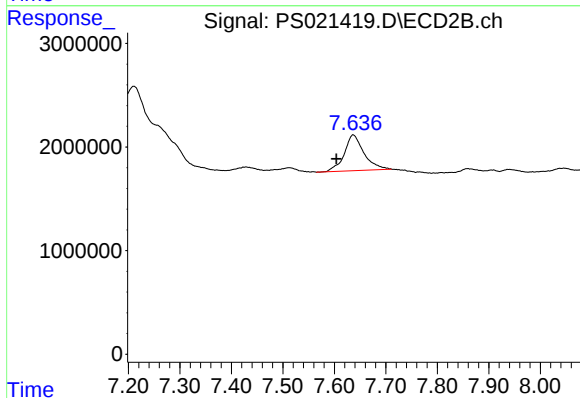


#8 DICHLORPROP

R.T.: 7.637 min
Delta R.T.: 0.033 min
Response: 9210299
Conc: 4.68 ng/ml

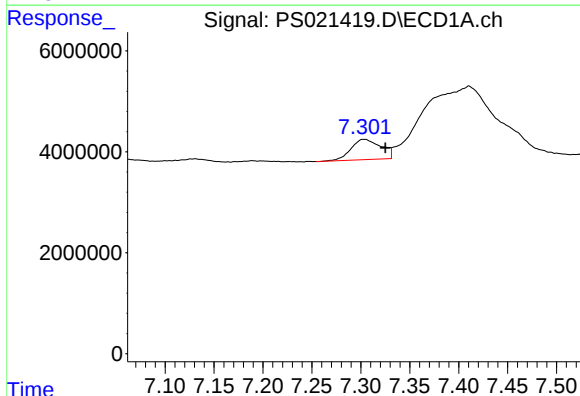


#9 2,4-D

R.T.: 7.303 min
Delta R.T.: -0.022 min
Response: 8605756
Conc: 2.25 ng/ml

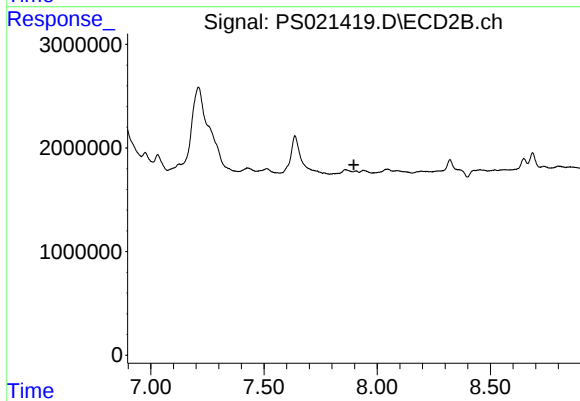

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 7.897 min
Response: 0
Conc: N.D.

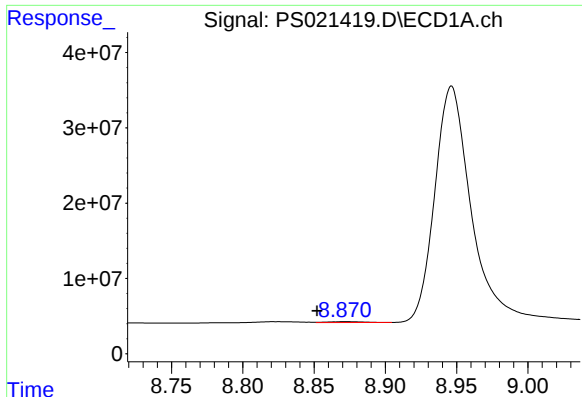

#13 2,4-DB


R.T.: 8.873 min
Delta R.T.: 0.020 min
Response: 2023172
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

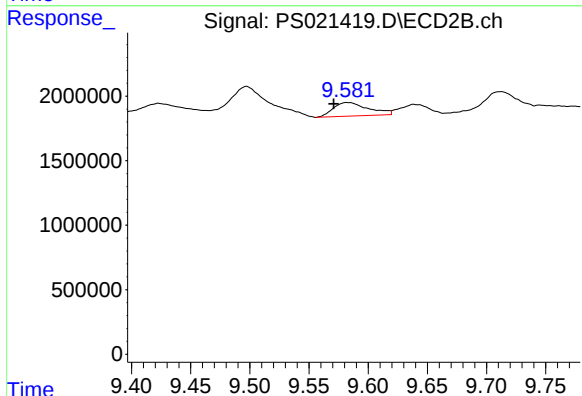


#13 2,4-DB

R.T.: 9.583 min
Delta R.T.: 0.012 min
Response: 2173097
Conc: 1.51 ng/ml

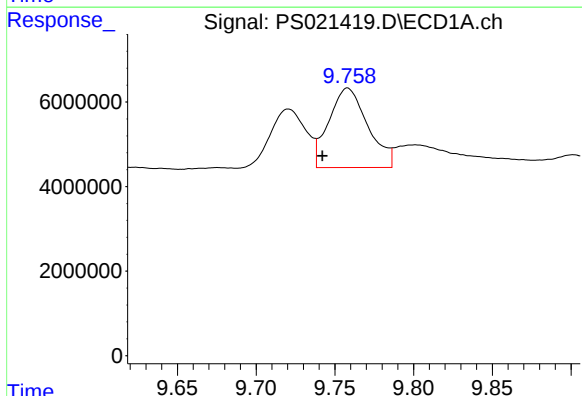

#15 Picloram

R.T.: 9.758 min
Delta R.T.: 0.016 min
Response: 32470746
Conc: 1.13 ng/ml

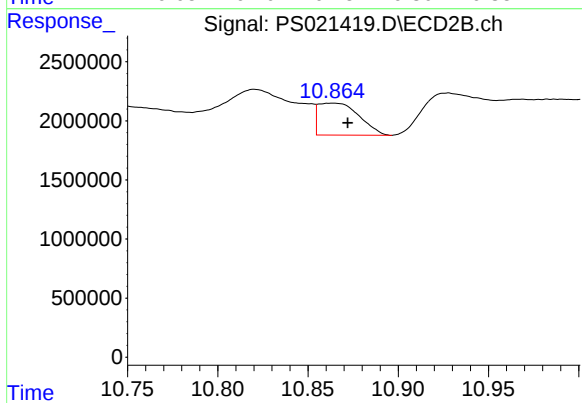

#15 Picloram

R.T.: 10.863 min
Delta R.T.: -0.009 min
Response: 4268606
Conc: N.D.