

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120925\
 Data File : PS032663.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 09 Dec 2025 20:18
 Operator : AR\AJ
 Sample : Q3806-01RE
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-01-12-5-2025RE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 02:16:43 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120925.M
 Quant Title : 8080.M
 QLast Update : Tue Dec 09 16:35:46 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.004	7.371	519.3E6	98002113	94.461	19.876 #
Target Compounds							
1) T	Dalapon	0.000	2.492f	0	1977.1E6	N.D.	273.234
2) T	3,5-DICHL...	0.000	6.354	0	4308770	N.D.	<MDL
3) T	4-Nitroph...	6.816	6.891f	38026633	63640832	21.250	28.096 #
5) T	DICAMBA	7.176	7.530f	61405579	12975284	2.731	<MDL #
6) T	MCPD	7.393f	0.000	195.5E6	0	14.578	N.D. #
7) T	MCPA	7.505	7.890	267.4E6	397.0E6	16.124	27.714 #
8) T	DICHLORPROP	7.850	8.256	41729928	32731911	7.553	7.010
10) T	Pentachlo...	8.392	9.046f	190.2E6	221.7E6	2.600	3.919 #
11) T	2,4,5-TP ...	8.931	9.456	859.2E6	3883.0E6	25.670	146.898 #
13) T	2,4-DB	9.839f	10.420f	618.8E6	993.1E6	147.272	237.597 #
14) T	DINOSEB	10.957f	10.828	434.4E6	489.8E6	17.851	29.755 #
15) T	Picloram	10.817	0.000	19804081	0	<MDL	N.D. #
16) T	DCPA	11.264	0.000	141.0E6	0	3.472	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS120925\
Data File : PS032663.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 09 Dec 2025 20:18
Operator : AR\AJ
Sample : Q3806-01RE
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-01-12-5-2025RE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 02:16:43 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120925.M
Quant Title : 8080.M
QLast Update : Tue Dec 09 16:35:46 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

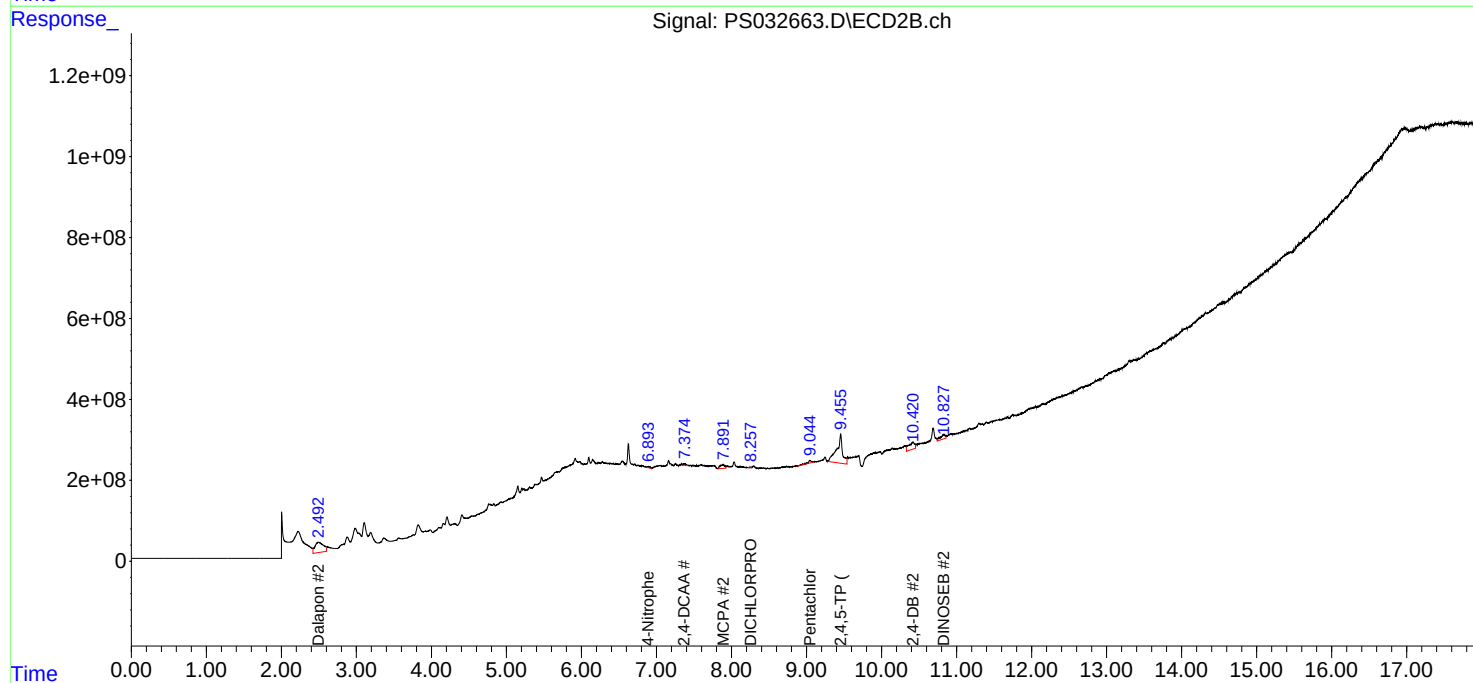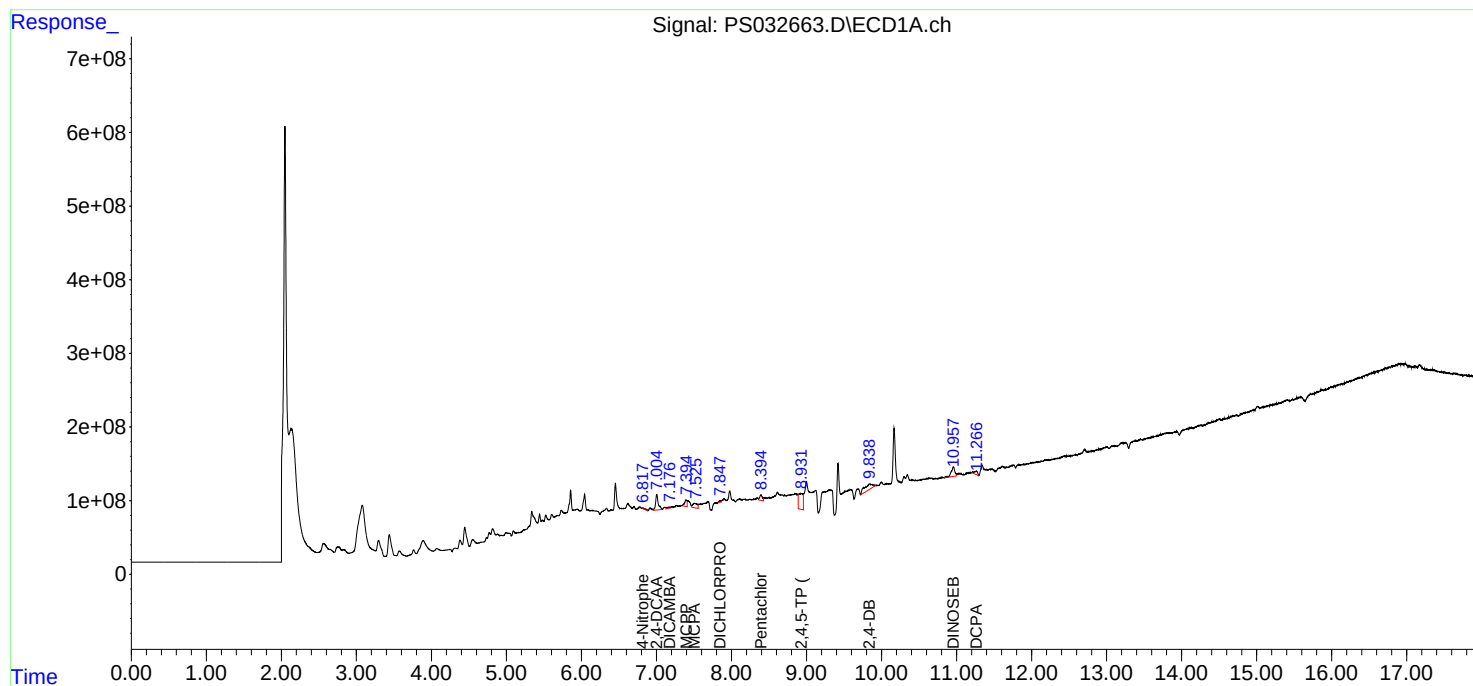


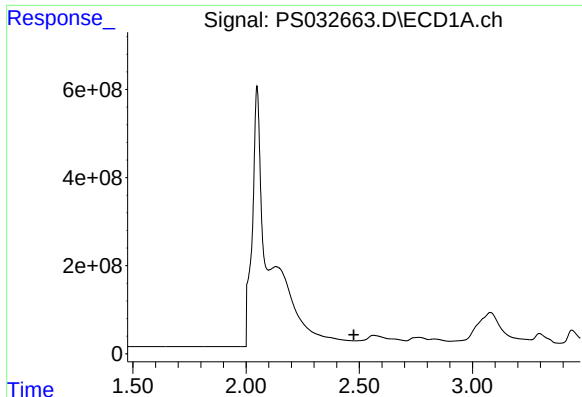

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.476 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-01-12-5-2025RE

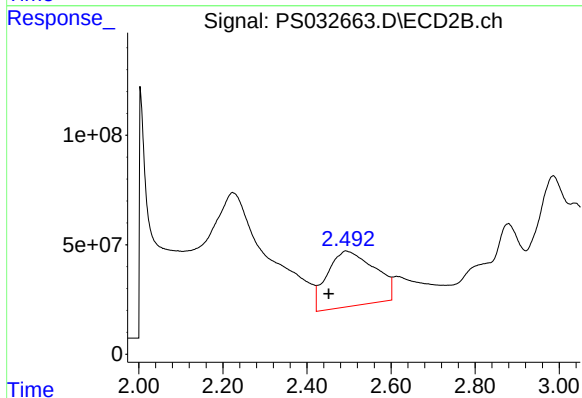


#1 Dalapon

R.T.: 2.492 min
Delta R.T.: 0.041 min
Response: 1977079665
Conc: 273.23 ng/ml

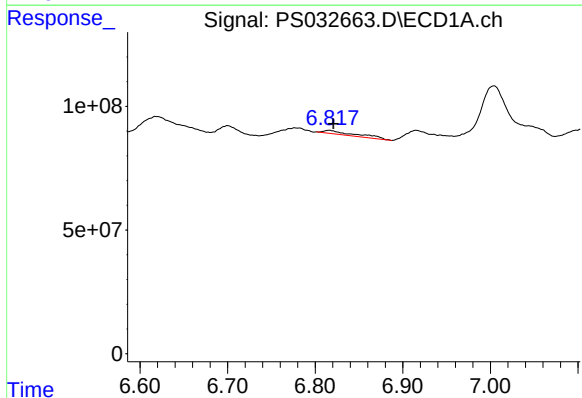


#3 4-Nitrophenol

R.T.: 6.816 min
Delta R.T.: -0.005 min
Response: 38026633
Conc: 21.25 ng/ml

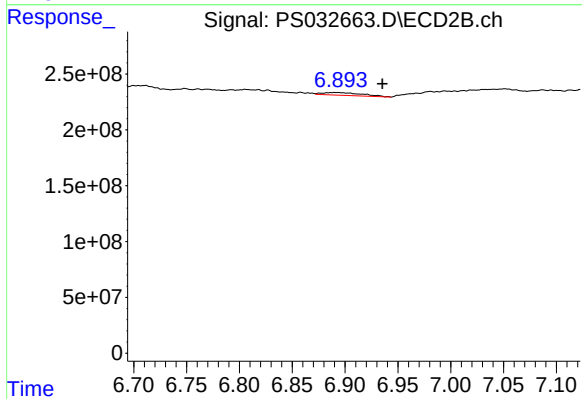

#3 4-Nitrophenol


R.T.: 6.891 min
Delta R.T.: -0.045 min
Response: 63640832
Conc: 28.10 ng/ml

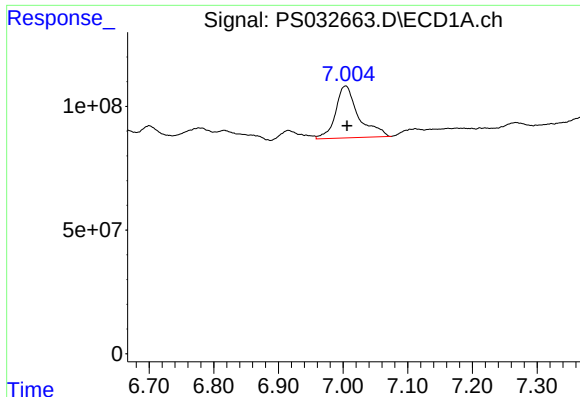

#4 2,4-DCAA


R.T.: 7.004 min
Delta R.T.: -0.003 min
Response: 519328043
Conc: 94.46 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-01-12-5-2025RE

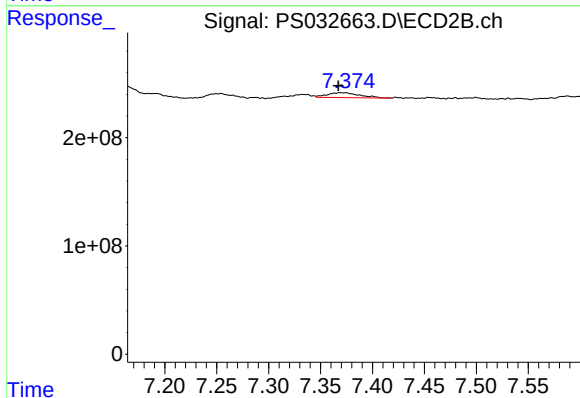


#4 2,4-DCAA

R.T.: 7.371 min
Delta R.T.: 0.003 min
Response: 98002113
Conc: 19.88 ng/ml

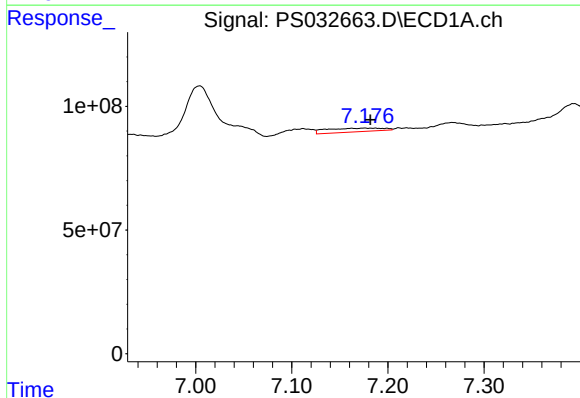


#5 DICAMBA

R.T.: 7.176 min
Delta R.T.: -0.006 min
Response: 61405579
Conc: 2.73 ng/ml

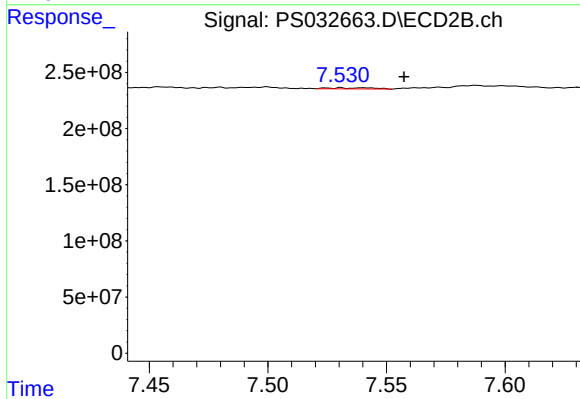

#5 DICAMBA


R.T.: 7.530 min
Delta R.T.: -0.027 min
Response: 12975284
Conc: N.D.

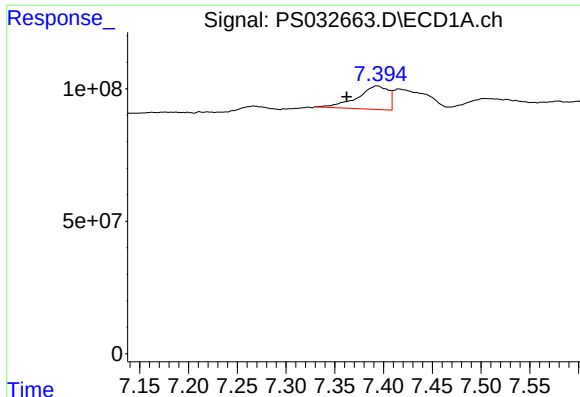

#6 MCPP


R.T.: 7.393 min
Delta R.T.: 0.031 min
Response: 195504842
Conc: 14.58 ug/ml

Instrument :
ECD_S
ClientSampleId :
TR-01-12-5-2025RE

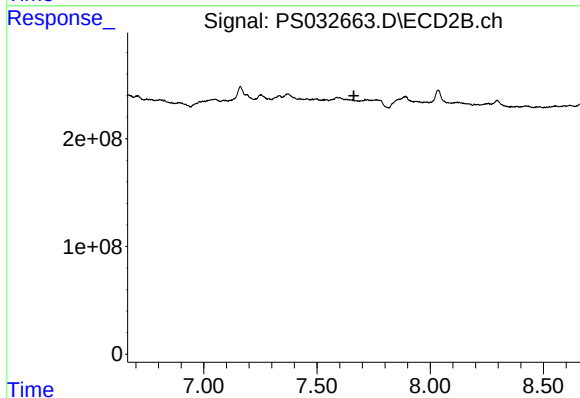


#6 MCPP

R.T.: 0.000 min
Exp R.T.: 7.663 min
Response: 0
Conc: N.D.

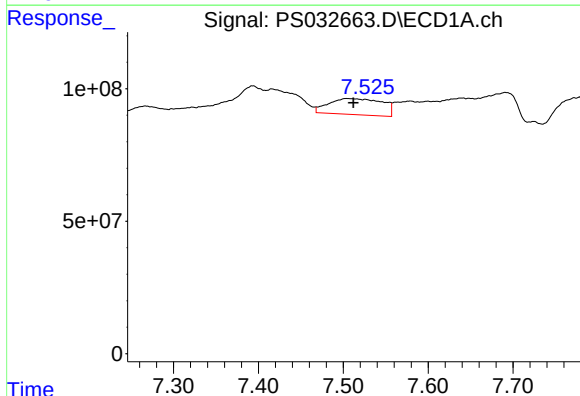


#7 MCPA

R.T.: 7.505 min
Delta R.T.: -0.007 min
Response: 267426371
Conc: 16.12 ug/ml

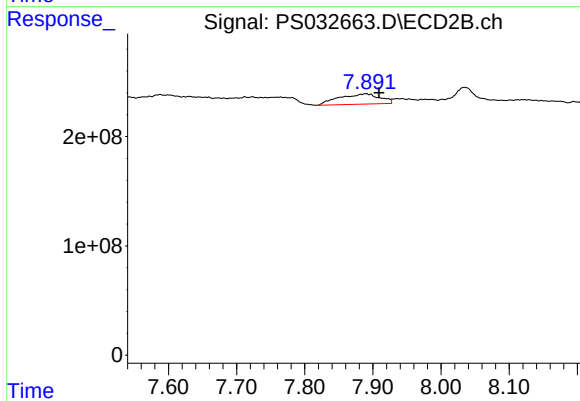

#7 MCPA


R.T.: 7.890 min
Delta R.T.: -0.020 min
Response: 396963588
Conc: 27.71 ug/ml

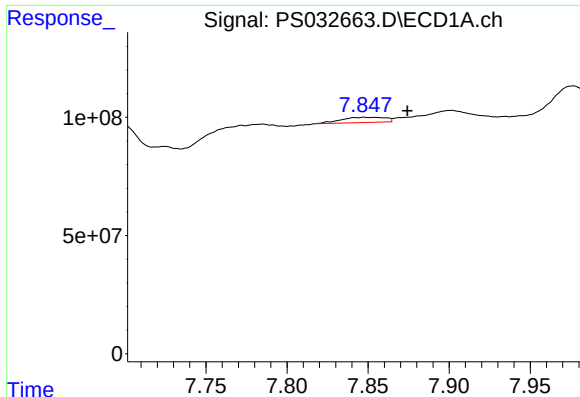

#8 DICHLORPROP


R.T.: 7.850 min
Delta R.T.: -0.025 min
Response: 41729928
Conc: 7.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-01-12-5-2025RE

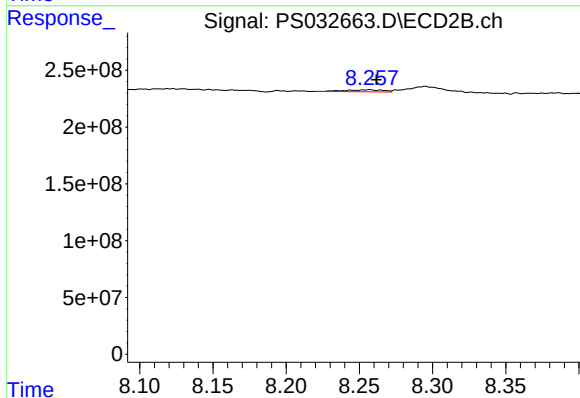


#8 DICHLORPROP

R.T.: 8.256 min
Delta R.T.: -0.005 min
Response: 32731911
Conc: 7.01 ng/ml

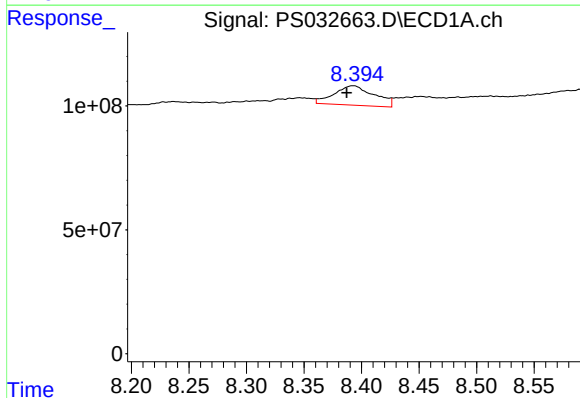


#10 Pentachlorophenol

R.T.: 8.392 min
Delta R.T.: 0.005 min
Response: 190176870
Conc: 2.60 ng/ml

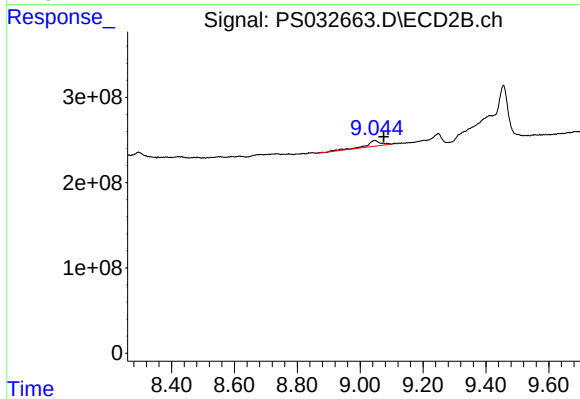

#10 Pentachlorophenol


R.T.: 9.046 min
Delta R.T.: -0.030 min
Response: 221672698
Conc: 3.92 ng/ml

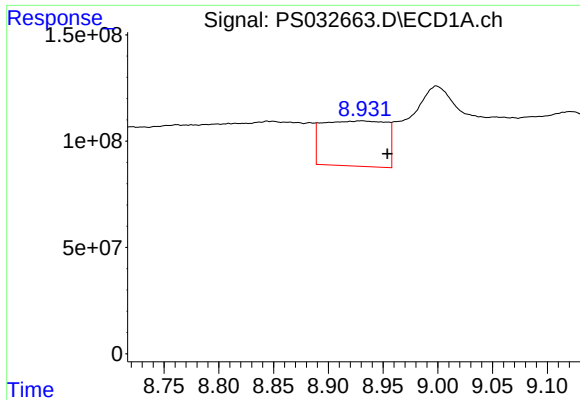

#11 2,4,5-TP (SILVEX)


R.T.: 8.931 min
Delta R.T.: -0.023 min
Response: 859160795
Conc: 25.67 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-01-12-5-2025RE

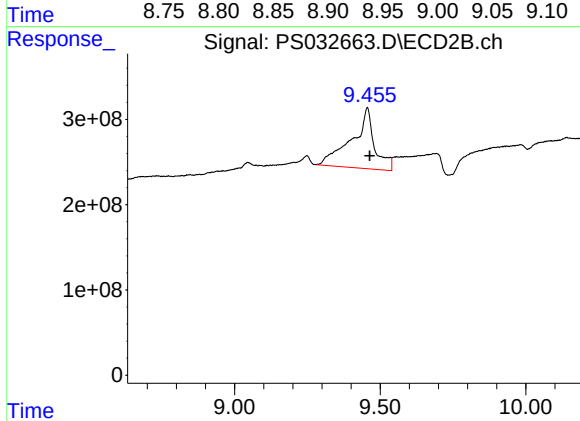


#11 2,4,5-TP (SILVEX)

R.T.: 9.456 min
Delta R.T.: -0.009 min
Response: 3883039530
Conc: 146.90 ng/ml

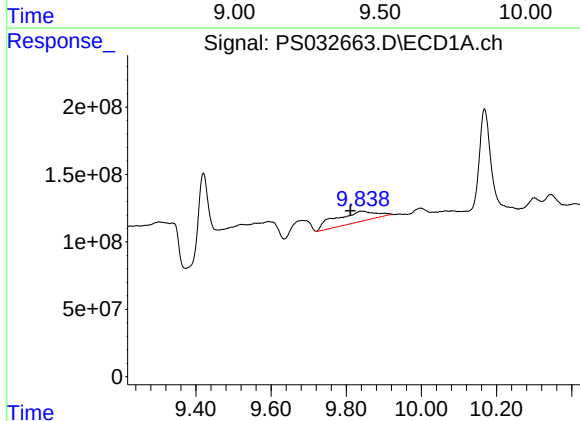


#13 2,4-DB

R.T.: 9.839 min
Delta R.T.: 0.028 min
Response: 618838659
Conc: 147.27 ng/ml

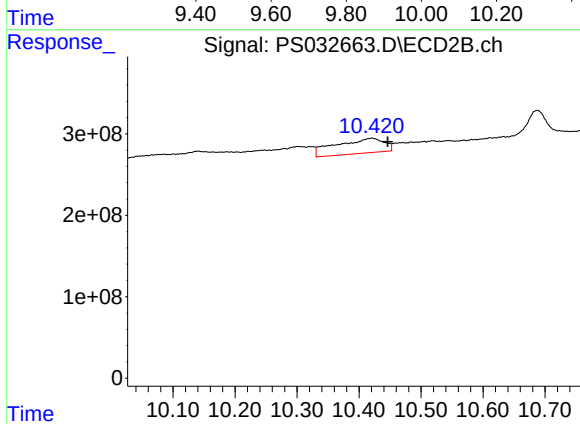

#13 2,4-DB


R.T.: 10.420 min
Delta R.T.: -0.026 min
Response: 993133961
Conc: 237.60 ng/ml

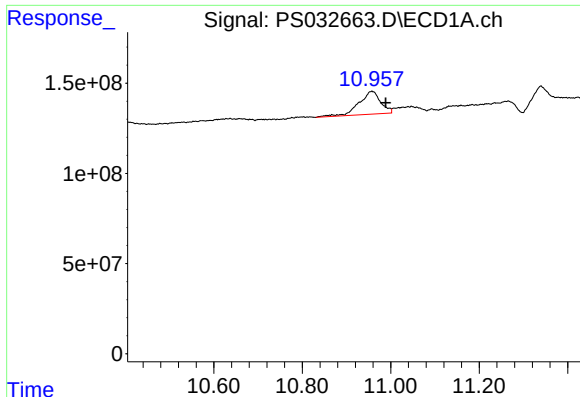

#14 DINOSEB


R.T.: 10.957 min
Delta R.T.: -0.031 min
Response: 434391350
Conc: 17.85 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-01-12-5-2025RE

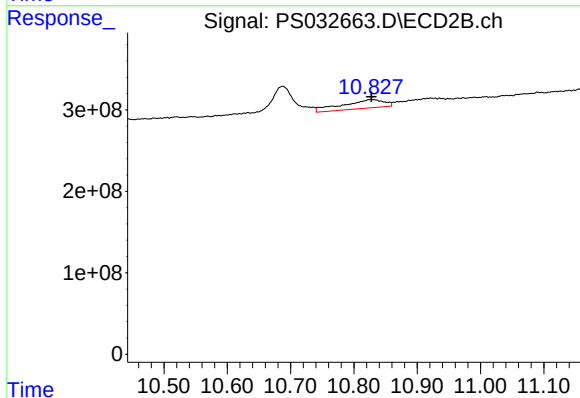


#14 DINOSEB

R.T.: 10.828 min
Delta R.T.: 0.000 min
Response: 489777475
Conc: 29.75 ng/ml

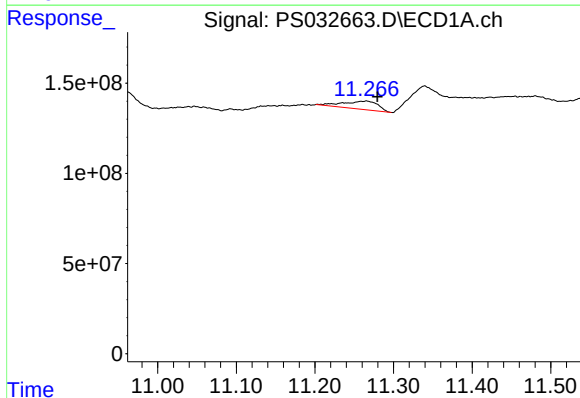

#16 DCPA

R.T.: 11.264 min
Delta R.T.: -0.015 min
Response: 141029688
Conc: 3.47 ng/ml

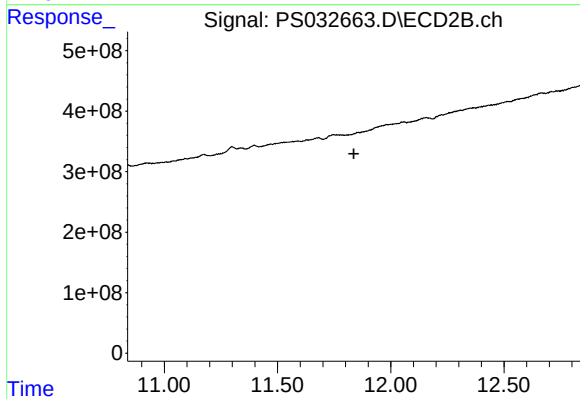

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.837 min
Response: 0
Conc: N.D.