

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121018\
 Data File : PS002545.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2018 15:18
 Operator : EI\SJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 10:09:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.461	10.896	2388142	424942	7.524	1.099 #
Target Compounds							
1) T	Dalapon	0.000	2.298	0	43786	N.D.	0.096 #
3) T	4-Nitroph...	11.033	10.001	2502169	448305	15.866	2.538 #
5) T	DICAMBA	0.000	11.144	0	1033112	N.D.	0.725 #
6) T	MCP	0.000	11.411	0	3826495	N.D.	4.093 #
7) T	MCPA	0.000	11.714	0	9322434	N.D.	6.127 #
15) T	Picloram	16.875	16.827	23027188	1408986	9.073	0.491 #
16) T	DCPA	0.000	16.827	0	1408986	N.D.	0.496 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121018\
Data File : PS002545.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2018 15:18
Operator : EI\SJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 10:09:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

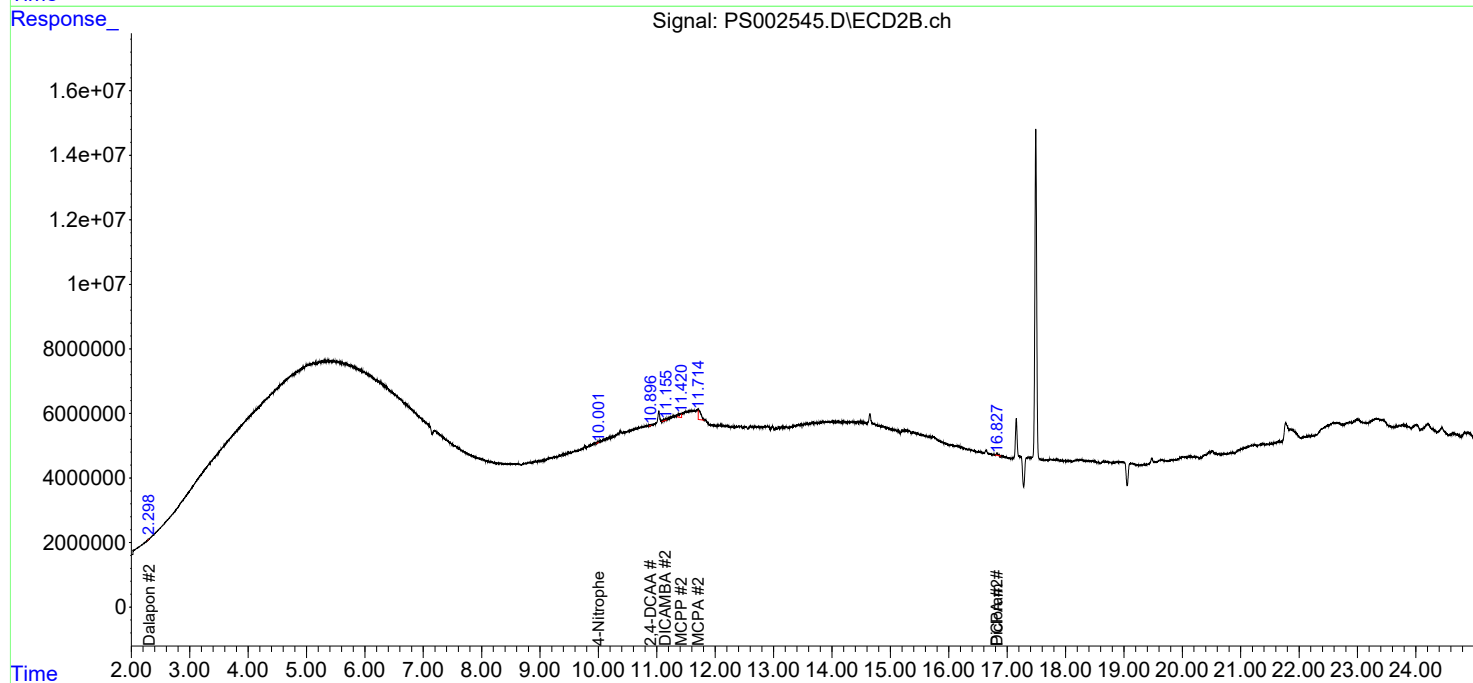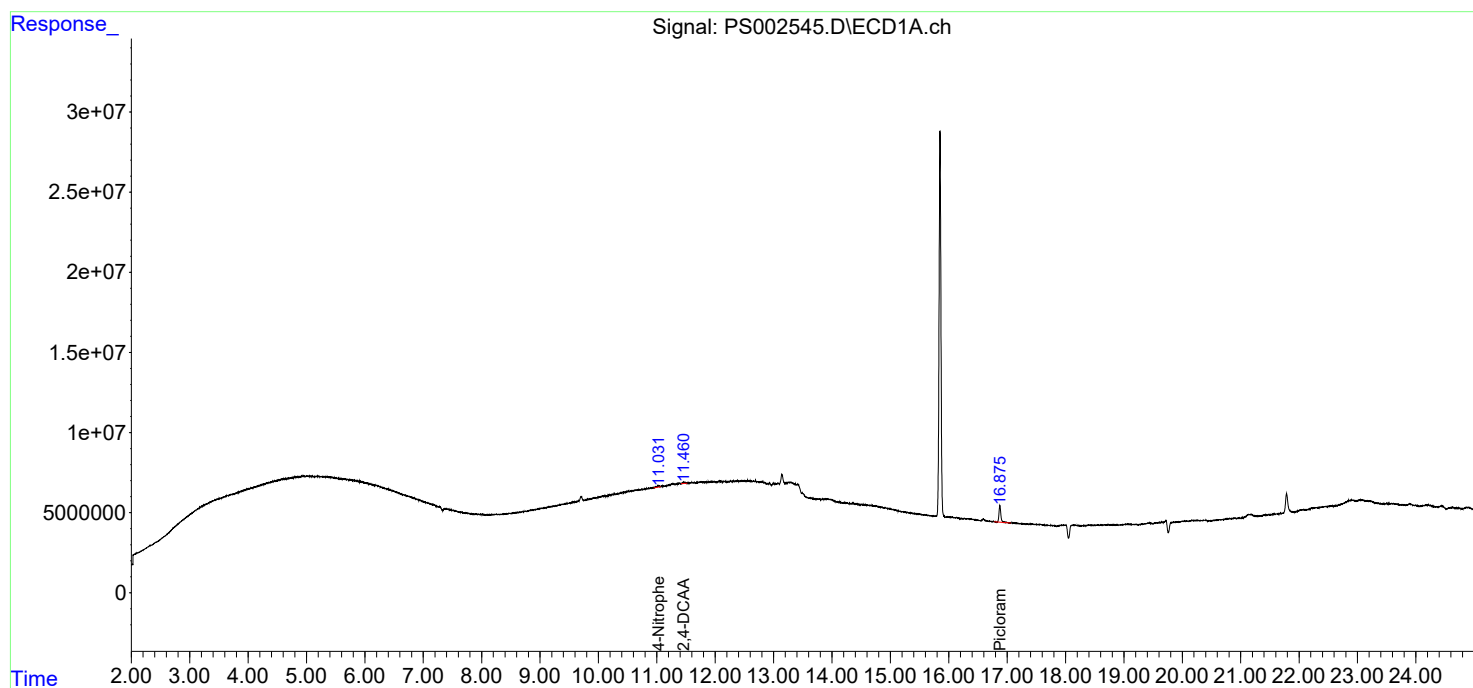


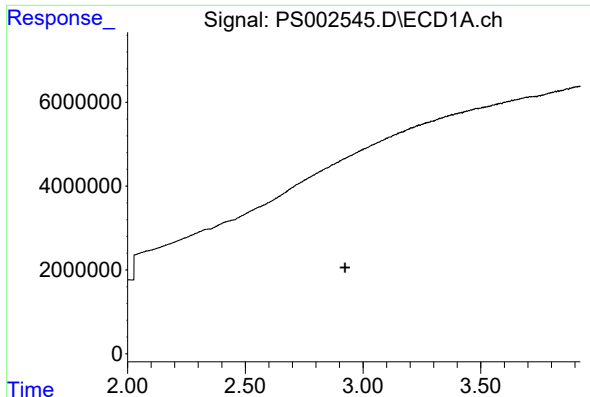

#1 Dalapon


R.T.: 0.000 min
Exp R.T.: 2.923 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

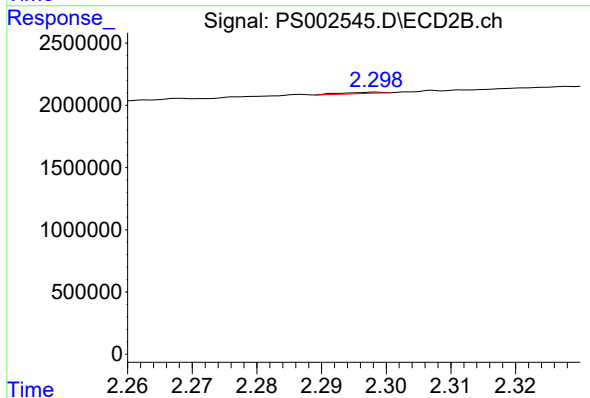


#1 Dalapon

R.T.: 2.298 min
Delta R.T.: -0.065 min
Response: 43786
Conc: 0.10 ng/ml

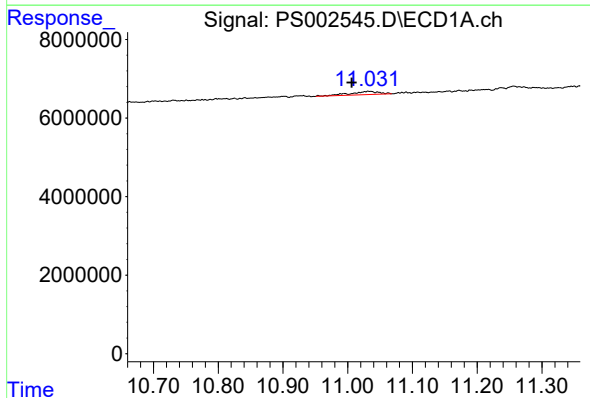


#3 4-Nitrophenol

R.T.: 11.033 min
Delta R.T.: 0.026 min
Response: 2502169
Conc: 15.87 ng/ml

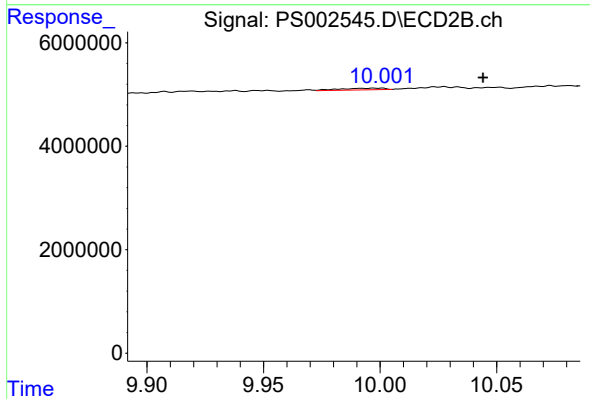

#3 4-Nitrophenol


R.T.: 10.001 min
Delta R.T.: -0.043 min
Response: 448305
Conc: 2.54 ng/ml

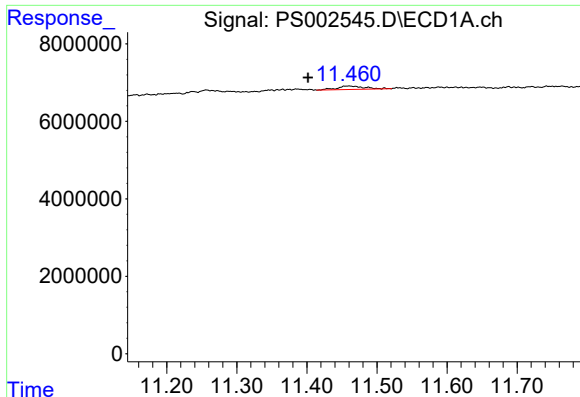

#4 2,4-DCAA


R.T.: 11.461 min
Delta R.T.: 0.059 min
Response: 2388142
Conc: 7.52 ng/ml

Instrument :
ECD_S
ClientSampleId :

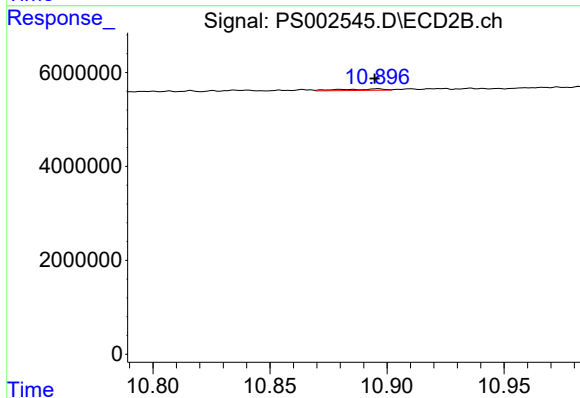


#4 2,4-DCAA

R.T.: 10.896 min
Delta R.T.: 0.001 min
Response: 424942
Conc: 1.10 ng/ml

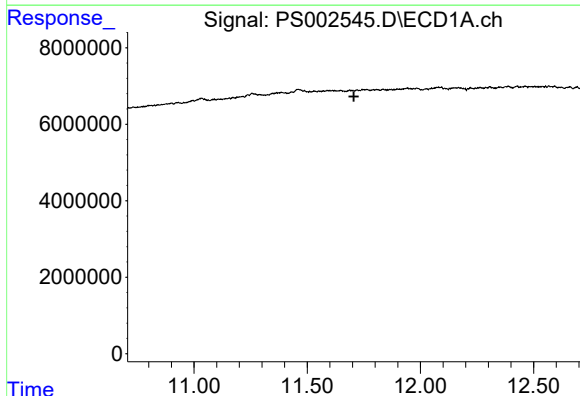


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.706 min
Response: 0
Conc: N.D.

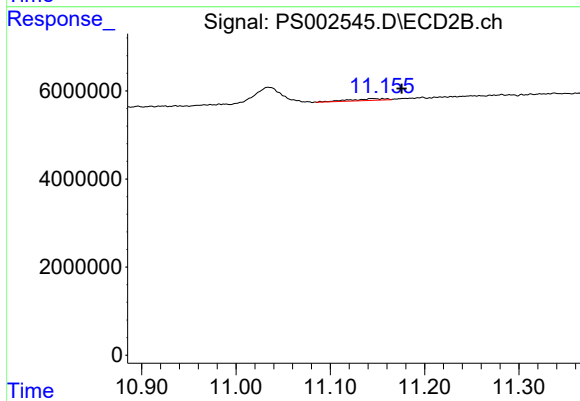

#5 DICAMBA


R.T.: 11.144 min
Delta R.T.: -0.032 min
Response: 1033112
Conc: 0.72 ng/ml

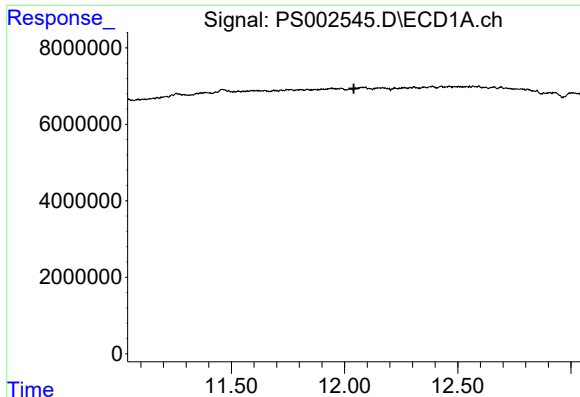

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 12.041 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

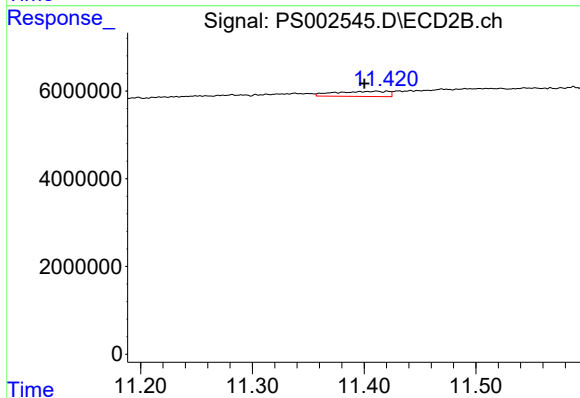


#6 MCPP

R.T.: 11.411 min
Delta R.T.: 0.011 min
Response: 3826495
Conc: 4.09 ug/ml

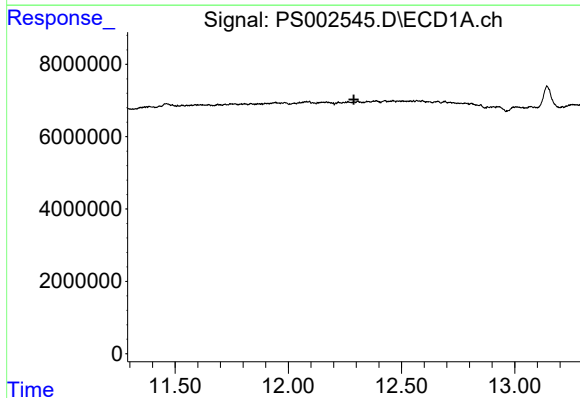


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 12.290 min
Response: 0
Conc: N.D.

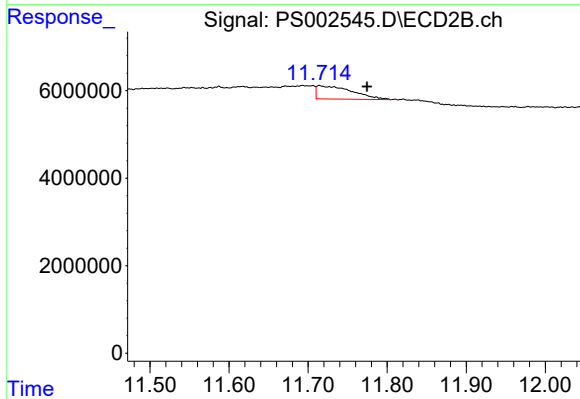

#7 MCPA


R.T.: 11.714 min
Delta R.T.: -0.060 min
Response: 9322434
Conc: 6.13 ug/ml

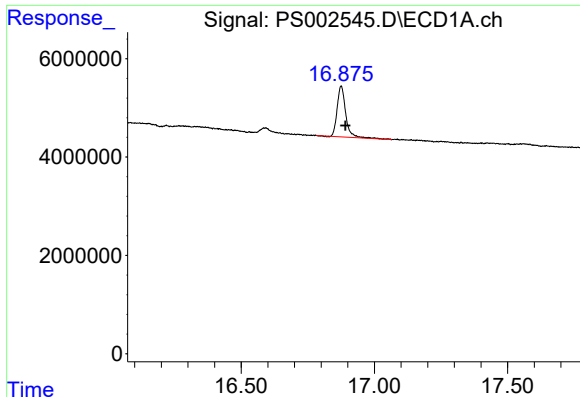

#15 Picloram


R.T.: 16.875 min
Delta R.T.: -0.015 min
Response: 23027188
Conc: 9.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

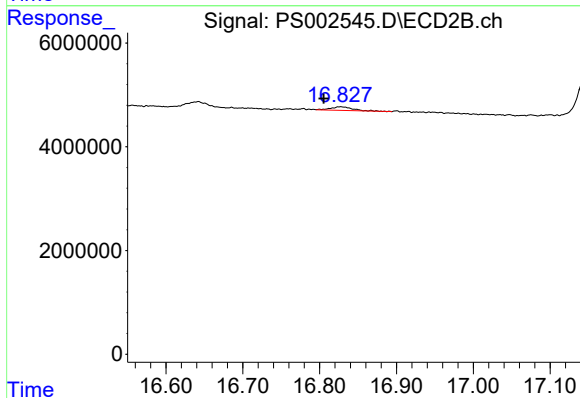


#15 Picloram

R.T.: 16.827 min
Delta R.T.: 0.022 min
Response: 1408986
Conc: 0.49 ng/ml

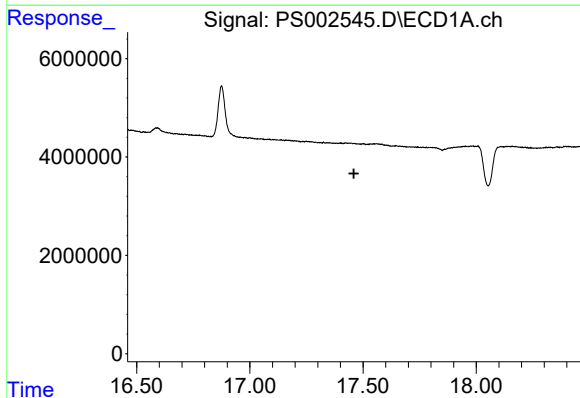

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.459 min
Response: 0
Conc: N.D.

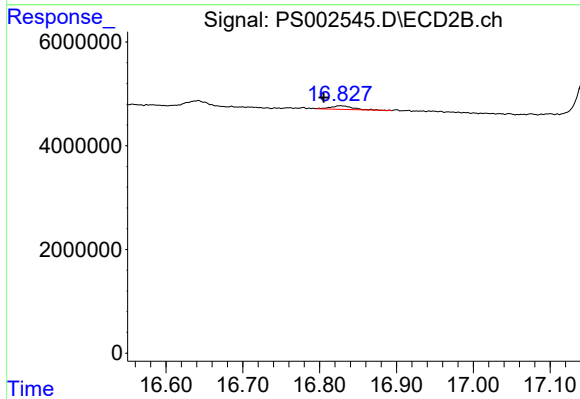

#16 DCPA

R.T.: 16.827 min
Delta R.T.: 0.022 min
Response: 1408986
Conc: 0.50 ng/ml