

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121019\
 Data File : PS008001.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2019 19:25
 Operator : SM\AJ
 Sample : K6117-03
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 TR-04-120619

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 04:17:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.426	5.154	692.3E6	377.8E6	442.558	486.960
Target Compounds							
1) T	Dalapon	1.990	1.714	132.8E6	252.6E6	65.104	212.674 #
2) T	3,5-DICHL...	0.000	4.447	0	7373276	N.D.	7.125
5) T	DICAMBA	5.516	5.292	42012973	13692904	7.384	4.789 #
8) T	DICHLORPROP	0.000	5.818	0	12308949	N.D.	17.171
9) T	2,4-D	6.474	6.058	86539877	7871704	53.792	8.908 #
10) T	Pentachlo...	0.000	6.367	0	24164501	N.D.	2.214
11) T	2,4,5-TP ...	0.000	6.796	0	194.5E6	N.D.	45.353



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121019\
Data File : PS008001.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2019 19:25
Operator : SM\AJ
Sample : K6117-03
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TR-04-120619

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 04:17:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

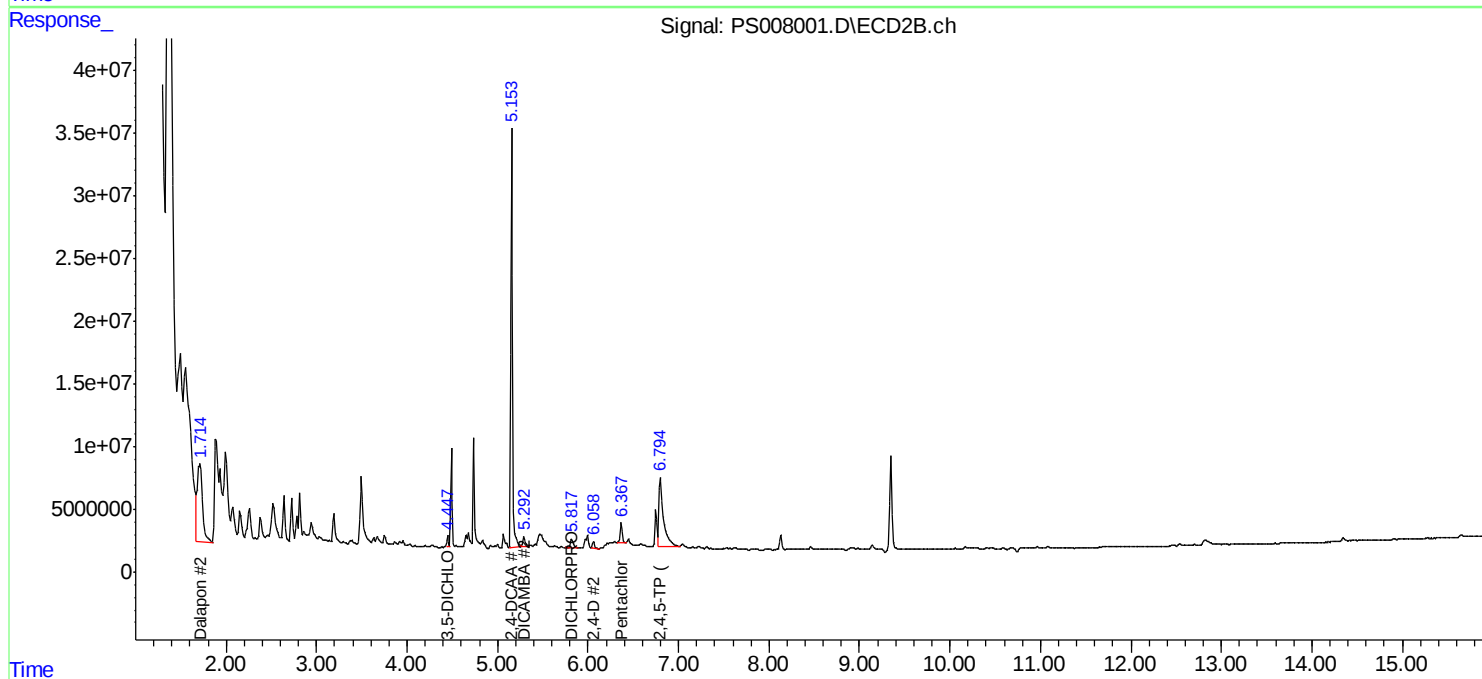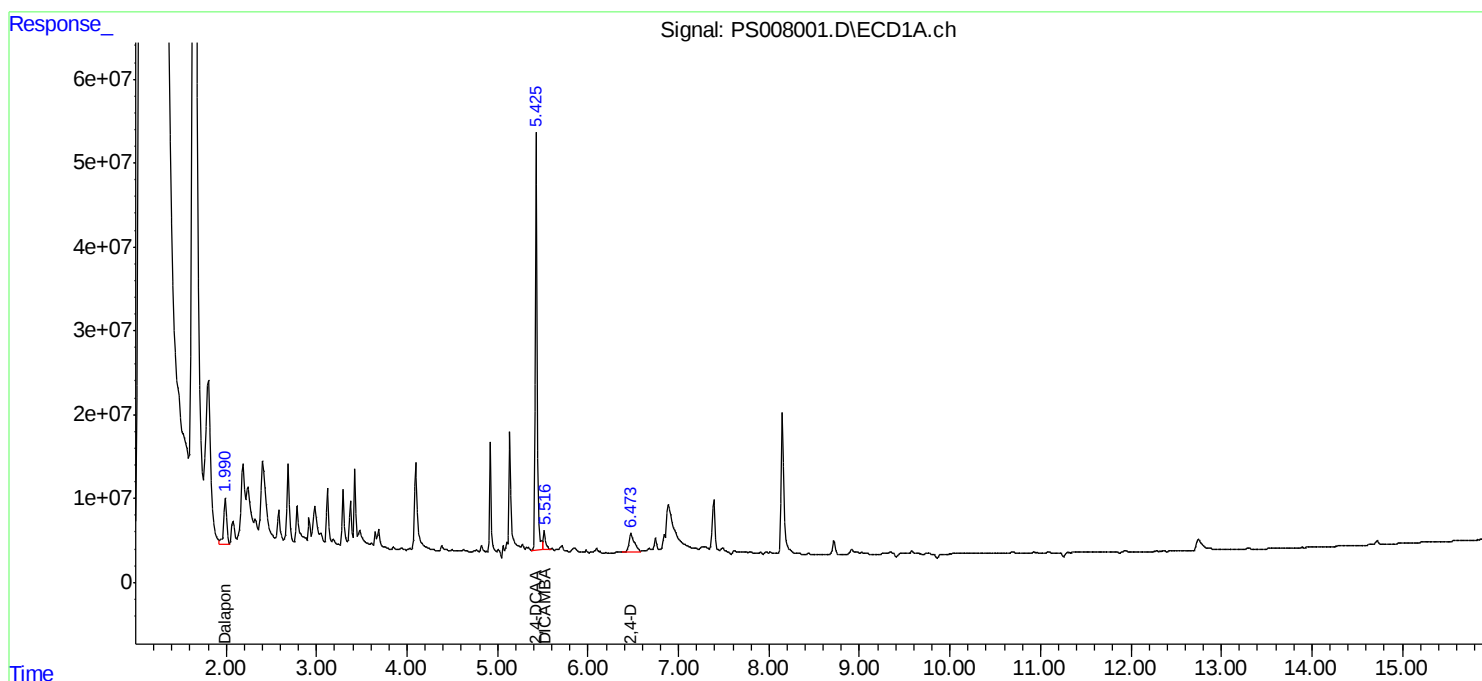


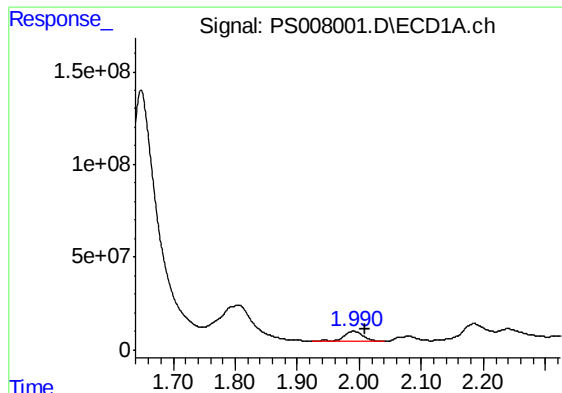

#1 Dalapon


R.T.: 1.990 min
Delta R.T.: -0.020 min
Response: 132767885
Conc: 65.10 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-120619

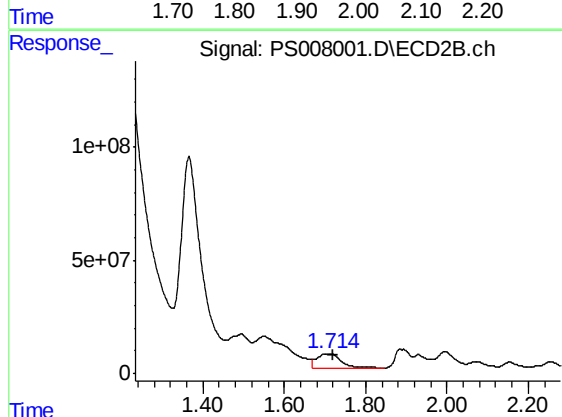


#1 Dalapon

R.T.: 1.714 min
Delta R.T.: -0.007 min
Response: 252612029
Conc: 212.67 ng/ml

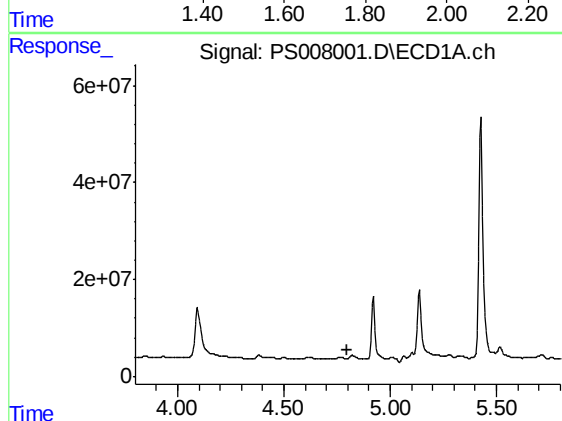


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

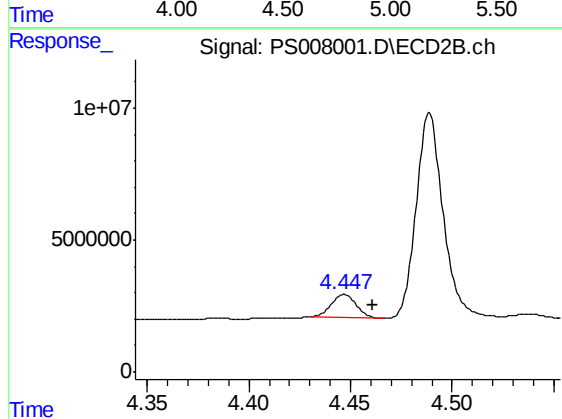

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.447 min
Delta R.T.: -0.014 min
Response: 7373276
Conc: 7.12 ng/ml

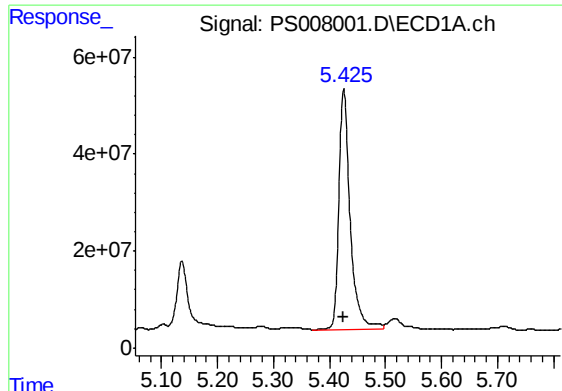

#4 2,4-DCAA


R.T.: 5.426 min
Delta R.T.: 0.000 min
Response: 692307830
Conc: 442.56 ng/ml

Instrument :
ECD_S
ClientSampleId :
TR-04-120619

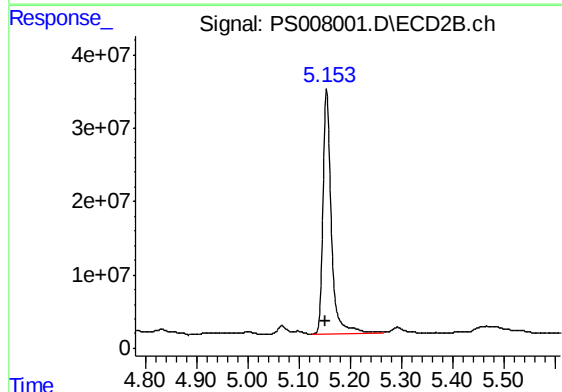


#4 2,4-DCAA

R.T.: 5.154 min
Delta R.T.: 0.002 min
Response: 377841321
Conc: 486.96 ng/ml

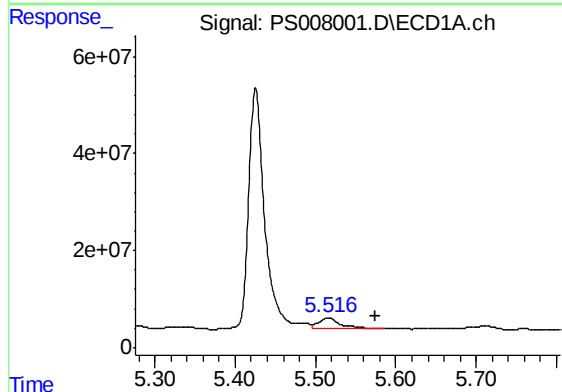


#5 DICAMBA

R.T.: 5.516 min
Delta R.T.: -0.058 min
Response: 42012973
Conc: 7.38 ng/ml

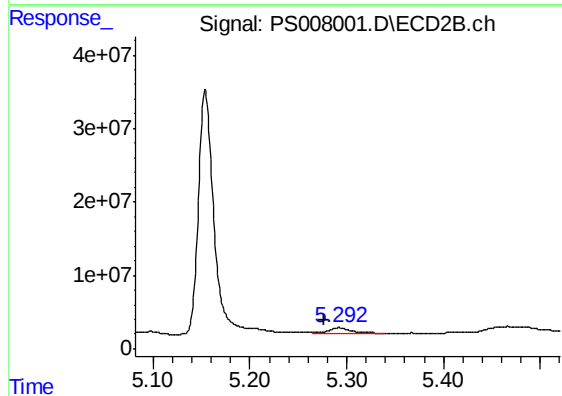

#5 DICAMBA


R.T.: 5.292 min
Delta R.T.: 0.015 min
Response: 13692904
Conc: 4.79 ng/ml

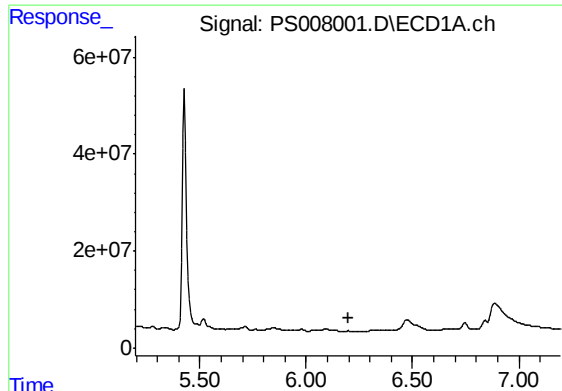

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-120619

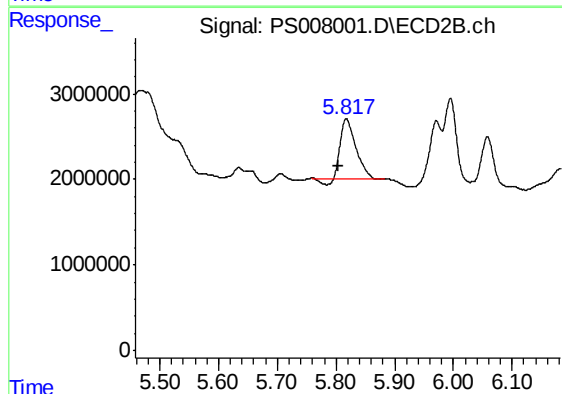


#8 DICHLORPROP

R.T.: 5.818 min
Delta R.T.: 0.014 min
Response: 12308949
Conc: 17.17 ng/ml

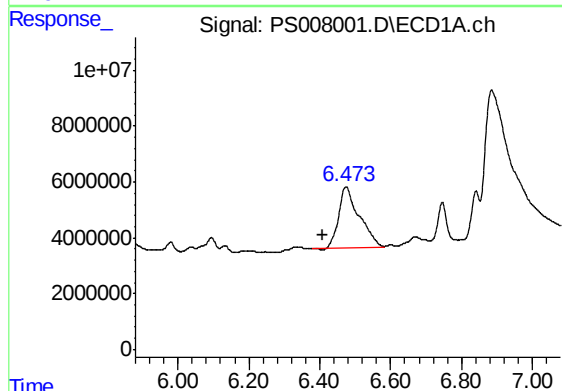


#9 2,4-D

R.T.: 6.474 min
Delta R.T.: 0.066 min
Response: 86539877
Conc: 53.79 ng/ml

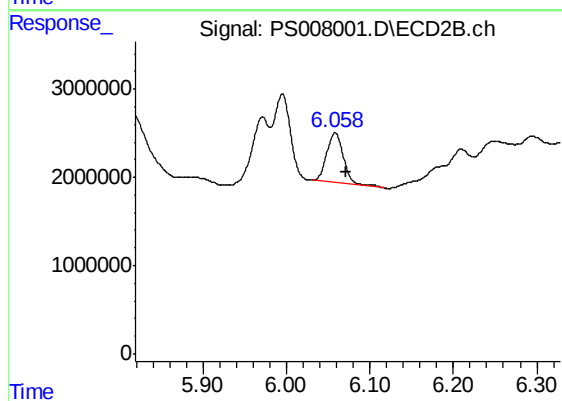

#9 2,4-D


R.T.: 6.058 min
Delta R.T.: -0.013 min
Response: 7871704
Conc: 8.91 ng/ml

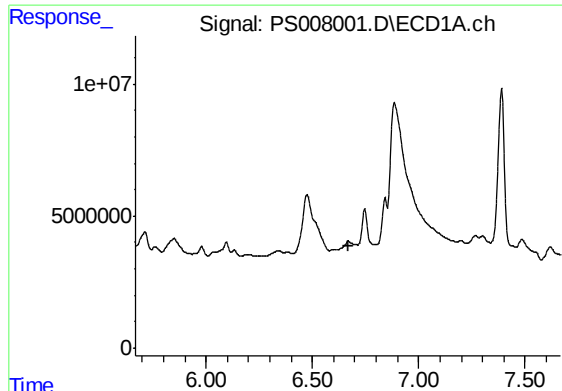

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 6.667 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
TR-04-120619

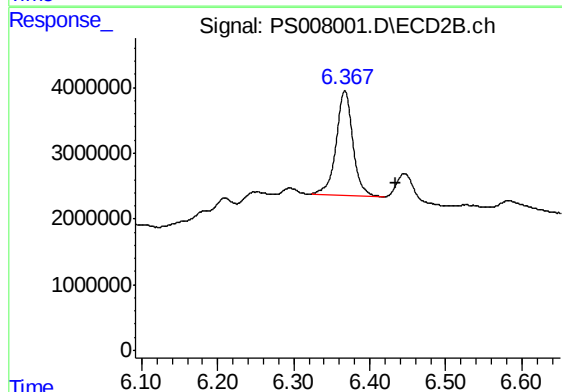


#10 Pentachlorophenol

R.T.: 6.367 min
Delta R.T.: -0.068 min
Response: 24164501
Conc: 2.21 ng/ml

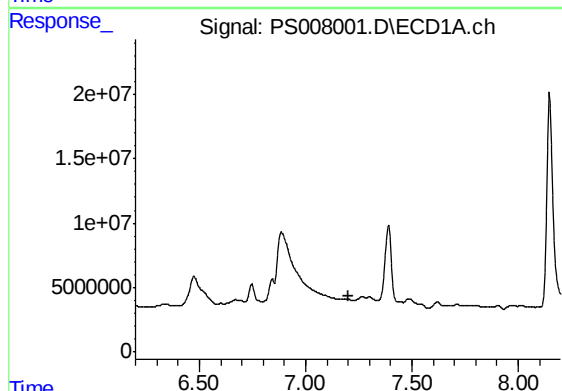

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

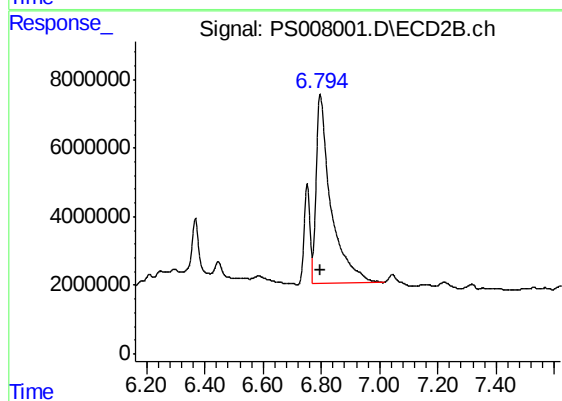

#11 2,4,5-TP (SILVEX)

R.T.: 6.796 min
Delta R.T.: -0.002 min
Response: 194512237
Conc: 45.35 ng/ml