

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121019\
 Data File : PS008004.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2019 20:31
 Operator : SM\AJ
 Sample : K6176-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 48-SPRUCE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 04:19:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.433	5.160	304.4E6	175.5E6	194.609	226.158
Target Compounds							
1) T	Dalapon	1.995	1.703	68553300	152.6E6	33.616	128.432 #
2) T	3,5-DICHL...	0.000	4.450	0	6020063	N.D.	5.817
3) T	4-Nitroph...	0.000	4.835	0	22264920	N.D.	49.166
5) T	DICAMBA	5.521	0.000	42882275	0	7.537	N.D. #
8) T	DICHLORPROP	0.000	5.824	0	7736815	N.D.	10.793
10) T	Pentachlo...	0.000	6.448	0	8104203	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.755	0	51020895	N.D.	11.896



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121019\
Data File : PS008004.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2019 20:31
Operator : SM\AJ
Sample : K6176-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
48-SPRUCE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 04:19:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

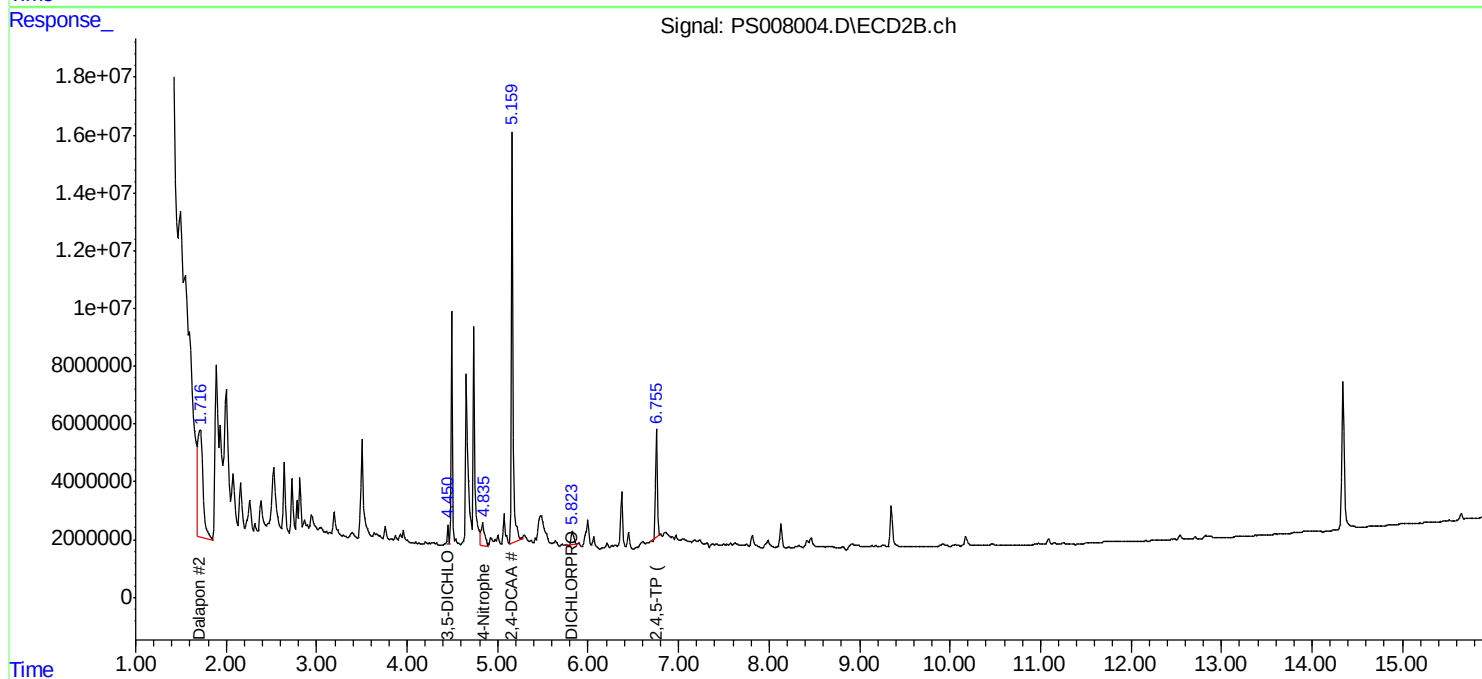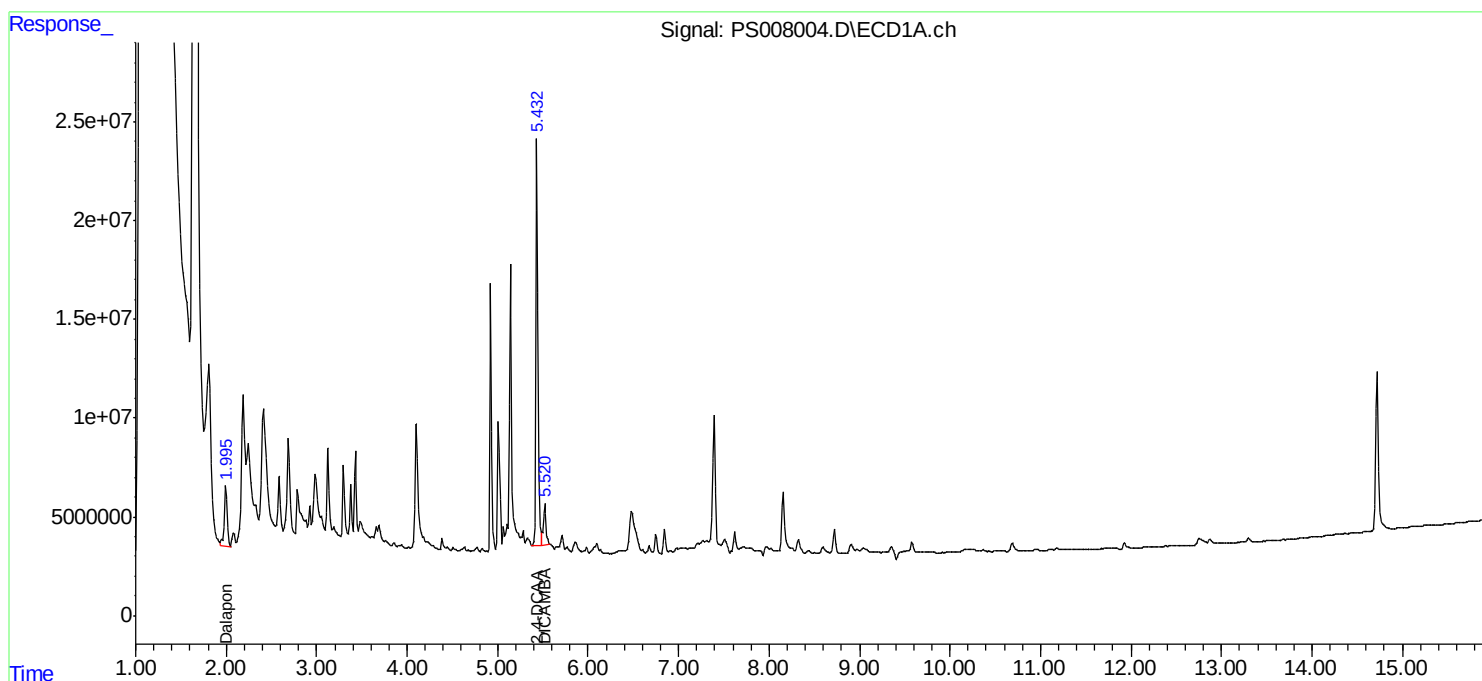


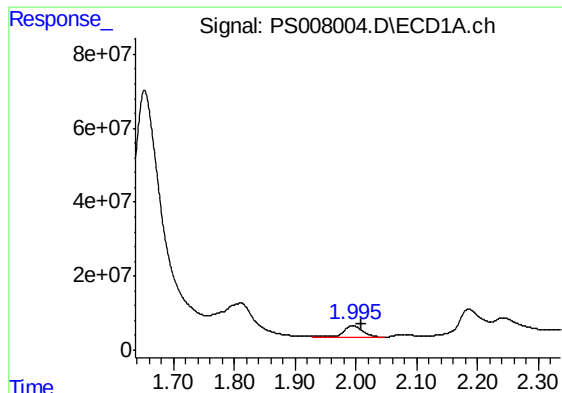

#1 Dalapon


R.T.: 1.995 min
Delta R.T.: -0.015 min
Response: 68553300
Conc: 33.62 ng/ml

Instrument :
ECD_S
ClientSampleId :
48-SPRUCE

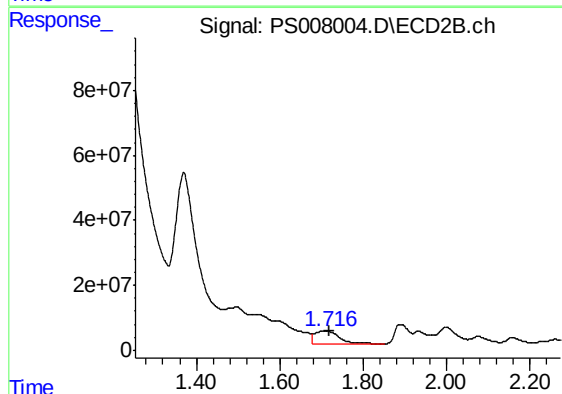


#1 Dalapon

R.T.: 1.703 min
Delta R.T.: -0.018 min
Response: 152550711
Conc: 128.43 ng/ml

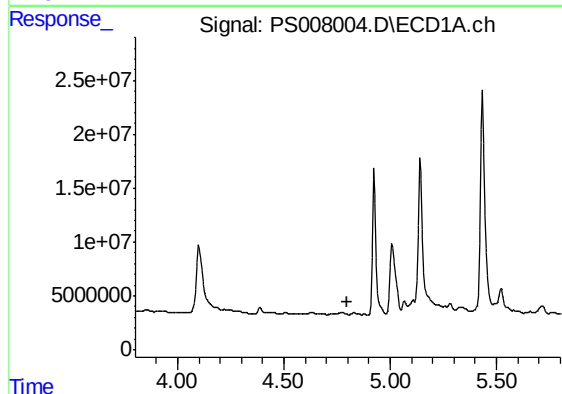


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

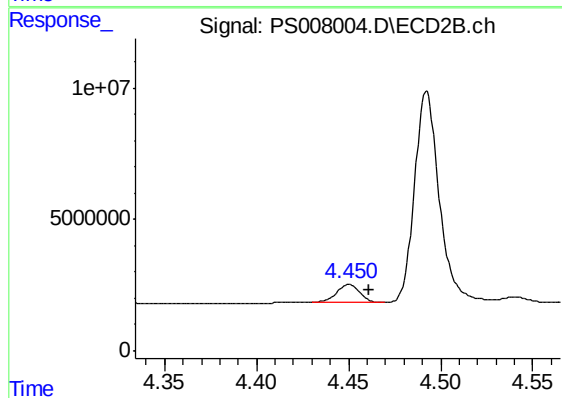

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.450 min
Delta R.T.: -0.011 min
Response: 6020063
Conc: 5.82 ng/ml

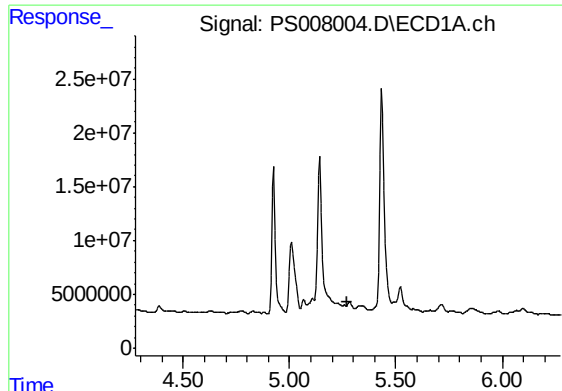

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
48-SPRUCE

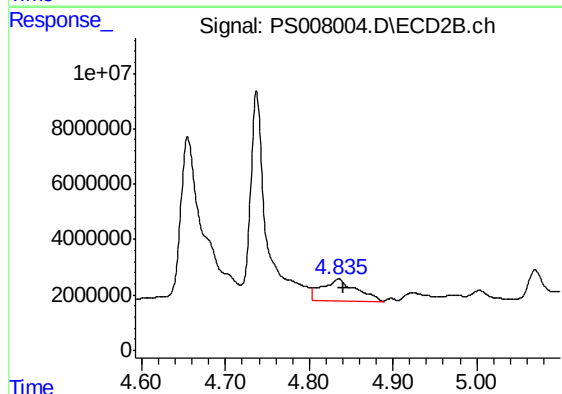


#3 4-Nitrophenol

R.T.: 4.835 min
Delta R.T.: -0.006 min
Response: 22264920
Conc: 49.17 ng/ml

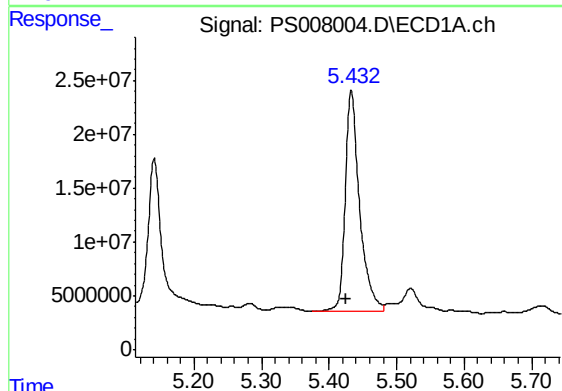


#4 2,4-DCAA

R.T.: 5.433 min
Delta R.T.: 0.008 min
Response: 304433842
Conc: 194.61 ng/ml

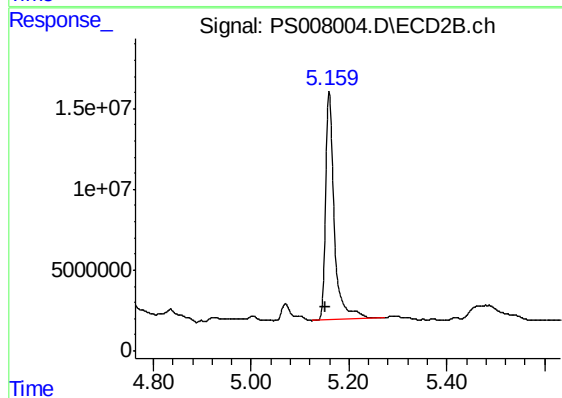

#4 2,4-DCAA


R.T.: 5.160 min
Delta R.T.: 0.008 min
Response: 175480097
Conc: 226.16 ng/ml

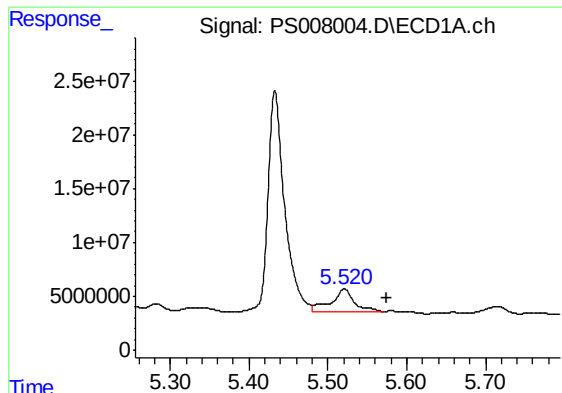

#5 DICAMBA


R.T.: 5.521 min
Delta R.T.: -0.054 min
Response: 42882275
Conc: 7.54 ng/ml

Instrument :
ECD_S
ClientSampleId :
48-SPRUCE

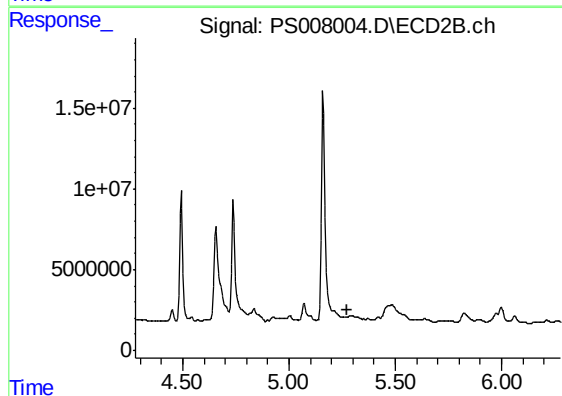


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 5.277 min
Response: 0
Conc: N.D.

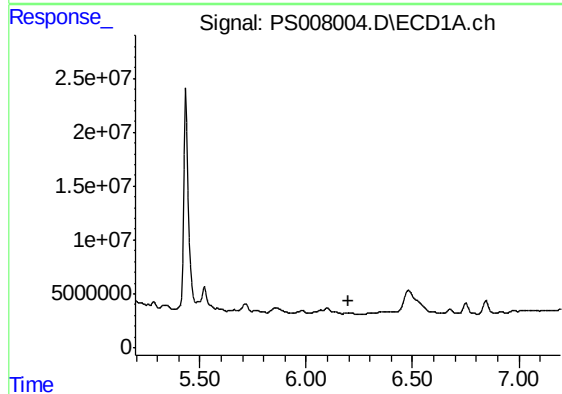


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

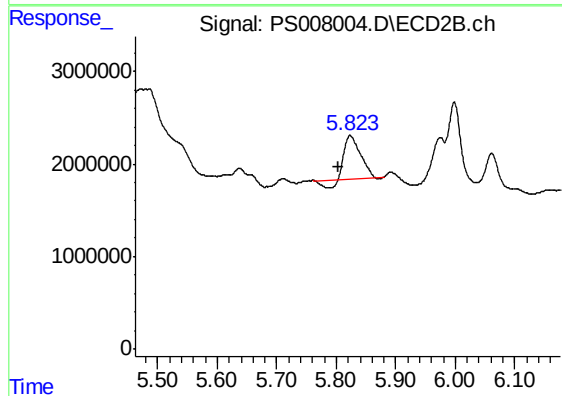

#8 DICHLORPROP


R.T.: 5.824 min
Delta R.T.: 0.019 min
Response: 7736815
Conc: 10.79 ng/ml

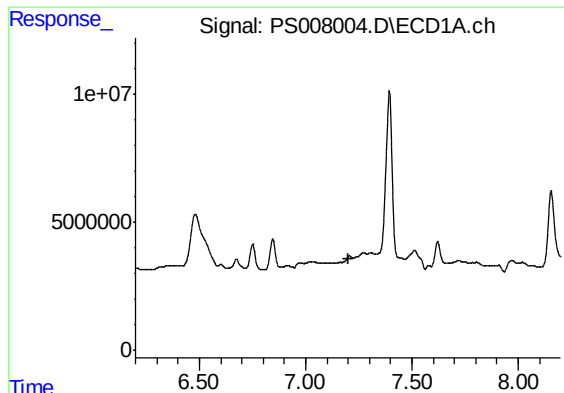

#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
48-SPRUCE

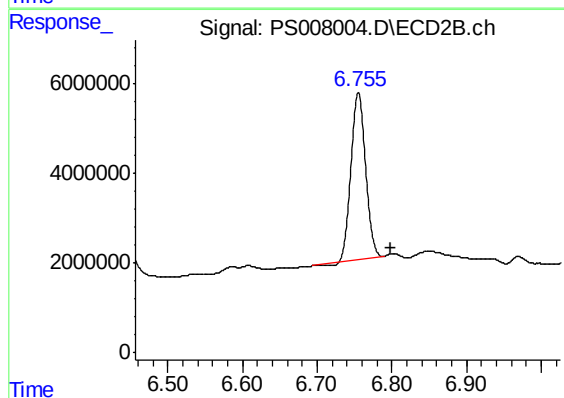

#11 2,4,5-TP (SILVEX)

R.T.: 6.755 min
Delta R.T.: -0.043 min
Response: 51020895
Conc: 11.90 ng/ml