

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121024\
 Data File : PS028745.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2024 08:53
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 11:31:48 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.659f	2.710	8544677	3639907	2.945	1.667 #
2) T	3,5-DICHL...	6.384	0.000	311629	0	<MDL	N.D. #
3) T	4-Nitroph...	7.011	0.000	3864136	0	2.248	N.D. #
5) T	DICAMBA	7.441f	7.908	-548385	3860781	N.D.	<MDL
7) T	MCPA	7.718f	0.000	1398119	0	<MDL	N.D. #
8) T	DICHLORPROP	8.156f	8.675f	605334	2859204	<MDL	1.789 #
9) T	2,4-D	8.332	0.000	1314797	0	<MDL	N.D. #
10) T	Pentachlo...	8.681f	0.000	1065255	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.209	0.000	727052	0	<MDL	N.D. #
12) T	2,4,5-T	9.472f	0.000	4073314	0	<MDL	N.D. #
14) T	DINOSEB	11.288	0.000	1702507	0	<MDL	N.D. #
15) T	Picloram	11.115	12.317	27540152	6059684	<MDL	<MDL #
16) T	DCPA	11.594	12.317f	351474	6059684	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121024\
Data File : PS028745.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2024 08:53
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 11:31:48 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

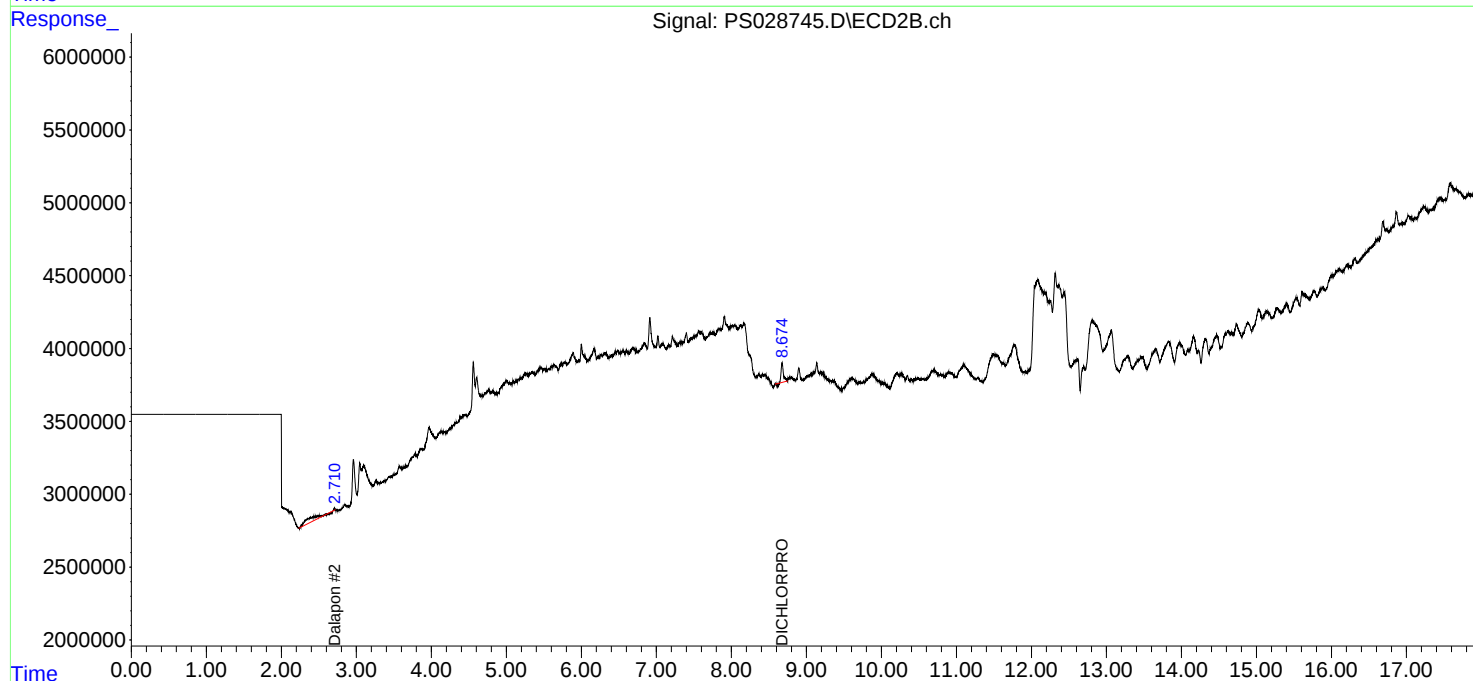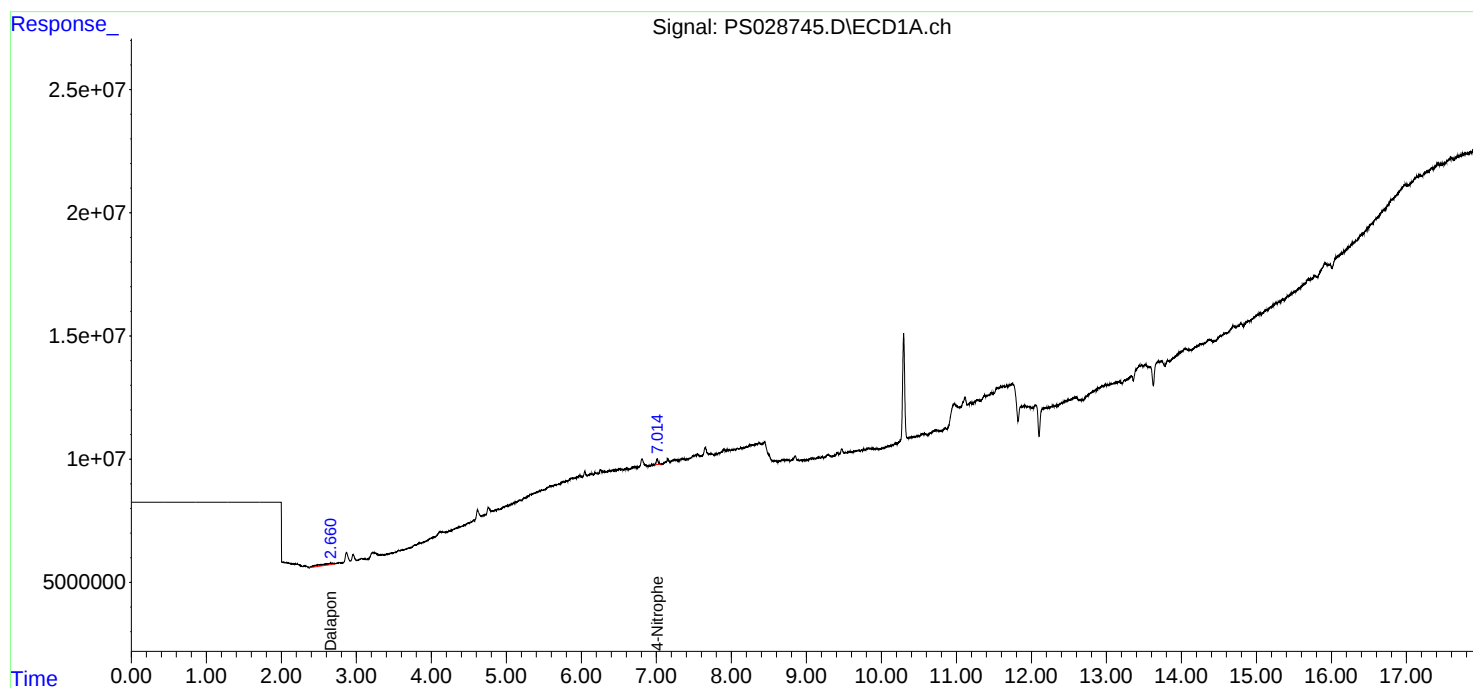


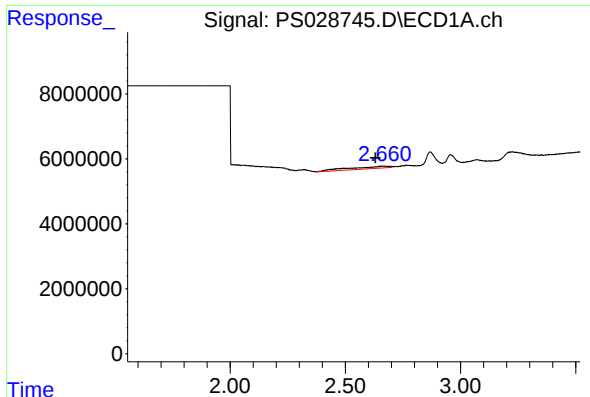

#1 Dalapon


R.T.: 2.659 min
Delta R.T.: 0.029 min
Response: 8544677
Conc: 2.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

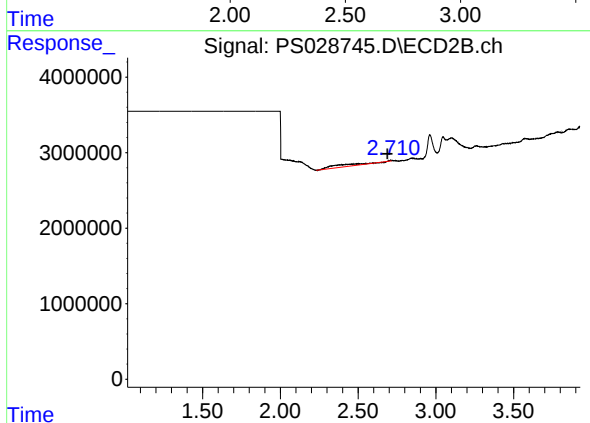


#1 Dalapon

R.T.: 2.710 min
Delta R.T.: 0.022 min
Response: 3639907
Conc: 1.67 ng/ml

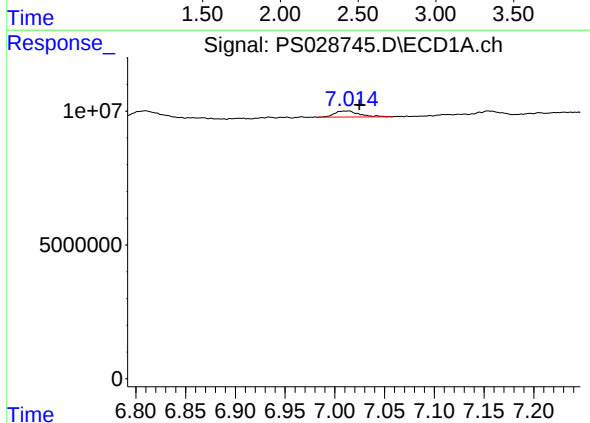


#3 4-Nitrophenol

R.T.: 7.011 min
Delta R.T.: -0.014 min
Response: 3864136
Conc: 2.25 ng/ml

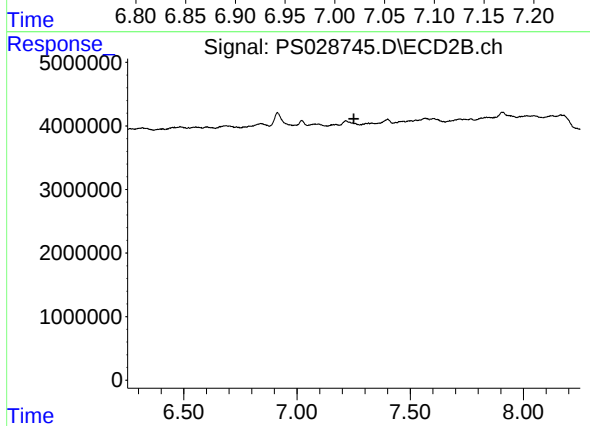

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

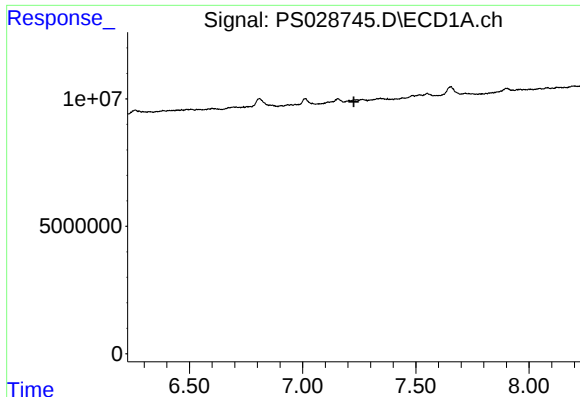

#4 2,4-DCAA


R.T.: 7.264 min
Delta R.T.: 0.038 min
Response: -1085190
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

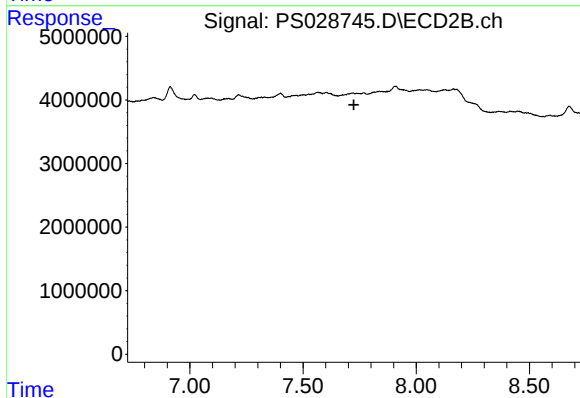


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.725 min
Response: 0
Conc: N.D.

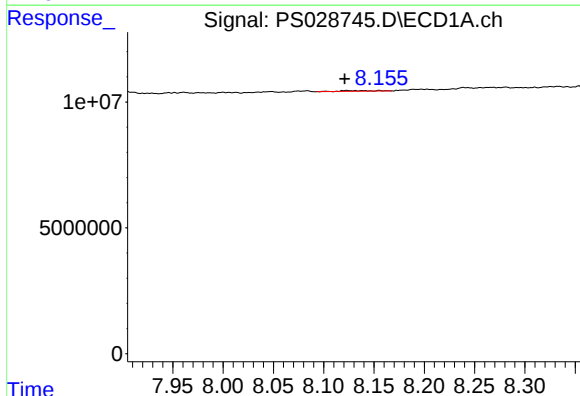

#8 DICHLORPROP

R.T.: 8.156 min
Delta R.T.: 0.035 min
Response: 605334
Conc: N.D.

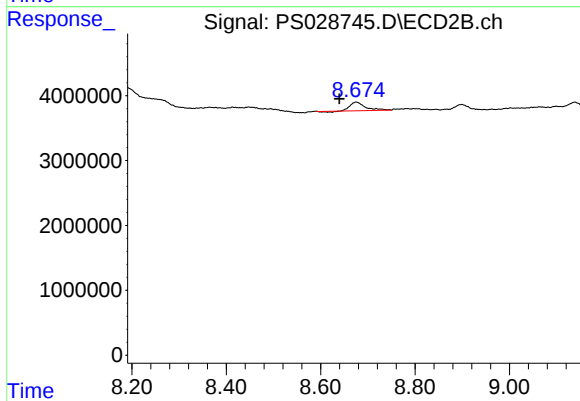

#8 DICHLORPROP

R.T.: 8.675 min
Delta R.T.: 0.036 min
Response: 2859204
Conc: 1.79 ng/ml