

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121024\
 Data File : PS028751.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2024 12:54
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 10 14:41:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.225	7.717	1324.4E6	585.1E6	493.737	434.364
Target Compounds							
1) T	Dalapon	2.670f	2.723f	9099629	4172664	3.136	1.911 #
2) T	3,5-DICHL...	6.414	0.000	592633	0	<MDL	N.D. #
3) T	4-Nitroph...	7.014	0.000	10275769	0	5.978	N.D. #
5) T	DICAMBA	0.000	7.914	0	4909260	N.D.	<MDL
7) T	MCPA	7.779f	8.271	1414730	5655153	<MDL	<MDL #
8) T	DICHLORPROP	8.088f	8.680f	1862250	8825026	<MDL	5.520 #
10) T	Pentachlo...	8.648	0.000	766260	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.222	9.862	-325541	6986749	N.D.	<MDL
12) T	2,4,5-T	9.520	10.282	7250557	9252204	<MDL	<MDL #
13) T	2,4-DB	10.095	0.000	1388508	0	<MDL	N.D. #
14) T	DINOSEB	11.279	0.000	6364943	0	<MDL	N.D. #
15) T	Picloram	11.117	12.322	60703149	17577605	2.041	1.364 #
16) T	DCPA	11.574	12.322f	7012333	17577605	<MDL	1.584 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121024\
Data File : PS028751.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2024 12:54
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 10 14:41:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

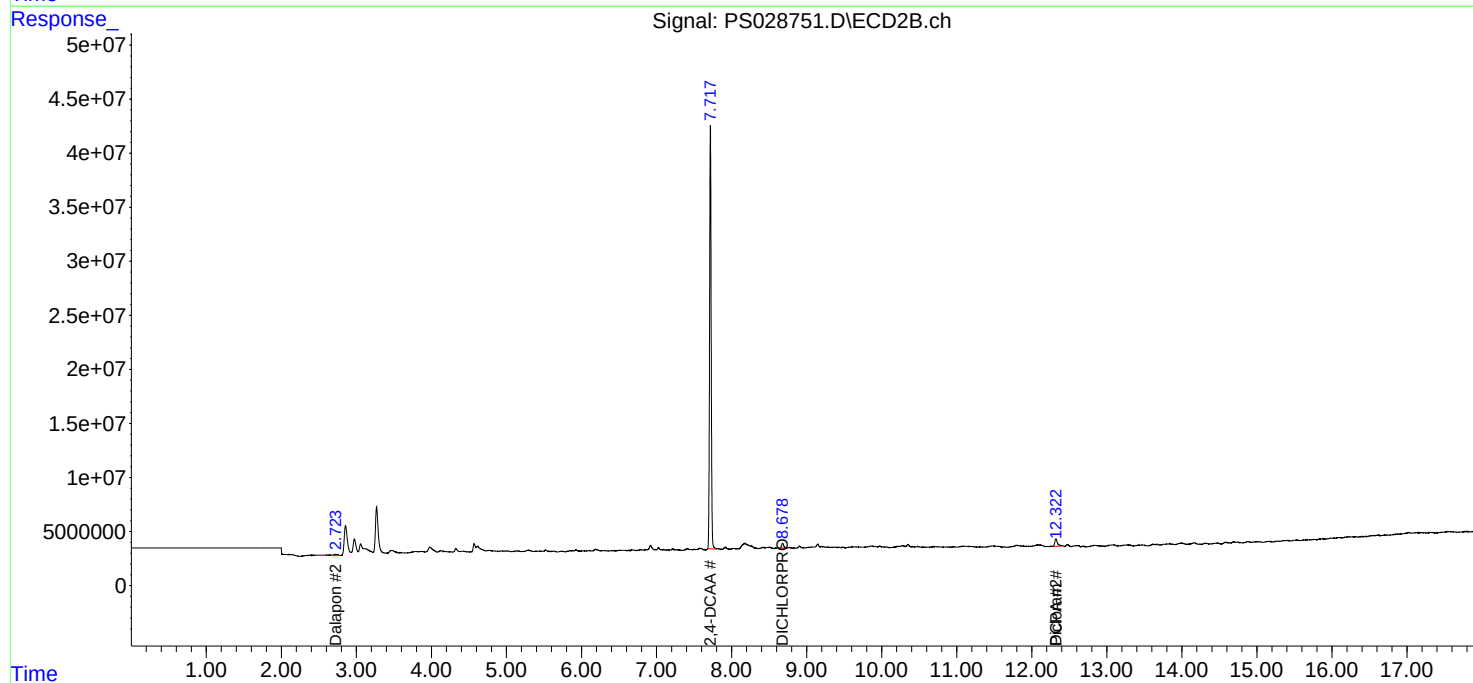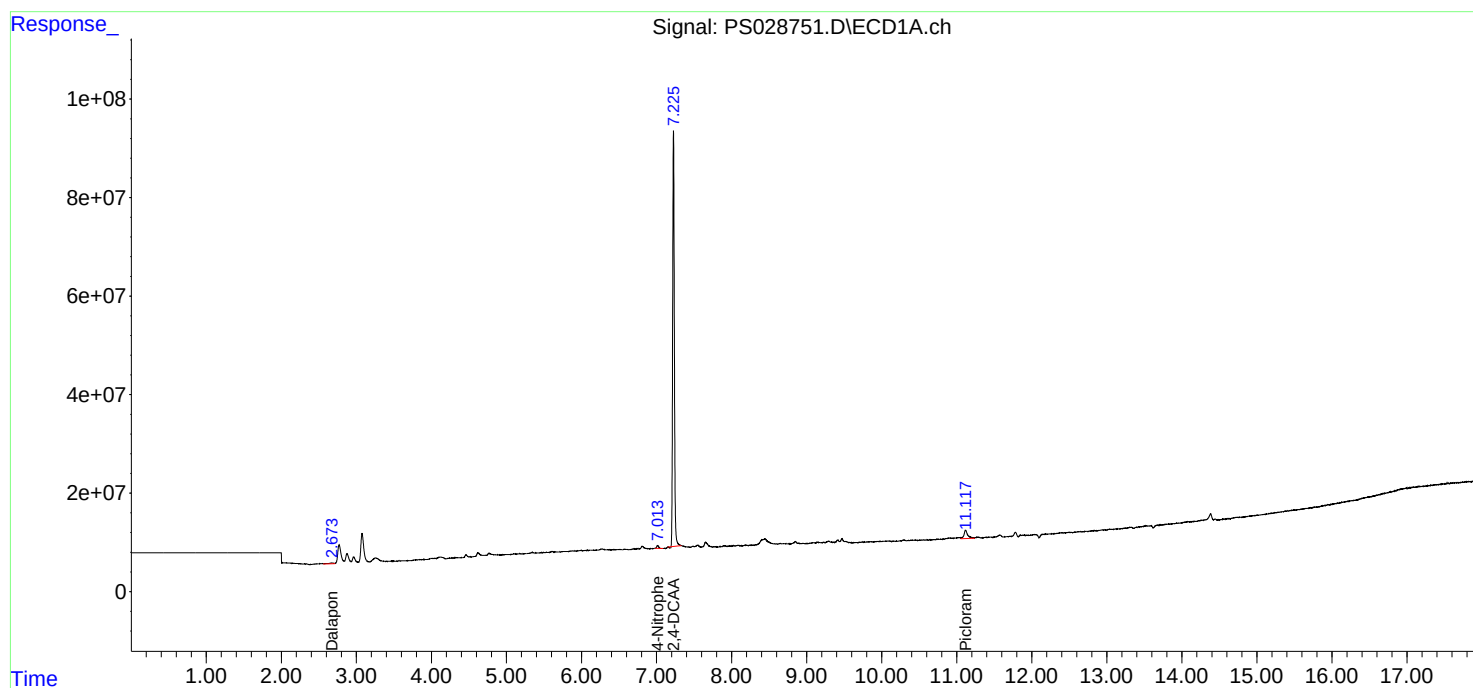


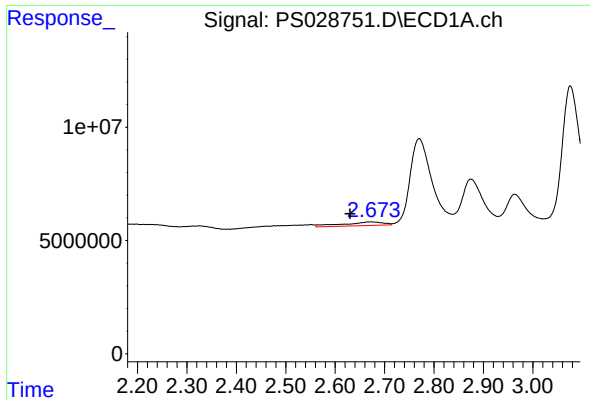

#1 Dalapon


R.T.: 2.670 min
Delta R.T.: 0.040 min
Response: 9099629
Conc: 3.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

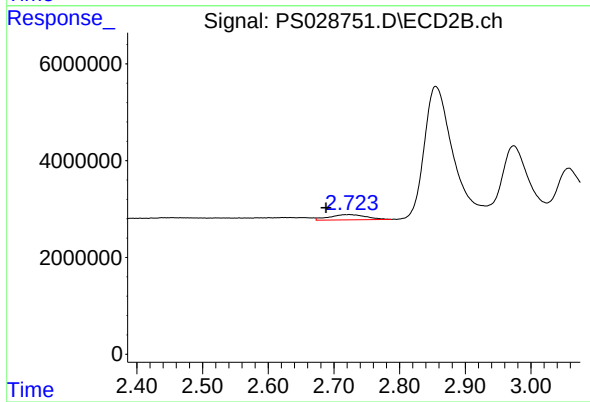


#1 Dalapon

R.T.: 2.723 min
Delta R.T.: 0.035 min
Response: 4172664
Conc: 1.91 ng/ml

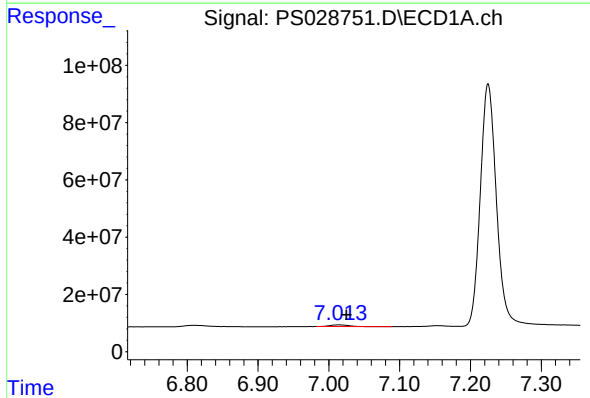


#3 4-Nitrophenol

R.T.: 7.014 min
Delta R.T.: -0.011 min
Response: 10275769
Conc: 5.98 ng/ml

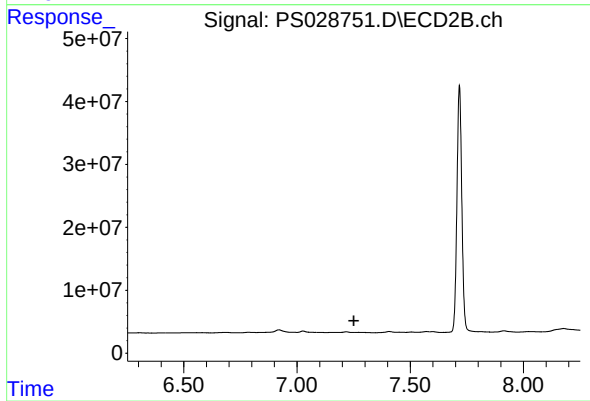

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

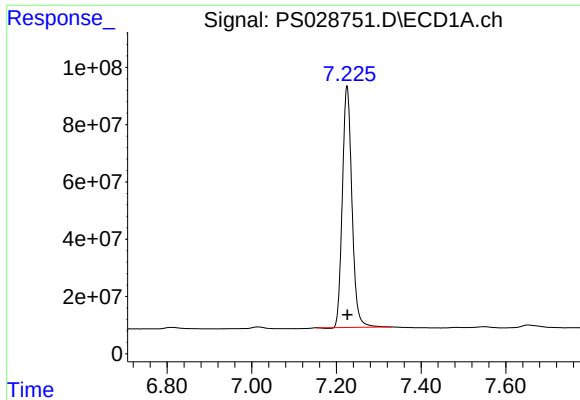

#4 2,4-DCAA


R.T.: 7.225 min
Delta R.T.: -0.001 min
Response: 1324371939
Conc: 493.74 ng/ml

Instrument :
ECD_S
ClientSampleId :

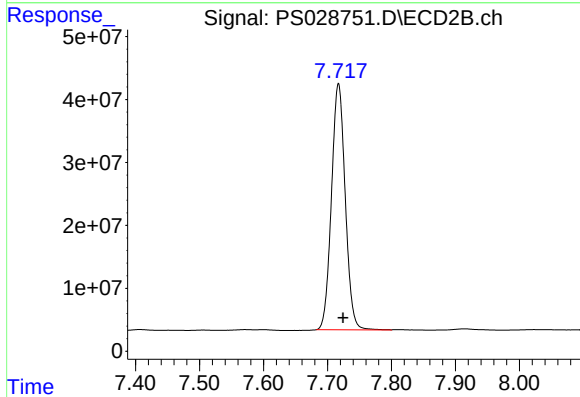


#4 2,4-DCAA

R.T.: 7.717 min
Delta R.T.: -0.007 min
Response: 585101410
Conc: 434.36 ng/ml

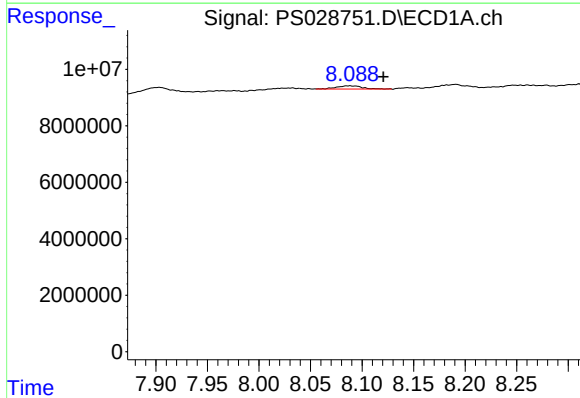


#8 DICHLORPROP

R.T.: 8.088 min
Delta R.T.: -0.032 min
Response: 1862250
Conc: N.D.

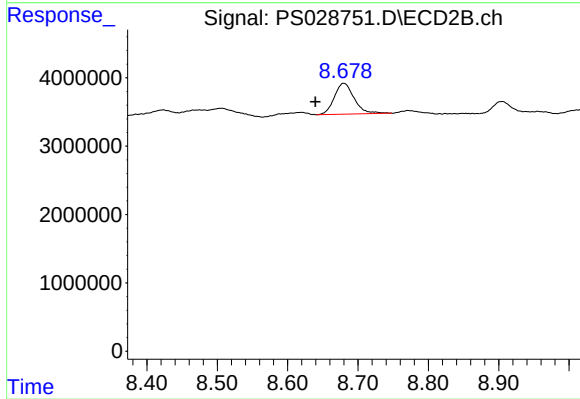

#8 DICHLORPROP


R.T.: 8.680 min
Delta R.T.: 0.040 min
Response: 8825026
Conc: 5.52 ng/ml

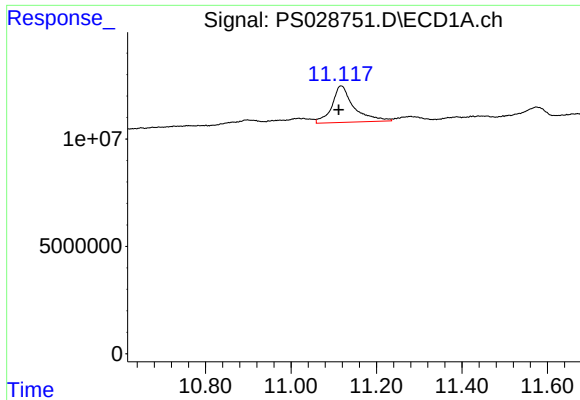

#15 Picloram


R.T.: 11.117 min
Delta R.T.: 0.006 min
Response: 60703149
Conc: 2.04 ng/ml

Instrument :
ECD_S
ClientSampleId :

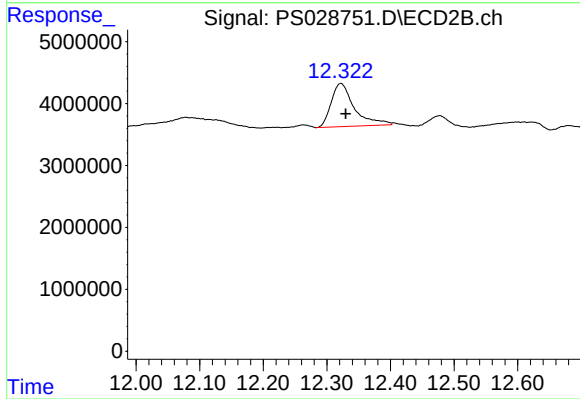


#15 Picloram

R.T.: 12.322 min
Delta R.T.: -0.008 min
Response: 17577605
Conc: 1.36 ng/ml

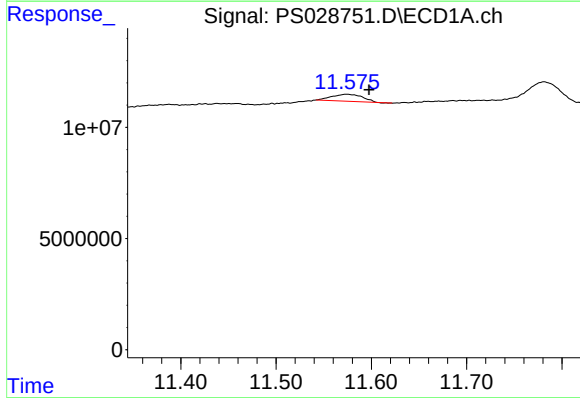

#16 DCPA

R.T.: 11.574 min
Delta R.T.: -0.023 min
Response: 7012333
Conc: N.D.

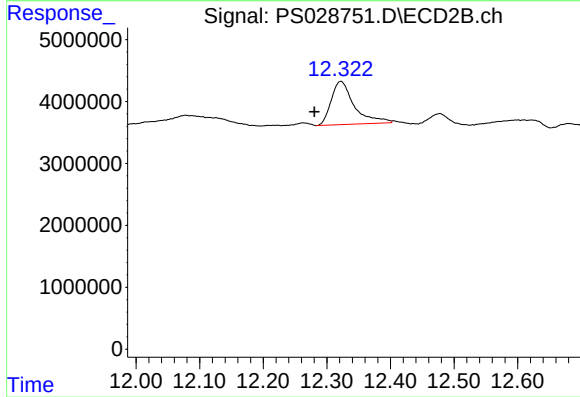

#16 DCPA

R.T.: 12.322 min
Delta R.T.: 0.042 min
Response: 17577605
Conc: 1.58 ng/ml