

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121025\
 Data File : PS032667.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 20:29
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 01:40:42 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 11 01:33:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds							
3) T	4-Nitroph...	7.095	0.000	3192281	0	<MDL	N.D. #
7) T	MCPA	7.873	0.000	1257847	0	<MDL	N.D. #
8) T	DICHLORPROP	8.198f	0.000	5530064	0	<MDL	N.D. #
10) T	Pentachlo...	8.830f	9.772f	14949335	7640325	<MDL	<MDL #
11) T	2,4,5-TP ...	0.000	10.167	0	5134706	N.D.	<MDL
12) T	2,4,5-T	9.688f	0.000	2123355	0	<MDL	N.D. #
13) T	2,4-DB	10.196f	0.000	33168267	0	5.243	N.D. #
15) T	Picloram	11.272	12.703	129.0E6	69464646	2.702	2.782
16) T	DCPA	11.747	0.000	48221254	0	1.002	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121025\
Data File : PS032667.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 20:29
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 01:40:42 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

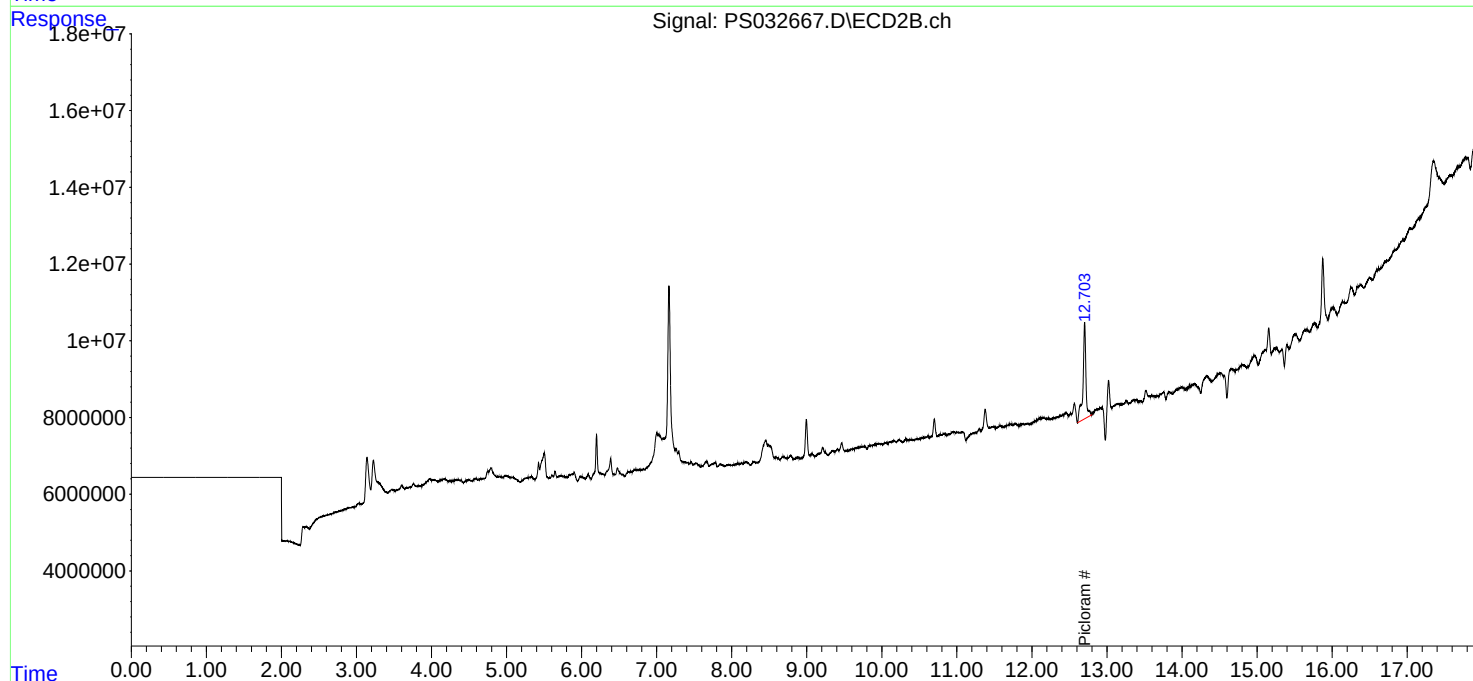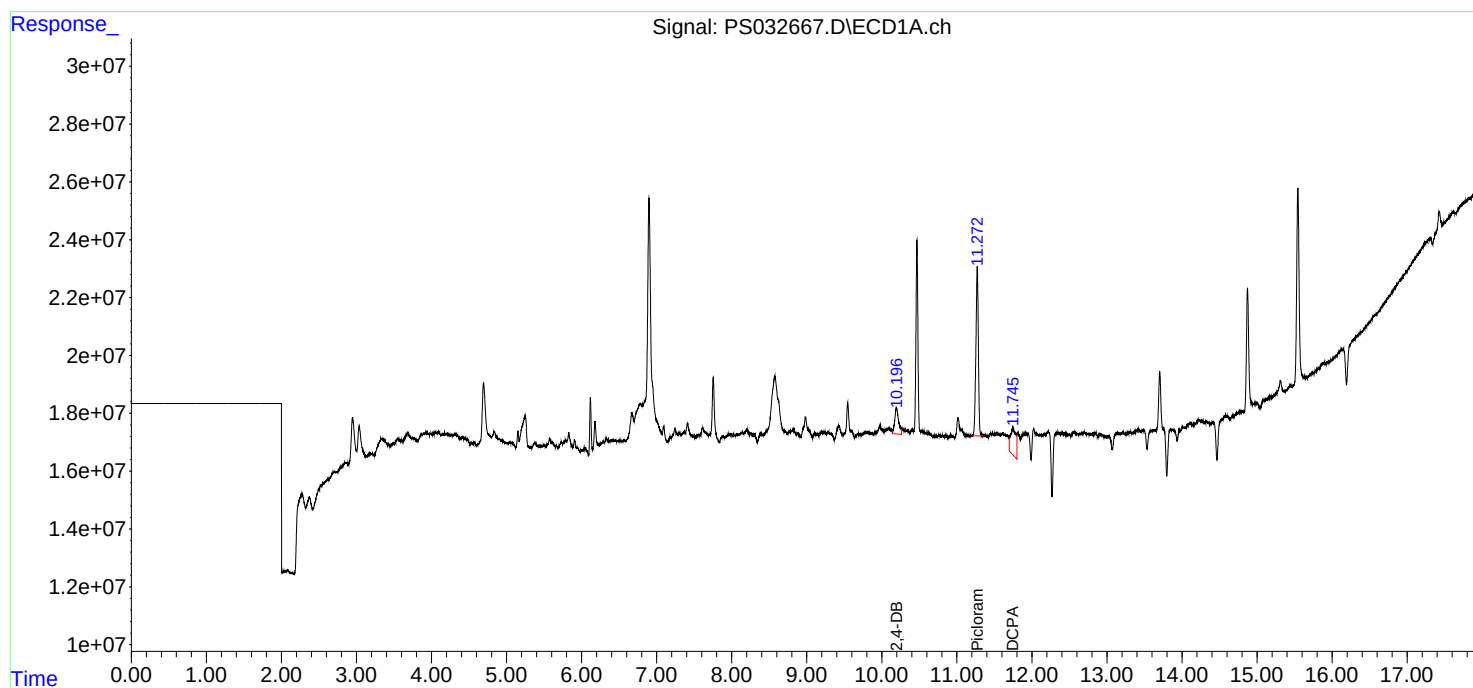


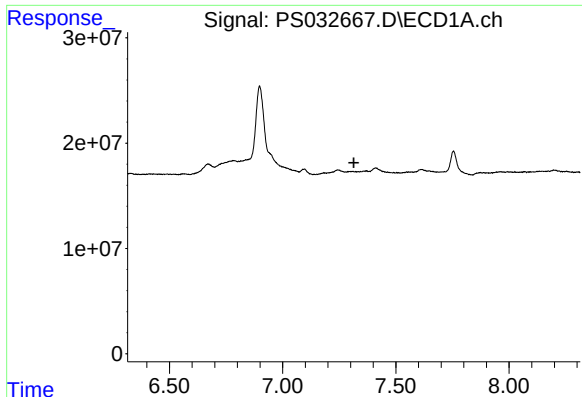

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T.: 7.314 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

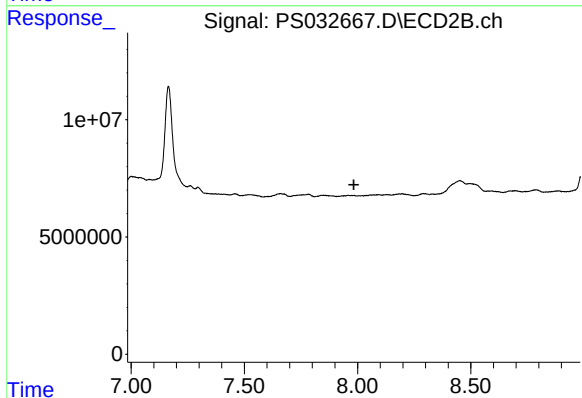


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T.: 7.984 min
Response: 0
Conc: N.D.

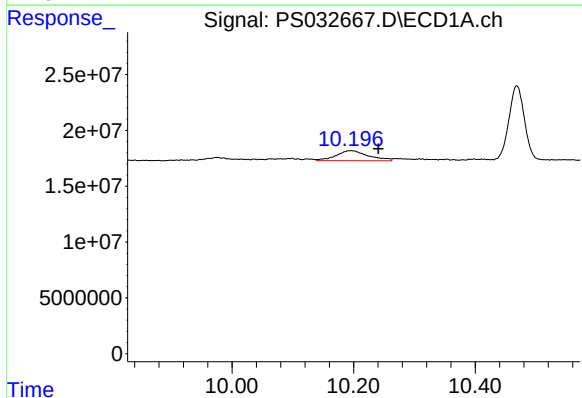


#13 2,4-DB

R.T.: 10.196 min
Delta R.T.: -0.045 min
Response: 33168267
Conc: 5.24 ng/ml

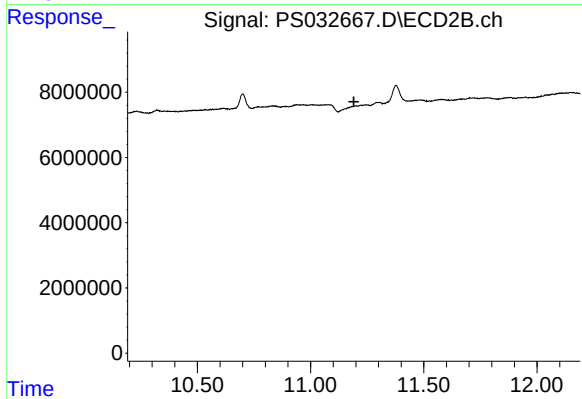

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 11.191 min
Response: 0
Conc: N.D.

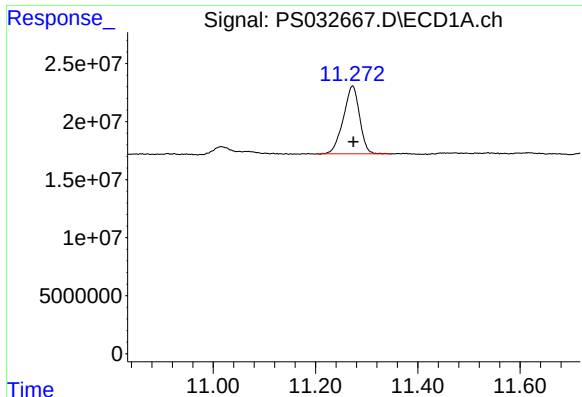

#15 Picloram


R.T.: 11.272 min
Delta R.T.: -0.002 min
Response: 129031201
Conc: 2.70 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

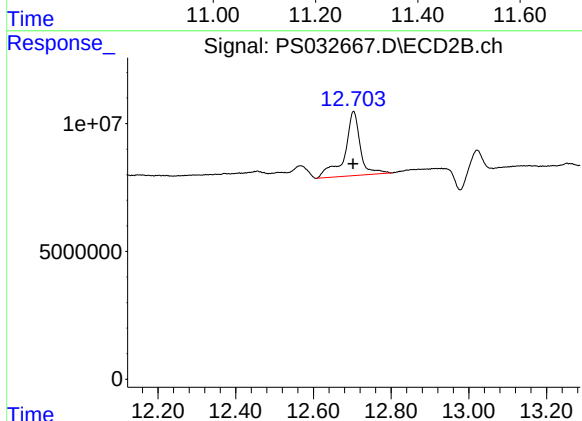


#15 Picloram

R.T.: 12.703 min
Delta R.T.: 0.001 min
Response: 69464646
Conc: 2.78 ng/ml

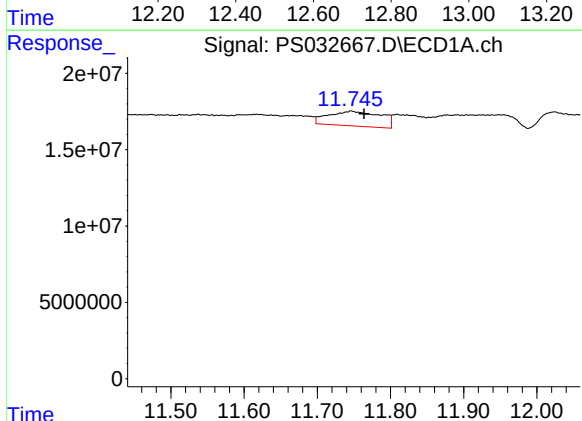

#16 DCPA

R.T.: 11.747 min
Delta R.T.: -0.017 min
Response: 48221254
Conc: 1.00 ng/ml

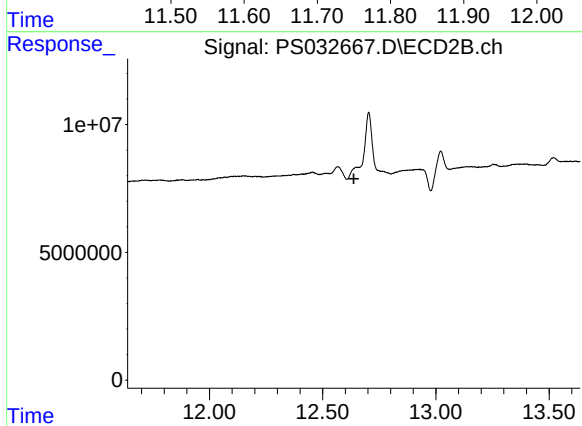

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 12.638 min
Response: 0
Conc: N.D.