

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121025\
 Data File : PS032668.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 10 Dec 2025 20:53
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 01:41:17 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 11 01:33:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.315	7.984	2519.4E6	1152.8E6	353.059	411.668
Target Compounds							
1) T	Dalapon	2.709	0.000	200.9E6	0	18.746	N.D. #
7) T	MCPA	7.896f	8.588f	4601265	2928144	<MDL	<MDL #
8) T	DICHLORPROP	8.198f	0.000	3641081	0	<MDL	N.D. #
10) T	Pentachlo...	8.798	9.827	19918216	1135339	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.619	0	5699256	N.D.	<MDL
13) T	2,4-DB	10.197f	0.000	36149554	0	5.714	N.D. #
14) T	DINOSEB	11.466	0.000	7095703	0	<MDL	N.D. #
15) T	Picloram	11.274	12.703	94025723	48867034	1.969	1.957
16) T	DCPA	11.752	12.651	22373025	15428503	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121025\
Data File : PS032668.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 10 Dec 2025 20:53
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 01:41:17 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

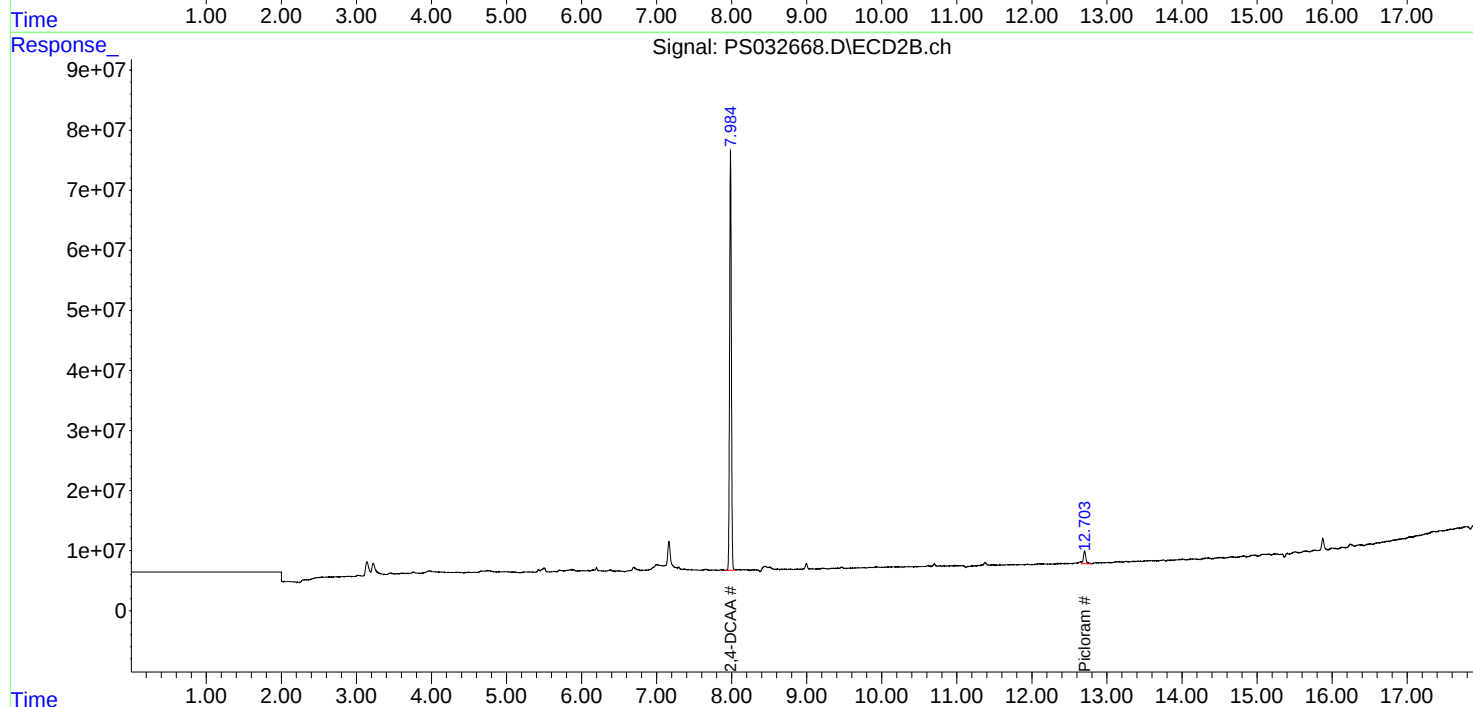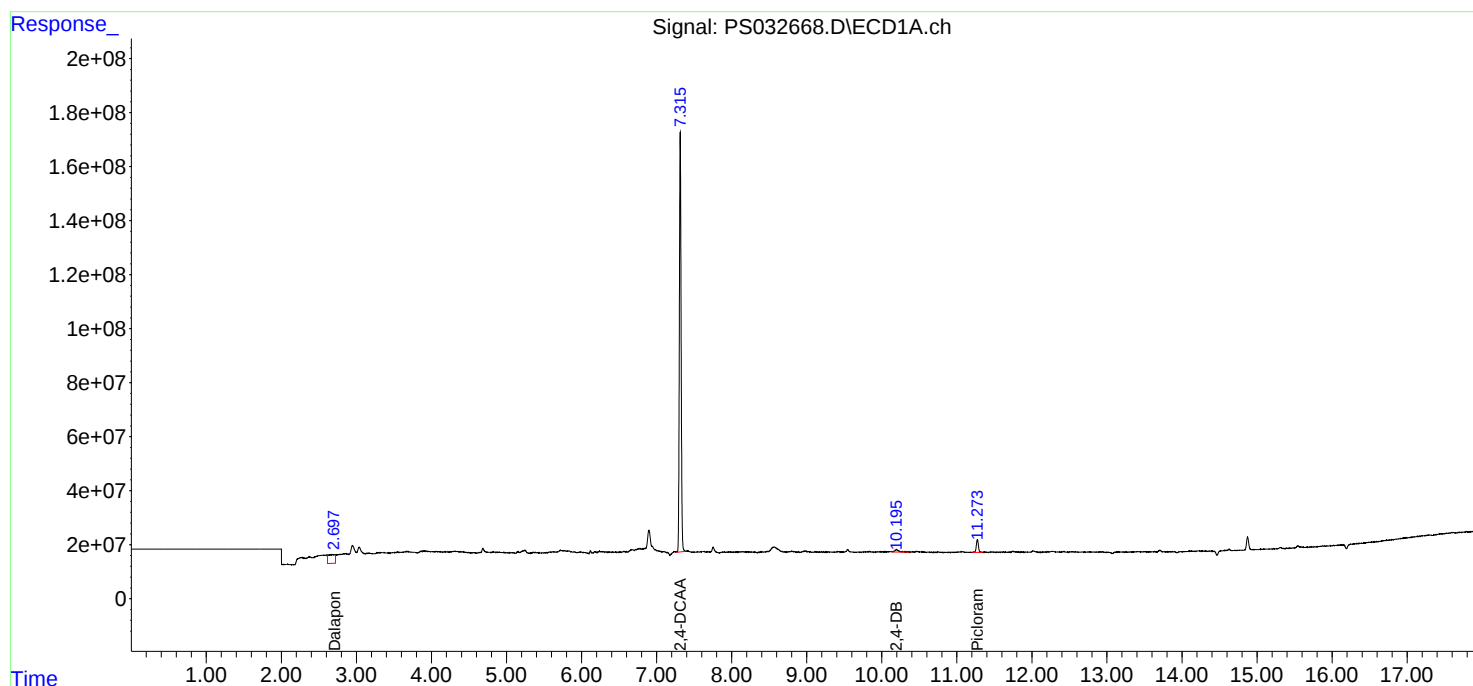


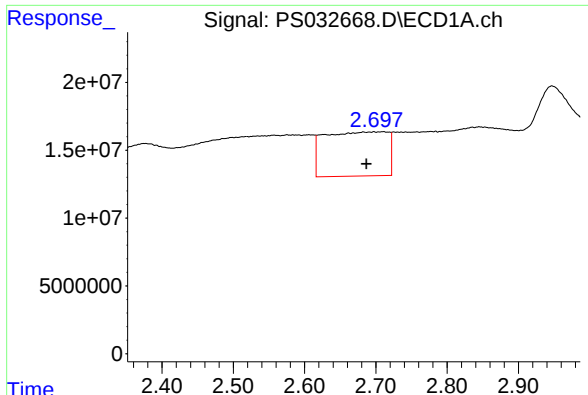

#1 Dalapon


R.T.: 2.709 min
Delta R.T.: 0.022 min
Response: 200949177
Conc: 18.75 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

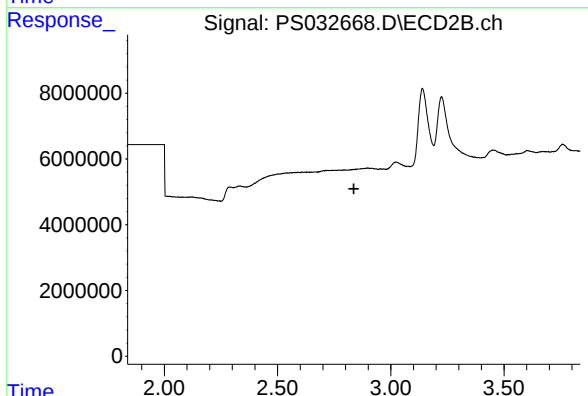


#1 Dalapon

R.T.: 0.000 min
Exp R.T.: 2.837 min
Response: 0
Conc: N.D.

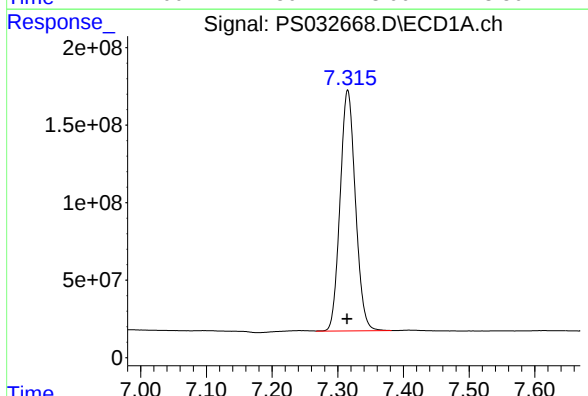


#4 2,4-DCAA

R.T.: 7.315 min
Delta R.T.: 0.000 min
Response: 2519407174
Conc: 353.06 ng/ml

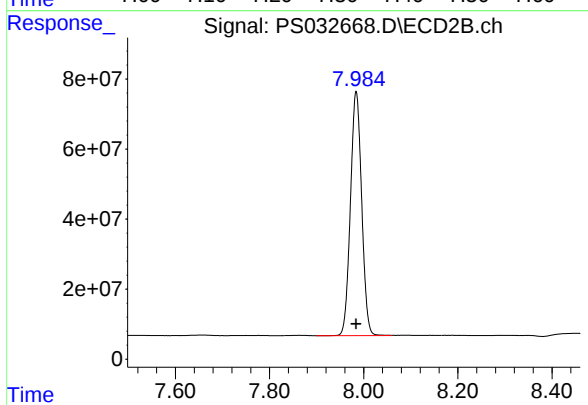

#4 2,4-DCAA


R.T.: 7.984 min
Delta R.T.: 0.000 min
Response: 1152804472
Conc: 411.67 ng/ml

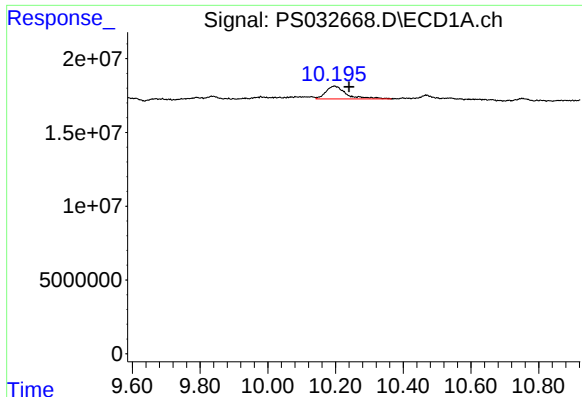

#13 2,4-DB


R.T.: 10.197 min
Delta R.T.: -0.044 min
Response: 36149554
Conc: 5.71 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

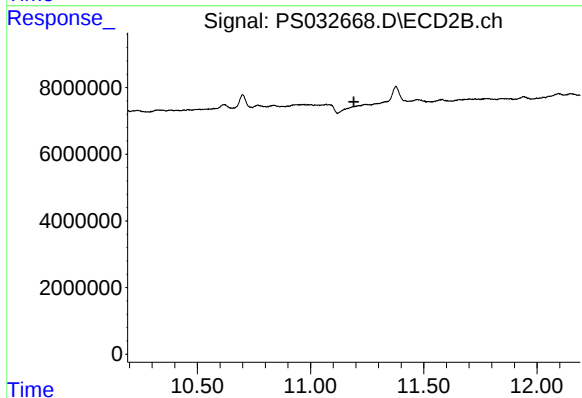


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 11.191 min
Response: 0
Conc: N.D.

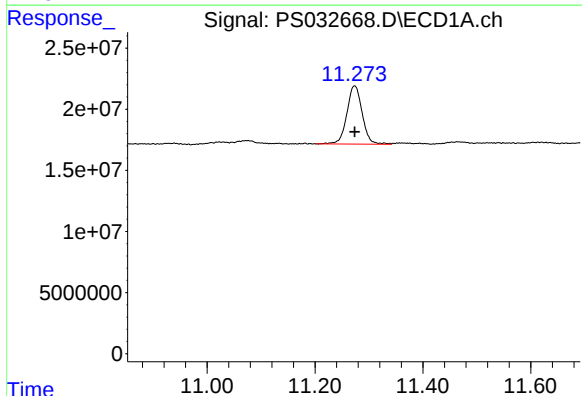

#15 Picloram

R.T.: 11.274 min
Delta R.T.: 0.000 min
Response: 94025723
Conc: 1.97 ng/ml

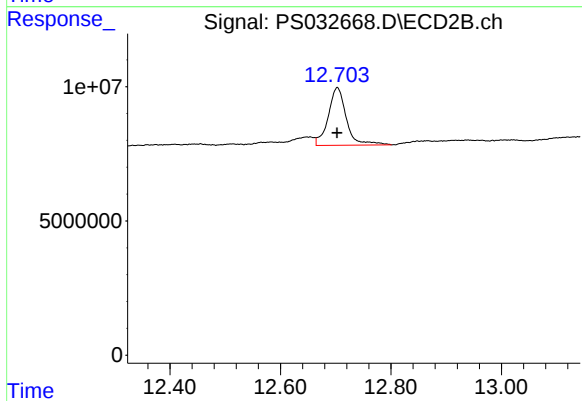

#15 Picloram

R.T.: 12.703 min
Delta R.T.: 0.000 min
Response: 48867034
Conc: 1.96 ng/ml