

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS121025\  
 Data File : PS032680.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 11 Dec 2025 01:42  
 Operator : AR\AJ  
 Sample : I.BLK  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_S  
 ClientSampleId :  
 I.BLK

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Dec 11 02:28:16 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS121025.M  
 Quant Title : 8080.M  
 QLast Update : Thu Dec 11 01:33:06 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

|                             | Compound     | RT#1    | RT#2   | Resp#1   | Resp#2   | ng/ml   | ng/ml   |
|-----------------------------|--------------|---------|--------|----------|----------|---------|---------|
| -----                       |              |         |        |          |          |         |         |
| System Monitoring Compounds |              |         |        |          |          |         |         |
| 4) S                        | 2,4-DCAA     | 7.315   | 7.985  | 2444.8E6 | 1110.1E6 | 342.597 | 396.401 |
| Target Compounds            |              |         |        |          |          |         |         |
| 1) T                        | Dalapon      | 0.000   | 2.843  | 0        | 3965404  | N.D.    | <MDL    |
| 7) T                        | MCPA         | 0.000   | 8.504f | 0        | 12637060 | N.D.    | 1.142   |
| 8) T                        | DICHLORPROP  | 8.213   | 0.000  | 5053703  | 0        | <MDL    | N.D. #  |
| 10) T                       | Pentachlo... | 8.795   | 9.783f | 12328976 | 9511502  | <MDL    | <MDL #  |
| 11) T                       | 2,4,5-TP ... | 0.000   | 10.186 | 0        | 5287510  | N.D.    | <MDL    |
| 12) T                       | 2,4,5-T      | 0.000   | 10.617 | 0        | 20292135 | N.D.    | 1.150   |
| 13) T                       | 2,4-DB       | 10.286f | 0.000  | 83428361 | 0        | 13.187  | N.D. #  |
| 14) T                       | DINOSEB      | 11.449  | 0.000  | 133.9E6  | 0        | 4.935   | N.D. #  |
| 15) T                       | Picloram     | 11.272  | 0.000  | 74988187 | 0        | 1.570   | N.D. #  |
| 16) T                       | DCPA         | 0.000   | 12.637 | 0        | 279.5E6  | N.D.    | 13.508  |
| -----                       |              |         |        |          |          |         |         |



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Data\PS121025\  
Data File : PS032680.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 11 Dec 2025 01:42  
Operator : AR\AJ  
Sample : I.BLK  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Dec 11 02:28:16 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_S\Method\PS121025.M  
Quant Title : 8080.M  
QLast Update : Thu Dec 11 01:33:06 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

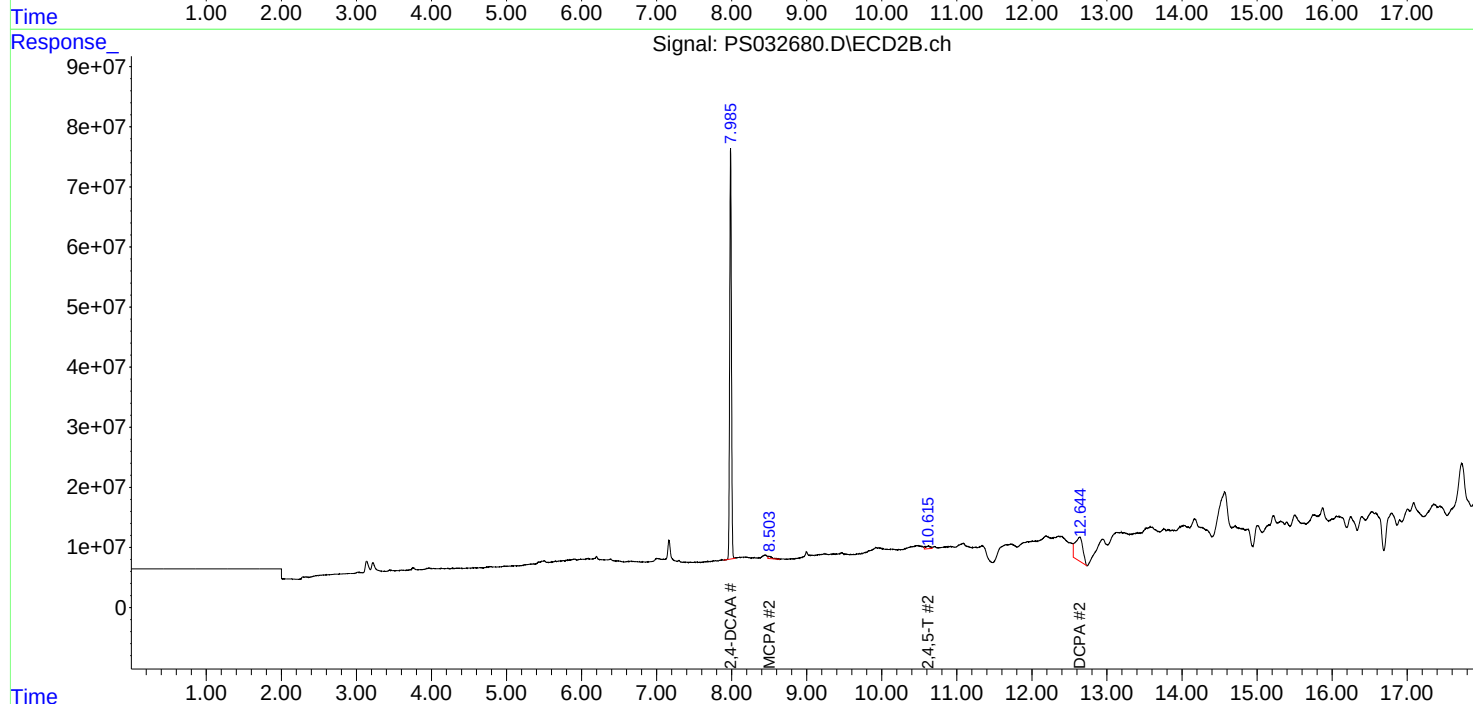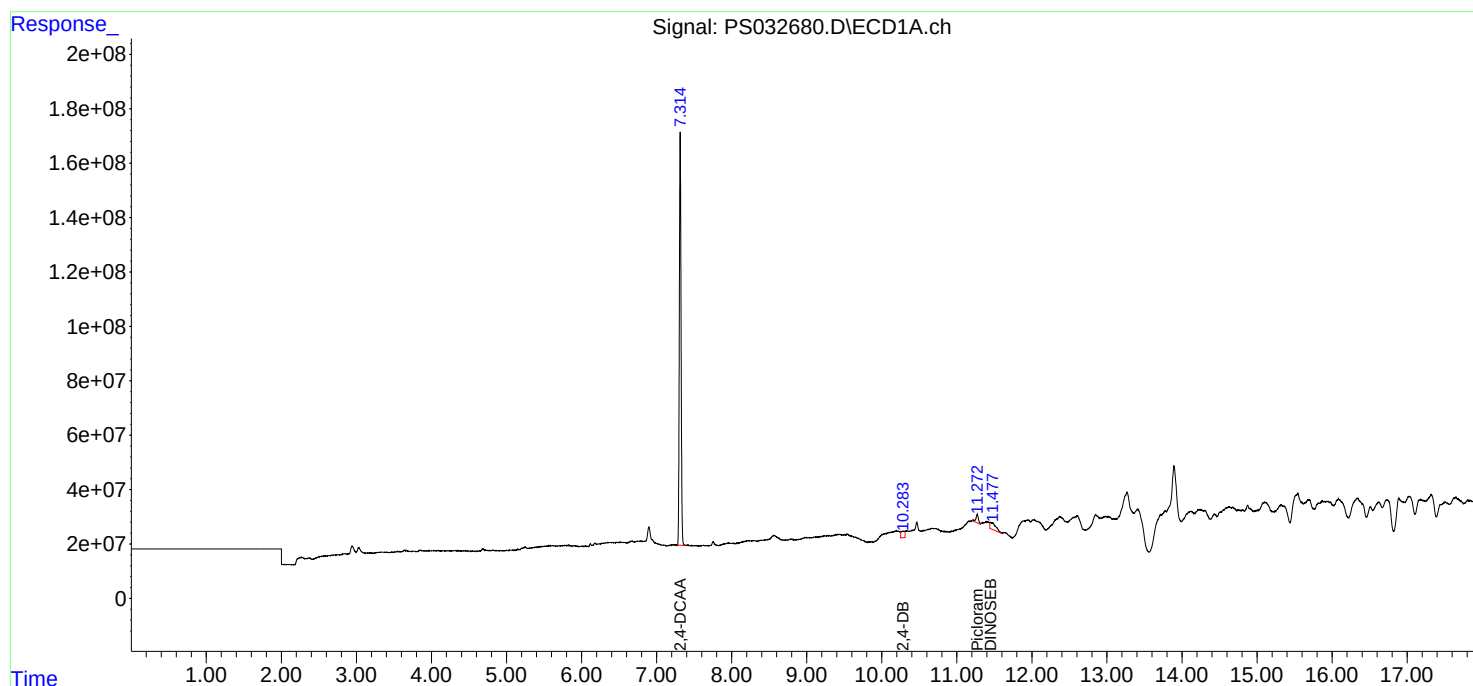


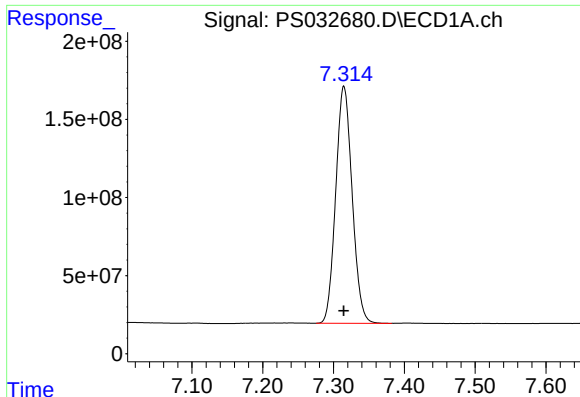

#4 2,4-DCAA


R.T.: 7.315 min  
Delta R.T.: 0.000 min  
Response: 2444750862  
Conc: 342.60 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

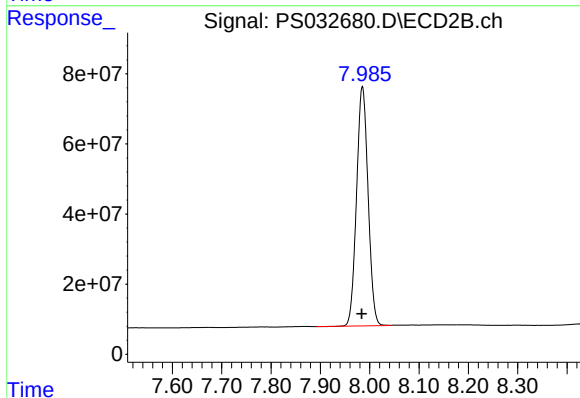


#4 2,4-DCAA

R.T.: 7.985 min  
Delta R.T.: 0.001 min  
Response: 1110051433  
Conc: 396.40 ng/ml

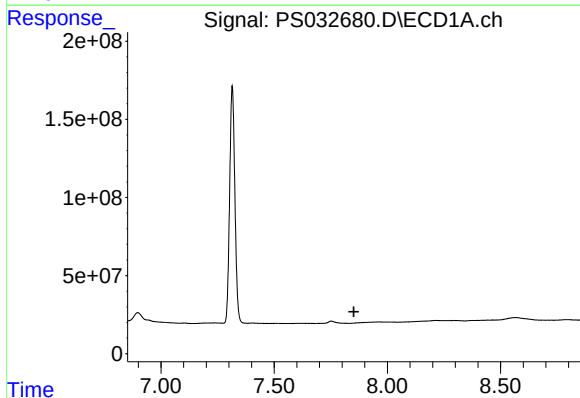


#7 MCPA

R.T.: 0.000 min  
Exp R.T. : 7.852 min  
Response: 0  
Conc: N.D.

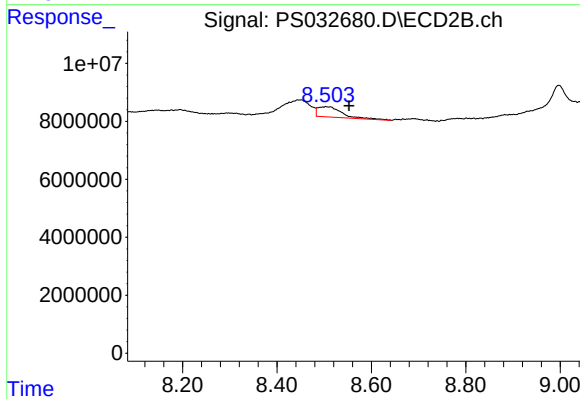

#7 MCPA


R.T.: 8.504 min  
Delta R.T.: -0.049 min  
Response: 12637060  
Conc: 1.14 ug/ml

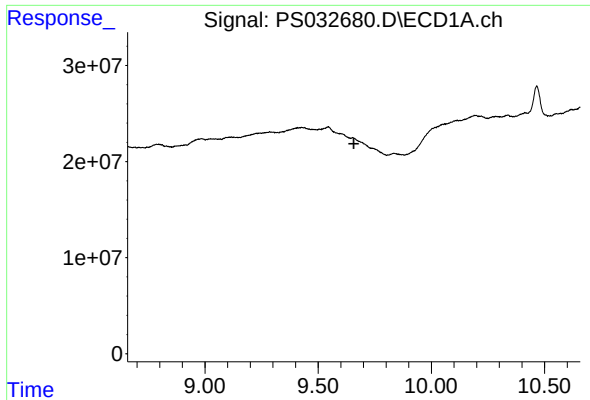

#12 2,4,5-T


R.T.: 0.000 min  
Exp R.T.: 9.658 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

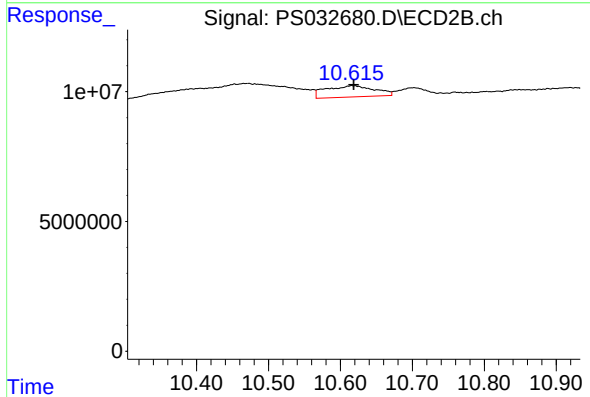


#12 2,4,5-T

R.T.: 10.617 min  
Delta R.T.: -0.002 min  
Response: 20292135  
Conc: 1.15 ng/ml

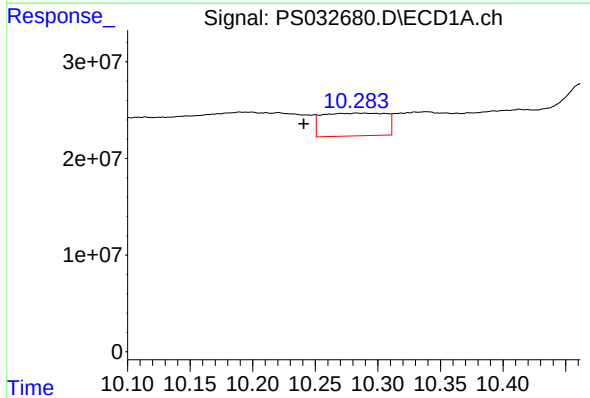


#13 2,4-DB

R.T.: 10.286 min  
Delta R.T.: 0.045 min  
Response: 83428361  
Conc: 13.19 ng/ml

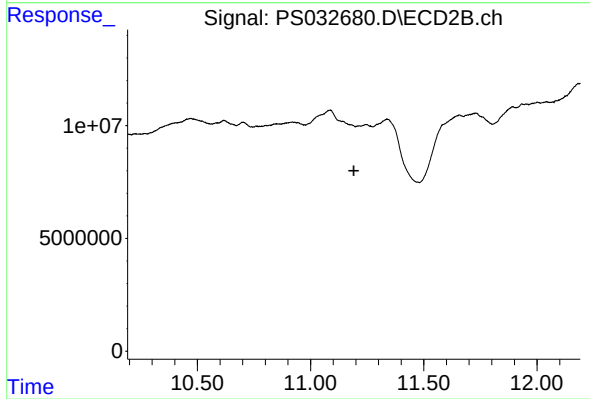

#13 2,4-DB


R.T.: 0.000 min  
Exp R.T.: 11.191 min  
Response: 0  
Conc: N.D.

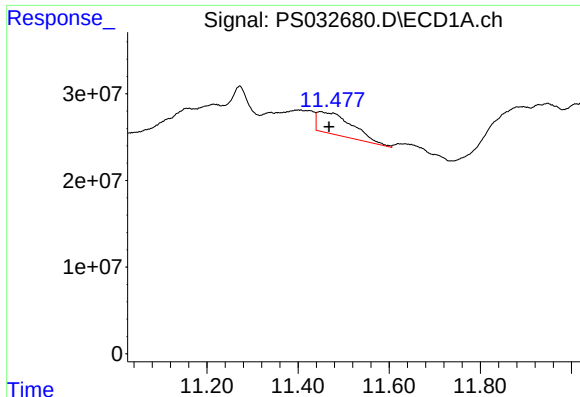

#14 DINOSEB


R.T.: 11.449 min  
Delta R.T.: -0.019 min  
Response: 133891120  
Conc: 4.93 ng/ml

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

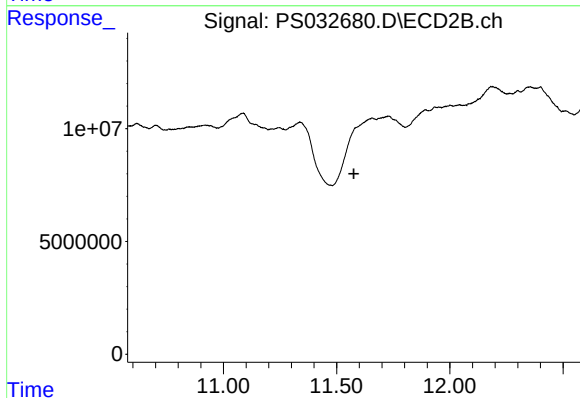


#14 DINOSEB

R.T.: 0.000 min  
Exp R.T. : 11.576 min  
Response: 0  
Conc: N.D.

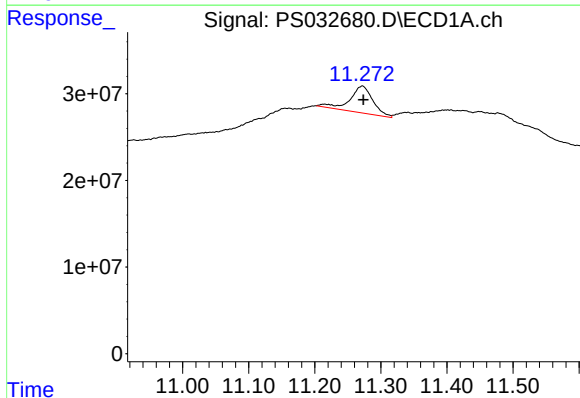


#15 Picloram

R.T.: 11.272 min  
Delta R.T.: -0.002 min  
Response: 74988187  
Conc: 1.57 ng/ml

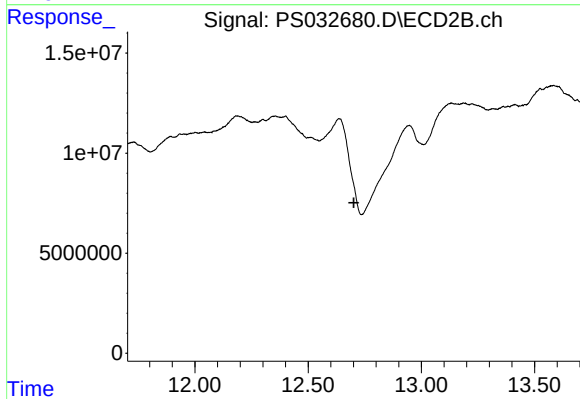

#15 Picloram


R.T.: 0.000 min  
Exp R.T. : 12.702 min  
Response: 0  
Conc: N.D.

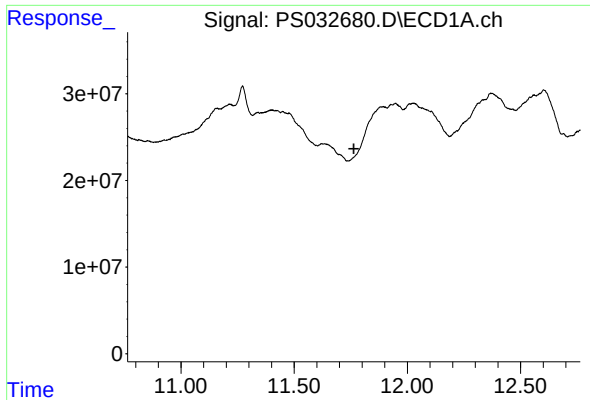

#16 DCPA

R.T.: 0.000 min  
Exp R.T.: 11.764 min  
Response: 0  
Conc: N.D.

Instrument :  
ECD\_S  
ClientSampleId :  
I.BLK

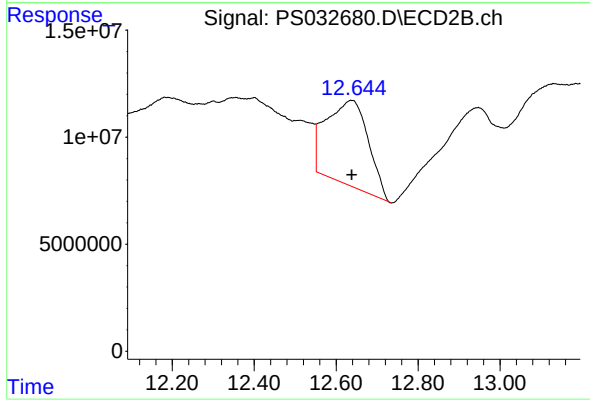

#16 DCPA

R.T.: 12.637 min  
Delta R.T.: -0.001 min  
Response: 279455237  
Conc: 13.51 ng/ml