

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121118\
 Data File : PS002556.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2018 16:12
 Operator : EI\SJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 18:24:52 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.392	10.888	203.4E6	205.0E6	640.726	529.924
Target Compounds							
7) T	MCPA	0.000	11.788	0	714499	N.D.	0.497 #
15) T	Picloram	16.853	16.745	180406	489013	0.071	0.178 #
16) T	DCPA	0.000	16.838	0	1259078	N.D.	0.433 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121118\
Data File : PS002556.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2018 16:12
Operator : EI\SJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 18:24:52 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

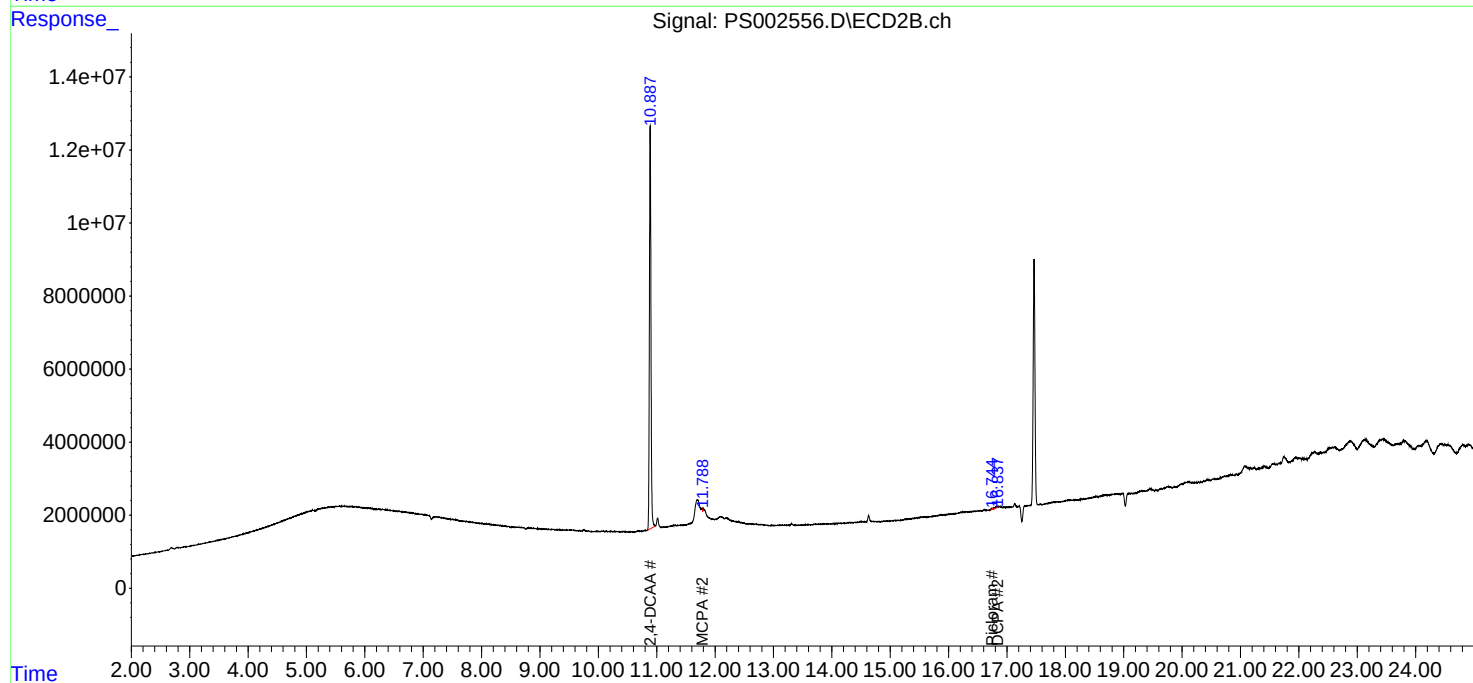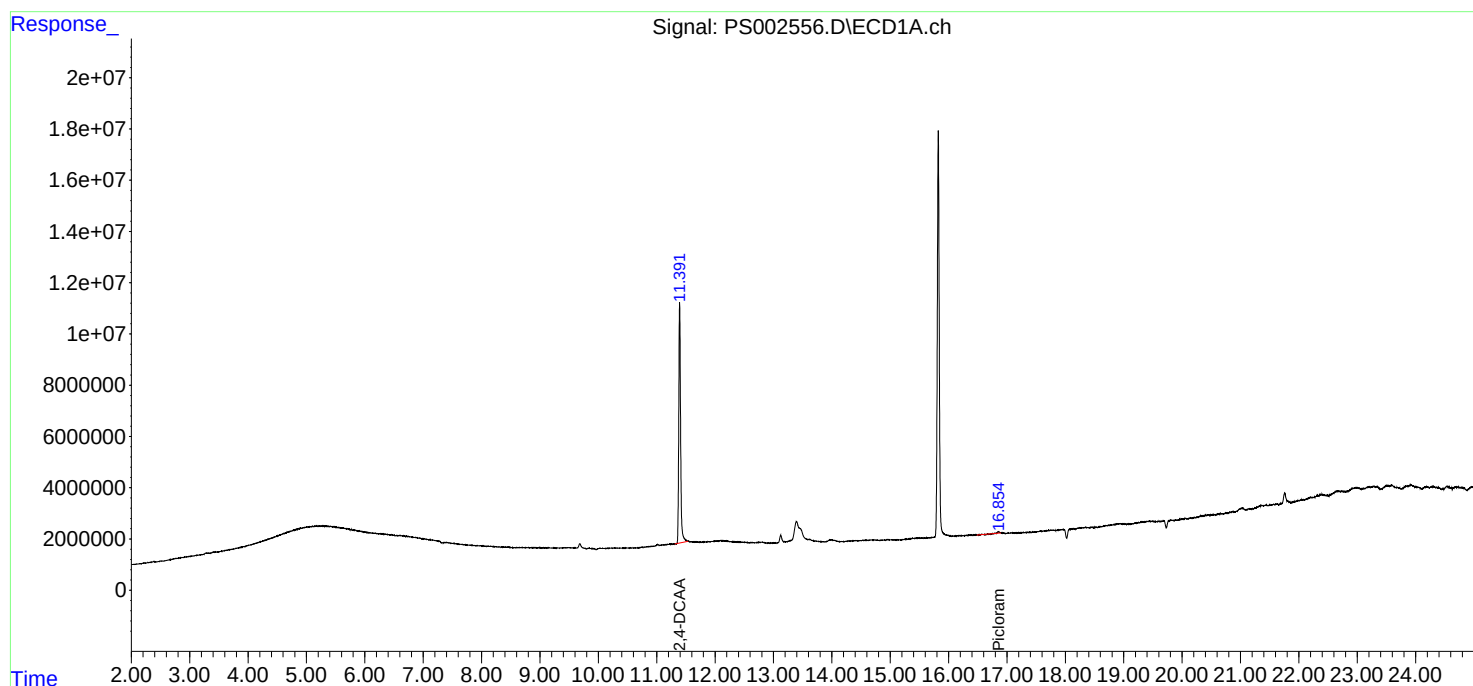


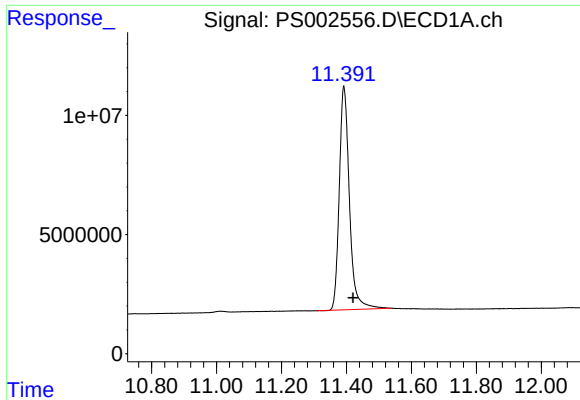

#4 2,4-DCAA


R.T.: 11.392 min
Delta R.T.: -0.028 min
Response: 203379152
Conc: 640.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

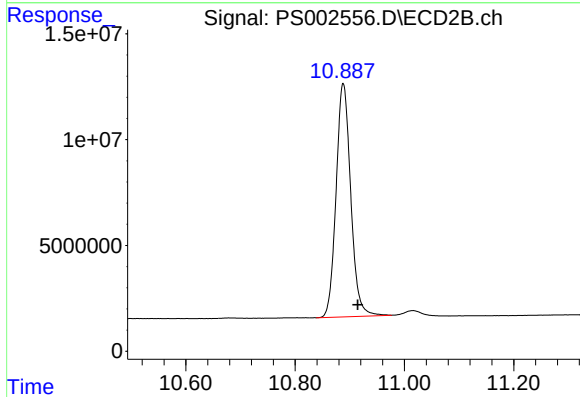


#4 2,4-DCAA

R.T.: 10.888 min
Delta R.T.: -0.027 min
Response: 204958591
Conc: 529.92 ng/ml

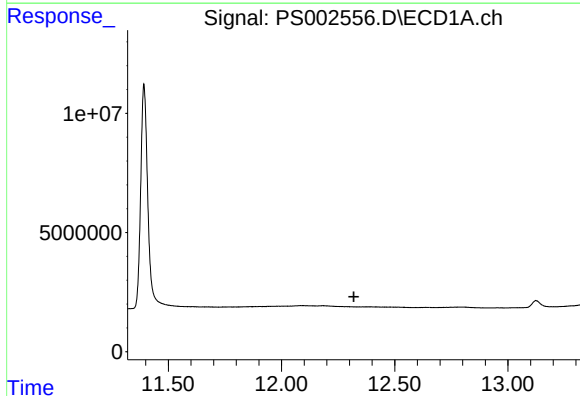


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.319 min
Response: 0
Conc: N.D.

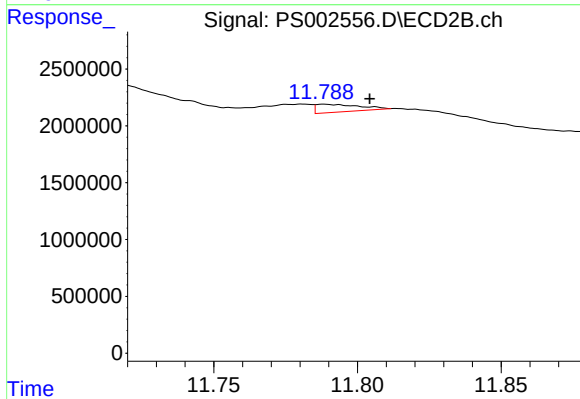

#7 MCPA


R.T.: 11.788 min
Delta R.T.: -0.016 min
Response: 714499
Conc: 0.50 ug/ml

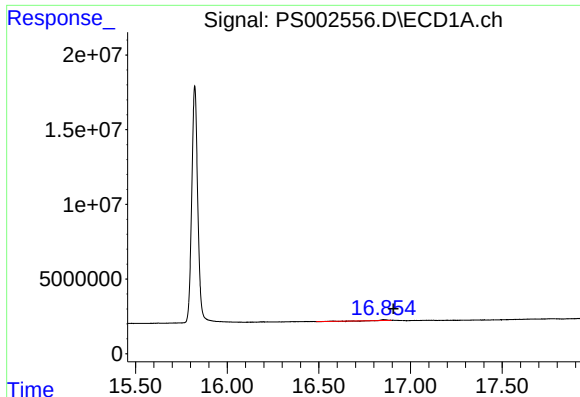

#15 Picloram


R.T.: 16.853 min
Delta R.T.: -0.053 min
Response: 180406
Conc: 0.07 ng/ml

Instrument :
ECD_S
ClientSampleId :

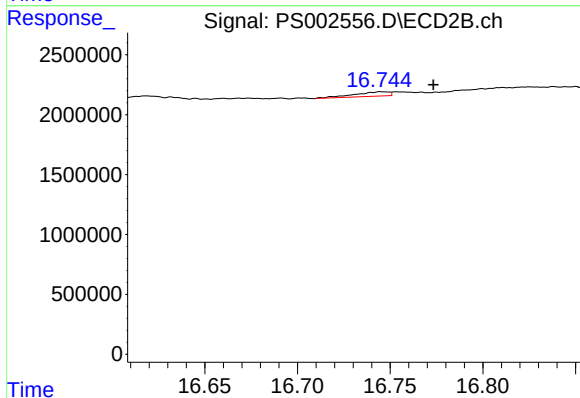


#15 Picloram

R.T.: 16.745 min
Delta R.T.: -0.028 min
Response: 489013
Conc: 0.18 ng/ml

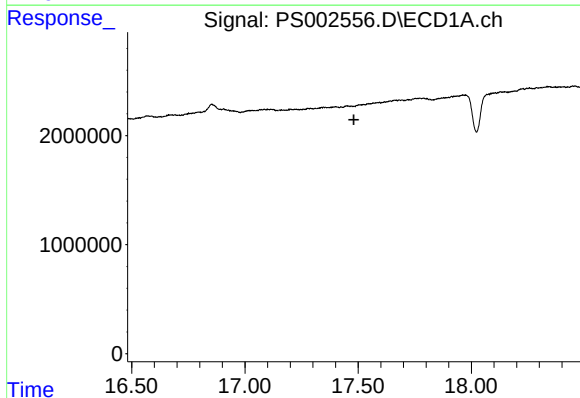

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.481 min
Response: 0
Conc: N.D.

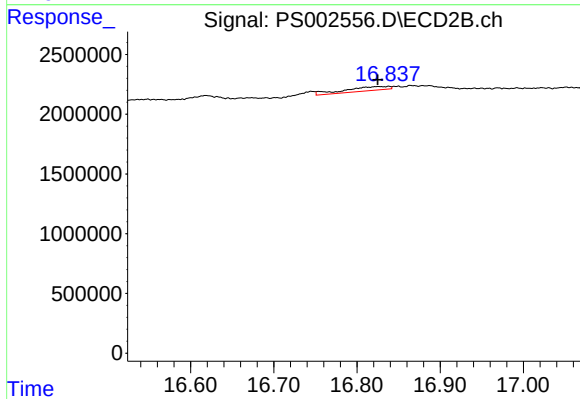

#16 DCPA

R.T.: 16.838 min
Delta R.T.: 0.013 min
Response: 1259078
Conc: 0.43 ng/ml