

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121119\
 Data File : PS008014.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 08:25
 Operator : SM\AJ
 Sample : K6176-06RE
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 48-SPRUCERE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 10:12:35 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.435	5.156	310.8E6	171.6E6	198.648	221.165
Target Compounds							
1) T	Dalapon	1.993	1.698	55550114	146.6E6	27.239	123.438 #
2) T	3,5-DICHL...	0.000	4.446	0	5223574	N.D.	5.048
3) T	4-Nitroph...	0.000	4.832	0	20042108	N.D.	44.258
5) T	DICAMBA	5.523	5.292	36546154	10880105	6.423	3.806 #
8) T	DICHLORPROP	0.000	5.819	0	14615533	N.D.	20.389
9) T	2,4-D	6.402	0.000	199.5E6	0	124.004	N.D. #
10) T	Pentachlo...	0.000	6.444	0	8581505	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.752	0	48233318	N.D.	11.246
15) T	Picloram	0.000	8.912	0	14260344	N.D.	2.309



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121119\
Data File : PS008014.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 08:25
Operator : SM\AJ
Sample : K6176-06RE
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
48-SPRUCERE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 10:12:35 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

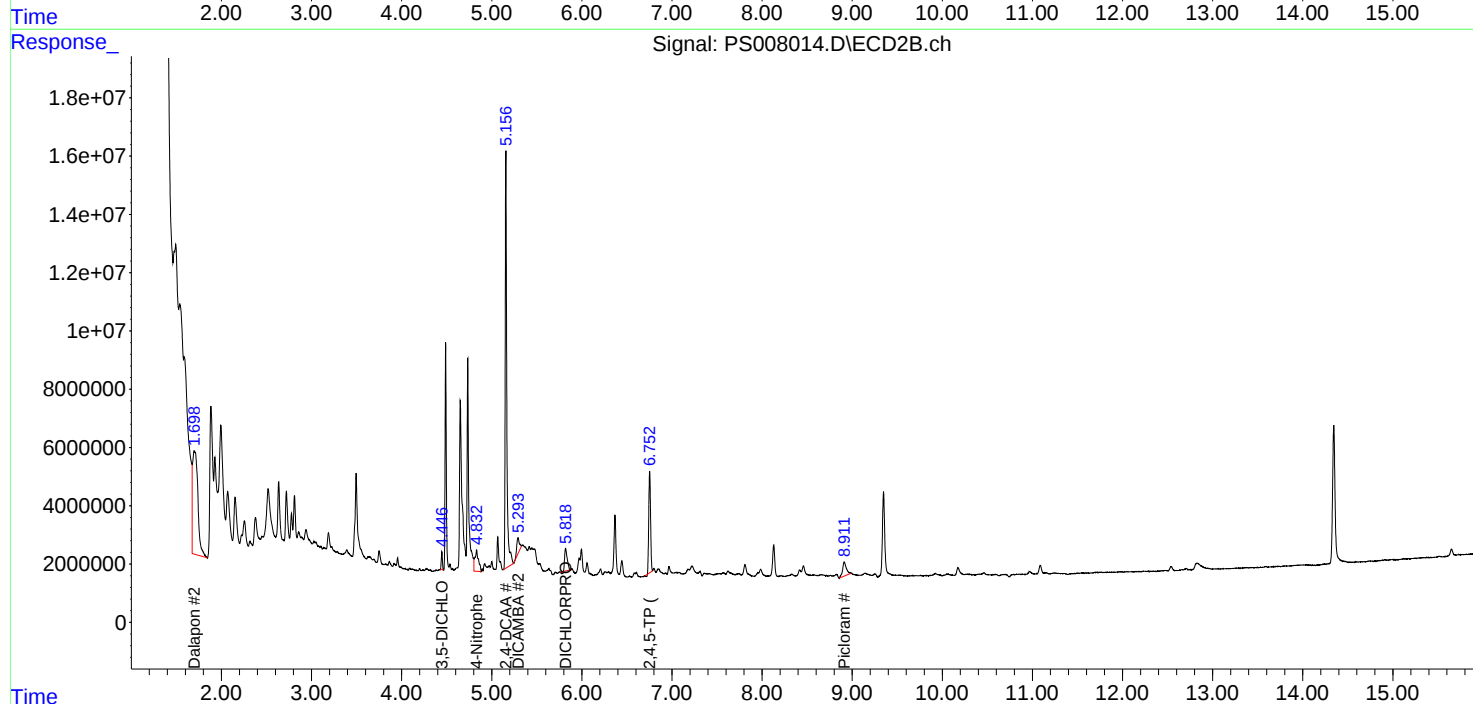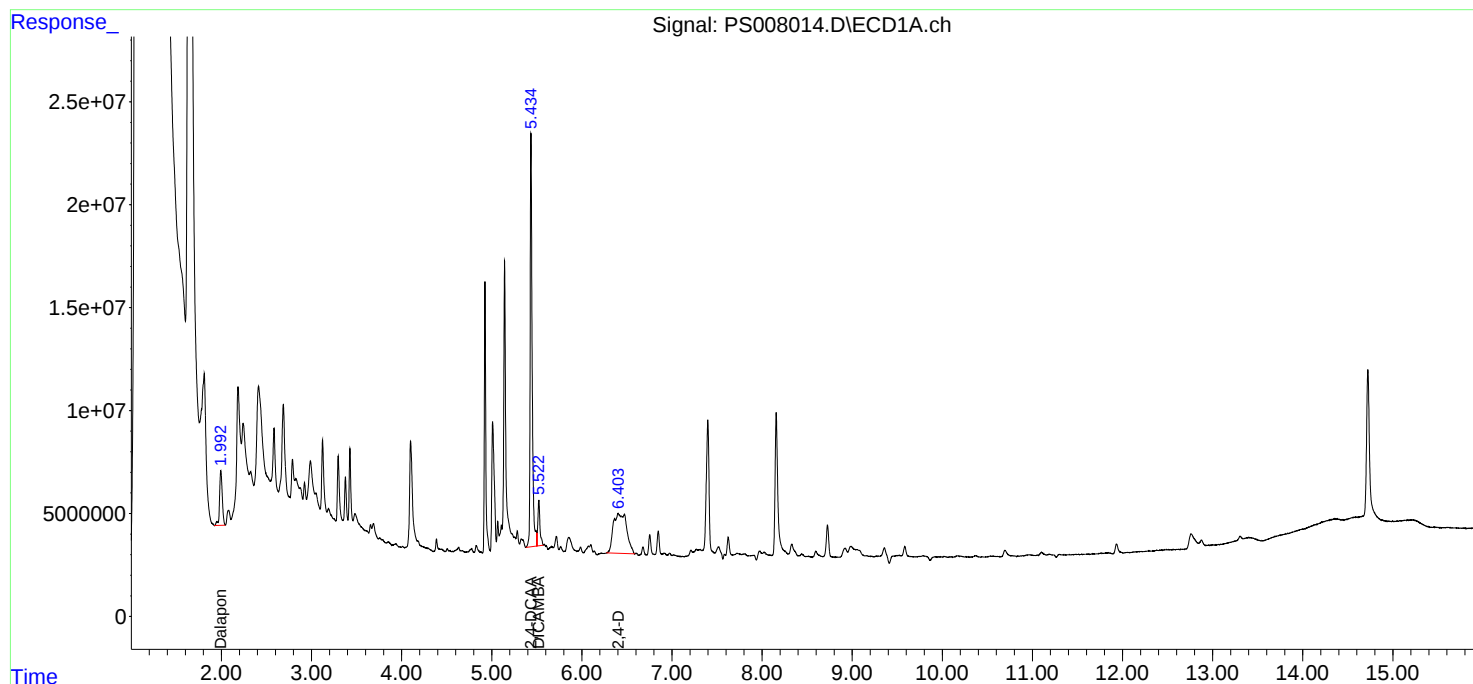


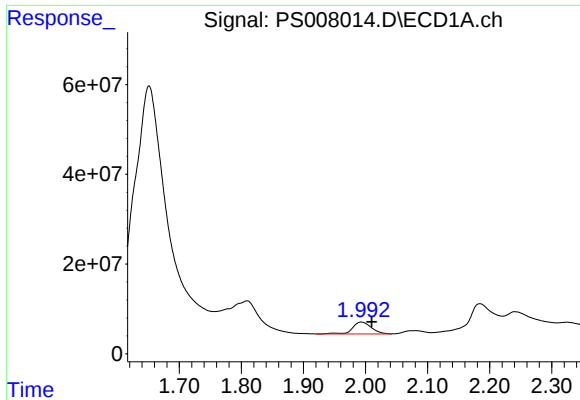

#1 Dalapon


R.T.: 1.993 min
Delta R.T.: -0.017 min
Response: 55550114
Conc: 27.24 ng/ml

Instrument :
ECD_S
ClientSampleId :
48-SPRUCERE

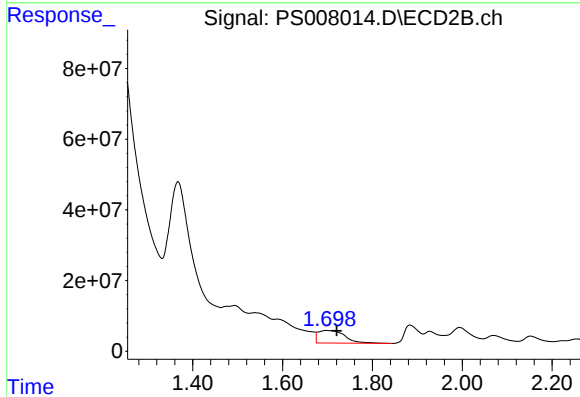


#1 Dalapon

R.T.: 1.698 min
Delta R.T.: -0.023 min
Response: 146618083
Conc: 123.44 ng/ml

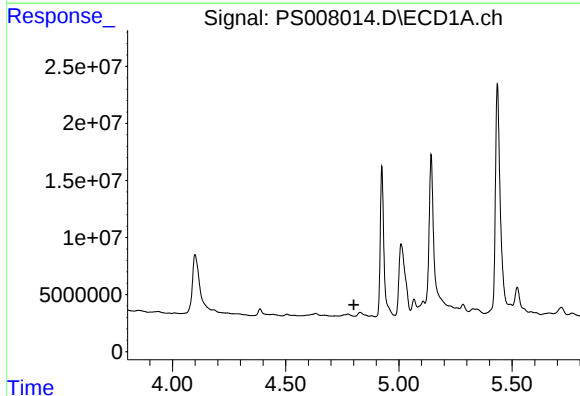


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

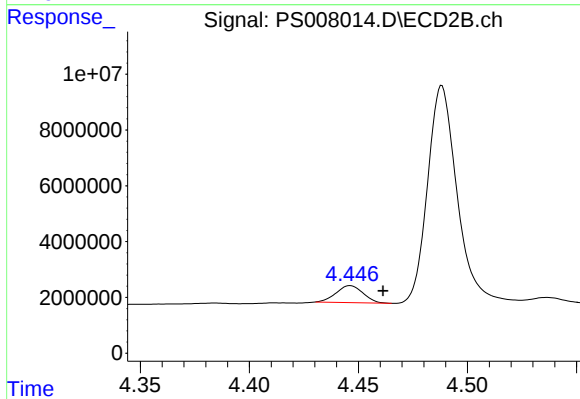

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.446 min
Delta R.T.: -0.015 min
Response: 5223574
Conc: 5.05 ng/ml

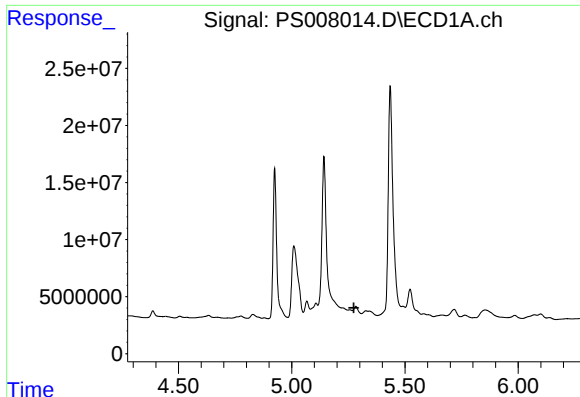

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 5.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
48-SPRUCERE

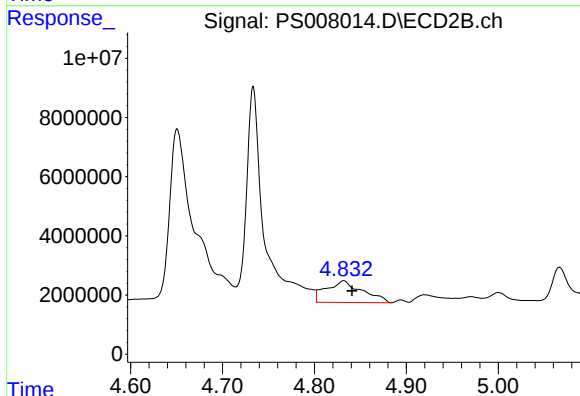


#3 4-Nitrophenol

R.T.: 4.832 min
Delta R.T.: -0.009 min
Response: 20042108
Conc: 44.26 ng/ml

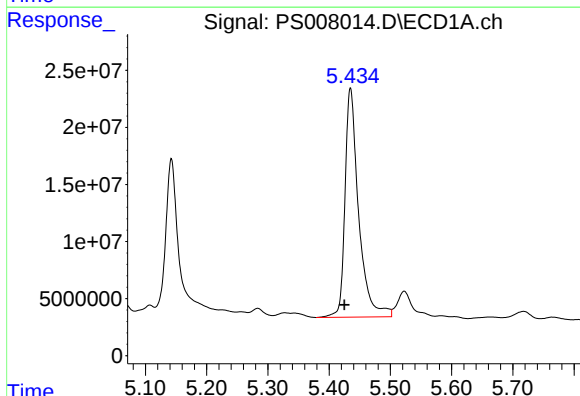


#4 2,4-DCAA

R.T.: 5.435 min
Delta R.T.: 0.010 min
Response: 310752476
Conc: 198.65 ng/ml

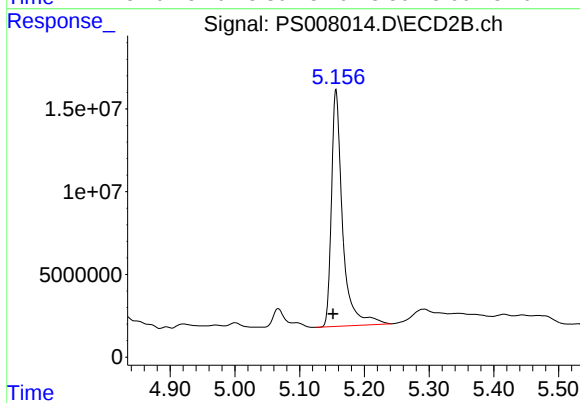

#4 2,4-DCAA


R.T.: 5.156 min
Delta R.T.: 0.005 min
Response: 171605542
Conc: 221.16 ng/ml

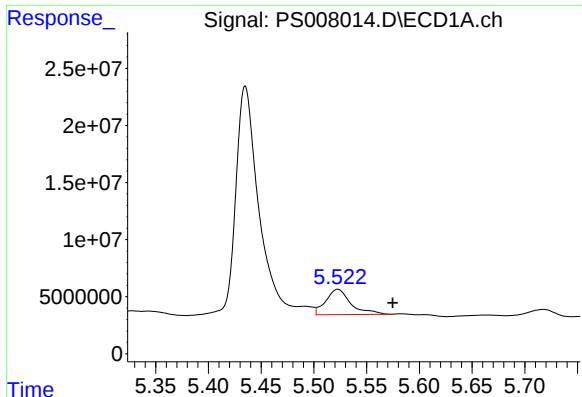

#5 DICAMBA


R.T.: 5.523 min
Delta R.T.: -0.052 min
Response: 36546154
Conc: 6.42 ng/ml

Instrument :
ECD_S
ClientSampleId :
48-SPRUCERE

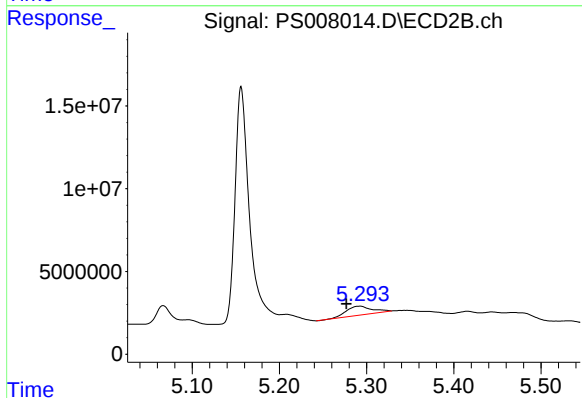


#5 DICAMBA

R.T.: 5.292 min
Delta R.T.: 0.015 min
Response: 10880105
Conc: 3.81 ng/ml

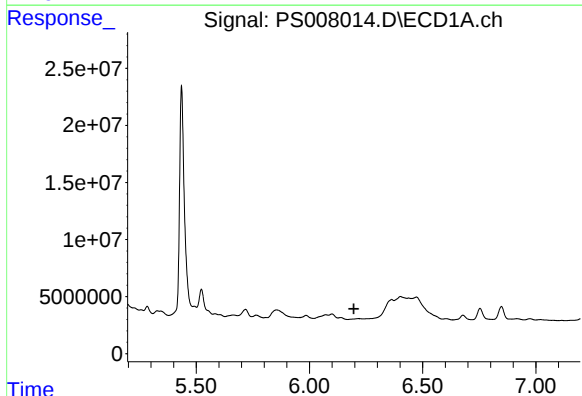


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 6.197 min
Response: 0
Conc: N.D.

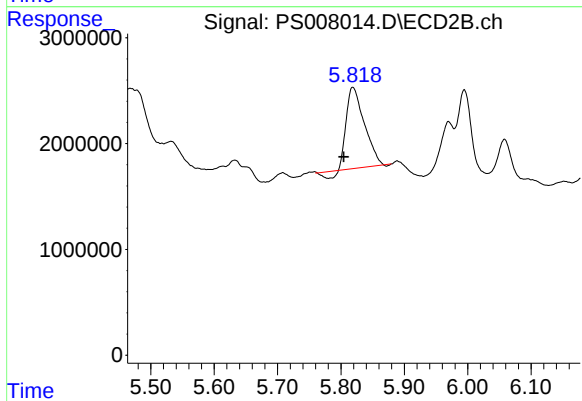

#8 DICHLORPROP


R.T.: 5.819 min
Delta R.T.: 0.015 min
Response: 14615533
Conc: 20.39 ng/ml

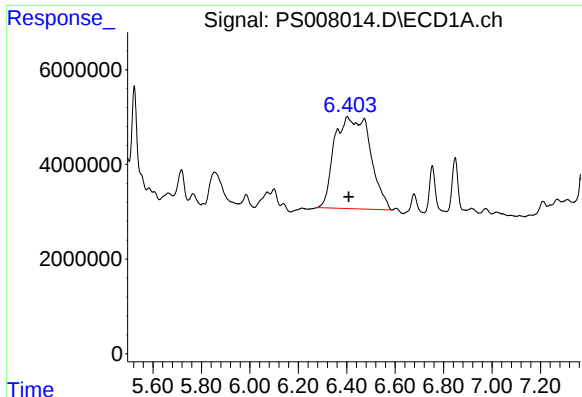

#9 2,4-D


R.T.: 6.402 min
Delta R.T.: -0.006 min
Response: 199495983
Conc: 124.00 ng/ml

Instrument :
ECD_S
ClientSampleId :
48-SPRUCERE

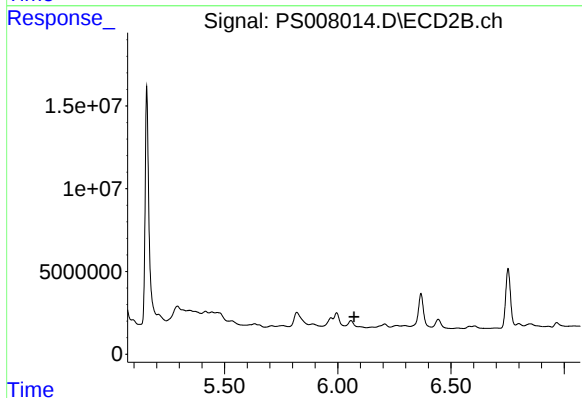


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.

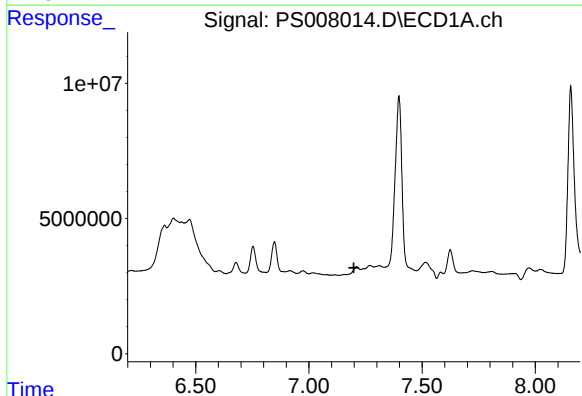


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 7.199 min
Response: 0
Conc: N.D.

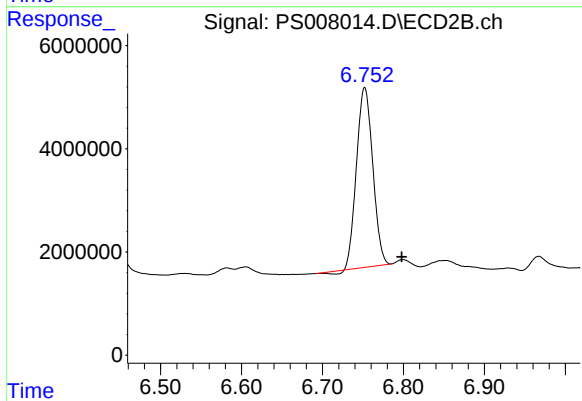

#11 2,4,5-TP (SILVEX)


R.T.: 6.752 min
Delta R.T.: -0.046 min
Response: 48233318
Conc: 11.25 ng/ml

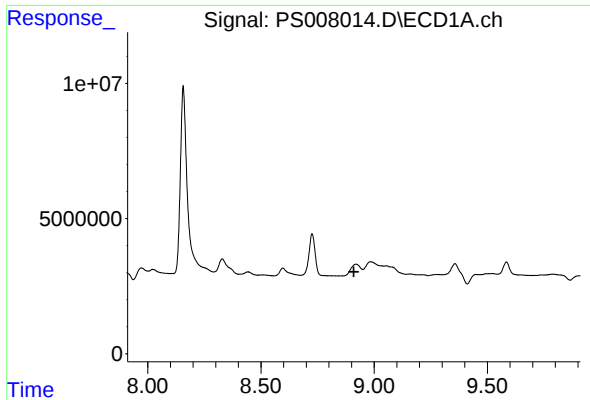

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 8.911 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
48-SPRUCERE

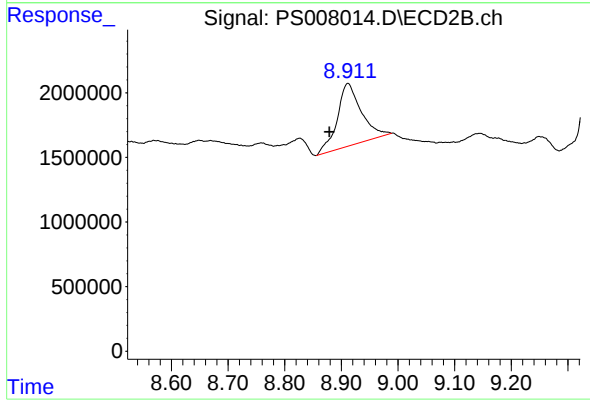

#15 Picloram

R.T.: 8.912 min
Delta R.T.: 0.032 min
Response: 14260344
Conc: 2.31 ng/ml