

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121119\
 Data File : PS008015.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 08:47
 Operator : SM\AJ
 Sample : K6118-05
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 SU-02-120619

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 10:12:48 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.442	5.170	1102.9E6	584.3E6	705.009	753.030
Target Compounds							
1) T	Dalapon	2.008	1.728	173.9E6	343.9E6	85.257	289.527 #
2) T	3,5-DICHL...	0.000	4.463	0	7238563	N.D.	6.995
5) T	DICAMBA	5.534	5.309	49203708	17687110	8.648	6.186 #
6) T	MCP	0.000	5.309	0	17687110	N.D.	8.529
7) T	MCPA	0.000	5.492	0	33725344	N.D.	10.583
8) T	DICHLORPROP	0.000	5.837	0	19524068	N.D.	27.237
9) T	2,4-D	0.000	6.075	0	5632127	N.D.	6.374
10) T	Pentachlo...	0.000	6.462	0	7555984	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	6.769	0	33392014	N.D.	7.786
12) T	2,4,5-T	7.407	0.000	107.8E6	0	11.650	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121119\
Data File : PS008015.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 08:47
Operator : SM\AJ
Sample : K6118-05
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
SU-02-120619

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 10:12:48 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

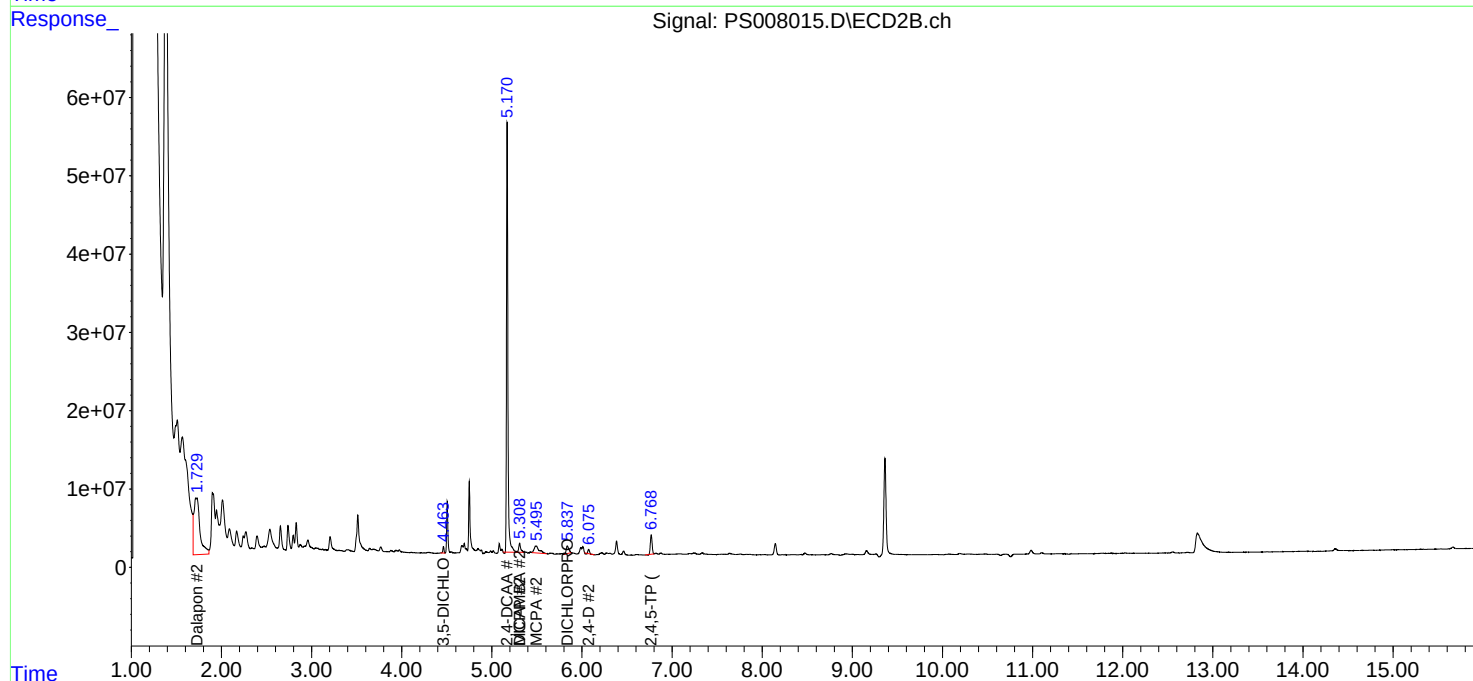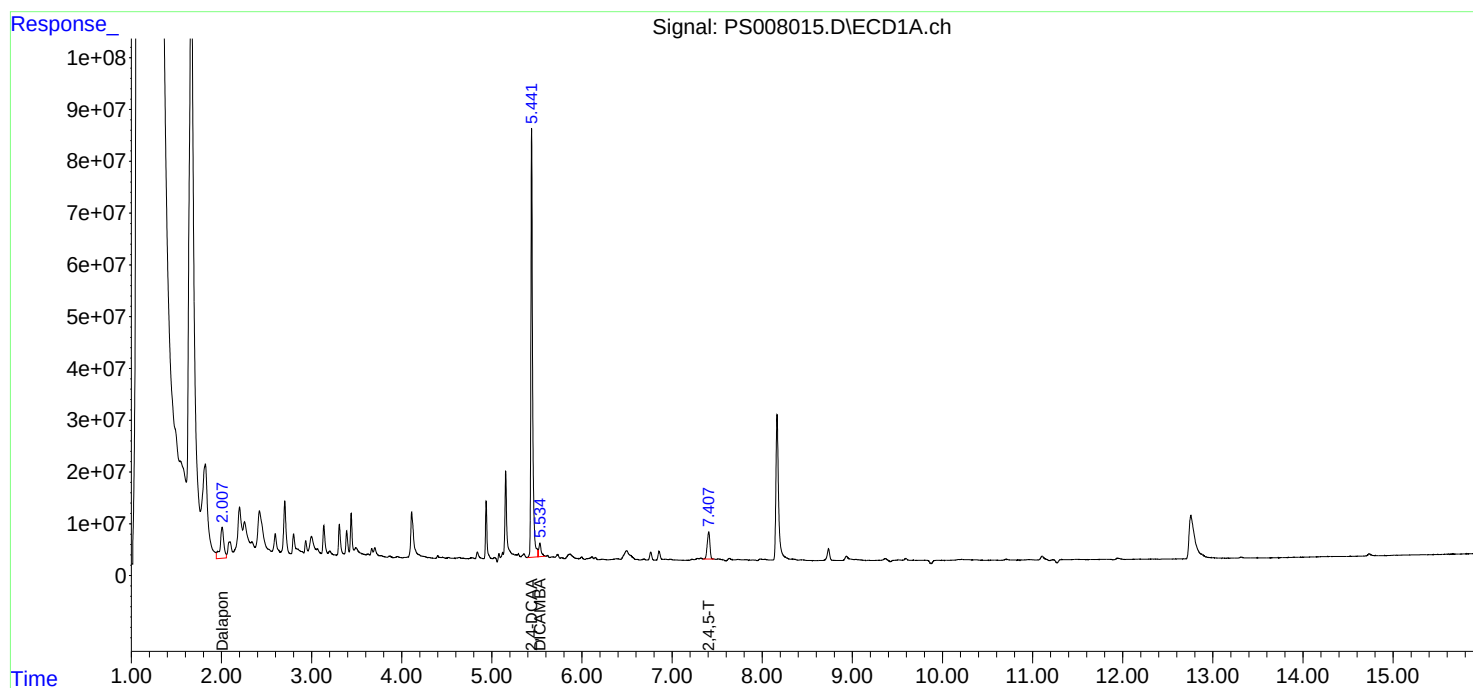


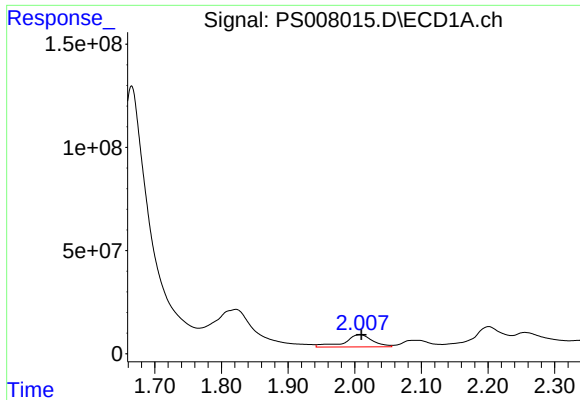

#1 Dalapon


R.T.: 2.008 min
Delta R.T.: -0.002 min
Response: 173867498
Conc: 85.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-02-120619

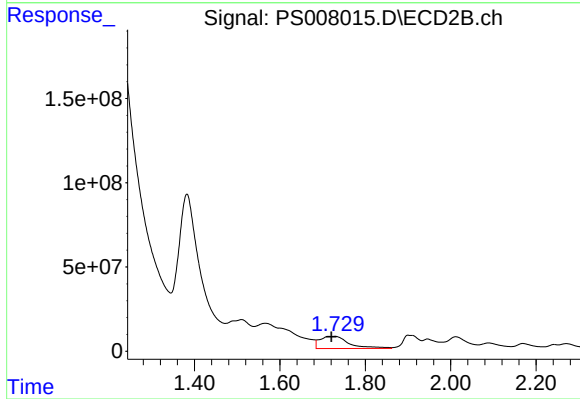


#1 Dalapon

R.T.: 1.728 min
Delta R.T.: 0.008 min
Response: 343897950
Conc: 289.53 ng/ml

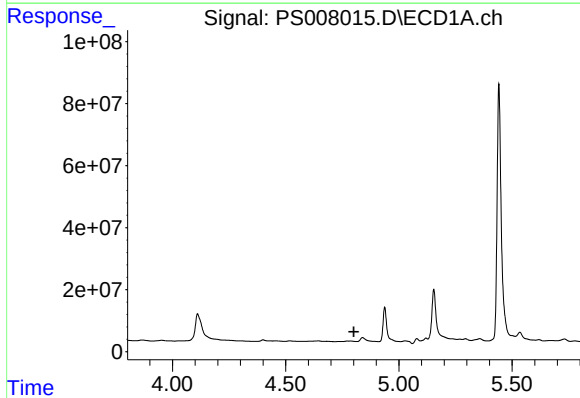


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 4.801 min
Response: 0
Conc: N.D.

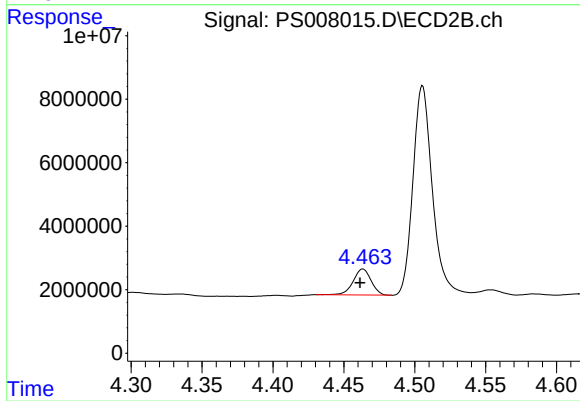

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 4.463 min
Delta R.T.: 0.002 min
Response: 7238563
Conc: 6.99 ng/ml

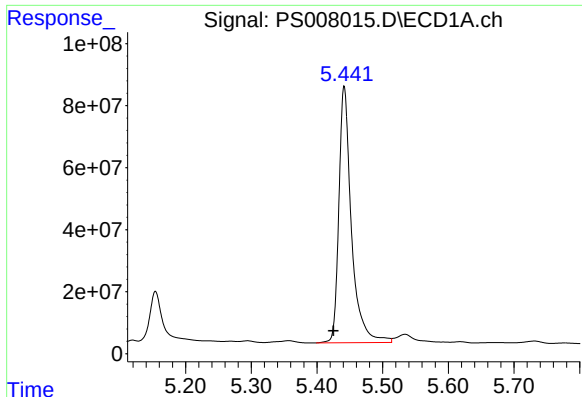

#4 2,4-DCAA


R.T.: 5.442 min
Delta R.T.: 0.017 min
Response: 1102869105
Conc: 705.01 ng/ml

Instrument :
ECD_S
ClientSampleId :
SU-02-120619

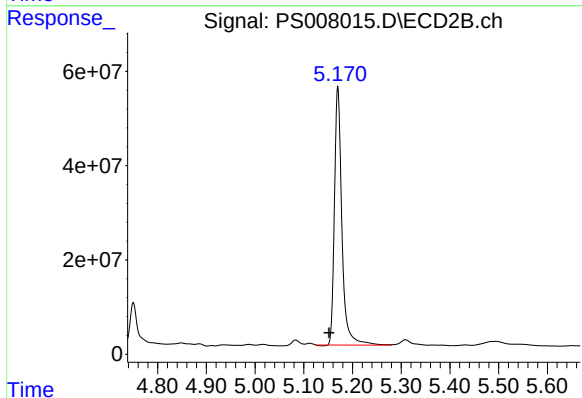


#4 2,4-DCAA

R.T.: 5.170 min
Delta R.T.: 0.018 min
Response: 584289474
Conc: 753.03 ng/ml

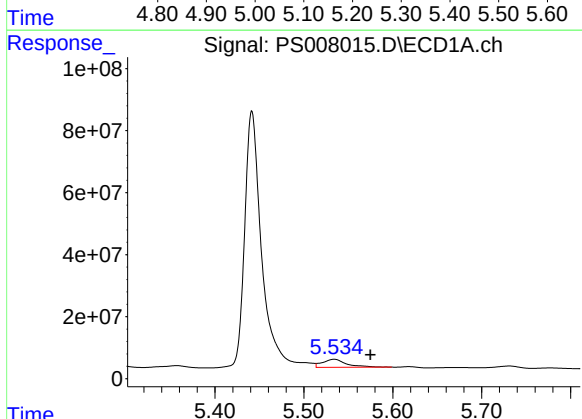


#5 DICAMBA

R.T.: 5.534 min
Delta R.T.: -0.041 min
Response: 49203708
Conc: 8.65 ng/ml

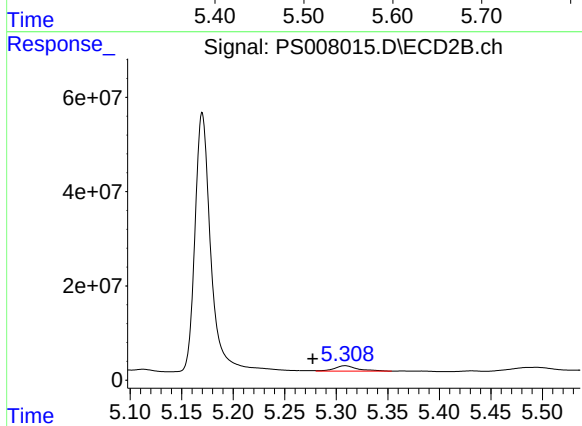

#5 DICAMBA


R.T.: 5.309 min
Delta R.T.: 0.032 min
Response: 17687110
Conc: 6.19 ng/ml

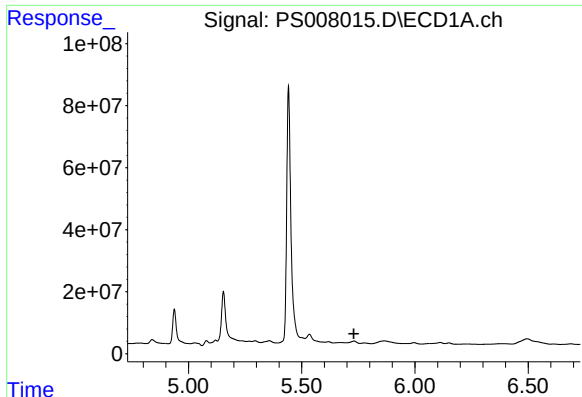

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 5.730 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-02-120619

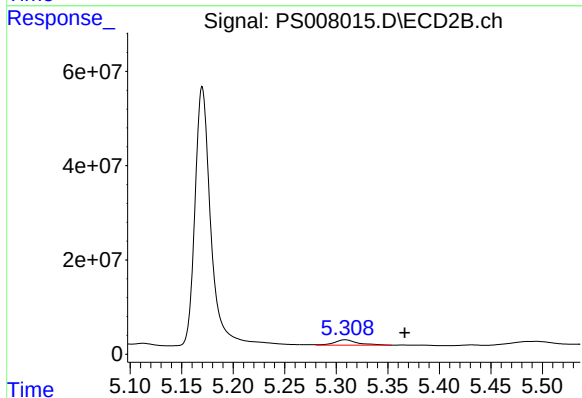


#6 MCPP

R.T.: 5.309 min
Delta R.T.: -0.058 min
Response: 17687110
Conc: 8.53 ug/ml

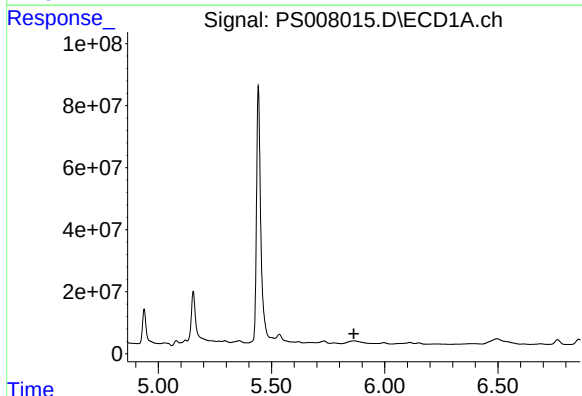


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 5.864 min
Response: 0
Conc: N.D.

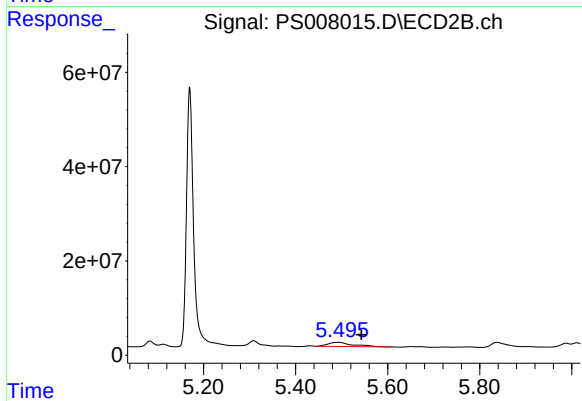

#7 MCPA


R.T.: 5.492 min
Delta R.T.: -0.050 min
Response: 33725344
Conc: 10.58 ug/ml

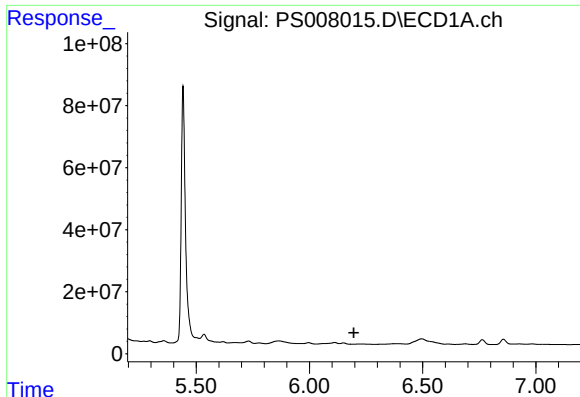

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 6.197 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-02-120619

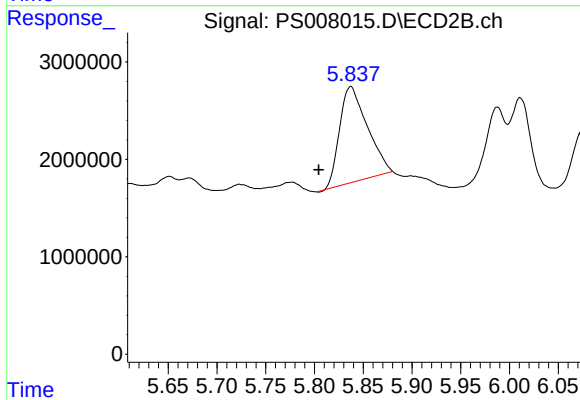


#8 DICHLORPROP

R.T.: 5.837 min
Delta R.T.: 0.033 min
Response: 19524068
Conc: 27.24 ng/ml

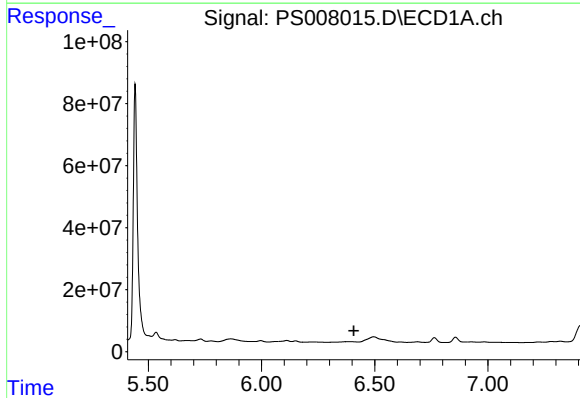


#9 2,4-D

R.T.: 0.000 min
Exp R.T.: 6.408 min
Response: 0
Conc: N.D.

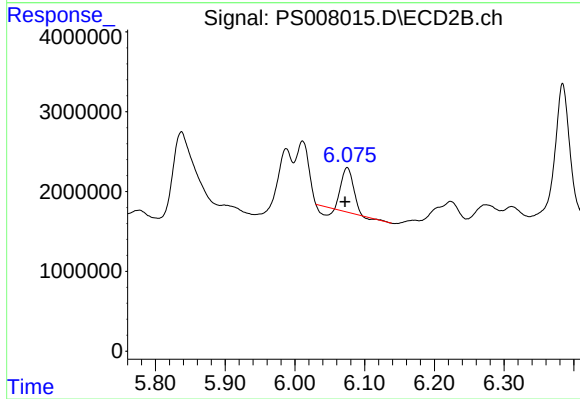

#9 2,4-D


R.T.: 6.075 min
Delta R.T.: 0.003 min
Response: 5632127
Conc: 6.37 ng/ml

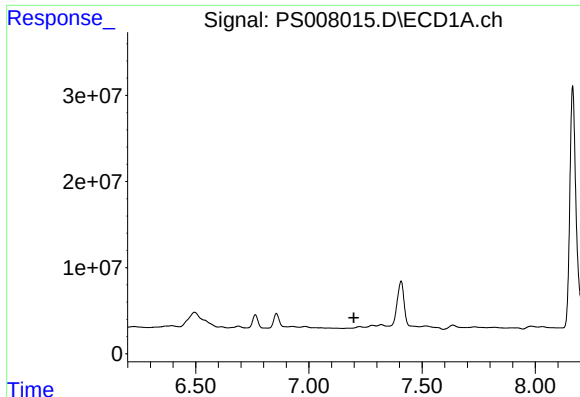

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 7.199 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
SU-02-120619

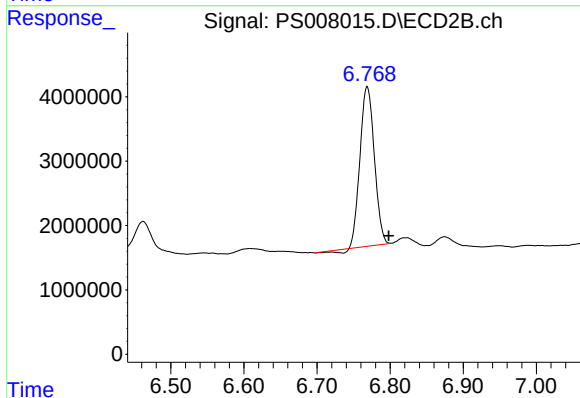


#11 2,4,5-TP (SILVEX)

R.T.: 6.769 min
Delta R.T.: -0.029 min
Response: 33392014
Conc: 7.79 ng/ml

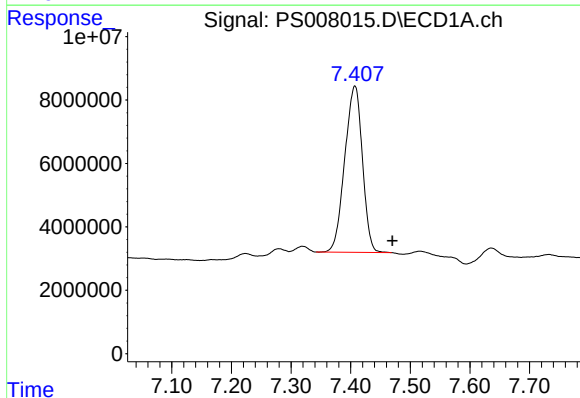

#12 2,4,5-T

R.T.: 7.407 min
Delta R.T.: -0.063 min
Response: 107819089
Conc: 11.65 ng/ml

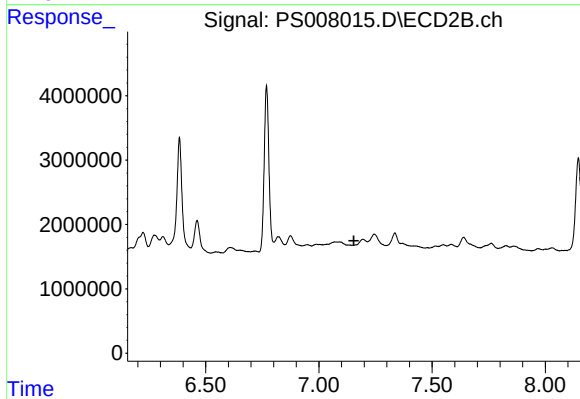

#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 7.155 min
Response: 0
Conc: N.D.