

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121119\
 Data File : PS008023.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2019 13:22
 Operator : SM\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 14:31:55 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 05 04:44:22 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	5.433	5.155	632.8E6	328.0E6	404.499	422.776
Target Compounds							
6) T	MCP	0.000	5.422	0	19253968	N.D.	9.285
9) T	2,4-D	6.462	0.000	155.6E6	0	96.719	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121119\
Data File : PS008023.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2019 13:22
Operator : SM\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 14:31:55 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120419.M
Quant Title : 8080.M
QLast Update : Thu Dec 05 04:44:22 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

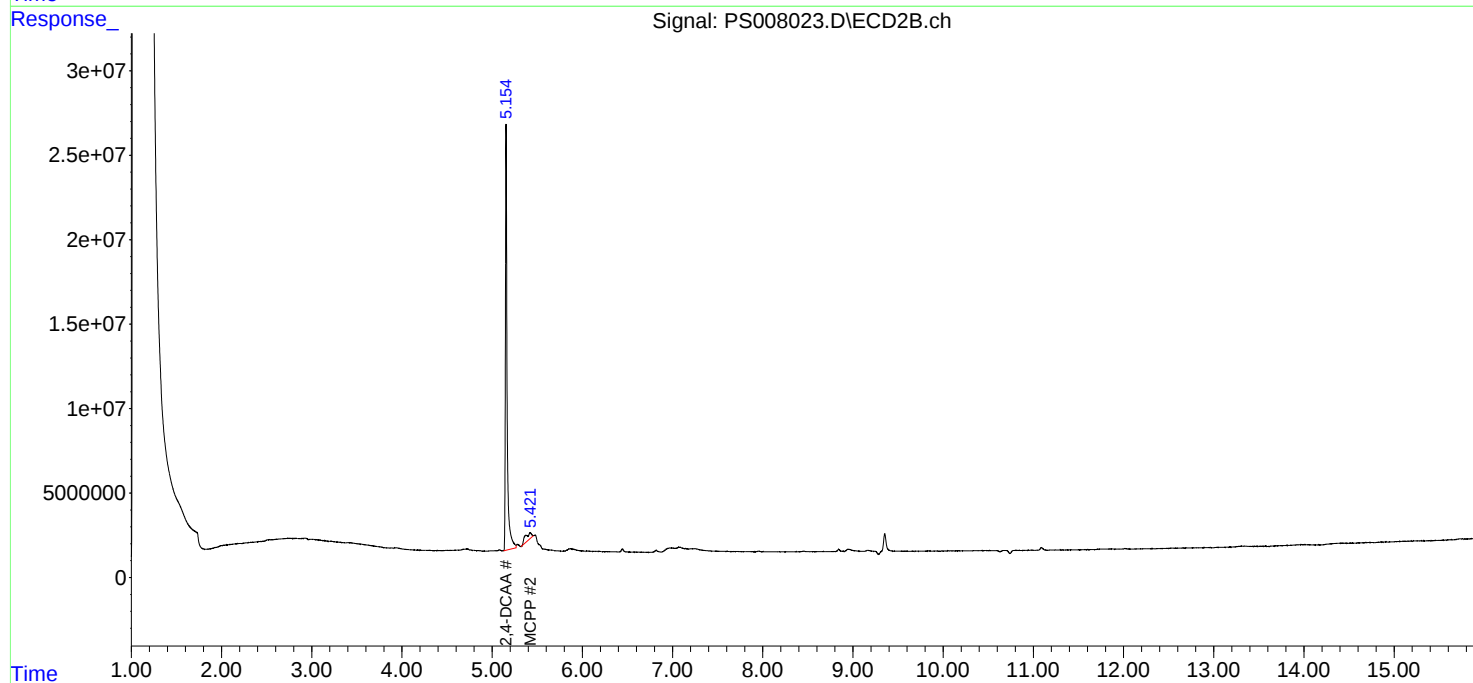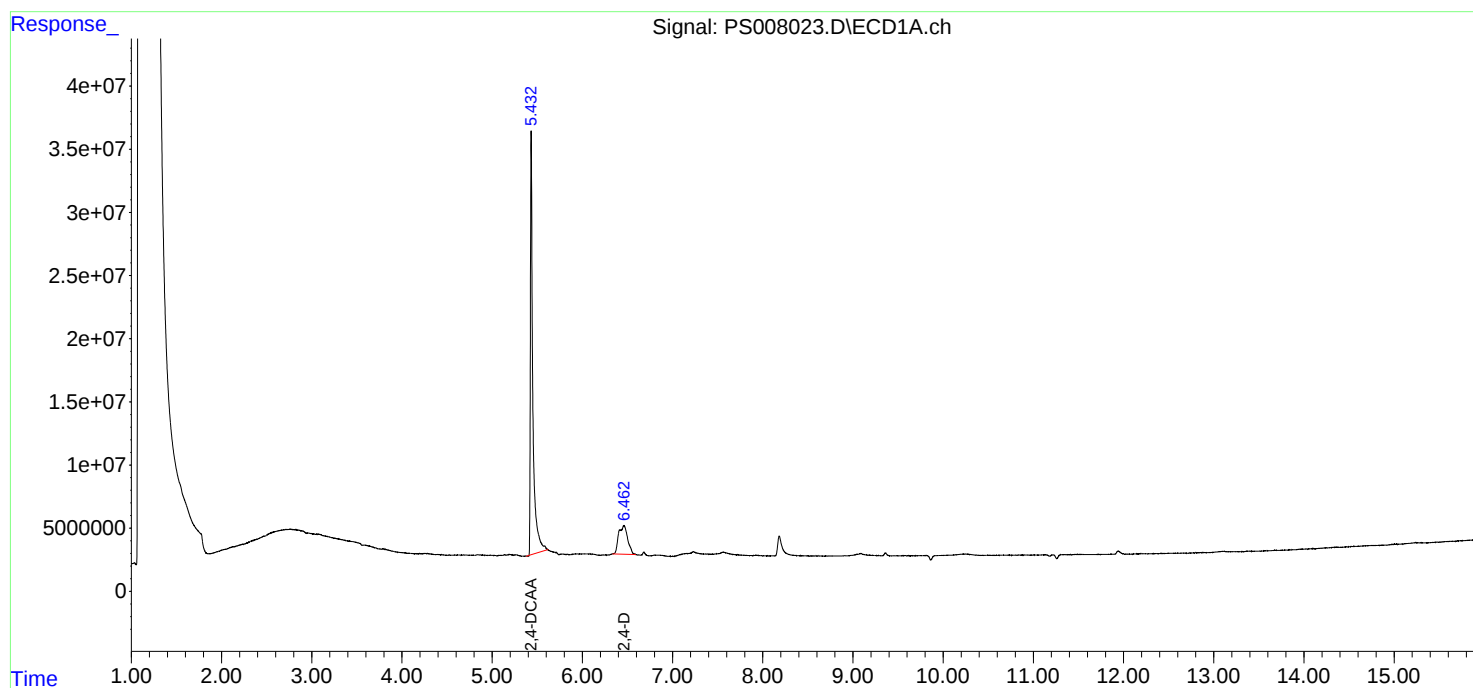


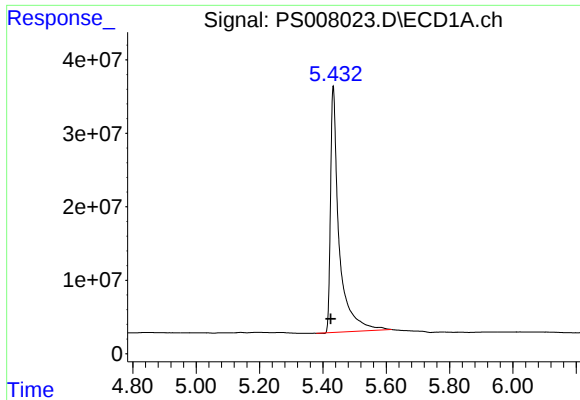

#4 2,4-DCAA


R.T.: 5.433 min
Delta R.T.: 0.008 min
Response: 632771681
Conc: 404.50 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

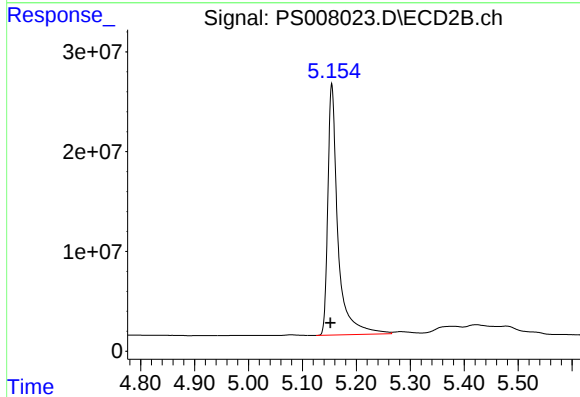


#4 2,4-DCAA

R.T.: 5.155 min
Delta R.T.: 0.003 min
Response: 328039438
Conc: 422.78 ng/ml

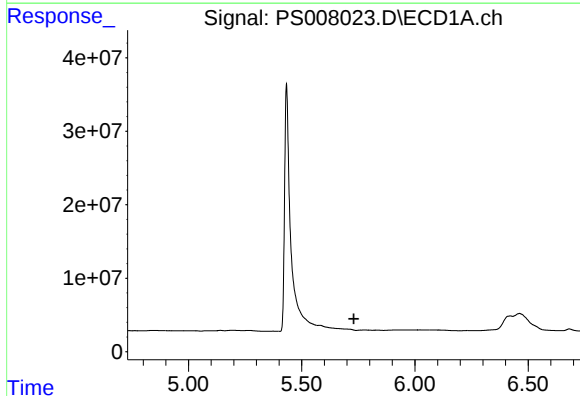


#6 MCP

R.T.: 0.000 min
Exp R.T. : 5.730 min
Response: 0
Conc: N.D.

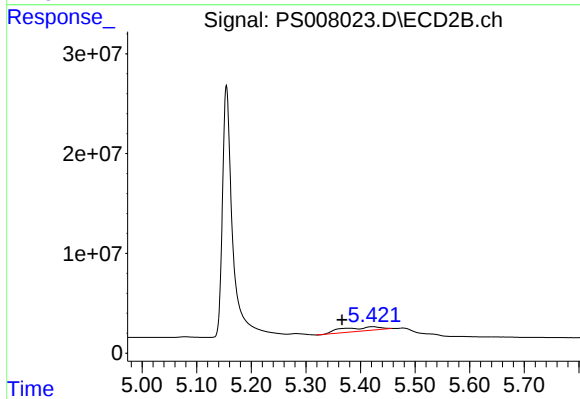

#6 MCP


R.T.: 5.422 min
Delta R.T.: 0.056 min
Response: 19253968
Conc: 9.28 ug/ml

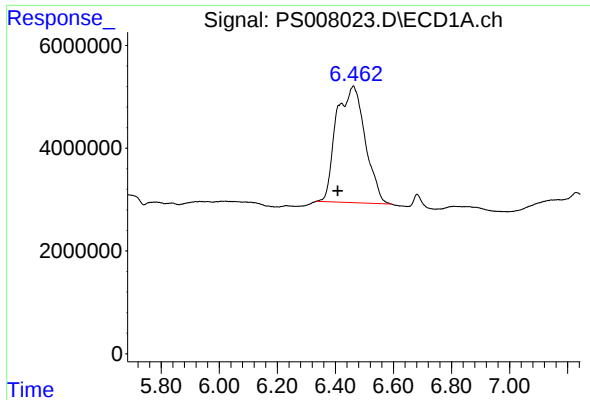

#9 2,4-D

R.T.: 6.462 min
Delta R.T.: 0.054 min
Response: 155601028
Conc: 96.72 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

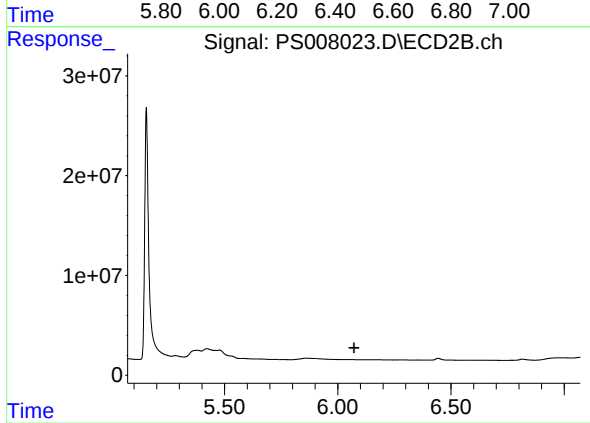

#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 6.072 min
Response: 0
Conc: N.D.