

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121123\
 Data File : PS025045.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2023 10:32
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 16:23:12 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds

1) T	Dalapon	2.511	2.562	10334692	3538770	3.584	3.085
7) T	MCPA	0.000	7.222	0	4285746	N.D.	1.303
8) T	DICHLORPROP	0.000	7.560	0	937863	N.D.	1.192
11) T	2,4,5-TP ...	0.000	8.560f	0	280368	N.D.	<MDL
12) T	2,4,5-T	0.000	9.021f	0	3867923	N.D.	<MDL
15) T	Picloram	9.681	10.761	43790833	11951828	2.247	1.826
16) T	DCPA	0.000	10.761	0	11951828	N.D.	2.205



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121123\
Data File : PS025045.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2023 10:32
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 16:23:12 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

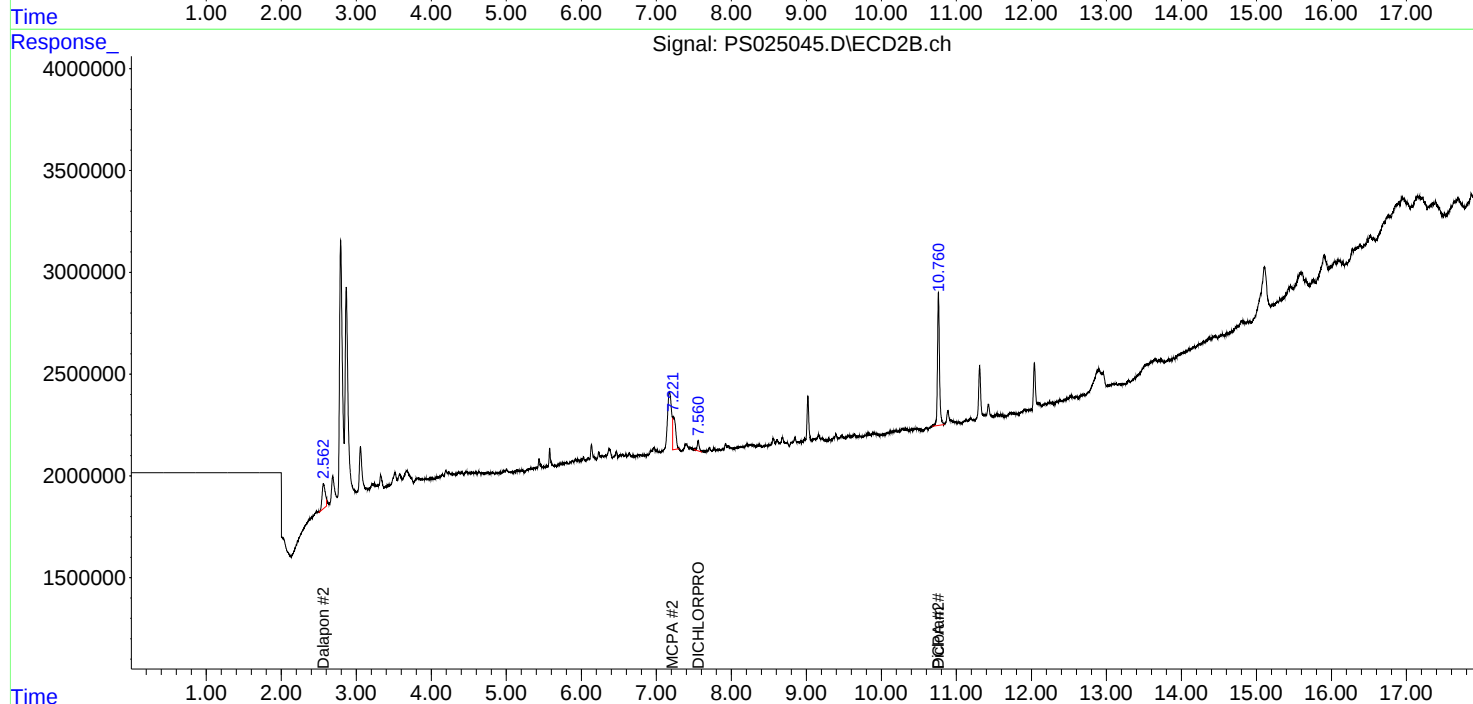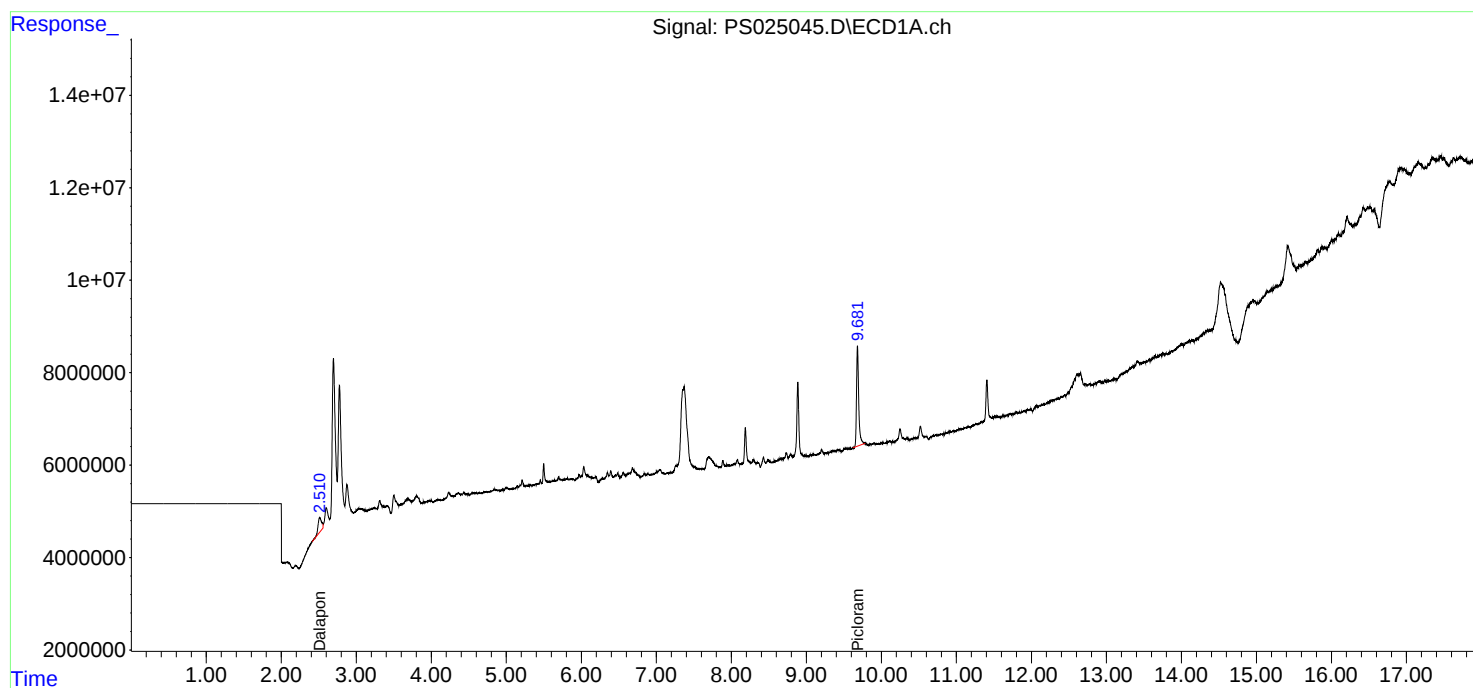


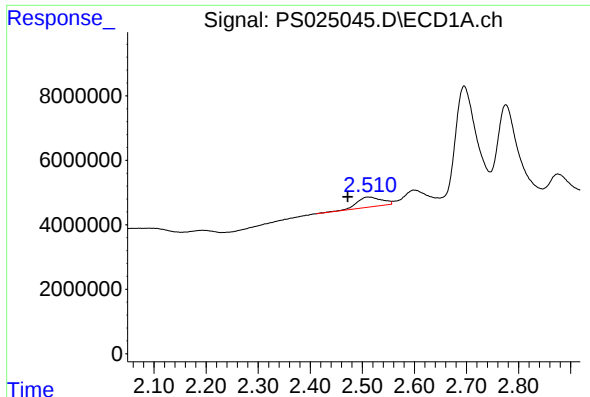

#1 Dalapon


R.T.: 2.511 min
Delta R.T.: 0.039 min
Response: 10334692
Conc: 3.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

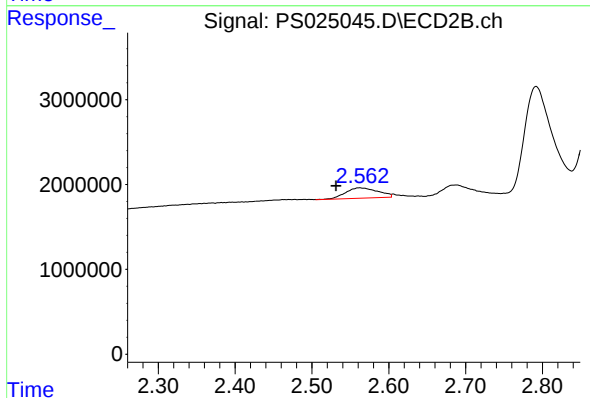


#1 Dalapon

R.T.: 2.562 min
Delta R.T.: 0.031 min
Response: 3538770
Conc: 3.09 ng/ml

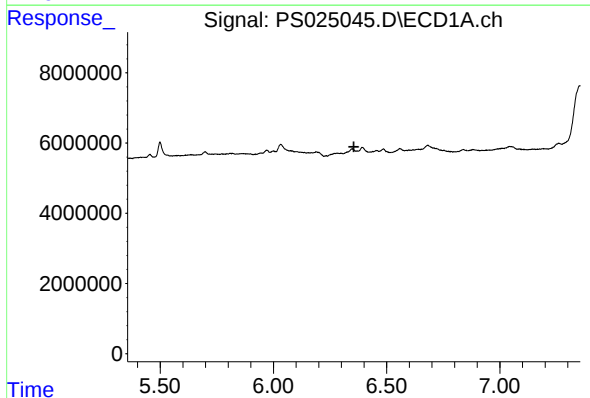


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

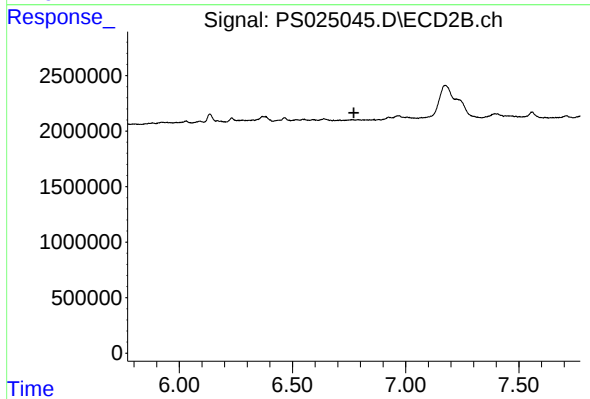

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

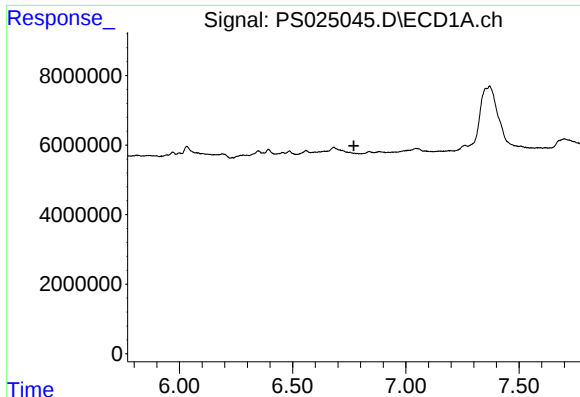

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

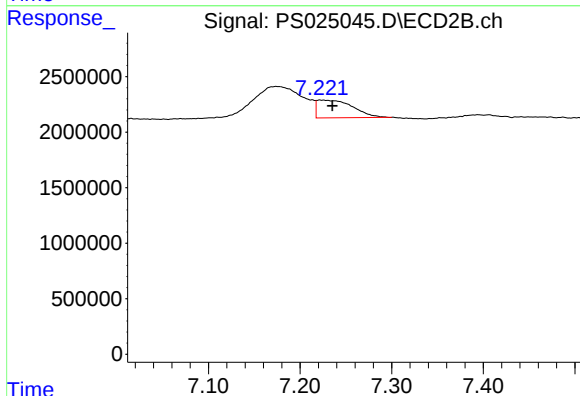


#7 MCPA

R.T.: 7.222 min
Delta R.T.: -0.014 min
Response: 4285746
Conc: 1.30 ug/ml

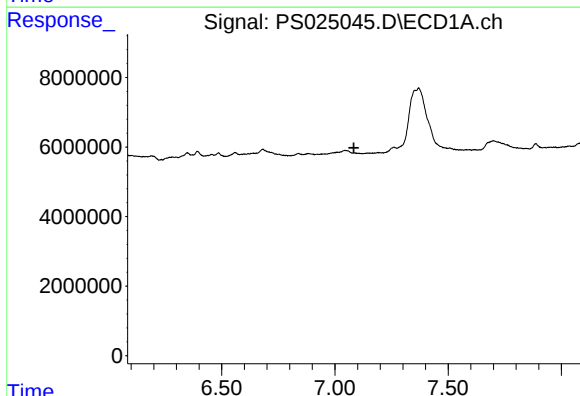


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

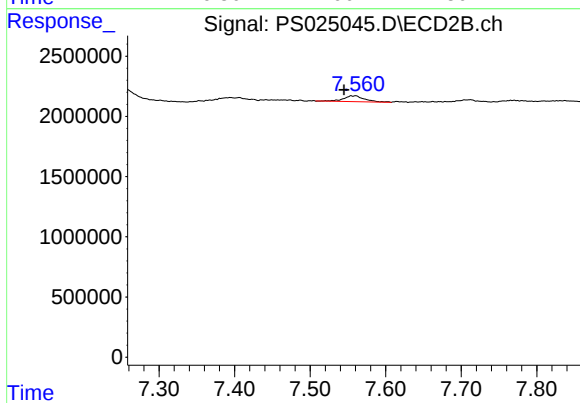

#8 DICHLORPROP


R.T.: 7.560 min
Delta R.T.: 0.015 min
Response: 937863
Conc: 1.19 ng/ml

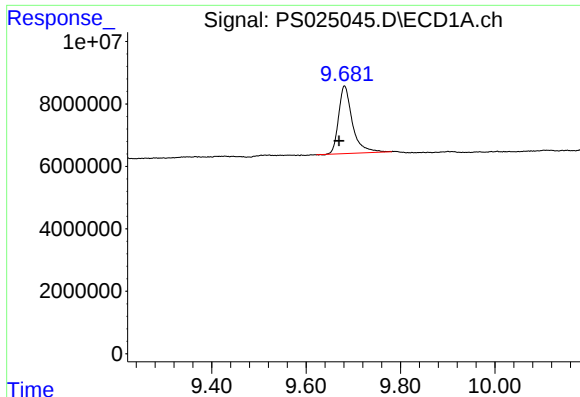

#15 Picloram


R.T.: 9.681 min
Delta R.T.: 0.012 min
Response: 43790833
Conc: 2.25 ng/ml

Instrument :
ECD_S
ClientSampleId :

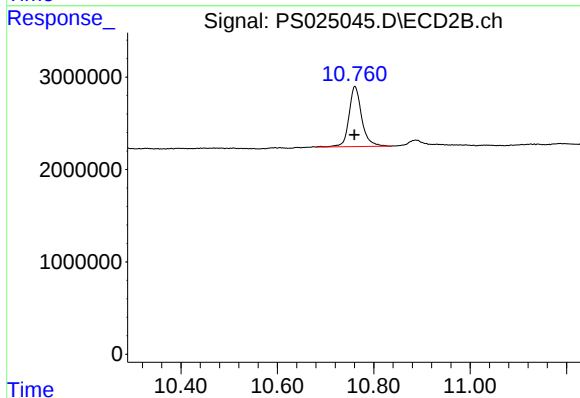


#15 Picloram

R.T.: 10.761 min
Delta R.T.: 0.001 min
Response: 11951828
Conc: 1.83 ng/ml

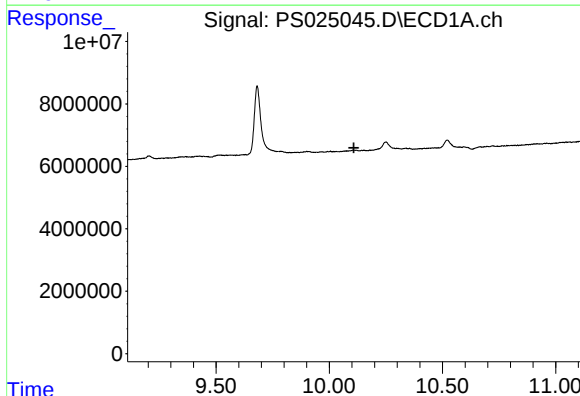

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.109 min
Response: 0
Conc: N.D.

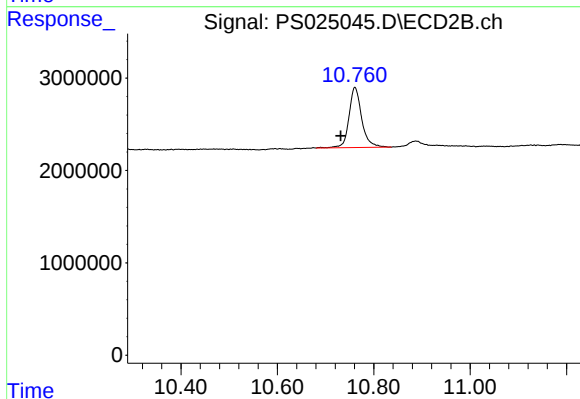

#16 DCPA

R.T.: 10.761 min
Delta R.T.: 0.029 min
Response: 11951828
Conc: 2.21 ng/ml