

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121123\
 Data File : PS025046.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2023 11:04
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 11 16:23:41 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.358	6.770	1197.3E6	376.6E6	535.028	519.712
Target Compounds							
1) T	Dalapon	2.509	2.559	11498820	2062898	3.988	1.798 #
3) T	4-Nitroph...	6.201	0.000	6682286	0	4.538	N.D. #
8) T	DICHLORPROP	0.000	7.532	0	330723	N.D.	<MDL
9) T	2,4-D	7.337f	7.771f	186.6E6	206399	61.440	<MDL #
11) T	2,4,5-TP ...	0.000	8.561f	0	412070	N.D.	<MDL
12) T	2,4,5-T	0.000	9.021f	0	2671311	N.D.	<MDL
15) T	Picloram	9.685	10.762	33667618	9370922	1.728	1.432
16) T	DCPA	0.000	10.762	0	9370922	N.D.	1.729



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121123\
Data File : PS025046.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2023 11:04
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 11 16:23:41 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

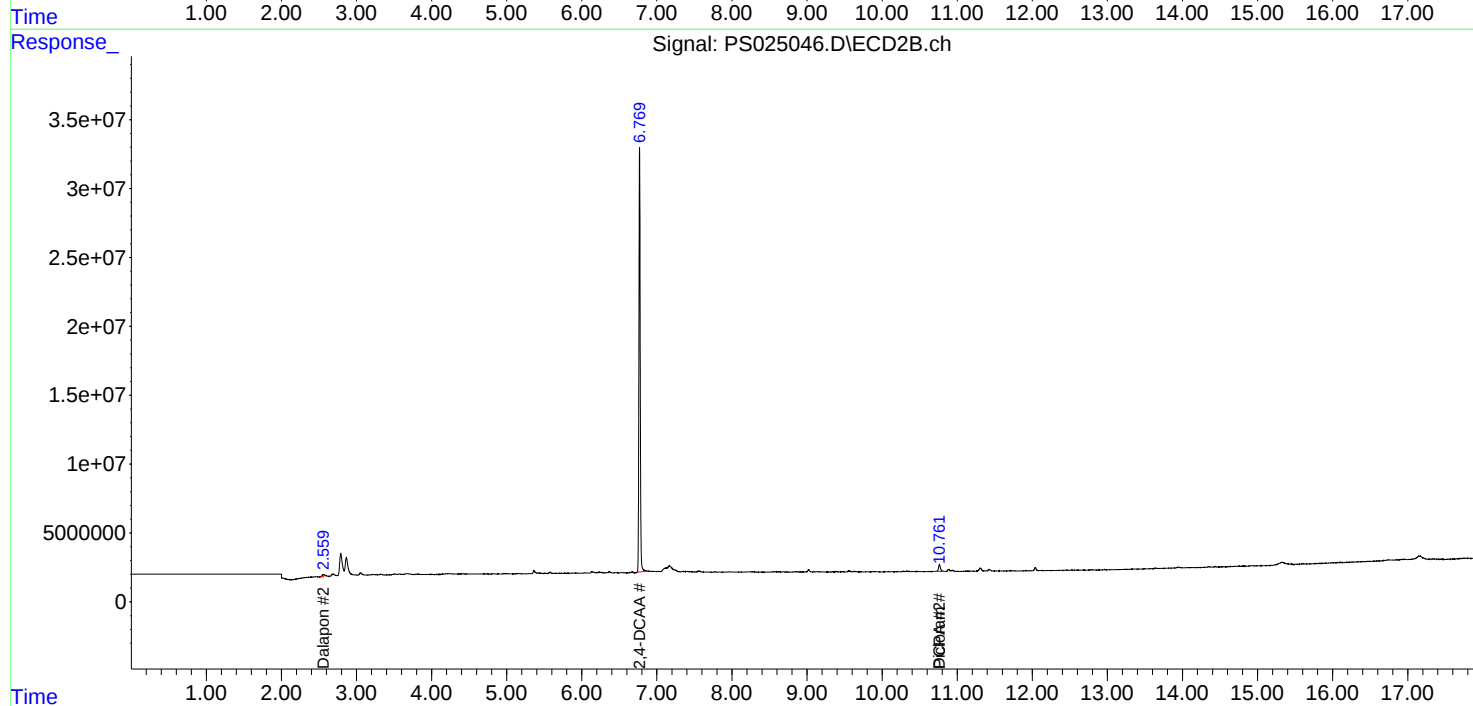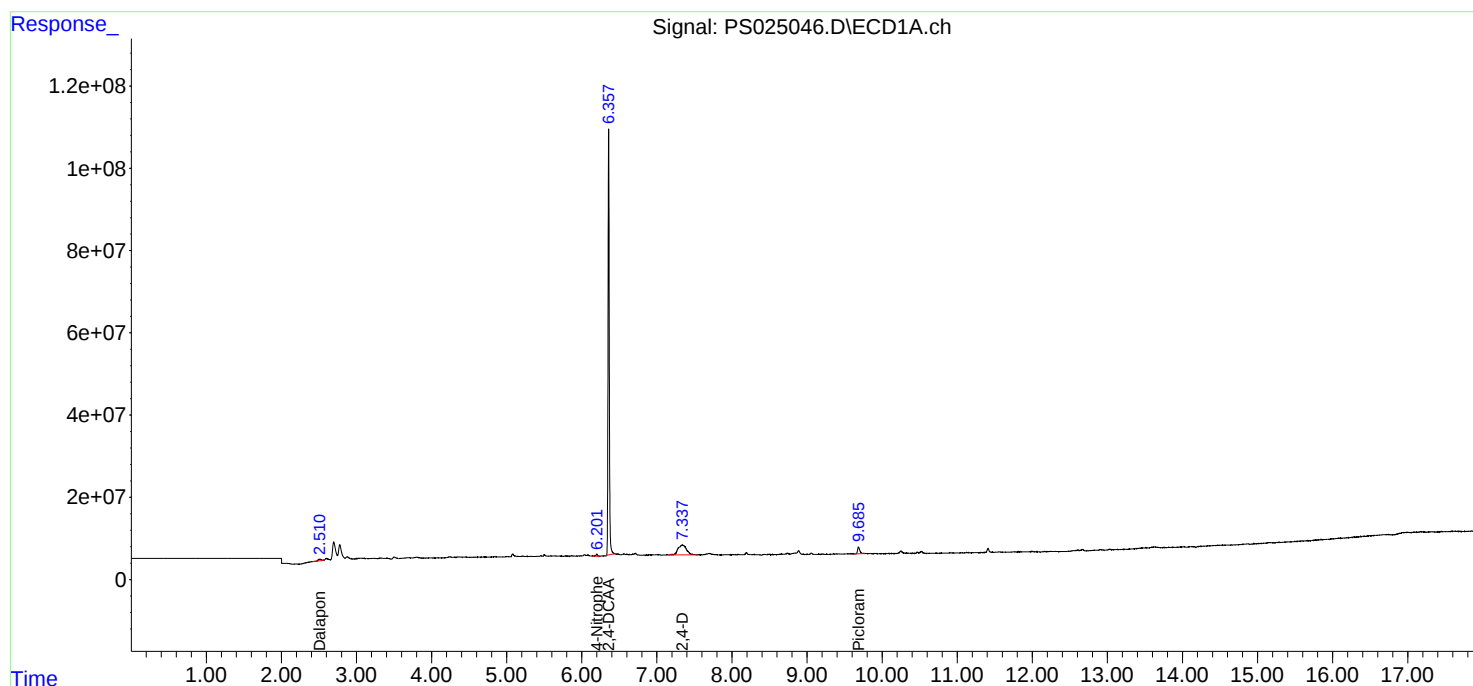


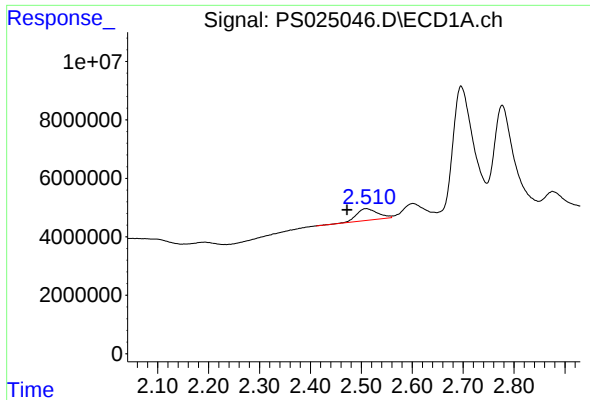

#1 Dalapon


R.T.: 2.509 min
Delta R.T.: 0.037 min
Response: 11498820
Conc: 3.99 ng/ml

Instrument :
ECD_S
ClientSampleId :

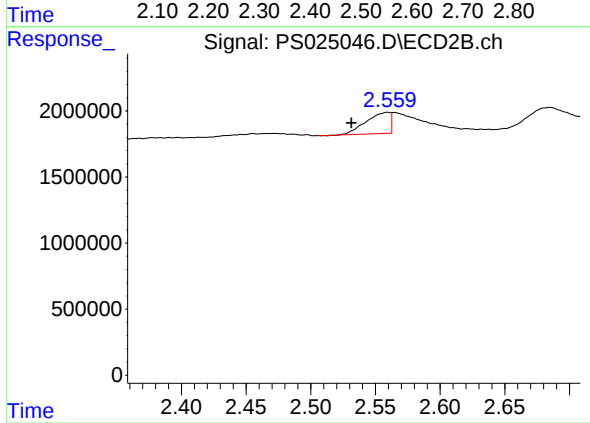


#1 Dalapon

R.T.: 2.559 min
Delta R.T.: 0.028 min
Response: 2062898
Conc: 1.80 ng/ml

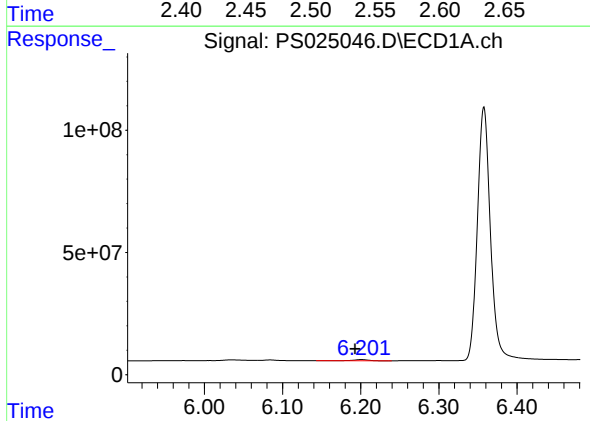


#3 4-Nitrophenol

R.T.: 6.201 min
Delta R.T.: 0.008 min
Response: 6682286
Conc: 4.54 ng/ml

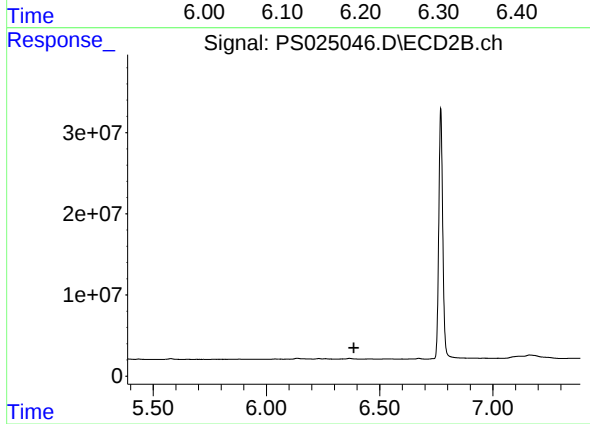

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.386 min
Response: 0
Conc: N.D.

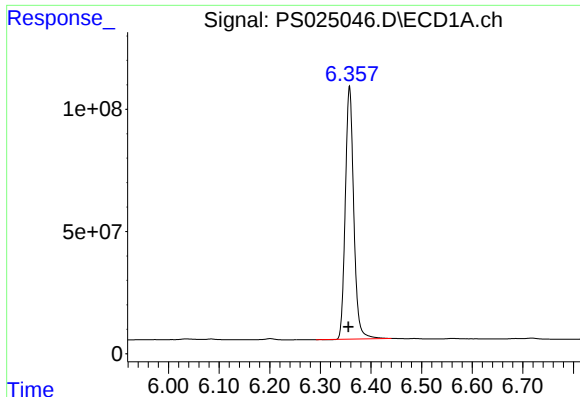

#4 2,4-DCAA


R.T.: 6.358 min
Delta R.T.: 0.002 min
Response: 1197308638
Conc: 535.03 ng/ml

Instrument :
ECD_S
ClientSampleId :

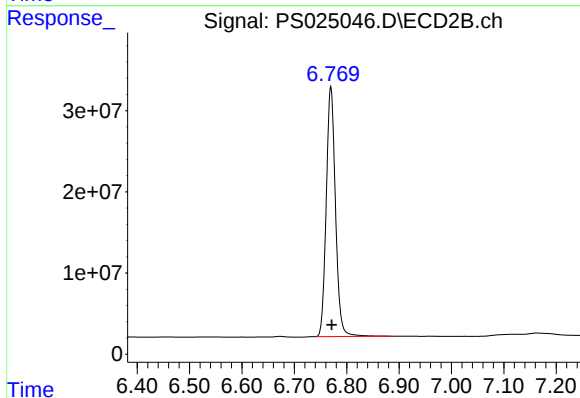


#4 2,4-DCAA

R.T.: 6.770 min
Delta R.T.: -0.001 min
Response: 376559549
Conc: 519.71 ng/ml

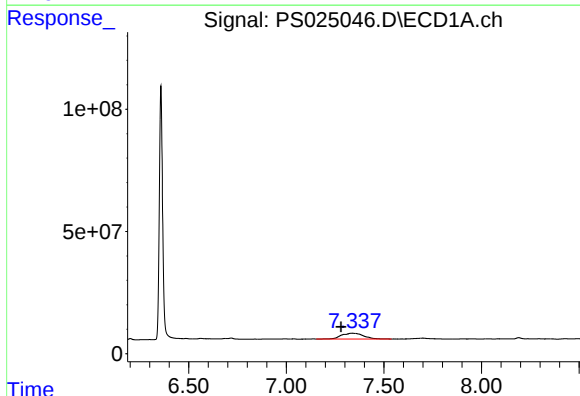


#9 2,4-D

R.T.: 7.337 min
Delta R.T.: 0.056 min
Response: 186615437
Conc: 61.44 ng/ml

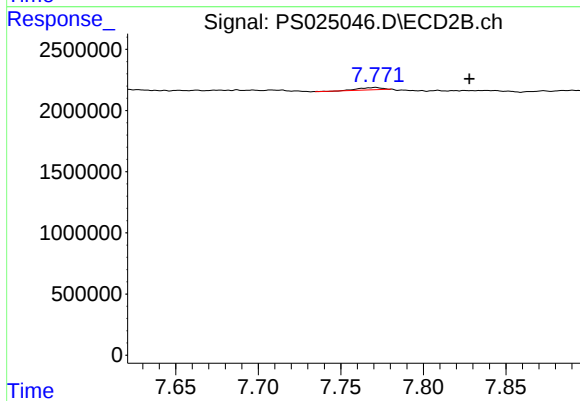

#9 2,4-D


R.T.: 7.771 min
Delta R.T.: -0.057 min
Response: 206399
Conc: N.D.

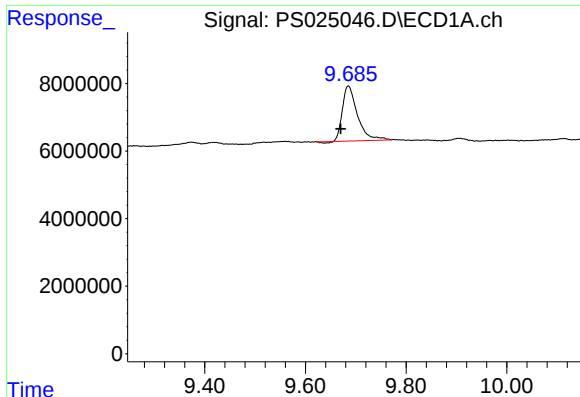

#15 Picloram


R.T.: 9.685 min
Delta R.T.: 0.016 min
Response: 33667618
Conc: 1.73 ng/ml

Instrument :
ECD_S
ClientSampleId :

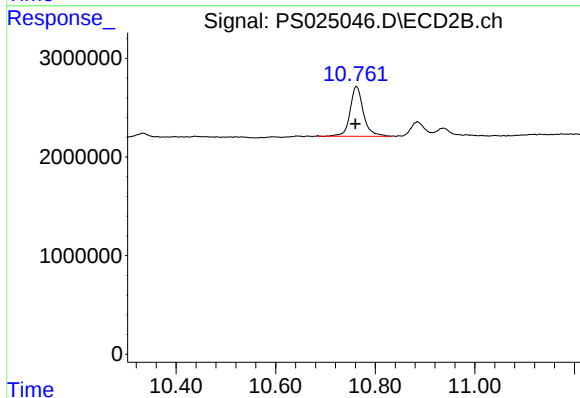


#15 Picloram

R.T.: 10.762 min
Delta R.T.: 0.002 min
Response: 9370922
Conc: 1.43 ng/ml

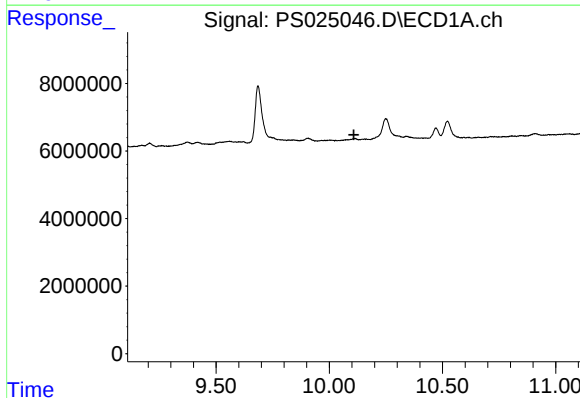

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 10.109 min
Response: 0
Conc: N.D.

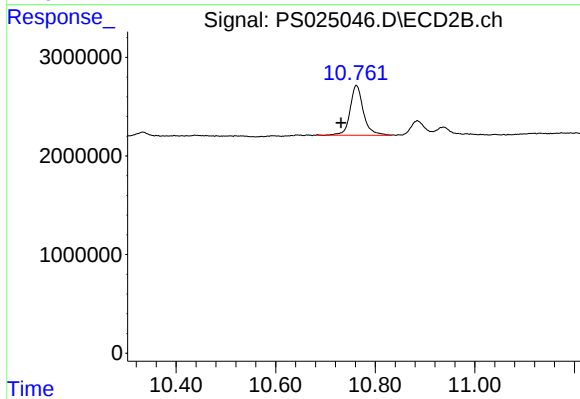

#16 DCPA

R.T.: 10.762 min
Delta R.T.: 0.030 min
Response: 9370922
Conc: 1.73 ng/ml