

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121124\
 Data File : PS028753.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2024 11:00
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 03:37:57 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.274f	0.000	2531985	0	<MDL	N.D. #
Target Compounds							
1) T	Dalapon	2.659f	0.000	3377916	0	1.164	N.D. #
2) T	3,5-DICHL...	6.402	0.000	561547	0	<MDL	N.D. #
3) T	4-Nitroph...	7.011	0.000	4839883	0	2.816	N.D. #
5) T	DICAMBA	7.379f	0.000	717898	0	<MDL	N.D. #
7) T	MCPA	7.755	0.000	405088	0	<MDL	N.D. #
8) T	DICHLORPROP	8.133	0.000	1249022	0	<MDL	N.D. #
9) T	2,4-D	8.337	0.000	1573972	0	<MDL	N.D. #
10) T	Pentachlo...	8.688f	0.000	1046687	0	<MDL	N.D. #
12) T	2,4,5-T	9.475f	10.266f	8194649	4368084	<MDL	<MDL #
13) T	2,4-DB	10.115	0.000	3141647	0	<MDL	N.D. #
14) T	DINOSEB	11.322	0.000	5732246	0	<MDL	N.D. #
15) T	Picloram	11.117	12.321	16888336	10361777	<MDL	<MDL #
16) T	DCPA	11.582	12.256	1795305	2670051	<MDL	<MDL #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121124\
Data File : PS028753.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2024 11:00
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 03:37:57 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

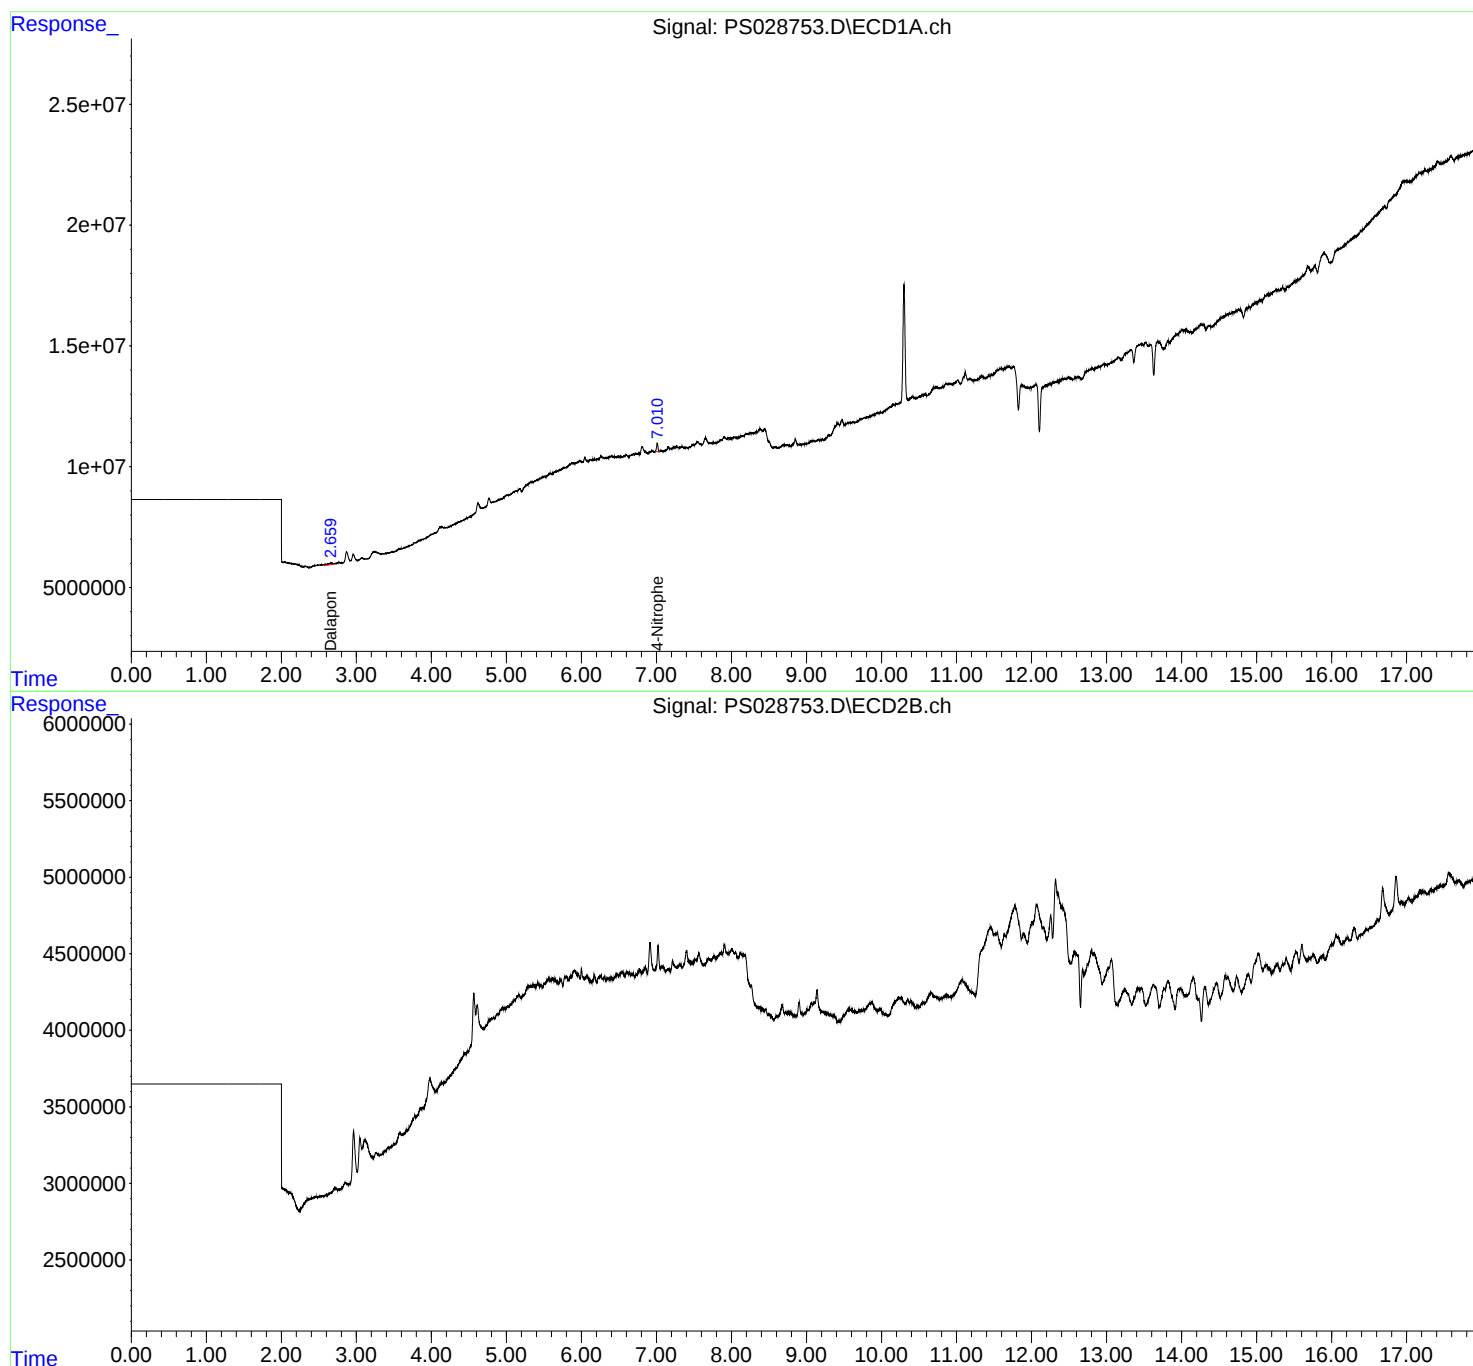


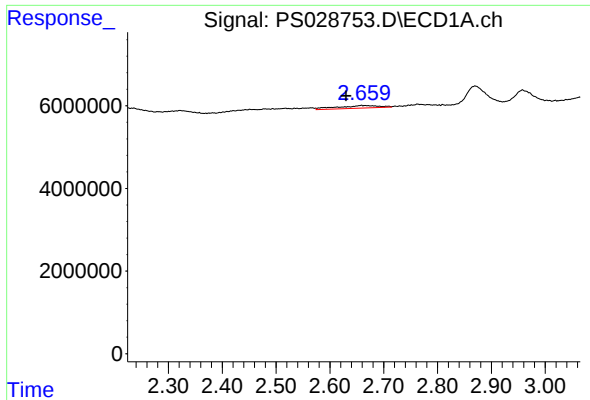

#1 Dalapon


R.T.: 2.659 min
Delta R.T.: 0.029 min
Response: 3377916
Conc: 1.16 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

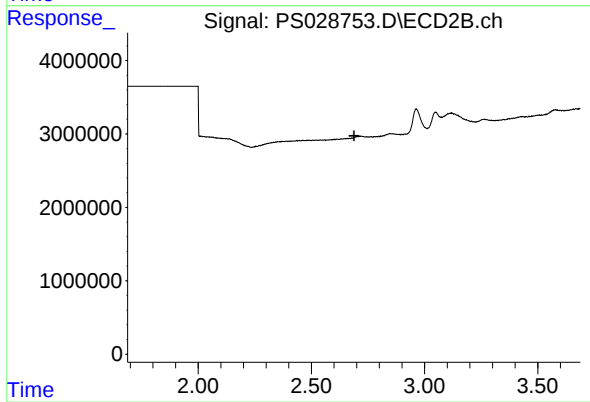


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

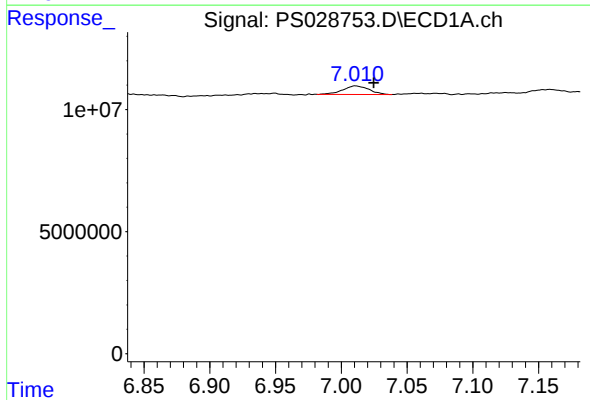


#3 4-Nitrophenol

R.T.: 7.011 min
Delta R.T.: -0.013 min
Response: 4839883
Conc: 2.82 ng/ml

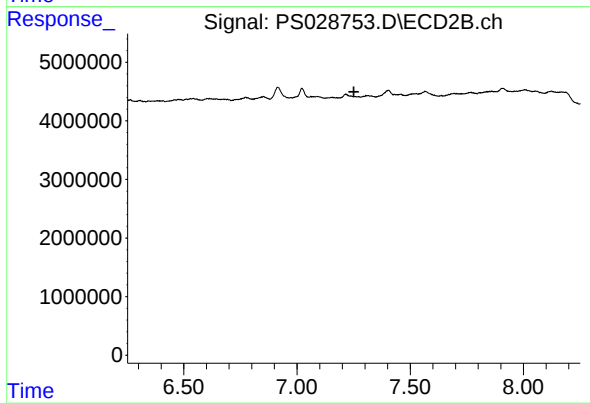

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

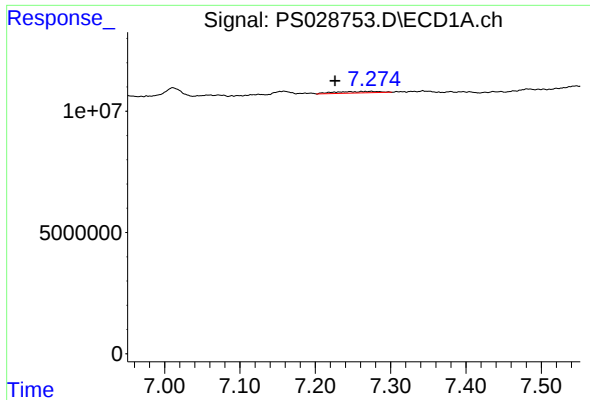

#4 2,4-DCAA

R.T.: 7.274 min
Delta R.T.: 0.048 min
Response: 2531985
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

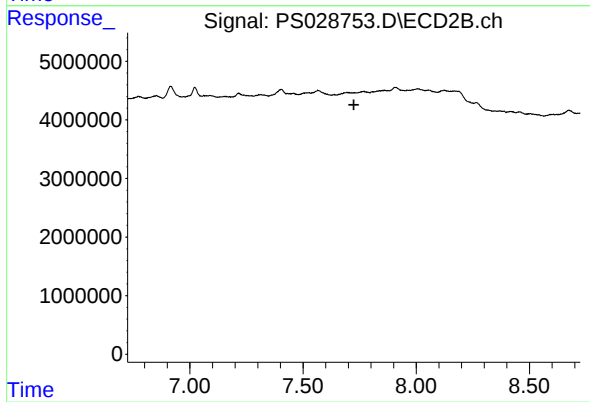

#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 7.725 min
Response: 0
Conc: N.D.