

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121124\
 Data File : PS028760.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2024 18:38
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 03:40:17 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.226	7.719	1374.1E6	592.0E6	512.275	439.466
Target Compounds							
1) T	Dalapon	2.671f	2.717f	19790215	19831289	6.820	9.081 #
3) T	4-Nitroph...	7.022	0.000	4721306	0	2.747	N.D. #
5) T	DICAMBA	7.410	7.916	22362	8807699	<MDL	1.431 #
6) T	MCP	0.000	8.022	0	5138001	N.D.	1.193
8) T	DICHLORPROP	0.000	8.682f	0	4125772	N.D.	2.581
10) T	Pentachlo...	8.650	0.000	934661	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.224	0.000	467321	0	<MDL	N.D. #
12) T	2,4,5-T	9.516	10.287	2386562	3126863	<MDL	<MDL #
14) T	DINOSEB	11.294	0.000	9052538	0	<MDL	N.D. #
15) T	Picloram	11.118	12.327	43790702	9893010	1.473	<MDL #
16) T	DCPA	11.592	12.327f	2837251	9893010	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121124\
Data File : PS028760.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2024 18:38
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 03:40:17 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

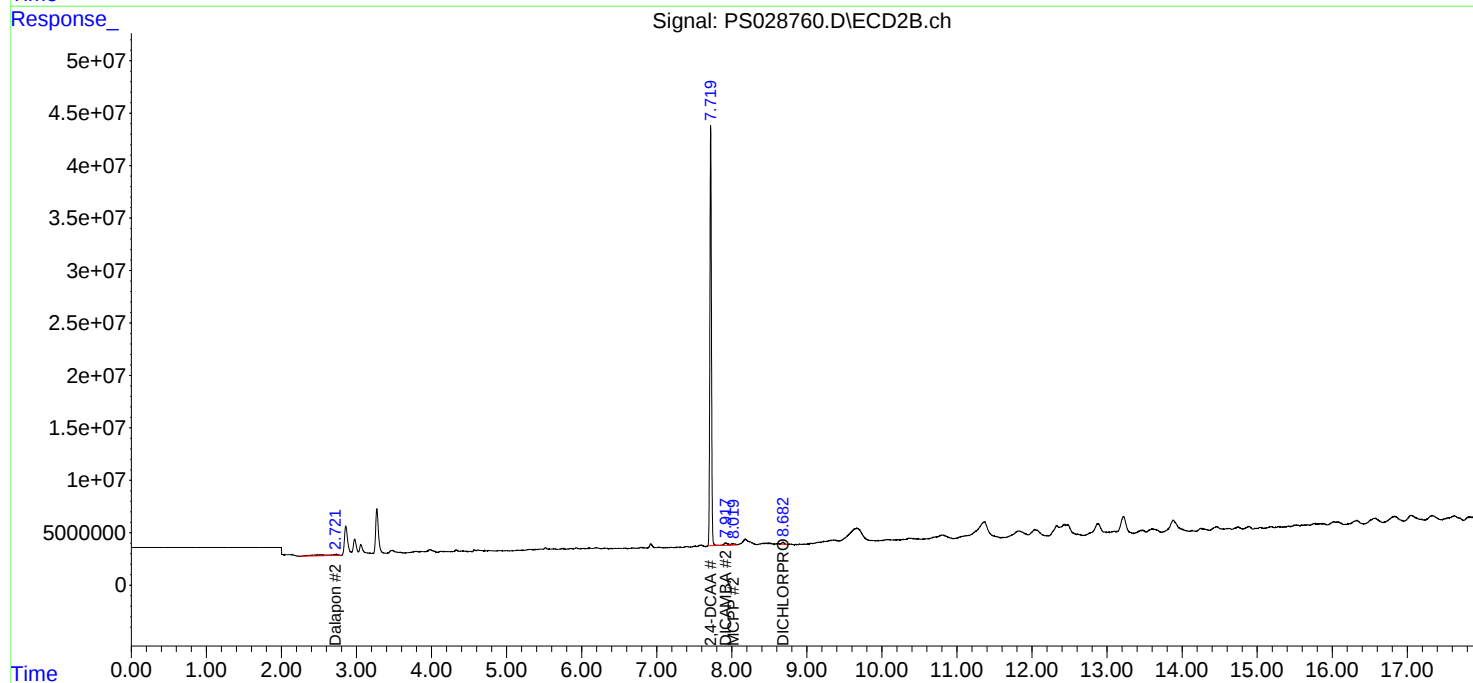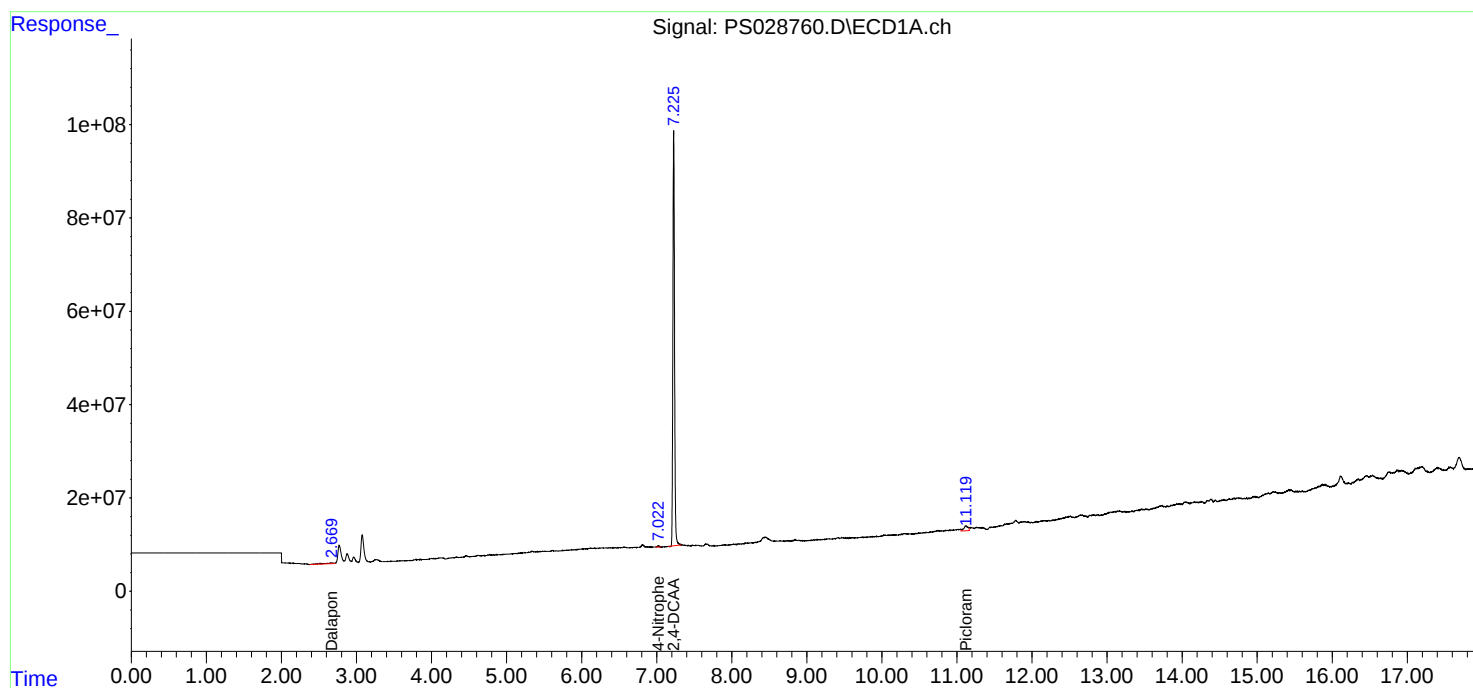


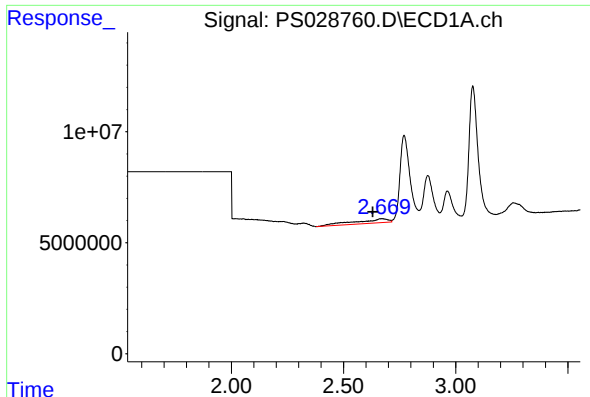

#1 Dalapon


R.T.: 2.671 min
Delta R.T.: 0.041 min
Response: 19790215
Conc: 6.82 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

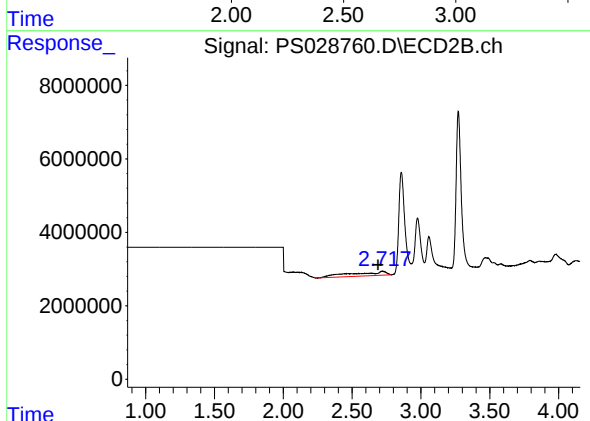


#1 Dalapon

R.T.: 2.717 min
Delta R.T.: 0.029 min
Response: 19831289
Conc: 9.08 ng/ml

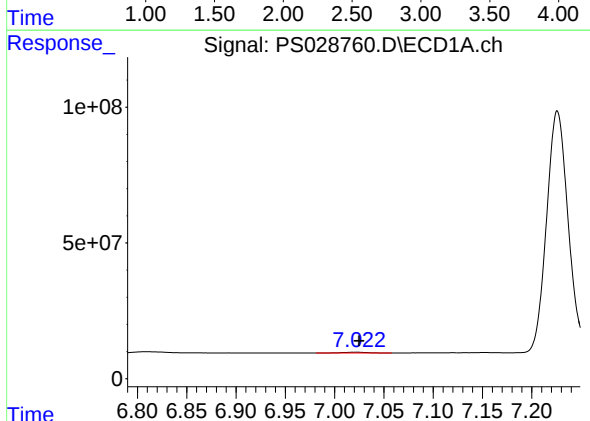


#3 4-Nitrophenol

R.T.: 7.022 min
Delta R.T.: -0.003 min
Response: 4721306
Conc: 2.75 ng/ml

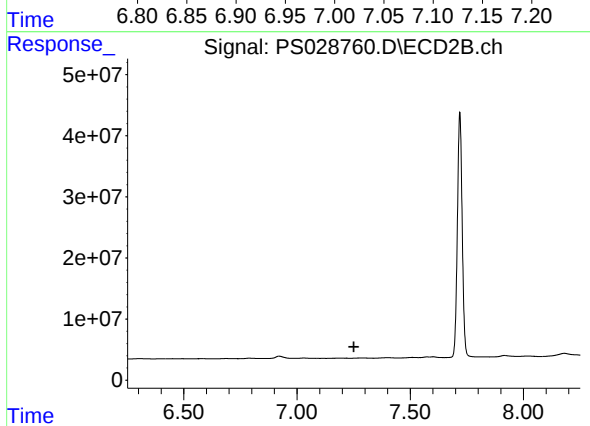

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

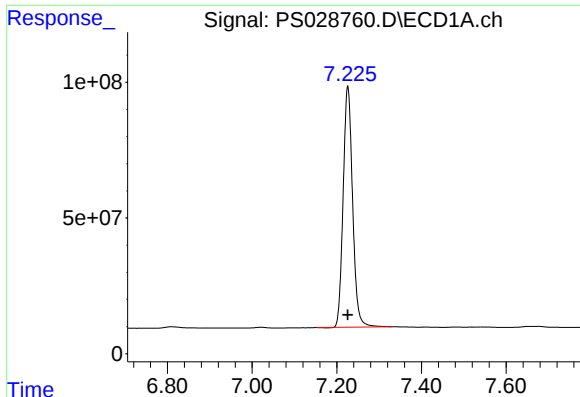

#4 2,4-DCAA


R.T.: 7.226 min
Delta R.T.: 0.000 min
Response: 1374096404
Conc: 512.27 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

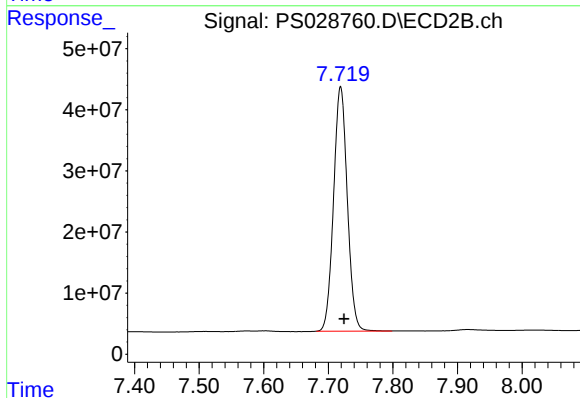


#4 2,4-DCAA

R.T.: 7.719 min
Delta R.T.: -0.006 min
Response: 591973415
Conc: 439.47 ng/ml

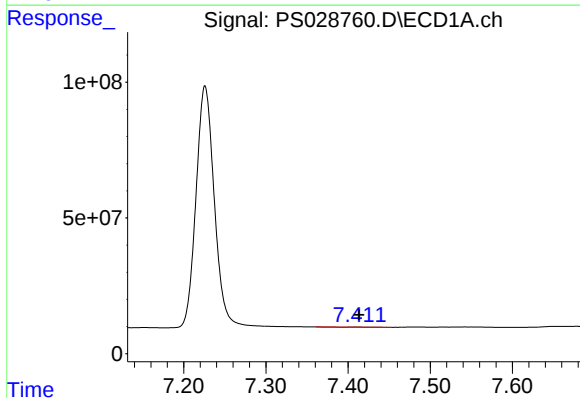


#5 DICAMBA

R.T.: 7.410 min
Delta R.T.: -0.003 min
Response: 22362
Conc: N.D.

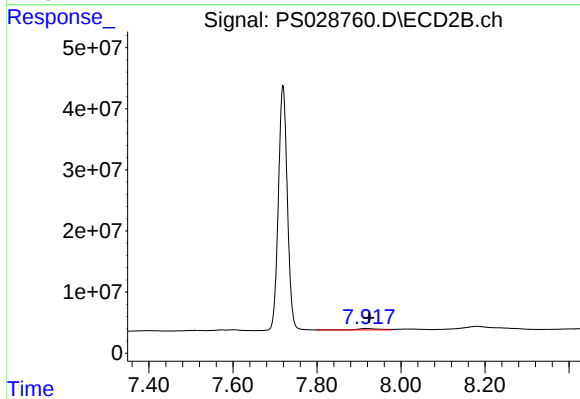

#5 DICAMBA


R.T.: 7.916 min
Delta R.T.: -0.008 min
Response: 8807699
Conc: 1.43 ng/ml

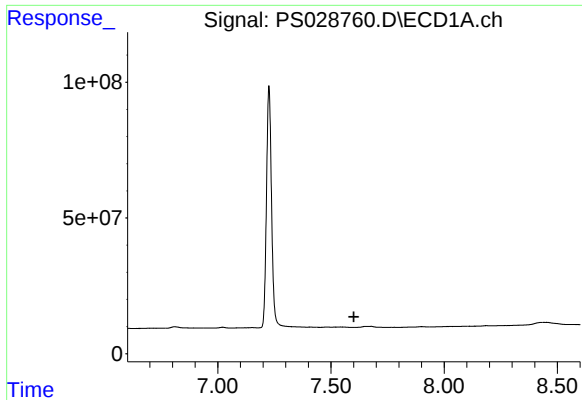

#6 MCP


R.T.: 0.000 min
Exp R.T.: 7.601 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

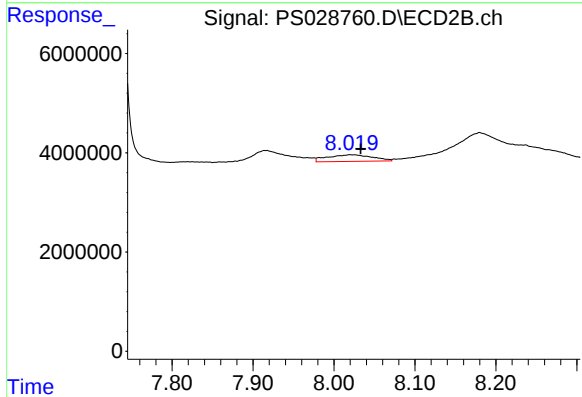


#6 MCP

R.T.: 8.022 min
Delta R.T.: -0.011 min
Response: 5138001
Conc: 1.19 ug/ml

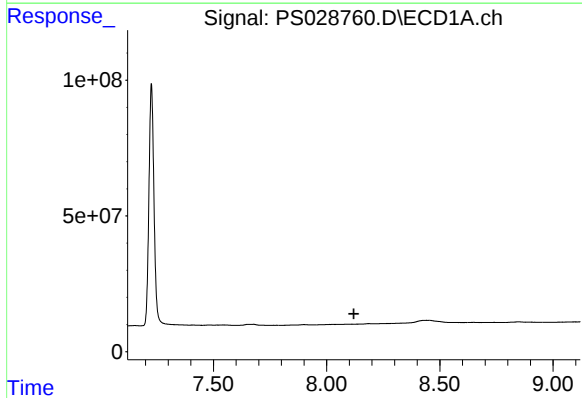


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 8.121 min
Response: 0
Conc: N.D.

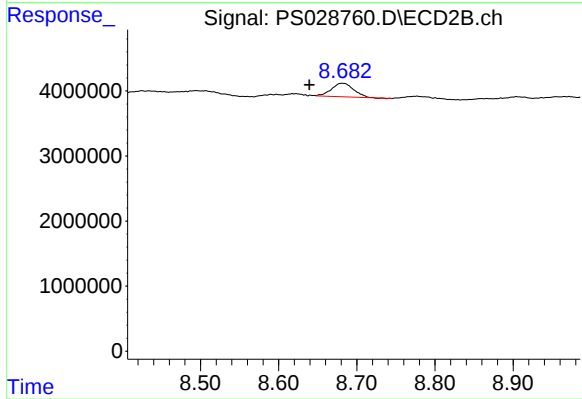

#8 DICHLORPROP


R.T.: 8.682 min
Delta R.T.: 0.042 min
Response: 4125772
Conc: 2.58 ng/ml

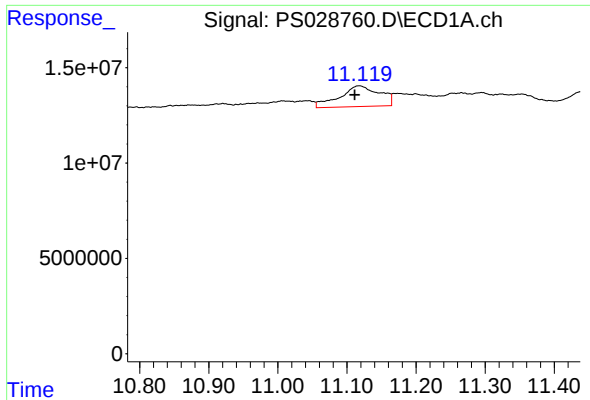

#15 Picloram

R.T.: 11.118 min
Delta R.T.: 0.006 min
Response: 43790702
Conc: 1.47 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

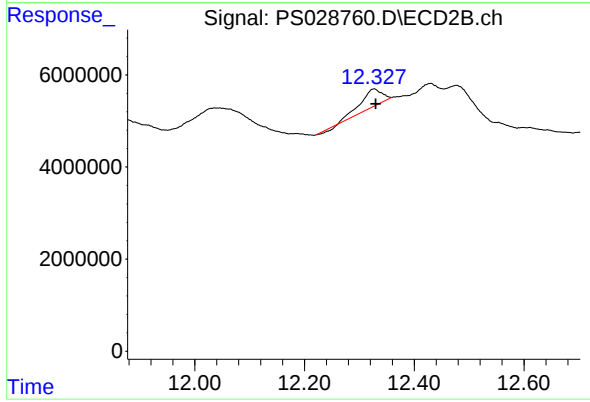

#15 Picloram

R.T.: 12.327 min
Delta R.T.: -0.003 min
Response: 9893010
Conc: N.D.