

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
 Data File : PS032686.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2025 18:30
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 00:28:36 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 11 01:33:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.313	7.983	2290.6E6	1071.0E6	320.988	382.463
Target Compounds							
1) T	Dalapon	2.685	2.815	417.6E6	1593919	38.957	<MDL #
2) T	3,5-DICHL...	6.457	0.000	3220946	0	<MDL	N.D. #
5) T	DICAMBA	7.506	8.190	3554234	7169350	<MDL	<MDL #
6) T	MCP	0.000	8.270f	0	1673427	N.D.	<MDL
7) T	MCPA	0.000	8.573	0	4329480	N.D.	<MDL
10) T	Pentachlo...	8.777	0.000	34167309	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.356	10.161f	8529884	6284576	<MDL	<MDL #
12) T	2,4,5-T	0.000	10.607	0	28787743	N.D.	1.632
13) T	2,4-DB	10.282f	11.149f	17965582	14722963	2.840	5.989 #
14) T	DINOSEB	11.448	0.000	287.0E6	0	10.578	N.D. #
15) T	Picloram	11.269	0.000	49443931	0	1.035	N.D. #
16) T	DCPA	0.000	12.641	0	714.2E6	N.D.	34.522



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
Data File : PS032686.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2025 18:30
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 00:28:36 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

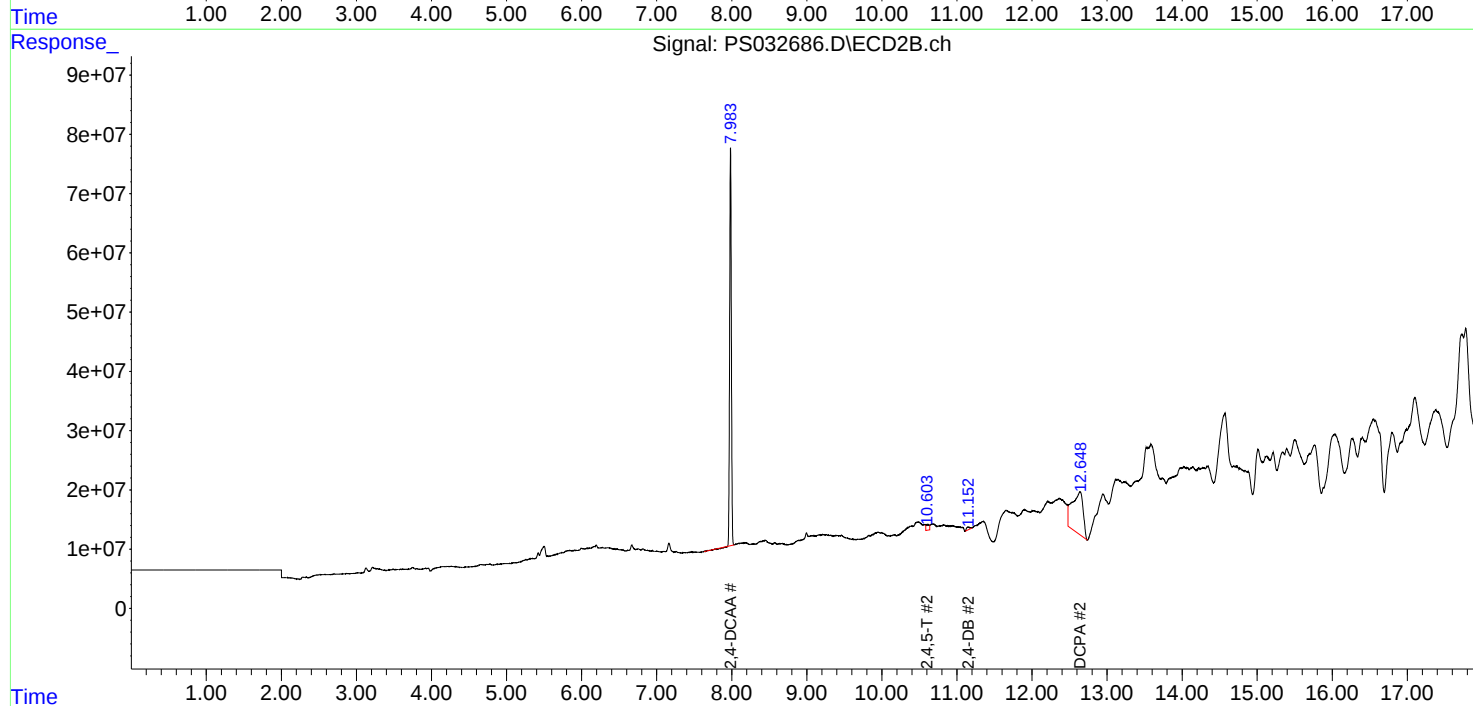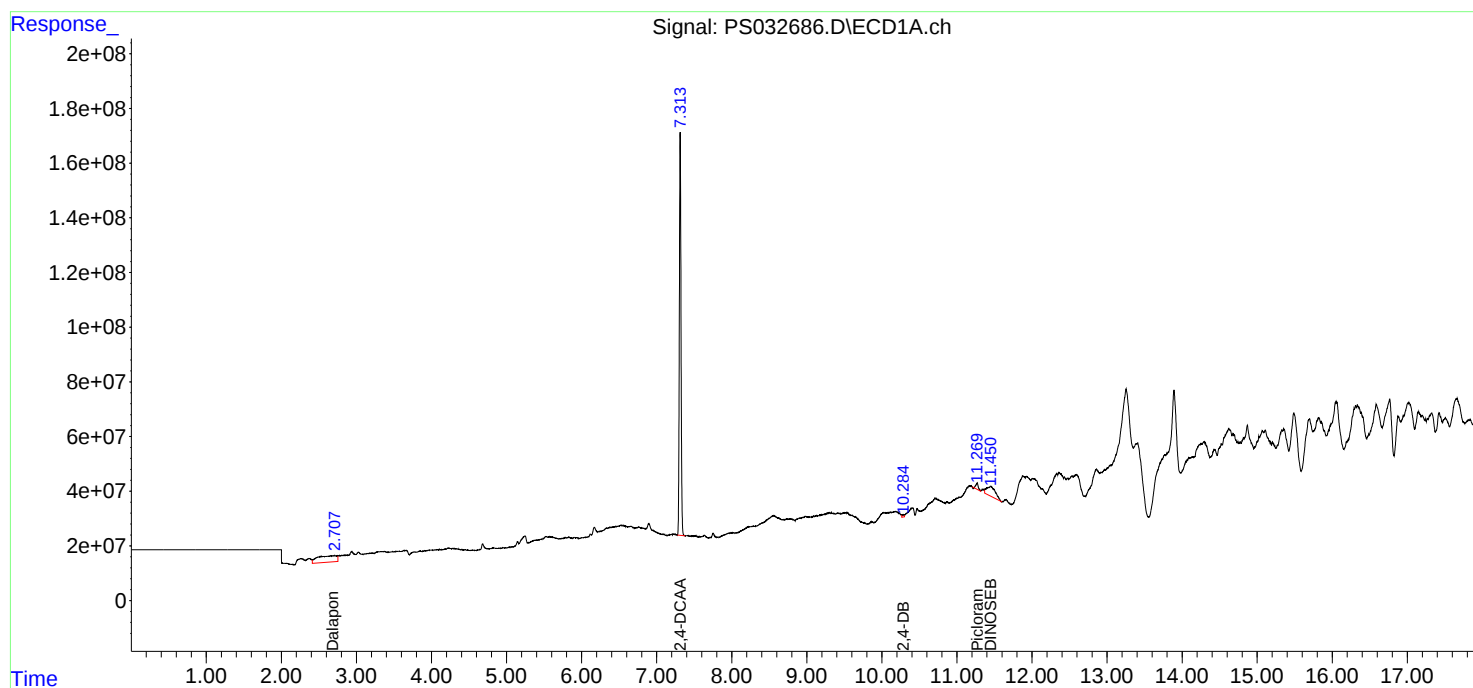


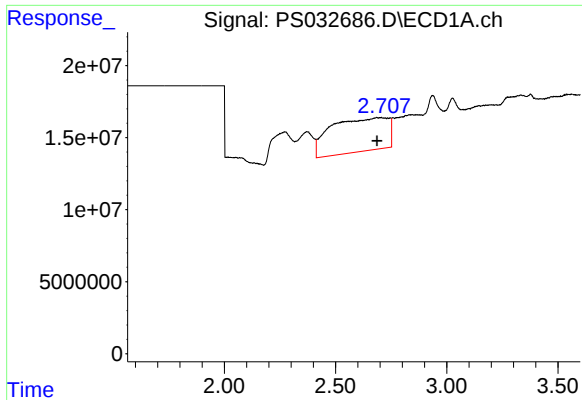

#1 Dalapon


R.T.: 2.685 min
Delta R.T.: -0.002 min
Response: 417598671
Conc: 38.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

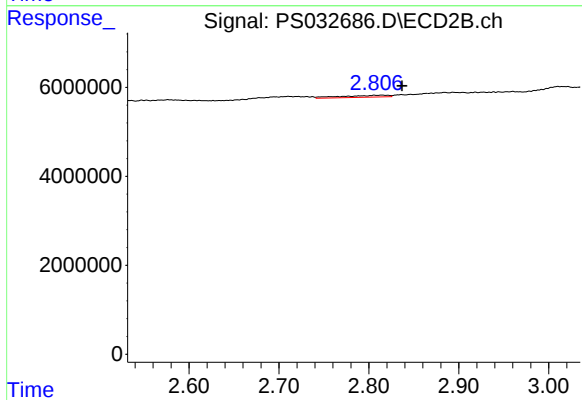


#1 Dalapon

R.T.: 2.815 min
Delta R.T.: -0.022 min
Response: 1593919
Conc: N.D.

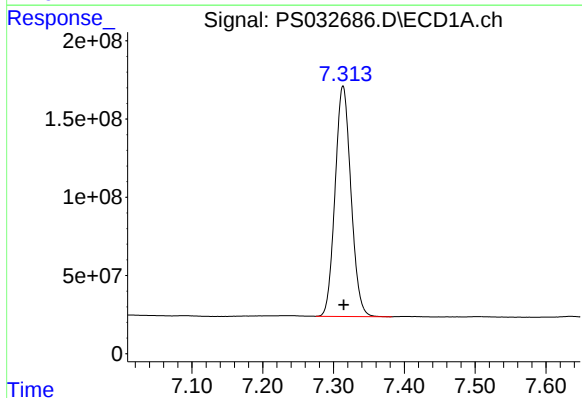


#4 2,4-DCAA

R.T.: 7.313 min
Delta R.T.: 0.000 min
Response: 2290550872
Conc: 320.99 ng/ml

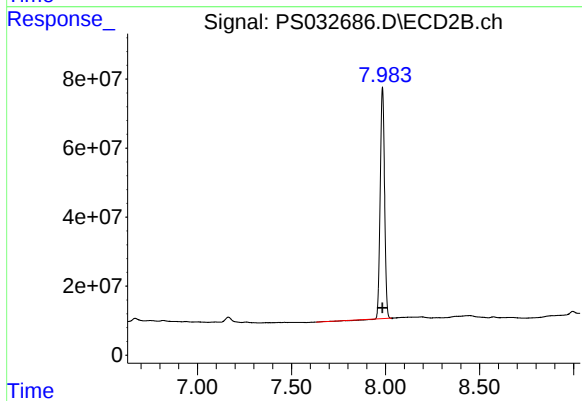

#4 2,4-DCAA


R.T.: 7.983 min
Delta R.T.: 0.000 min
Response: 1071021177
Conc: 382.46 ng/ml

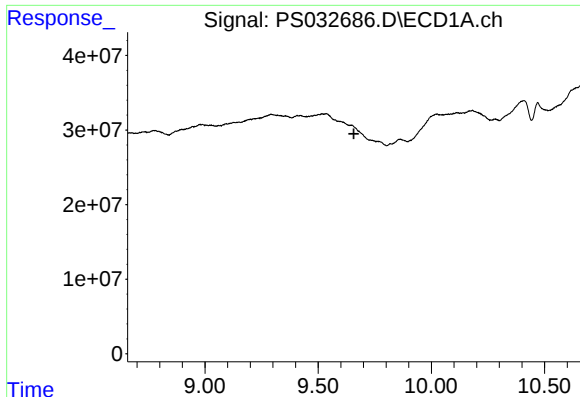

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 9.658 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

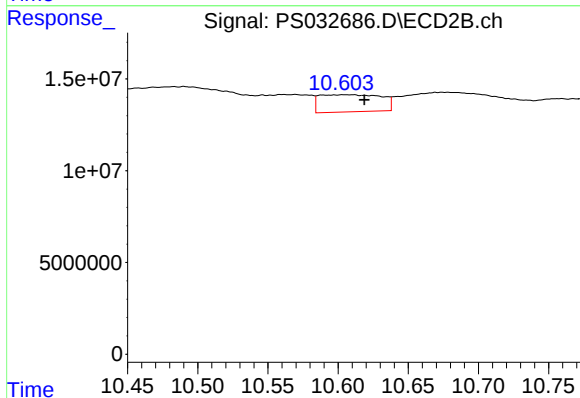


#12 2,4,5-T

R.T.: 10.607 min
Delta R.T.: -0.012 min
Response: 28787743
Conc: 1.63 ng/ml

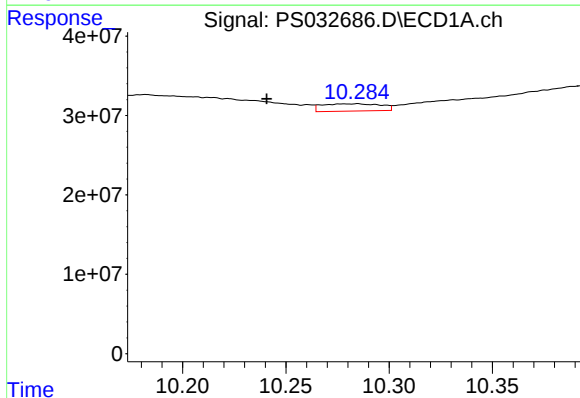


#13 2,4-DB

R.T.: 10.282 min
Delta R.T.: 0.041 min
Response: 17965582
Conc: 2.84 ng/ml

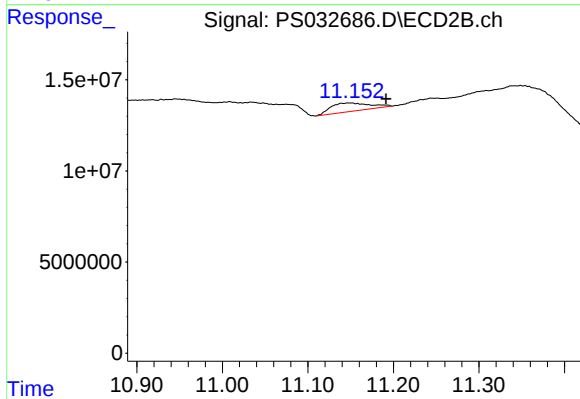

#13 2,4-DB


R.T.: 11.149 min
Delta R.T.: -0.042 min
Response: 14722963
Conc: 5.99 ng/ml

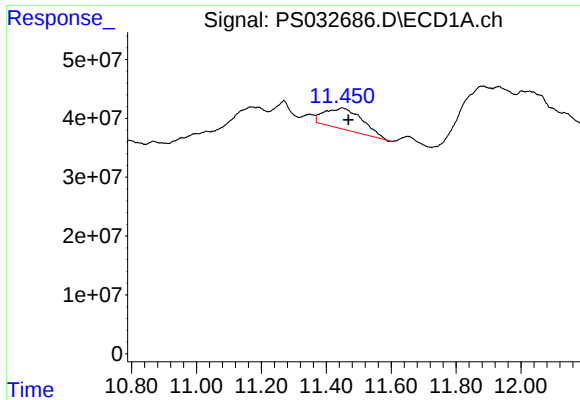

#14 DINOSEB


R.T.: 11.448 min
Delta R.T.: -0.020 min
Response: 286996245
Conc: 10.58 ng/ml

Instrument :
ECD_S
ClientSampleId :

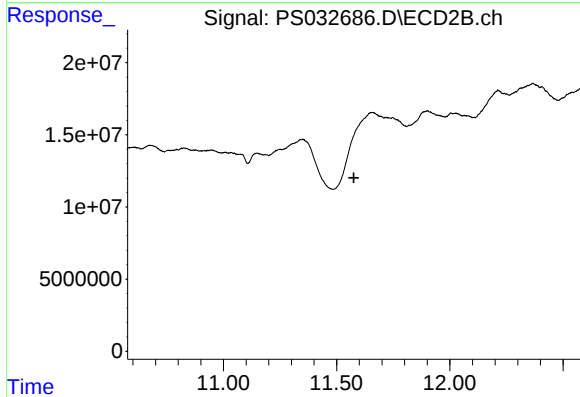


#14 DINOSEB

R.T.: 0.000 min
Exp R.T. : 11.576 min
Response: 0
Conc: N.D.

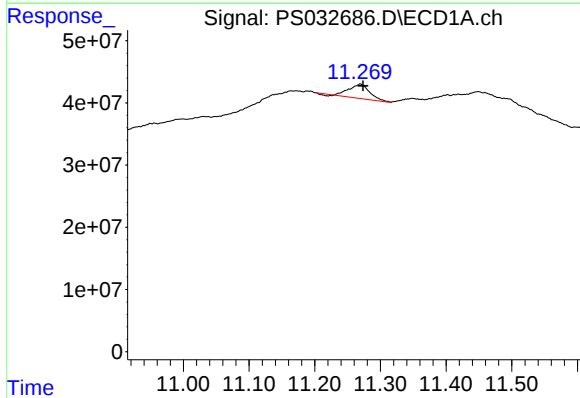


#15 Picloram

R.T.: 11.269 min
Delta R.T.: -0.005 min
Response: 49443931
Conc: 1.04 ng/ml

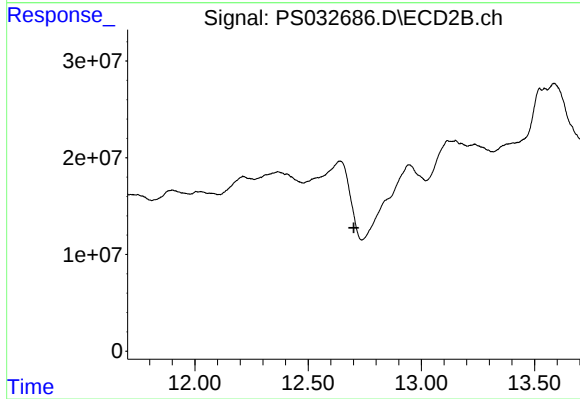

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 12.702 min
Response: 0
Conc: N.D.

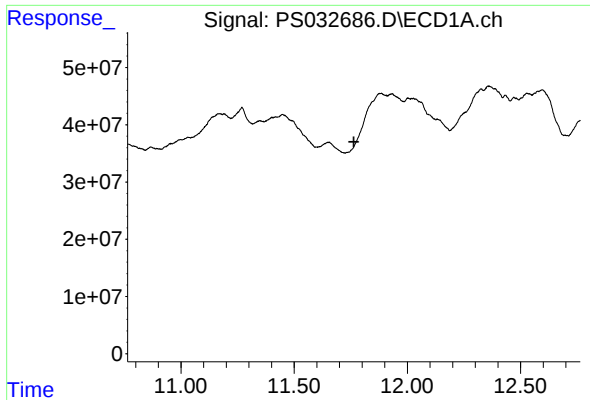

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 11.764 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

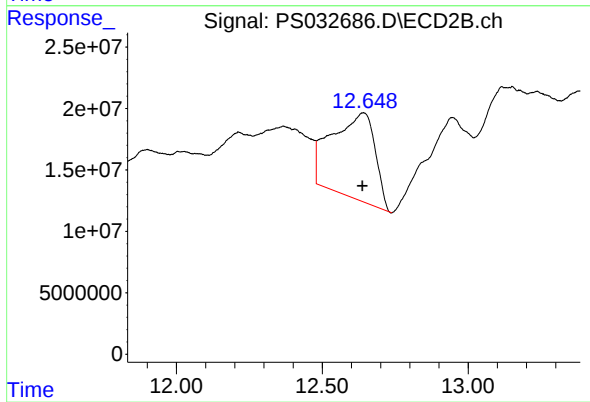

#16 DCPA

R.T.: 12.641 min
Delta R.T.: 0.002 min
Response: 714173384
Conc: 34.52 ng/ml