

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
 Data File : PS032698.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2025 23:19
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 00:33:40 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 11 01:33:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.311	7.986	2427.2E6	1201.0E6	340.131	428.887 #
Target Compounds							
3) T	4-Nitroph...	7.090	0.000	7471725	0	1.659	N.D. #
6) T	MCP	0.000	8.291	0	1949806	N.D.	<MDL
7) T	MCPA	0.000	8.577	0	5727525	N.D.	<MDL
8) T	DICHLORPROP	8.209	0.000	8357871	0	1.304	N.D. #
10) T	Pentachlo...	8.796	9.828	23124255	1883019	<MDL	<MDL #
11) T	2,4,5-TP ...	9.361	10.187	9787758	1473317	<MDL	<MDL #
12) T	2,4,5-T	9.656	10.620	3585210	19904731	<MDL	1.128 #
15) T	Picloram	11.266	12.704	32851623	13942451	<MDL	<MDL #
16) T	DCPA	11.753	12.646	63269306	10059307	1.315	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
Data File : PS032698.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2025 23:19
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 00:33:40 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

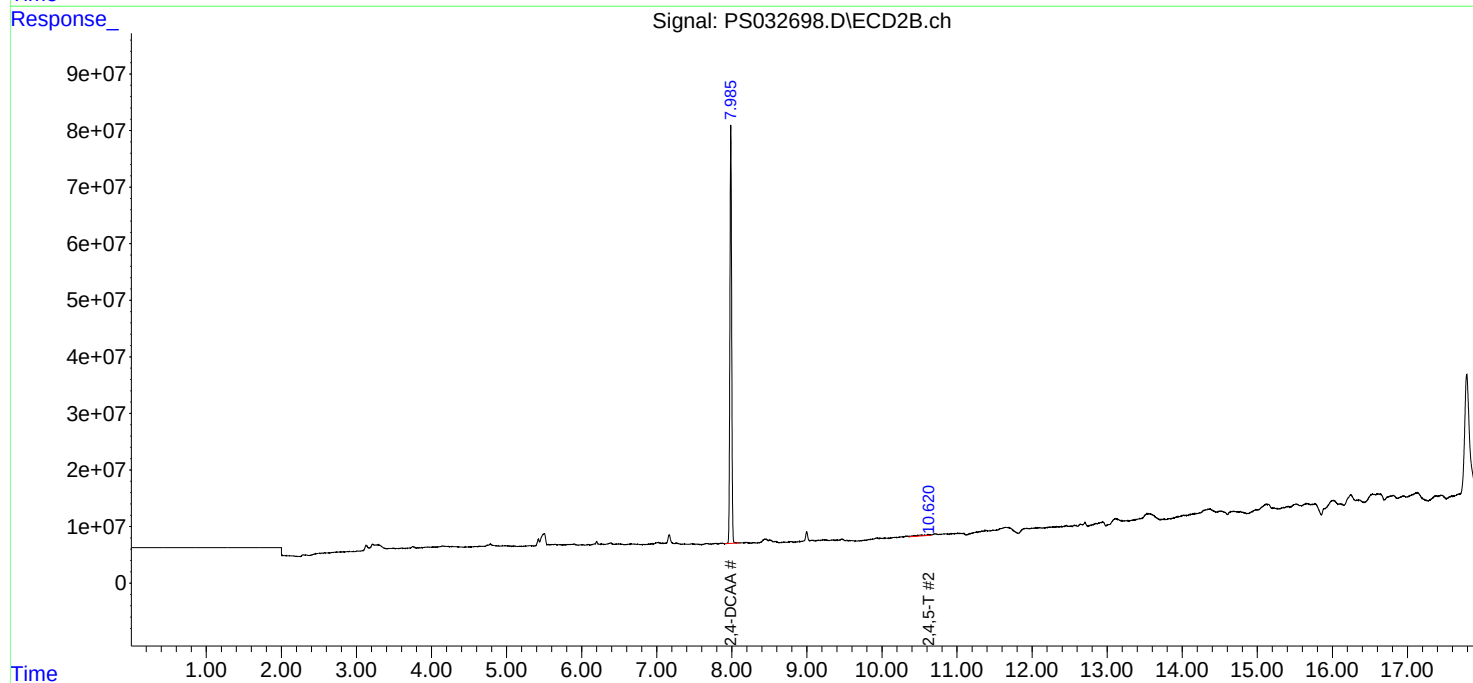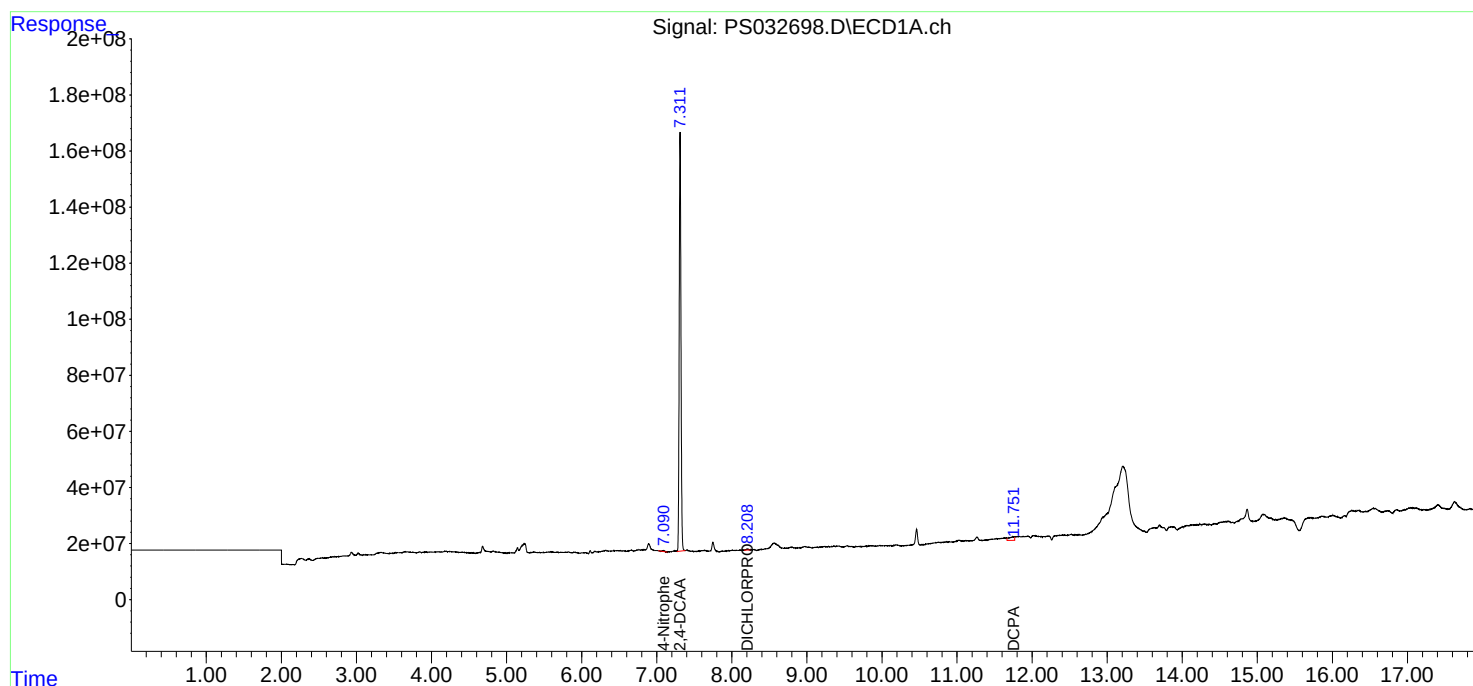


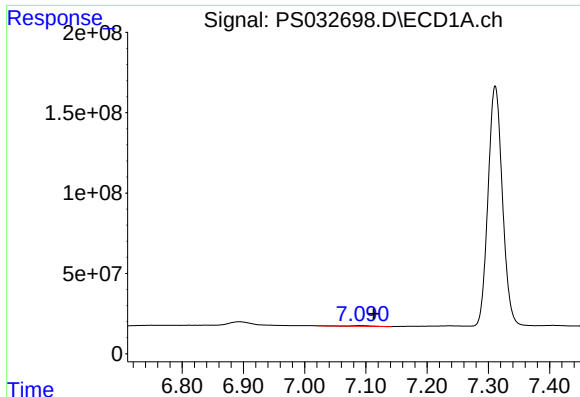

#3 4-Nitrophenol


R.T.: 7.090 min
Delta R.T.: -0.023 min
Response: 7471725
Conc: 1.66 ng/ml

Instrument :
ECD_S
ClientSampleId :

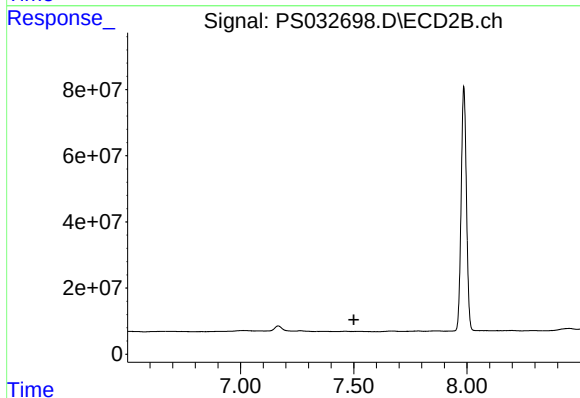


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 7.500 min
Response: 0
Conc: N.D.

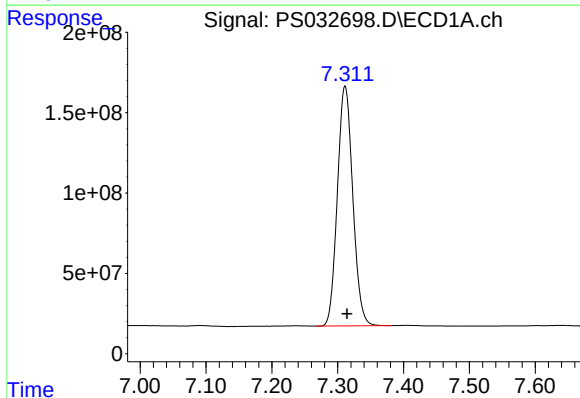


#4 2,4-DCAA

R.T.: 7.311 min
Delta R.T.: -0.003 min
Response: 2427159044
Conc: 340.13 ng/ml

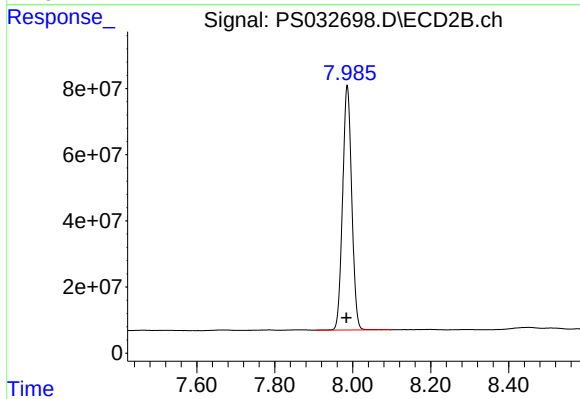

#4 2,4-DCAA


R.T.: 7.986 min
Delta R.T.: 0.002 min
Response: 1201024815
Conc: 428.89 ng/ml

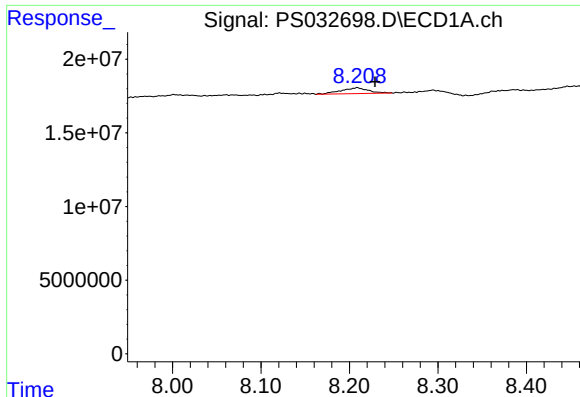

#8 DICHLORPROP


R.T.: 8.209 min
Delta R.T.: -0.020 min
Response: 8357871
Conc: 1.30 ng/ml

Instrument :
ECD_S
ClientSampleId :

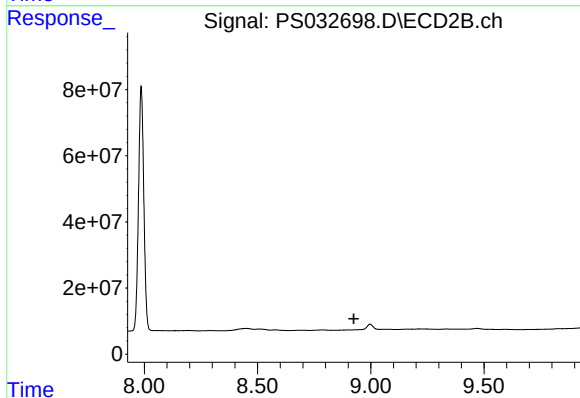


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T. : 8.925 min
Response: 0
Conc: N.D.

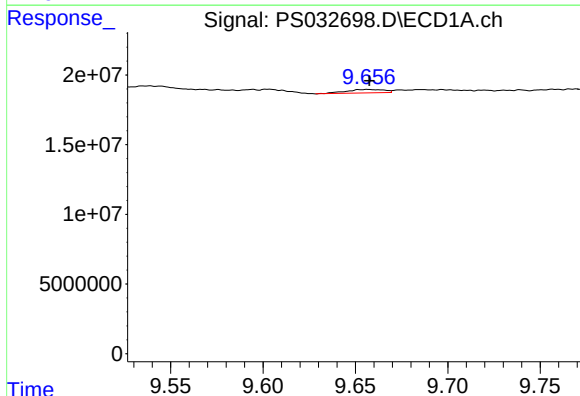


#12 2,4,5-T

R.T.: 9.656 min
Delta R.T.: -0.001 min
Response: 3585210
Conc: N.D.

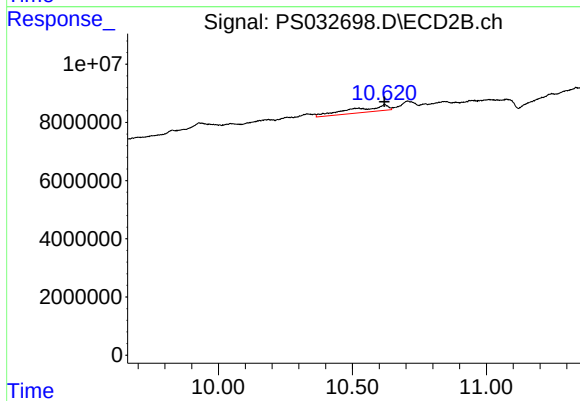

#12 2,4,5-T


R.T.: 10.620 min
Delta R.T.: 0.001 min
Response: 19904731
Conc: 1.13 ng/ml

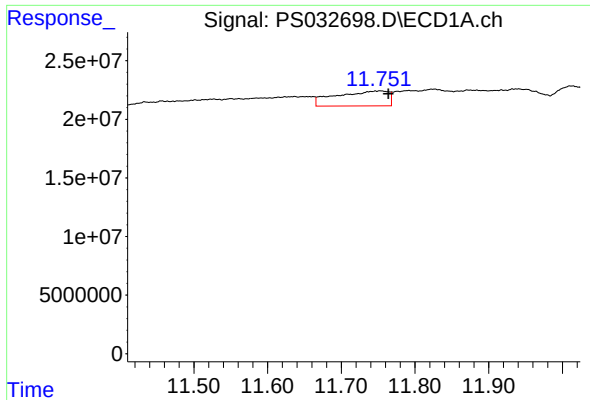

#16 DCPA

R.T.: 11.753 min
Delta R.T.: -0.011 min
Response: 63269306
Conc: 1.32 ng/ml

Instrument :
ECD_S
ClientSampleId :

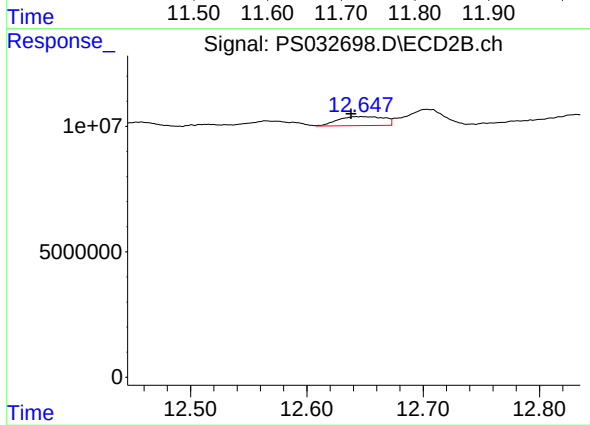

#16 DCPA

R.T.: 12.646 min
Delta R.T.: 0.008 min
Response: 10059307
Conc: N.D.