

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
 Data File : PS032706.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2025 02:55
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 06:13:56 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 11 01:33:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.311	7.987	2421.9E6	1195.0E6	339.399	426.729 #
Target Compounds							
1) T	Dalapon	2.703	2.794f	124.4E6	1501887	11.609	<MDL #
2) T	3,5-DICHL...	6.458	6.898	8815077	2801323	1.021	<MDL #
3) T	4-Nitroph...	7.089	7.465f	19086416	3652009	4.239	1.851 #
5) T	DICAMBA	0.000	8.203	0	3622700	N.D.	<MDL
6) T	MCPD	0.000	8.294	0	1770606	N.D.	<MDL
7) T	MCPA	7.870	8.577	-355843	11023667	N.D.	<MDL
8) T	DICHLORPROP	8.202f	8.909	19257290	1109993	3.004	<MDL #
10) T	Pentachlo...	8.799	9.868f	31282514	7254587	<MDL	<MDL #
11) T	2,4,5-TP ...	9.352	10.186	19415311	7659621	<MDL	<MDL #
12) T	2,4,5-T	9.665	10.625	8344643	12613321	<MDL	<MDL #
13) T	2,4-DB	10.215f	0.000	80098094	0	12.661	N.D. #
14) T	DINOSEB	11.473	11.573	74655903	149.5E6	2.752	11.858 #
15) T	Picloram	11.267	0.000	54554694	0	1.142	N.D. #
16) T	DCPA	11.743	12.646	139.1E6	125.7E6	2.892	6.077 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
Data File : PS032706.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2025 02:55
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 06:13:56 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

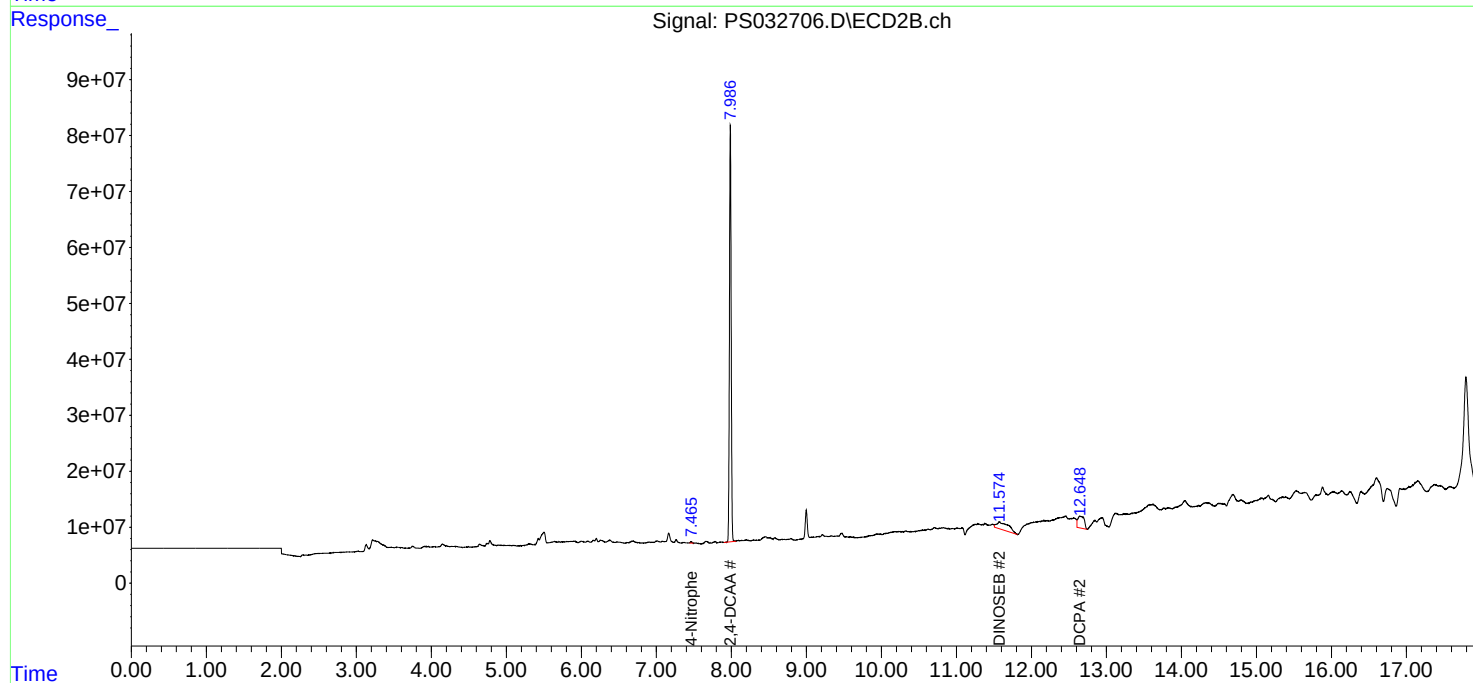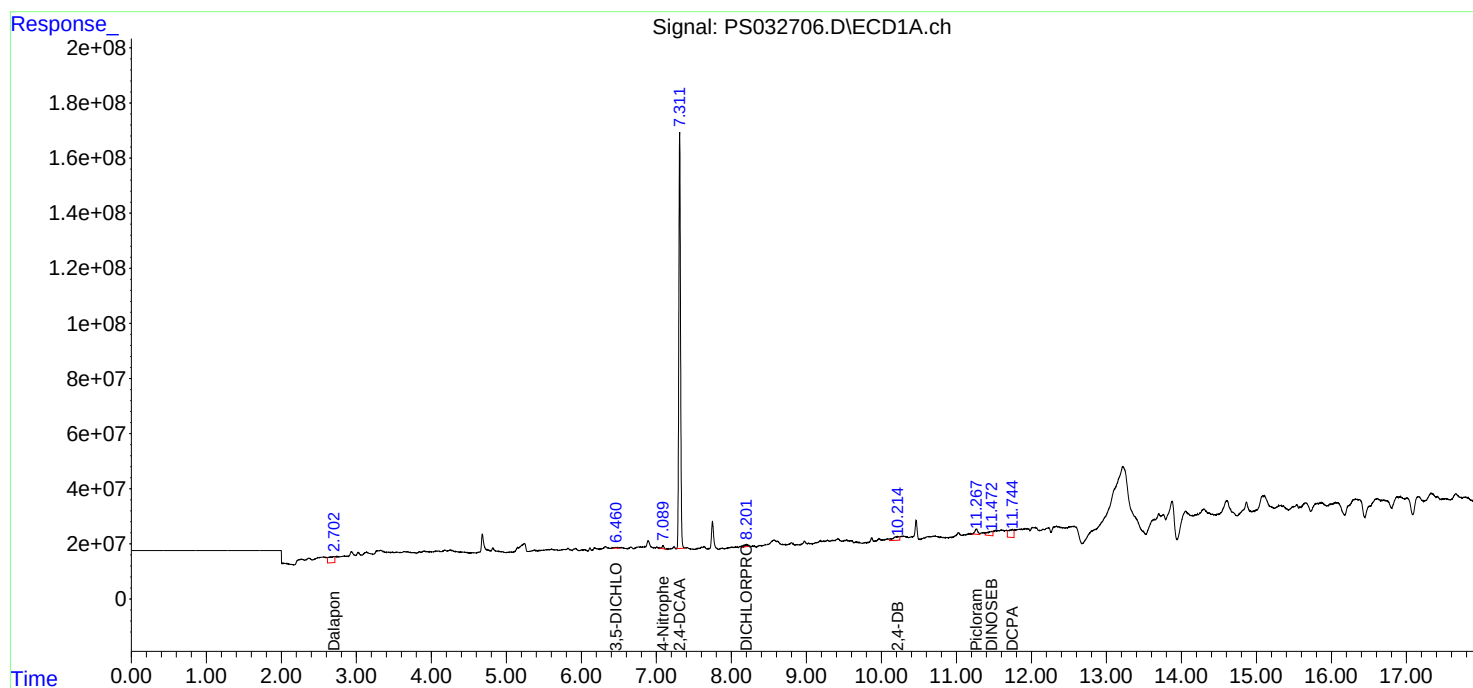


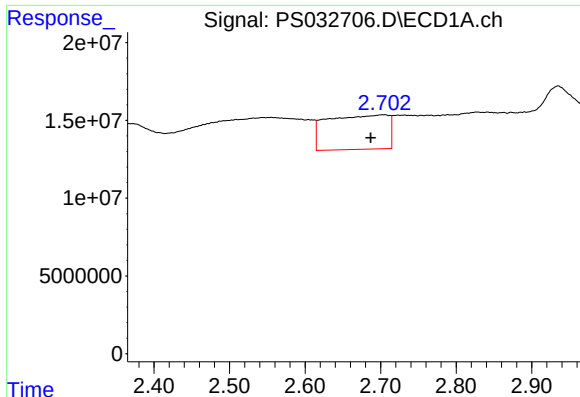

#1 Dalapon


R.T.: 2.703 min
Delta R.T.: 0.016 min
Response: 124443870
Conc: 11.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

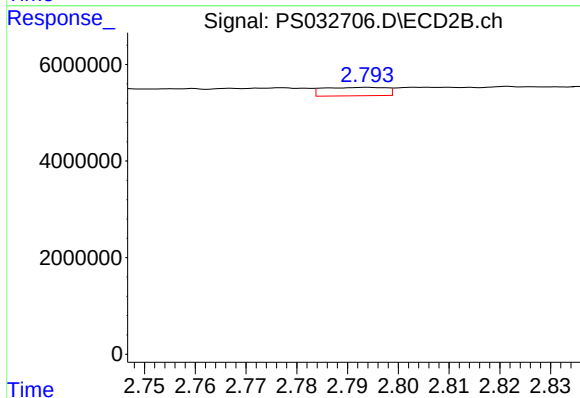


#1 Dalapon

R.T.: 2.794 min
Delta R.T.: -0.043 min
Response: 1501887
Conc: N.D.

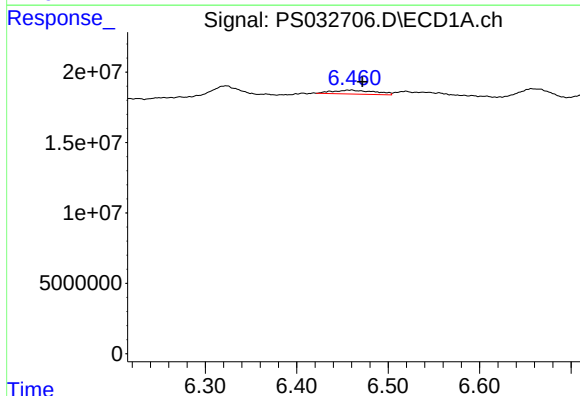


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 6.458 min
Delta R.T.: -0.014 min
Response: 8815077
Conc: 1.02 ng/ml

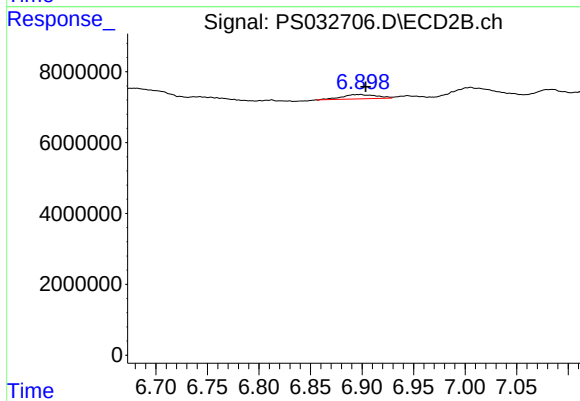

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 6.898 min
Delta R.T.: -0.005 min
Response: 2801323
Conc: N.D.

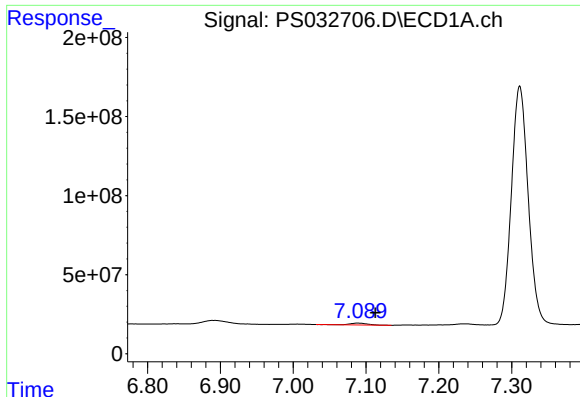

#3 4-Nitrophenol


R.T.: 7.089 min
Delta R.T.: -0.024 min
Response: 19086416
Conc: 4.24 ng/ml

Instrument :
ECD_S
ClientSampleId :

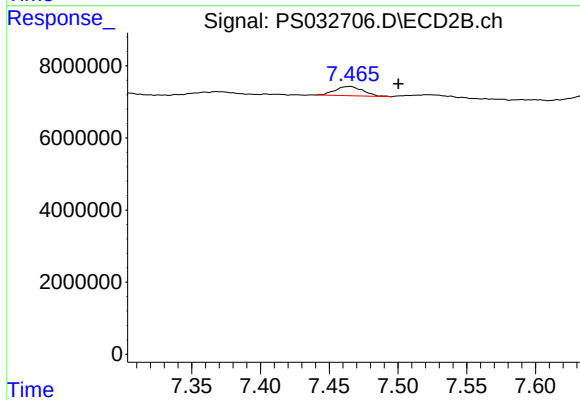


#3 4-Nitrophenol

R.T.: 7.465 min
Delta R.T.: -0.035 min
Response: 3652009
Conc: 1.85 ng/ml

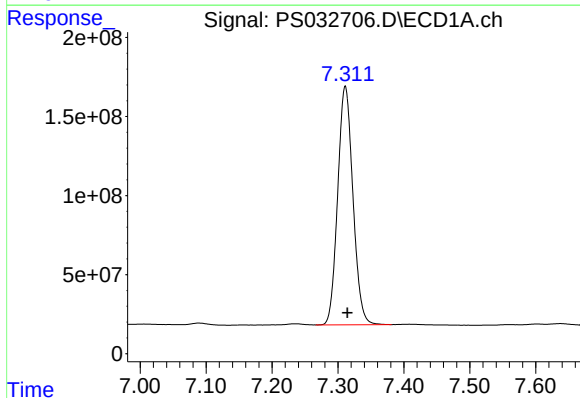


#4 2,4-DCAA

R.T.: 7.311 min
Delta R.T.: -0.003 min
Response: 2421934978
Conc: 339.40 ng/ml

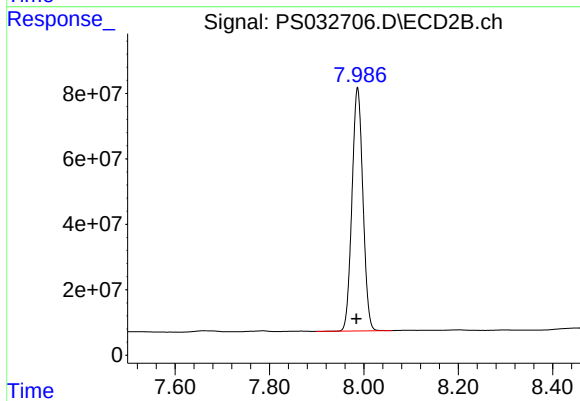

#4 2,4-DCAA


R.T.: 7.987 min
Delta R.T.: 0.003 min
Response: 1194981425
Conc: 426.73 ng/ml

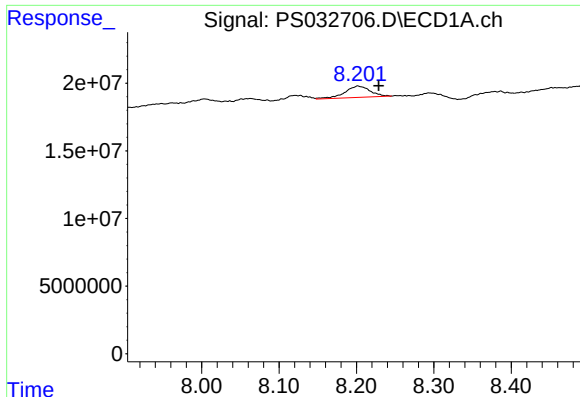

#8 DICHLORPROP


R.T.: 8.202 min
Delta R.T.: -0.026 min
Response: 19257290
Conc: 3.00 ng/ml

Instrument :
ECD_S
ClientSampleId :

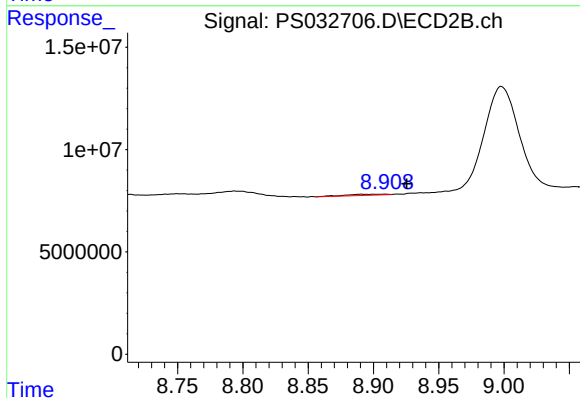


#8 DICHLORPROP

R.T.: 8.909 min
Delta R.T.: -0.017 min
Response: 1109993
Conc: N.D.

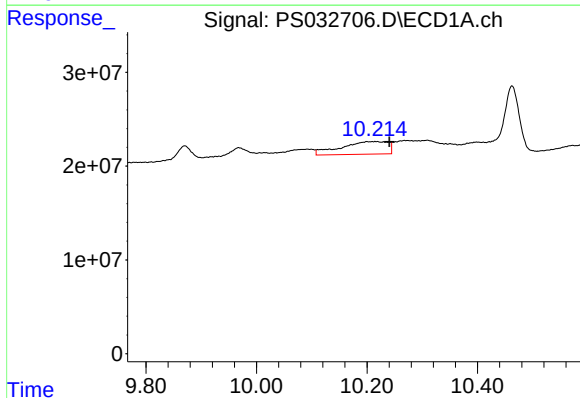


#13 2,4-DB

R.T.: 10.215 min
Delta R.T.: -0.026 min
Response: 80098094
Conc: 12.66 ng/ml

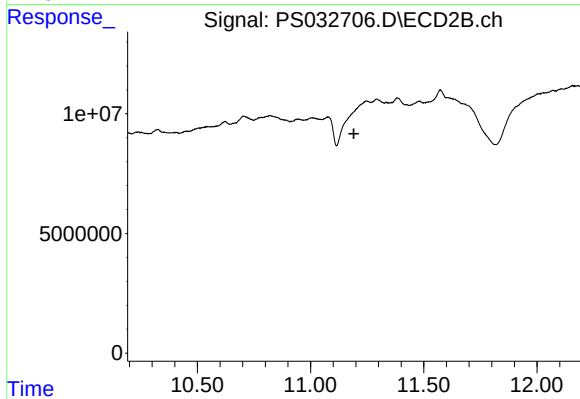

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 11.191 min
Response: 0
Conc: N.D.

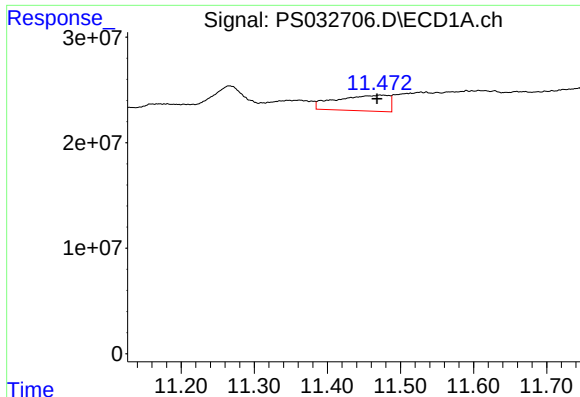

#14 DINOSEB


R.T.: 11.473 min
Delta R.T.: 0.005 min
Response: 74655903
Conc: 2.75 ng/ml

Instrument :
ECD_S
ClientSampleId :

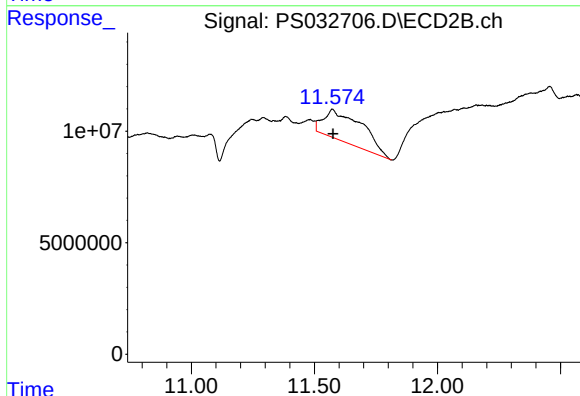


#14 DINOSEB

R.T.: 11.573 min
Delta R.T.: -0.004 min
Response: 149477304
Conc: 11.86 ng/ml

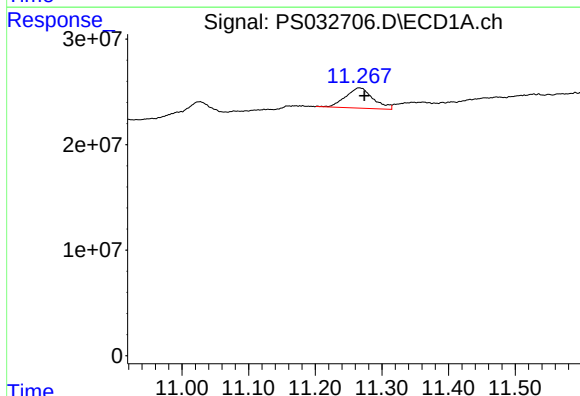


#15 Picloram

R.T.: 11.267 min
Delta R.T.: -0.007 min
Response: 54554694
Conc: 1.14 ng/ml

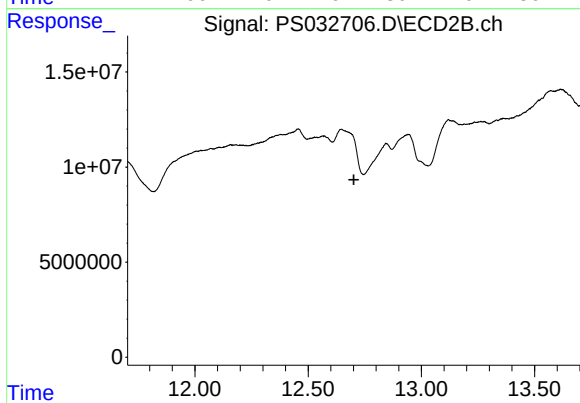

#15 Picloram


R.T.: 0.000 min
Exp R.T. : 12.702 min
Response: 0
Conc: N.D.

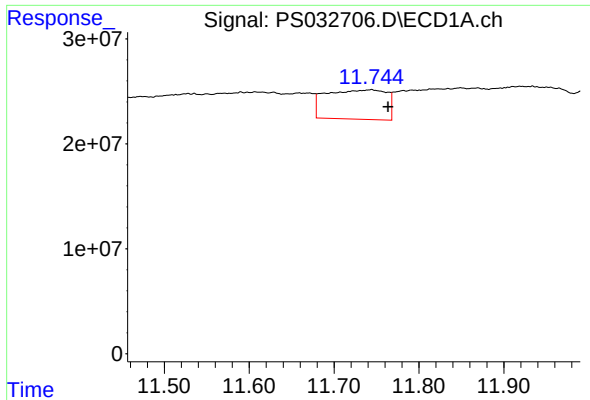

#16 DCPA

R.T.: 11.743 min
Delta R.T.: -0.020 min
Response: 139114330
Conc: 2.89 ng/ml

Instrument :
ECD_S
ClientSampleId :

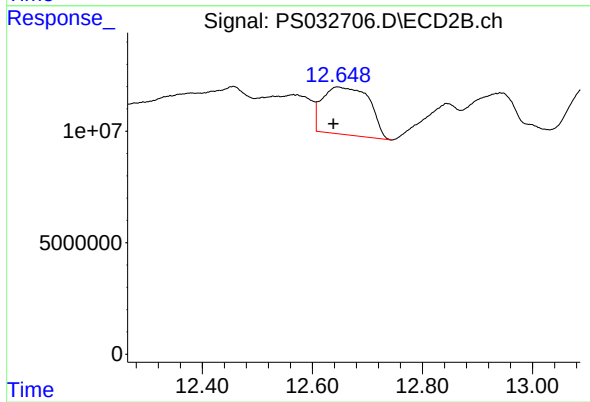

#16 DCPA

R.T.: 12.646 min
Delta R.T.: 0.008 min
Response: 125710587
Conc: 6.08 ng/ml