

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
 Data File : PS032688.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2025 19:18
 Operator : AR\AJ
 Sample : Q3812-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 OR-02-120825

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/12/2025
 Supervised By :Yogesh Patel 12/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 00:29:34 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 11 01:33:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.312	7.984	2522.9E6	1202.5E6	353.552	429.406
Target Compounds							
15) T	Picloram	11.268	12.703	2398.1E6	1077.4E6	50.210	43.146m
16) T	DCPA	11.757	12.638	1392.4E6	999.9E6	28.945m	48.336m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
Data File : PS032688.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2025 19:18
Operator : AR\AJ
Sample : Q3812-01
Misc :
ALS Vial : 6 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
OR-02-120825


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/12/2025
Supervised By : Yogesh Patel 12/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 00:29:34 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

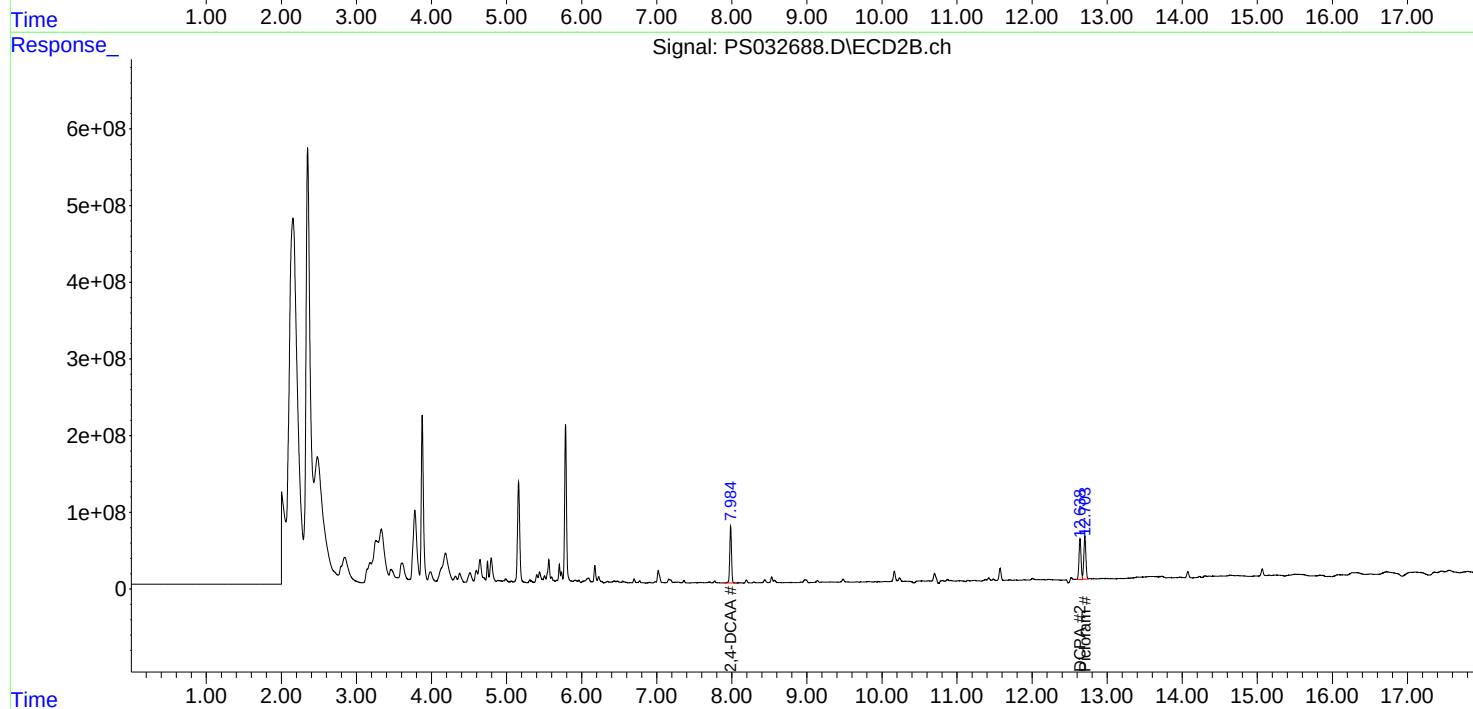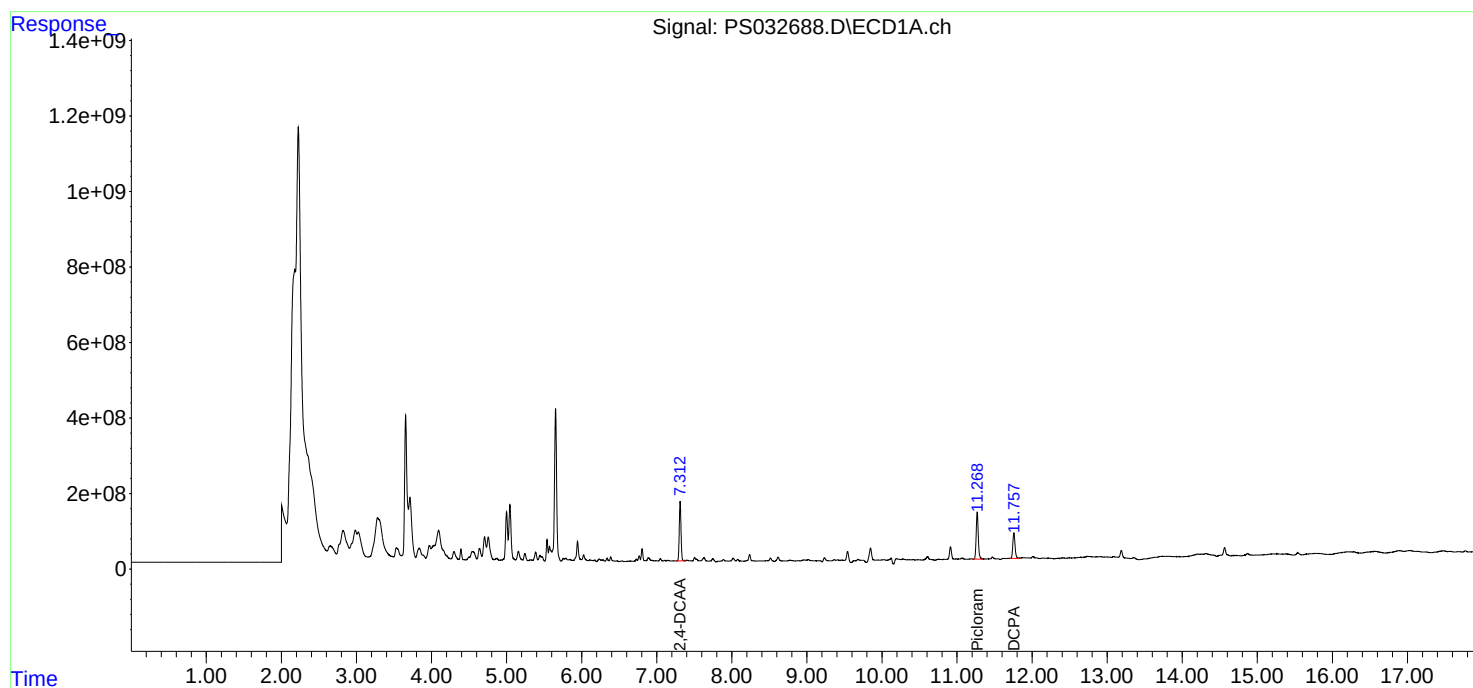

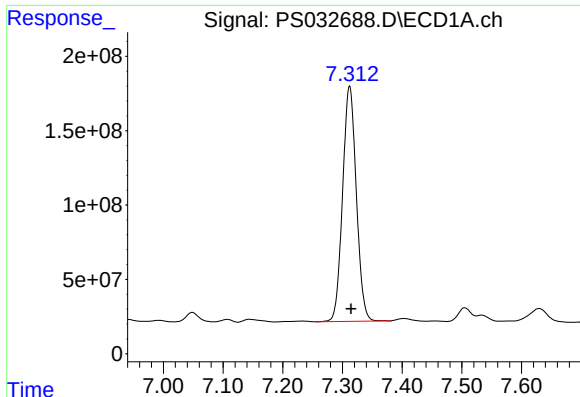


#4 2,4-DCAA

R.T.: 7.312 min
Delta R.T.: -0.002 min
Response: 2522929503
Conc: 353.55 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-120825


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/12/2025
Supervised By :Yogesh Patel 12/12/2025

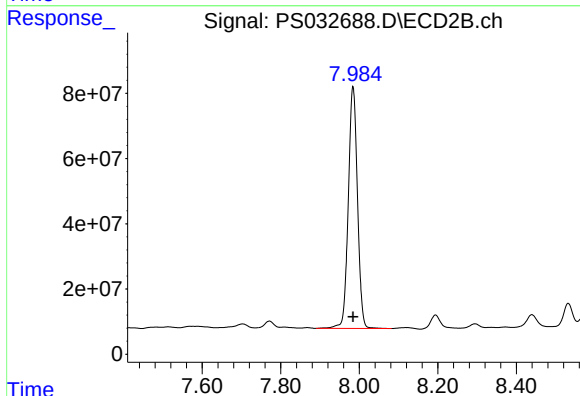


#4 2,4-DCAA

R.T.: 7.984 min
Delta R.T.: 0.000 min
Response: 1202477252
Conc: 429.41 ng/ml

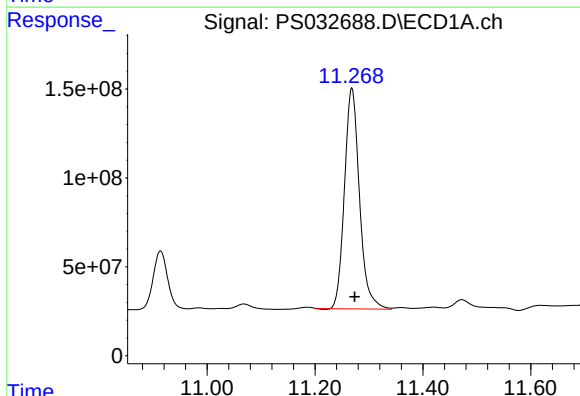


#15 Picloram

R.T.: 11.268 min
Delta R.T.: -0.005 min
Response: 2398137868
Conc: 50.21 ng/ml

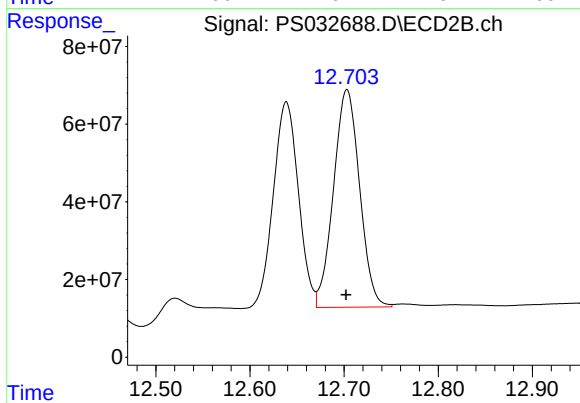

#15 Picloram

R.T.: 12.703 min
Delta R.T.: 0.000 min
Response: 1077394281
Conc: 43.15 ng/ml m

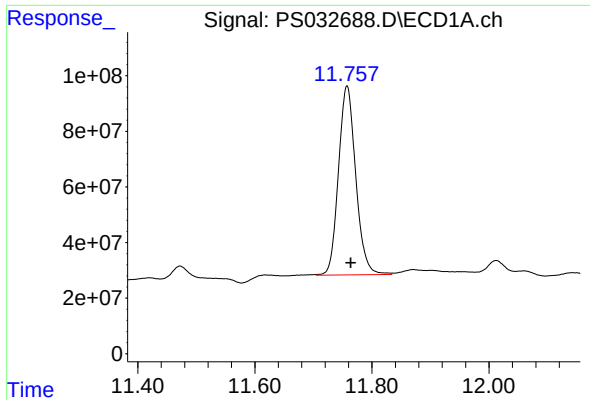


#16 DCPA

R.T.: 11.757 min
Delta R.T.: -0.007 min
Response: 1392373204
Conc: 28.94 ng/ml

Instrument :
ECD_S
ClientSampleId :
OR-02-120825

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/12/2025
Supervised By :Yogesh Patel 12/12/2025

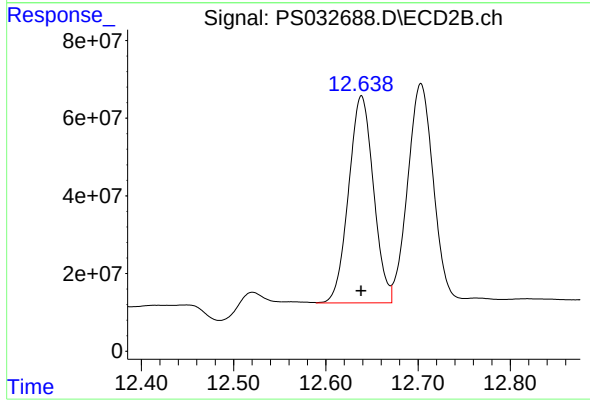

#16 DCPA

R.T.: 12.638 min
Delta R.T.: 0.000 min
Response: 999949837
Conc: 48.34 ng/ml m