

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
 Data File : PS032691.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 11 Dec 2025 20:30
 Operator : AR\AJ
 Sample : Q3831-01 (Sig #1); PB170882BS (Sig #2)
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 PL-01-12102025

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 12/12/2025
 Supervised By :Yogesh Patel 12/12/2025

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 00:30:45 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
 Quant Title : 8080.M
 QLast Update : Thu Dec 11 01:33:06 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
4) S 2,4-DCAA	7.309	7.987	334.4E6	86011352	46.864m	30.715 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
Data File : PS032691.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 11 Dec 2025 20:30
Operator : AR\AJ
Sample : Q3831-01 (Sig #1); PB170882BS (Sig #2)
Misc :
ALS Vial : 9 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
PL-01-12102025


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/12/2025
Supervised By : Yogesh Patel 12/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 00:30:45 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

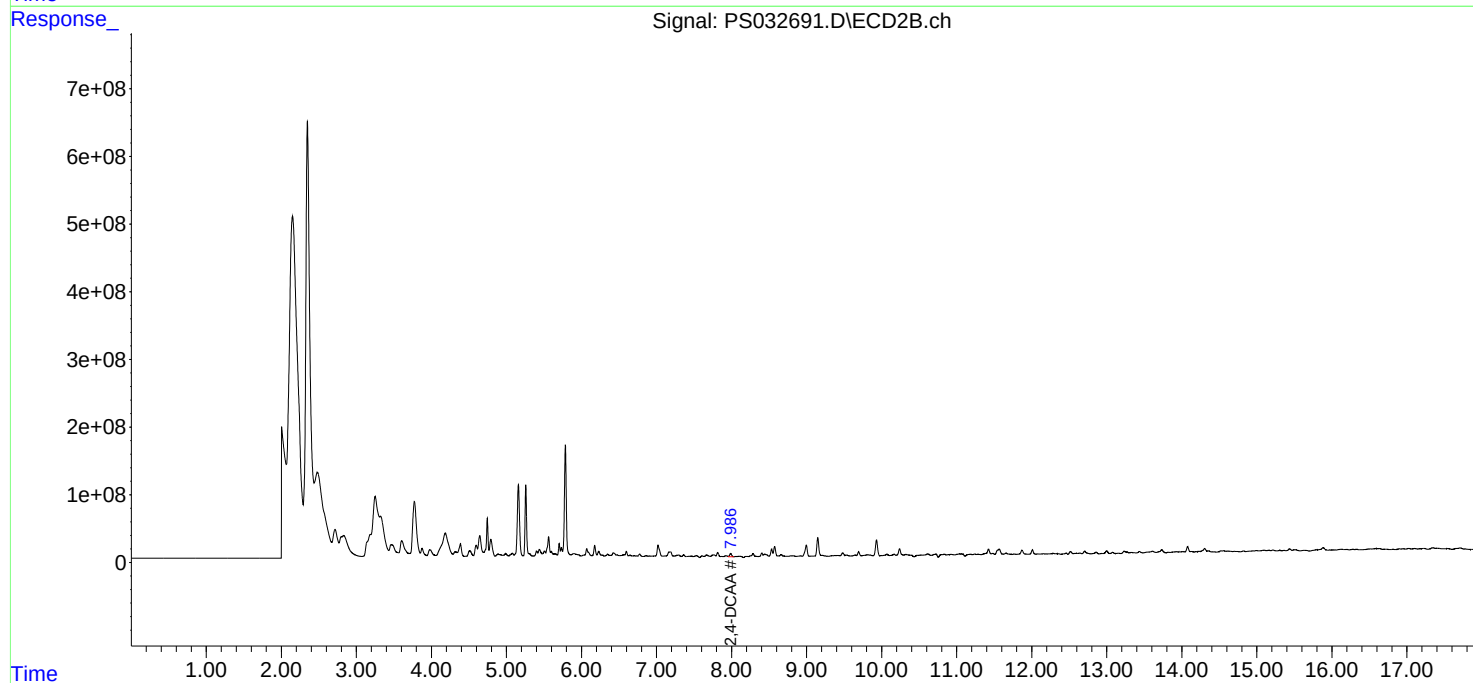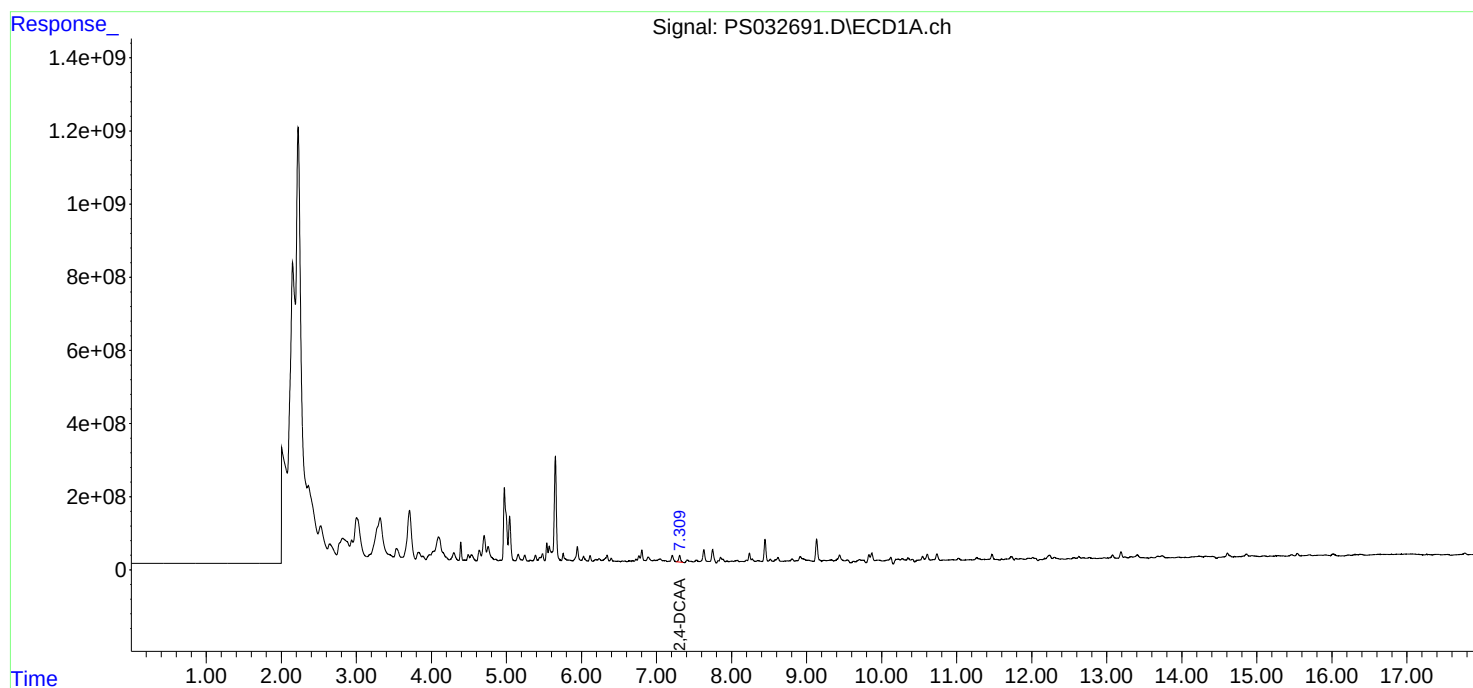

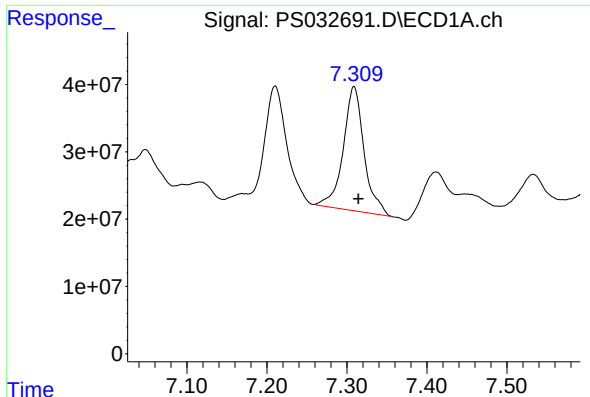


#4 2,4-DCAA

R.T.: 7.309 min
Delta R.T.: -0.006 min
Response: 334417404
Conc: 46.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
PL-01-12102025

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/12/2025
Supervised By :Yogesh Patel 12/12/2025

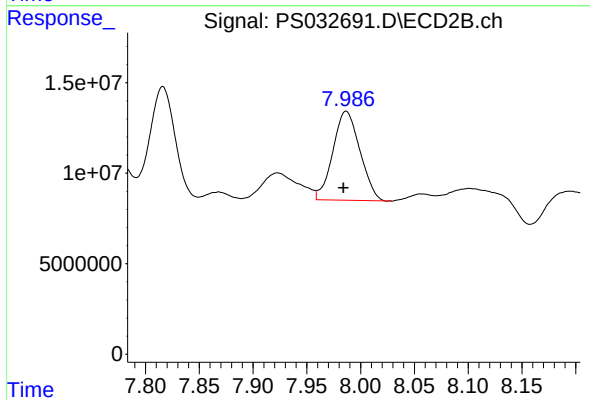

#4 2,4-DCAA

R.T.: 7.987 min
Delta R.T.: 0.003 min
Response: 86011352
Conc: 30.71 ng/ml