

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
Data File : PS032716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2025 07:19
Operator : AR\AJ
Sample : Q3826-13
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
TP-3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/12/2025
Supervised By :Yogesh Patel 12/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 08:12:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

4) S	2,4-DCAA	7.310	7.985	1768.7E6	821.4E6	247.865m	293.317m
------	----------	-------	-------	----------	---------	----------	----------

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121125\
Data File : PS032716.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2025 07:19
Operator : AR\AJ
Sample : Q3826-13
Misc :
ALS Vial : 30 Sample Multiplier: 1



Instrument :
ECD_S
ClientSampleId :
TP-3


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 12/12/2025
Supervised By : Yogesh Patel 12/12/2025

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 08:12:26 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS121025.M
Quant Title : 8080.M
QLast Update : Thu Dec 11 01:33:06 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

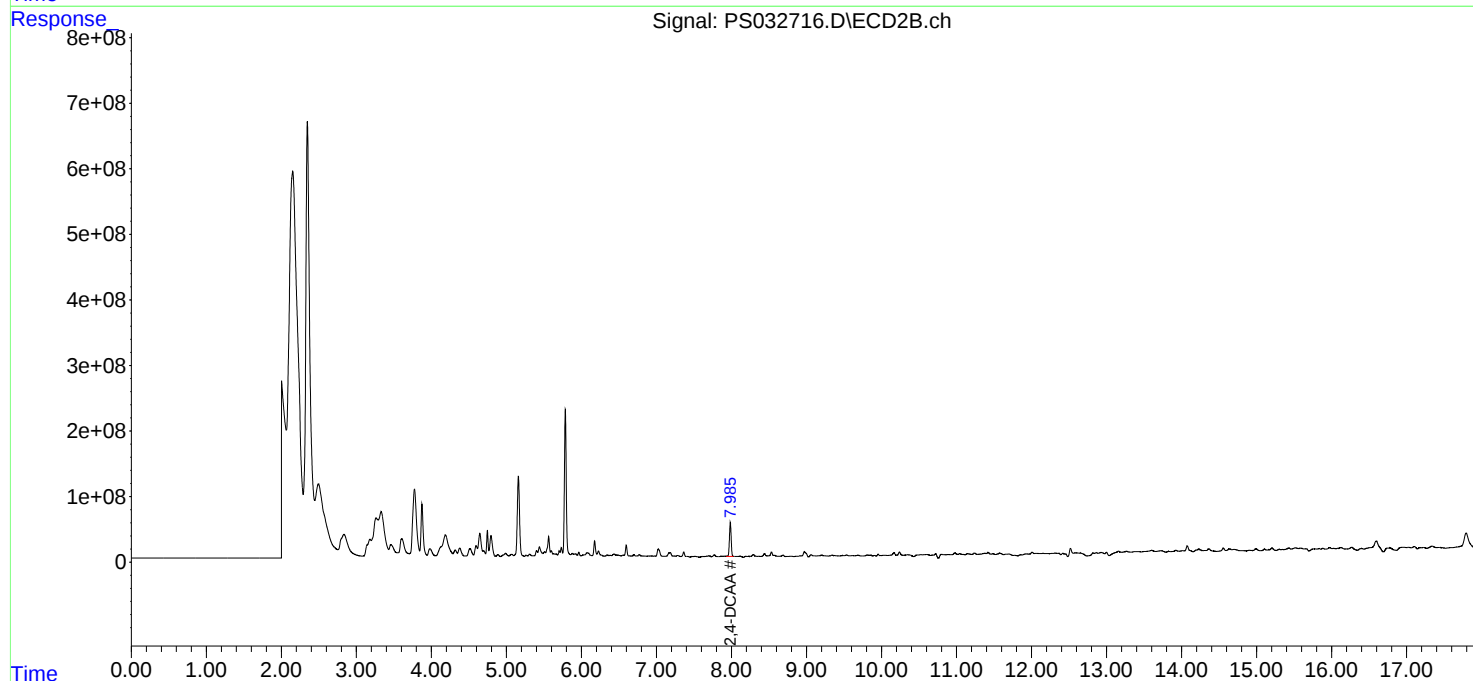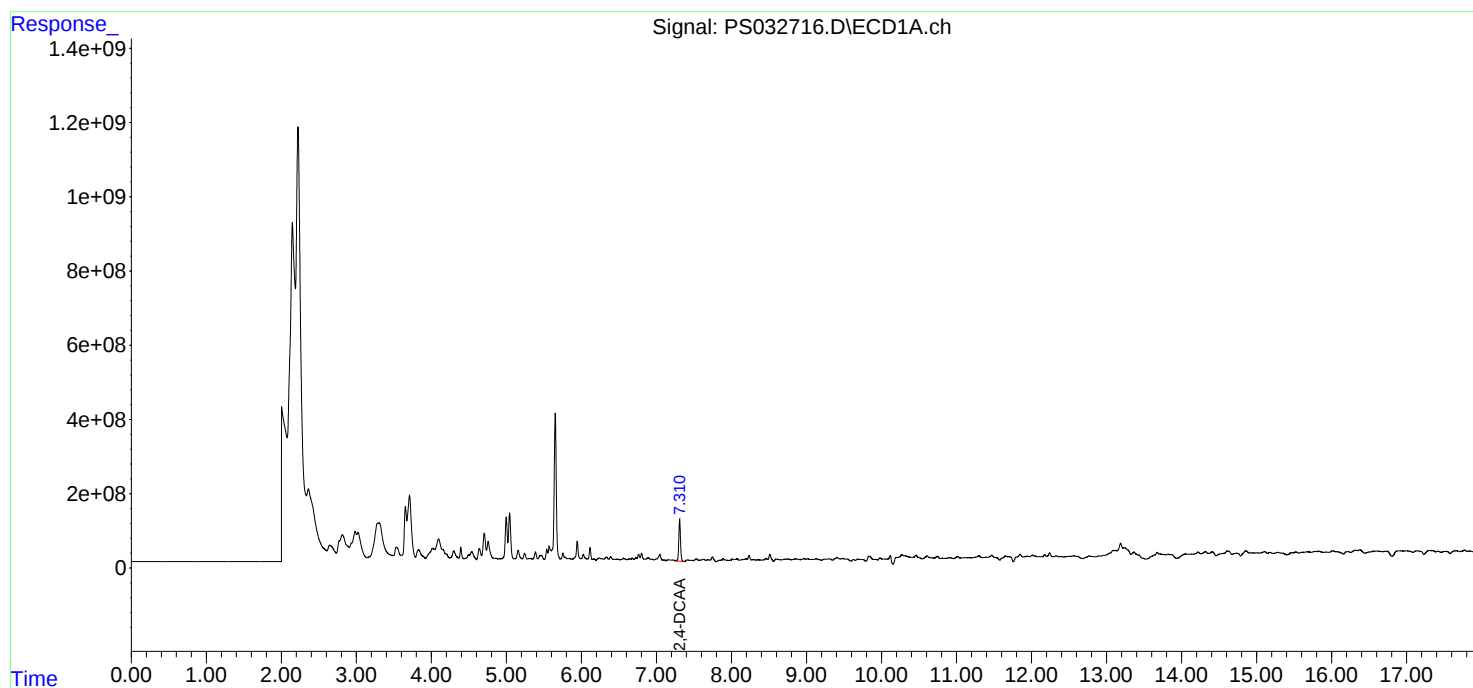

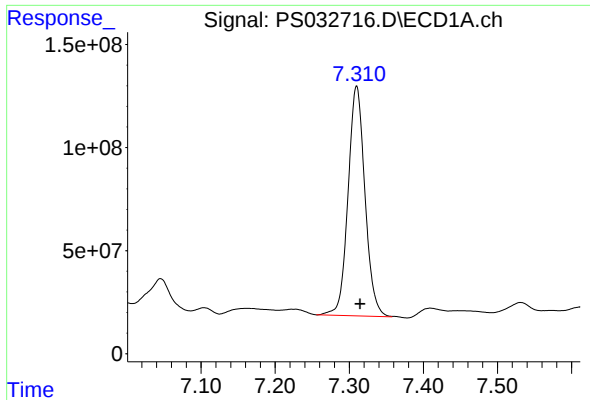


#4 2,4-DCAA

R.T.: 7.310 min
Delta R.T.: -0.005 min
Response: 1768749592
Conc: 247.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
TP-3

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 12/12/2025
Supervised By :Yogesh Patel 12/12/2025

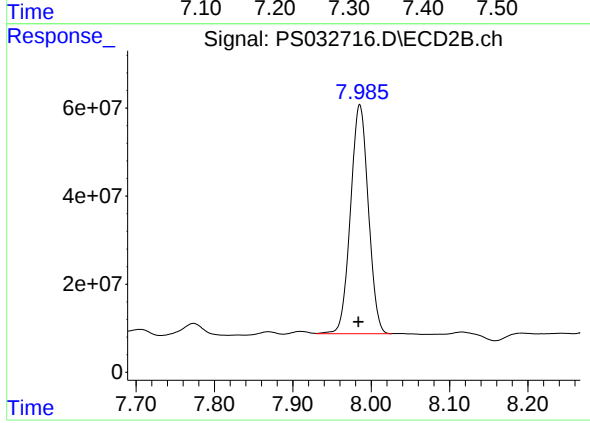

#4 2,4-DCAA

R.T.: 7.985 min
Delta R.T.: 0.001 min
Response: 821383148
Conc: 293.32 ng/ml m