

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\ps121222\
 Data File : PS021422.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2022 09:31
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 02:23:40 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
 Quant Title : 8080.M
 QLast Update : Wed Dec 07 15:59:29 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.384	6.810	1339.6E6	884.6E6	461.057	513.098
Target Compounds							
1) T	Dalapon	2.521f	0.000	525943	0	<MDL	N.D. #
2) T	3,5-DICHL...	5.730	0.000	4565831	0	1.149	N.D. #
3) T	4-Nitroph...	6.230	0.000	4308945	0	2.396	N.D. #
5) T	DICAMBA	0.000	6.994	0	25176252	N.D.	3.297
6) T	MCPD	0.000	7.065	0	22405783	N.D.	3.808
7) T	MCPA	6.762	7.214f	1715179	36964212	<MDL	4.180 #
8) T	DICHLORPROP	7.083	0.000	201731	0	<MDL	N.D. #
9) T	2,4-D	7.320	0.000	17738107	0	4.642	N.D. #
11) T	2,4,5-TP ...	8.093	0.000	9679249	0	<MDL	N.D. #
12) T	2,4,5-T	8.305	0.000	15639799	0	<MDL	N.D. #
13) T	2,4-DB	8.834	9.640f	3162836	1021936	<MDL	<MDL #
15) T	Picloram	0.000	10.895	0	25746762	N.D.	1.583
16) T	DCPA	10.218f	10.895f	549553	25746762	<MDL	1.898 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\ps121222\
Data File : PS021422.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2022 09:31
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 02:23:40 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120722.M
Quant Title : 8080.M
QLast Update : Wed Dec 07 15:59:29 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

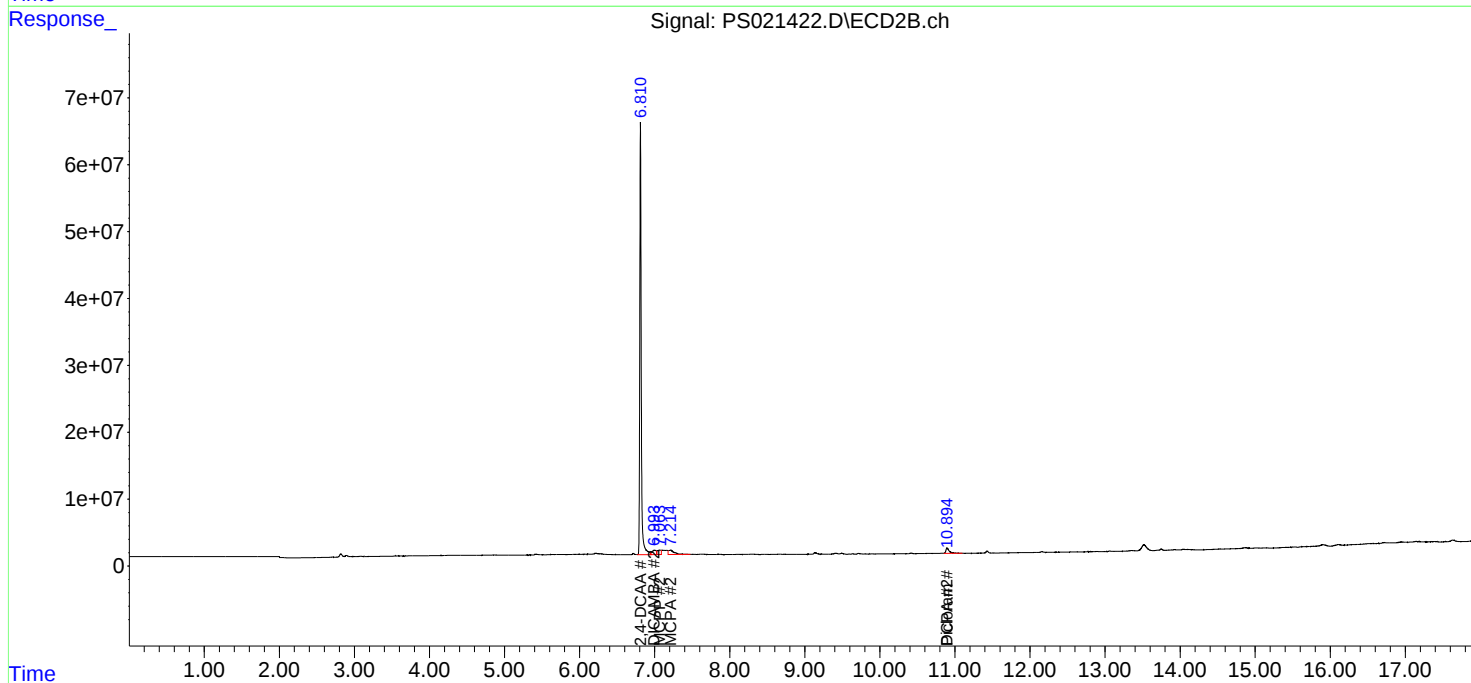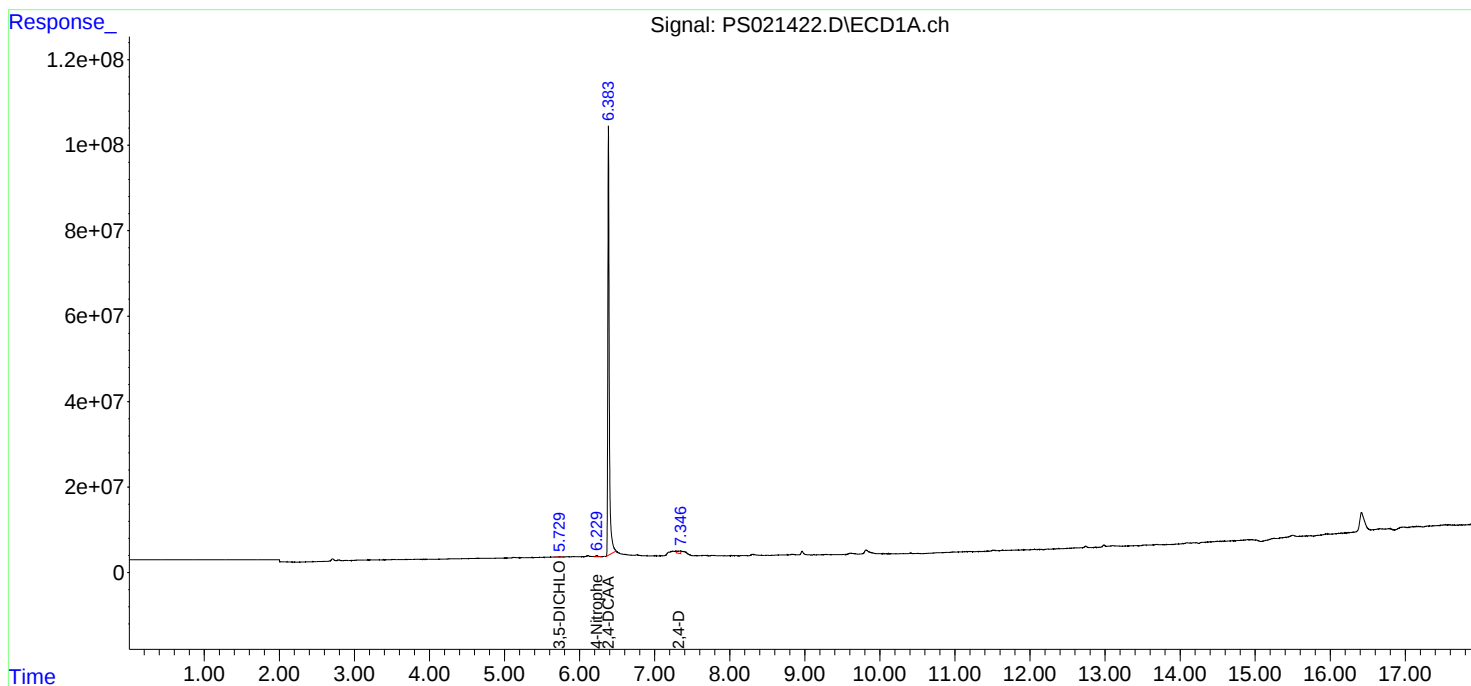


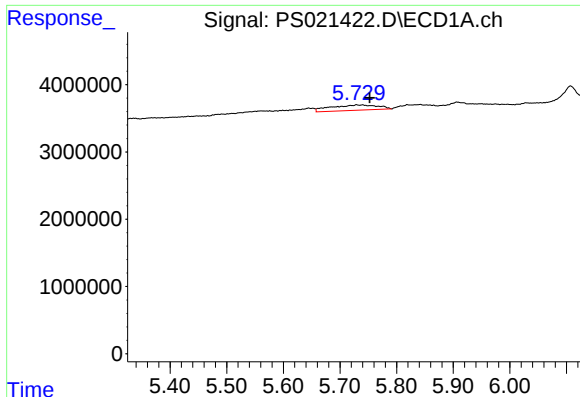

#2 3,5-DICHLOROBENZOIC ACID


R.T.: 5.730 min
Delta R.T.: -0.023 min
Response: 4565831
Conc: 1.15 ng/ml

Instrument :
ECD_S
ClientSampleId :

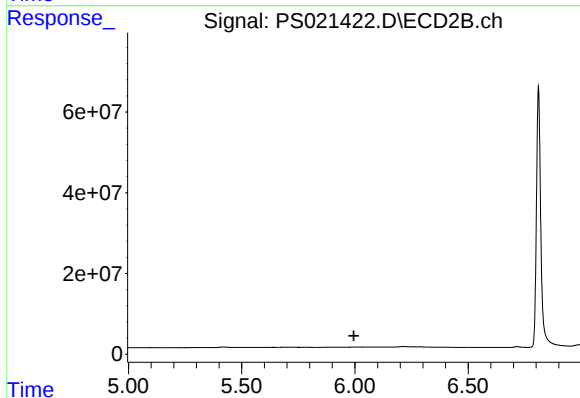


#2 3,5-DICHLOROBENZOIC ACID

R.T.: 0.000 min
Exp R.T. : 5.996 min
Response: 0
Conc: N.D.

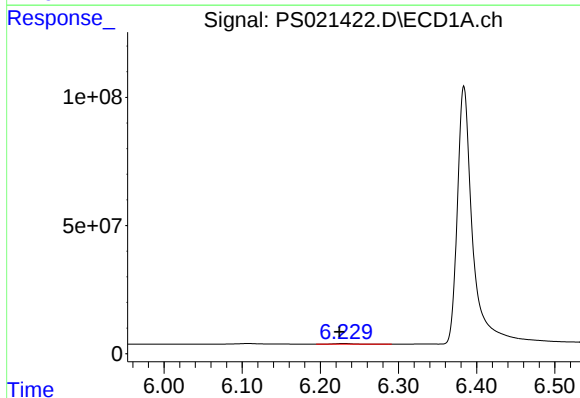


#3 4-Nitrophenol

R.T.: 6.230 min
Delta R.T.: 0.005 min
Response: 4308945
Conc: 2.40 ng/ml

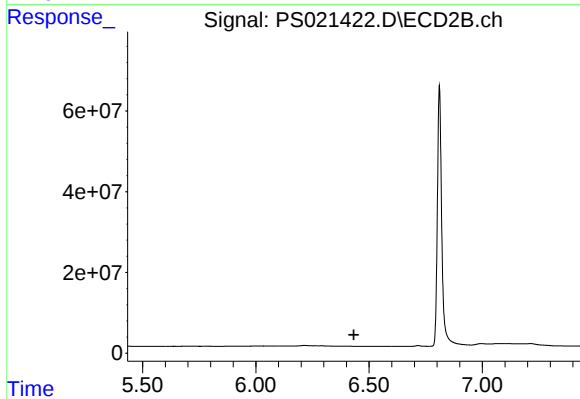

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 6.433 min
Response: 0
Conc: N.D.

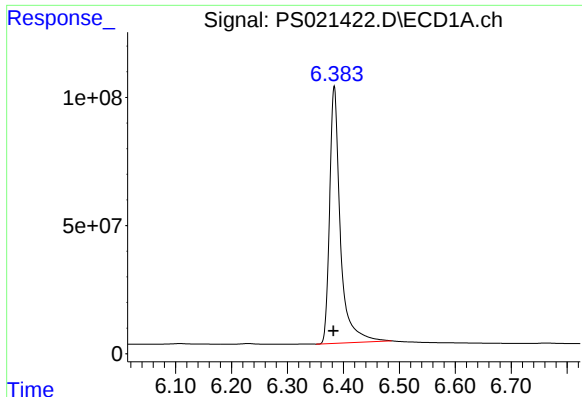

#4 2,4-DCAA


R.T.: 6.384 min
Delta R.T.: 0.002 min
Response: 1339597516
Conc: 461.06 ng/ml

Instrument :
ECD_S
ClientSampleId :

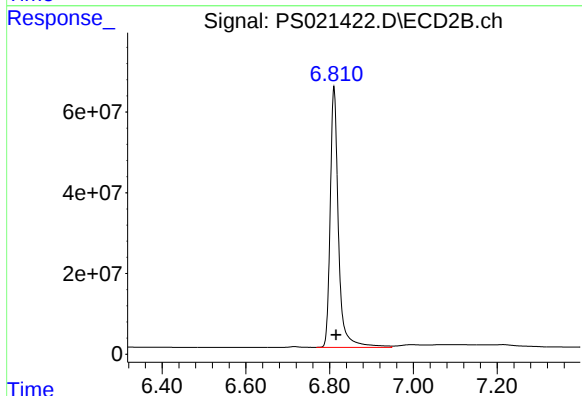


#4 2,4-DCAA

R.T.: 6.810 min
Delta R.T.: -0.005 min
Response: 884576718
Conc: 513.10 ng/ml

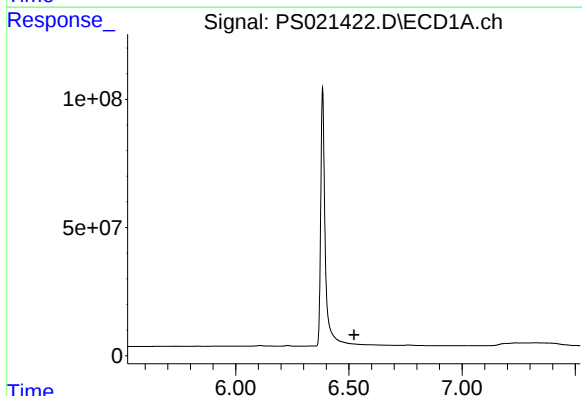


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 6.522 min
Response: 0
Conc: N.D.

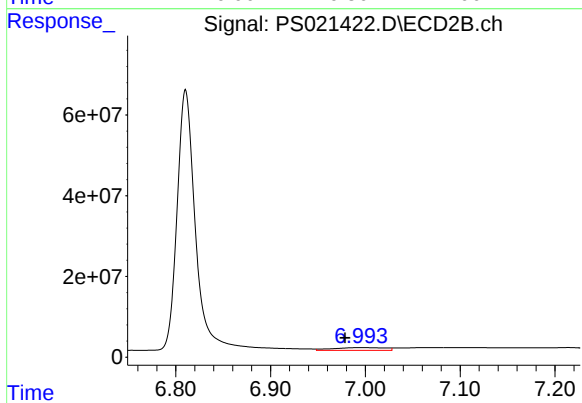

#5 DICAMBA


R.T.: 6.994 min
Delta R.T.: 0.015 min
Response: 25176252
Conc: 3.30 ng/ml

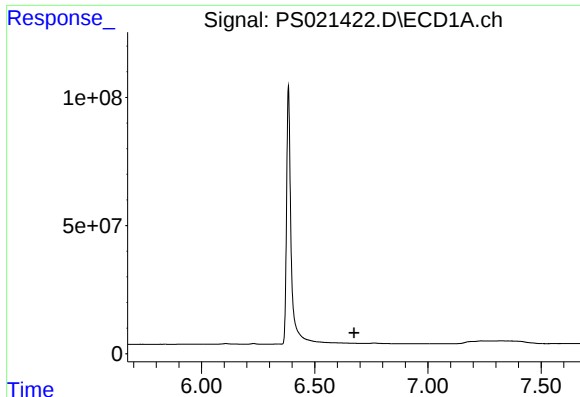

#6 MCPP


R.T.: 0.000 min
Exp R.T.: 6.673 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

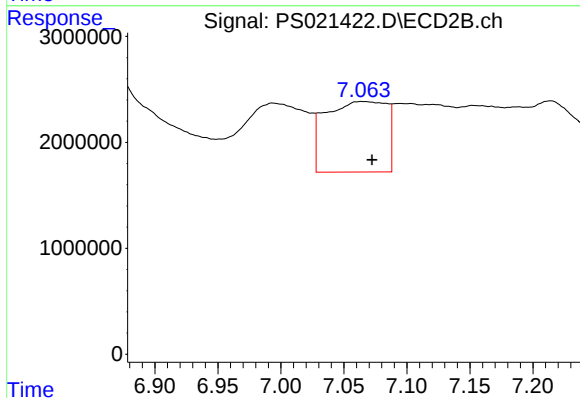


#6 MCPP

R.T.: 7.065 min
Delta R.T.: -0.008 min
Response: 22405783
Conc: 3.81 ug/ml

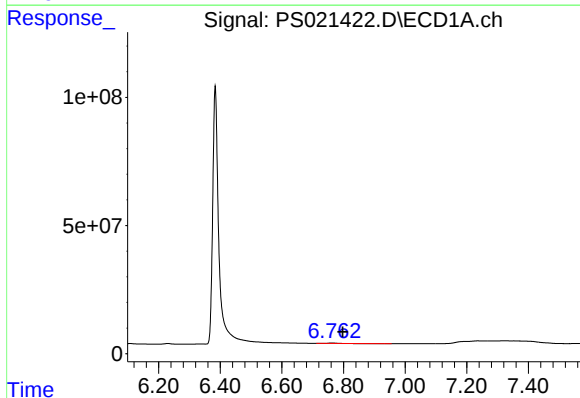


#7 MCPA

R.T.: 6.762 min
Delta R.T.: -0.036 min
Response: 1715179
Conc: N.D.

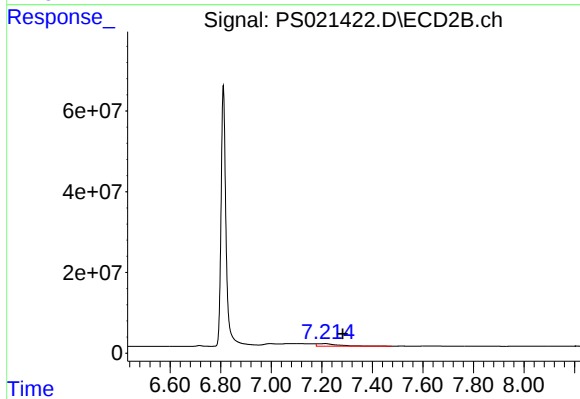

#7 MCPA


R.T.: 7.214 min
Delta R.T.: -0.069 min
Response: 36964212
Conc: 4.18 ug/ml

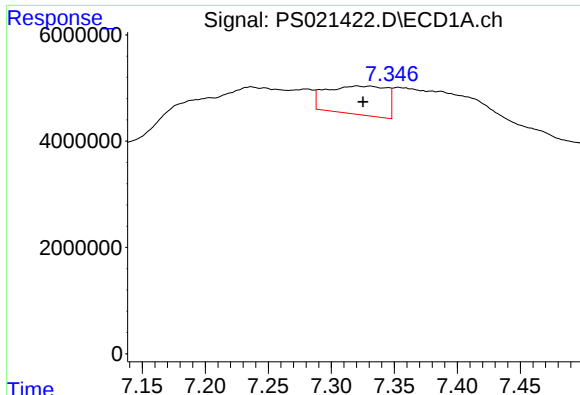

#9 2,4-D


R.T.: 7.320 min
Delta R.T.: -0.005 min
Response: 17738107
Conc: 4.64 ng/ml

Instrument :
ECD_S
ClientSampleId :

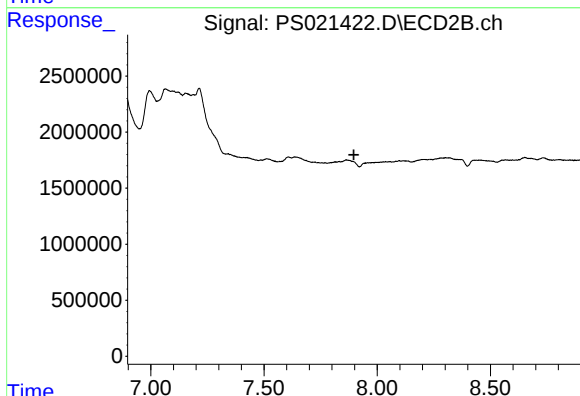


#9 2,4-D

R.T.: 0.000 min
Exp R.T. : 7.897 min
Response: 0
Conc: N.D.

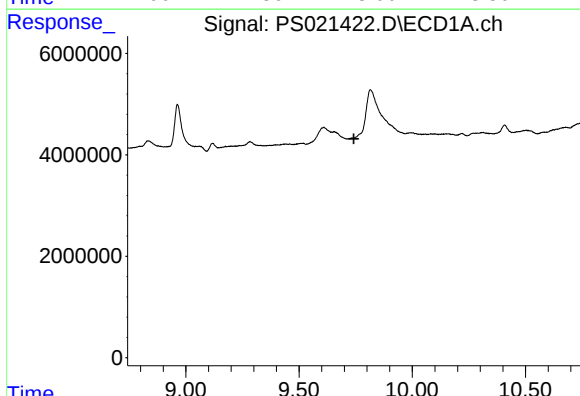


#15 Picloram

R.T.: 0.000 min
Exp R.T. : 9.742 min
Response: 0
Conc: N.D.

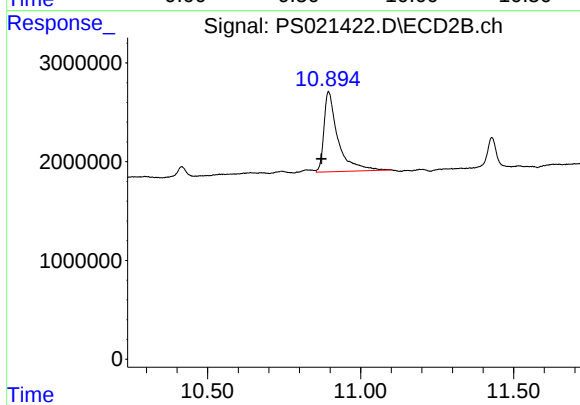

#15 Picloram


R.T.: 10.895 min
Delta R.T.: 0.023 min
Response: 25746762
Conc: 1.58 ng/ml

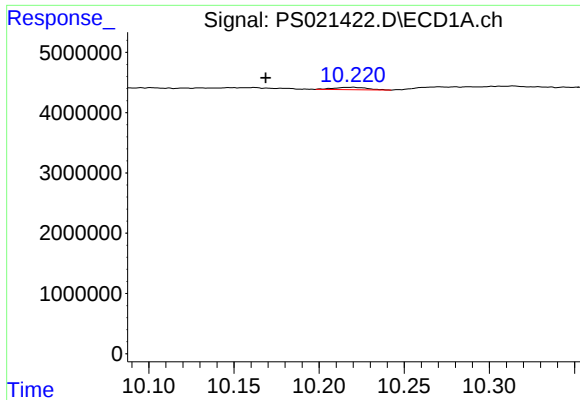

#16 DCPA

R.T.: 10.218 min
Delta R.T.: 0.050 min
Response: 549553
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

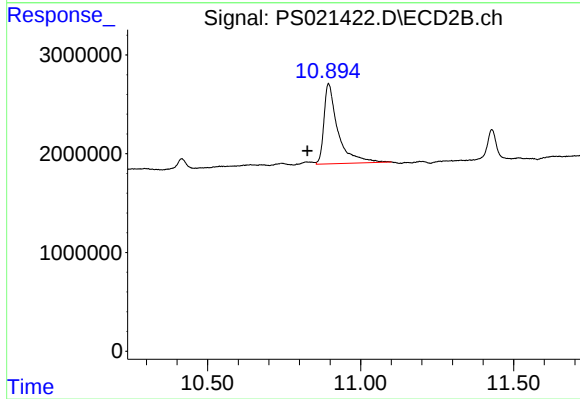

#16 DCPA

R.T.: 10.895 min
Delta R.T.: 0.069 min
Response: 25746762
Conc: 1.90 ng/ml