

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121223\
 Data File : PS025063.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 11:00
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 HEXANE

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 13:23:09 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds						
1) T	Dalapon	2.509	2.558	8565105	3933294	2.970 3.429
2) T	3,5-DICHL...	5.697	0.000	1007920	0	<MDL N.D. #
5) T	DICAMBA	0.000	6.968	0	2637558	N.D. <MDL
6) T	MCP	0.000	6.968f	0	2637558	N.D. 1.272
8) T	DICHLORPROP	0.000	7.552	0	1902746	N.D. 2.419
9) T	2,4-D	7.247	7.766f	22035115	345421	7.255 <MDL #
10) T	Pentachlo...	0.000	8.245	0	629973	N.D. <MDL
11) T	2,4,5-TP ...	0.000	8.606	0	499254	N.D. <MDL
12) T	2,4,5-T	0.000	8.975	0	479573	N.D. <MDL
15) T	Picloram	9.679	10.757	81712694	25077157	4.193 3.831
16) T	DCPA	0.000	10.757	0	25077157	N.D. 4.627



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121223\
Data File : PS025063.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 11:00
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
HEXANE

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 13:23:09 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

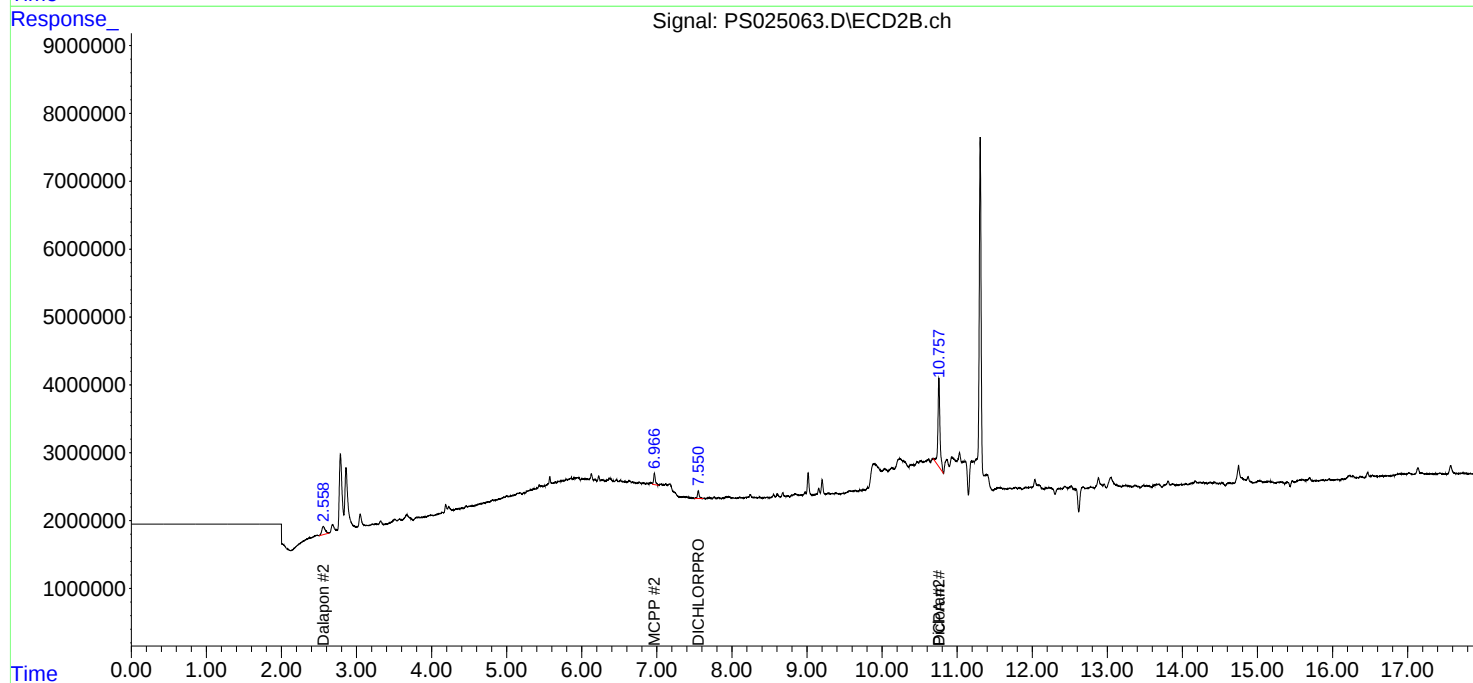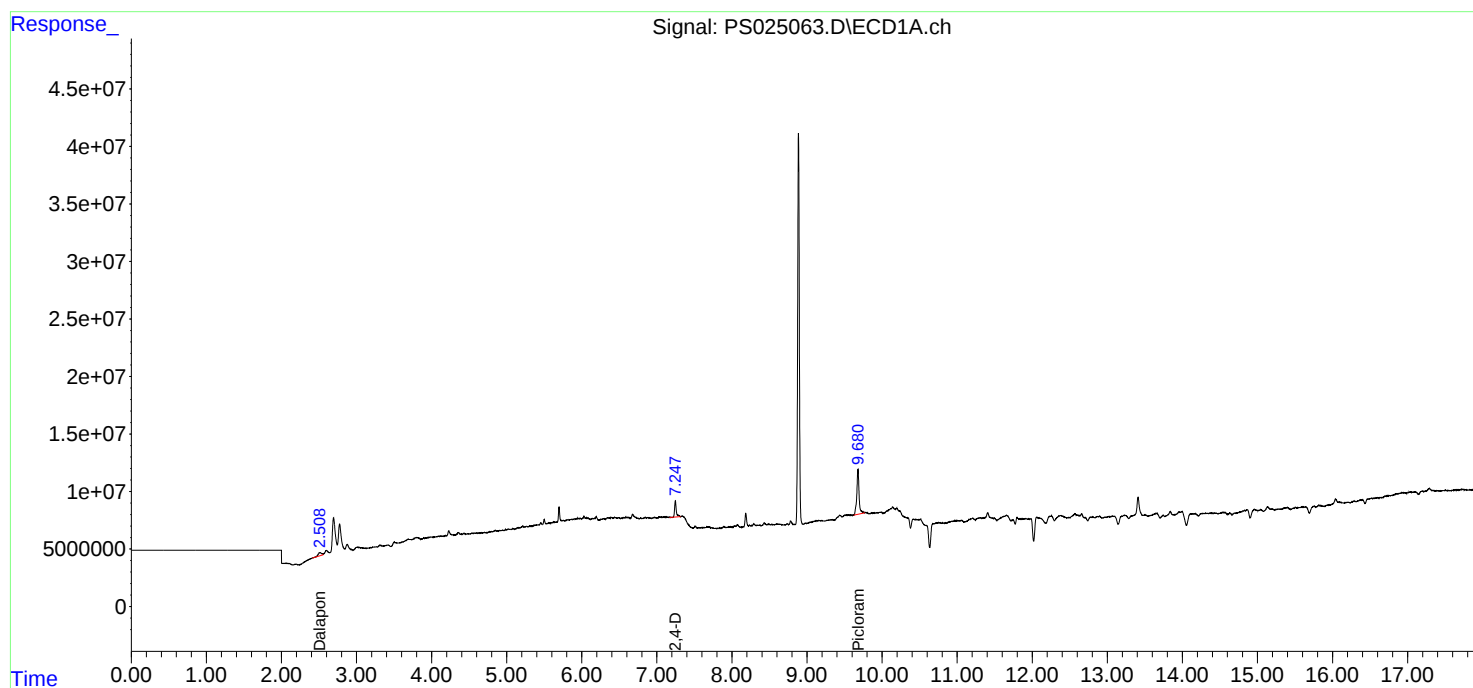


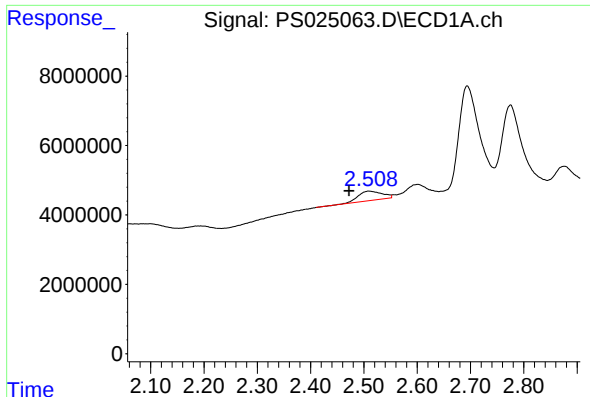

#1 Dalapon


R.T.: 2.509 min
Delta R.T.: 0.037 min
Response: 8565105
Conc: 2.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

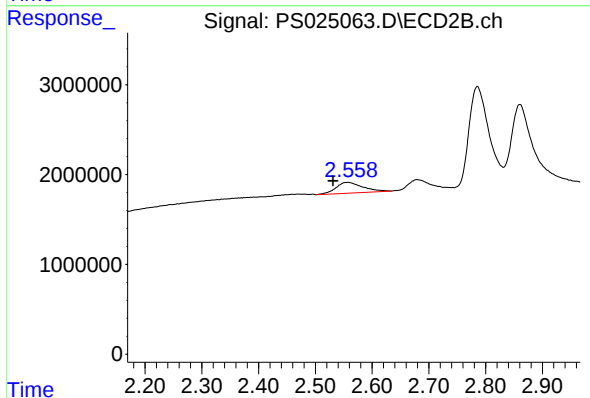


#1 Dalapon

R.T.: 2.558 min
Delta R.T.: 0.027 min
Response: 3933294
Conc: 3.43 ng/ml

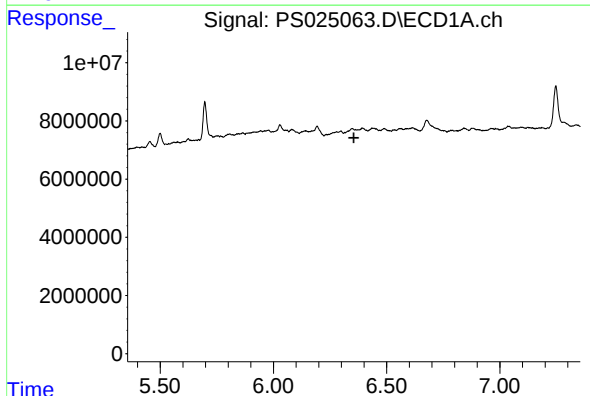


#4 2,4-DCAA

R.T.: 0.000 min
Exp R.T. : 6.355 min
Response: 0
Conc: N.D.

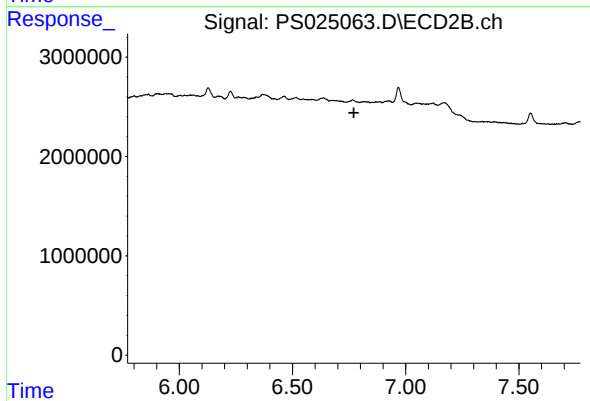

#4 2,4-DCAA


R.T.: 0.000 min
Exp R.T. : 6.771 min
Response: 0
Conc: N.D.

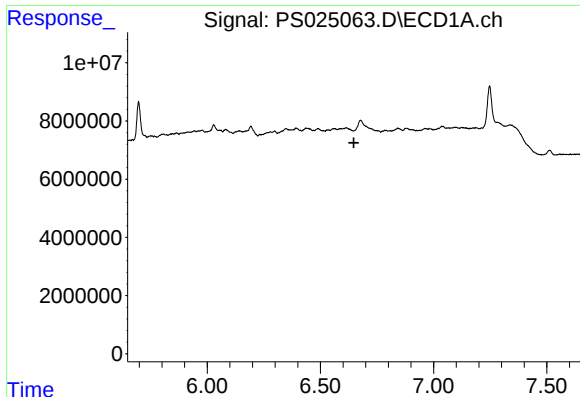

#6 MCP


R.T.: 0.000 min
Exp R.T.: 6.648 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

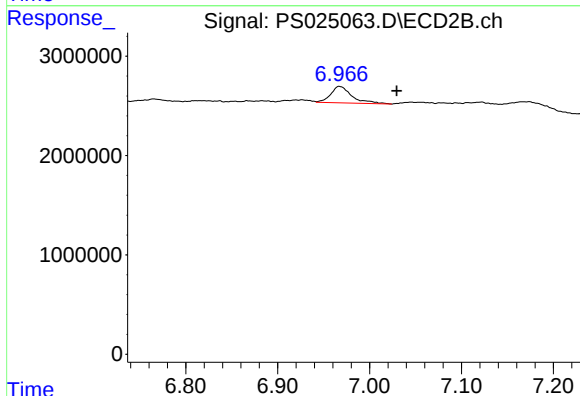


#6 MCP

R.T.: 6.968 min
Delta R.T.: -0.062 min
Response: 2637558
Conc: 1.27 ug/ml

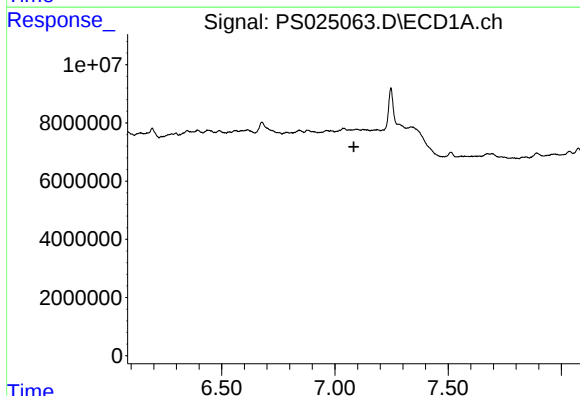


#8 DICHLORPROP

R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

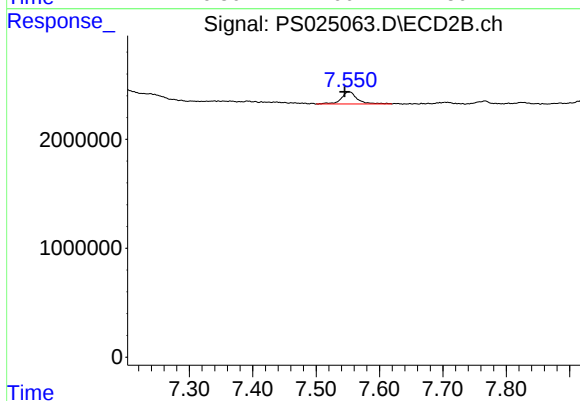

#8 DICHLORPROP


R.T.: 7.552 min
Delta R.T.: 0.007 min
Response: 1902746
Conc: 2.42 ng/ml

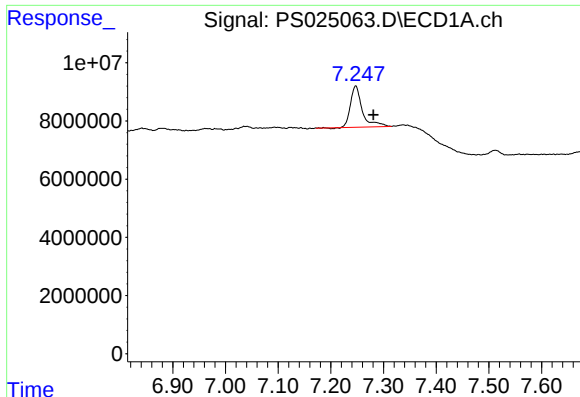

#9 2,4-D


R.T.: 7.247 min
Delta R.T.: -0.034 min
Response: 22035115
Conc: 7.25 ng/ml

Instrument :
ECD_S
ClientSampleId :
HEXANE

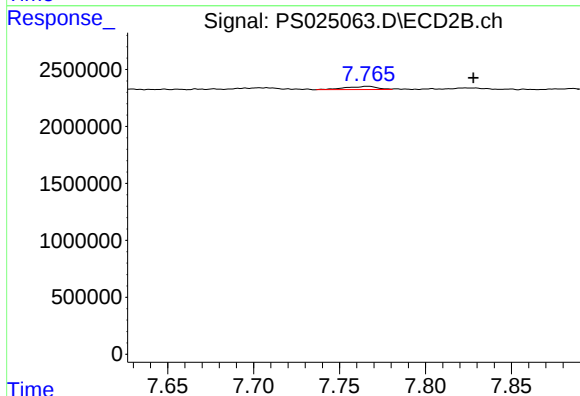


#9 2,4-D

R.T.: 7.766 min
Delta R.T.: -0.062 min
Response: 345421
Conc: N.D.

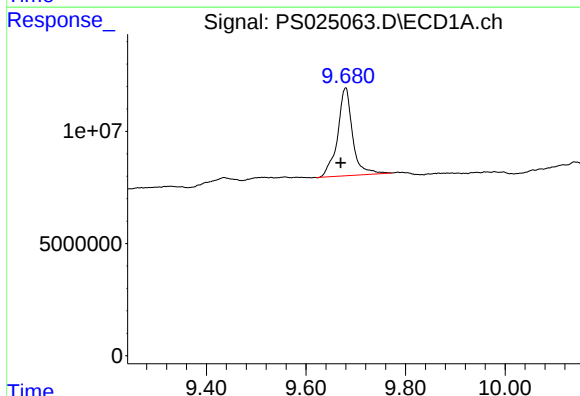


#15 Picloram

R.T.: 9.679 min
Delta R.T.: 0.010 min
Response: 81712694
Conc: 4.19 ng/ml

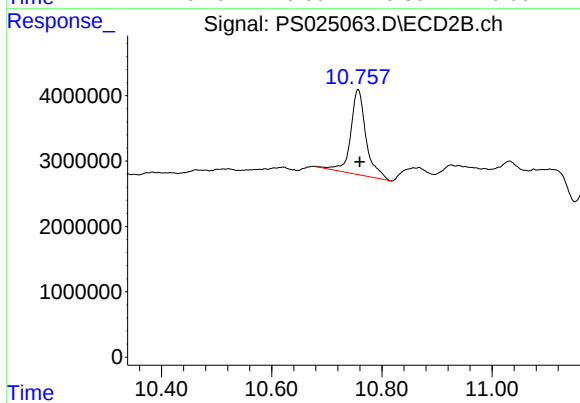

#15 Picloram


R.T.: 10.757 min
Delta R.T.: -0.003 min
Response: 25077157
Conc: 3.83 ng/ml

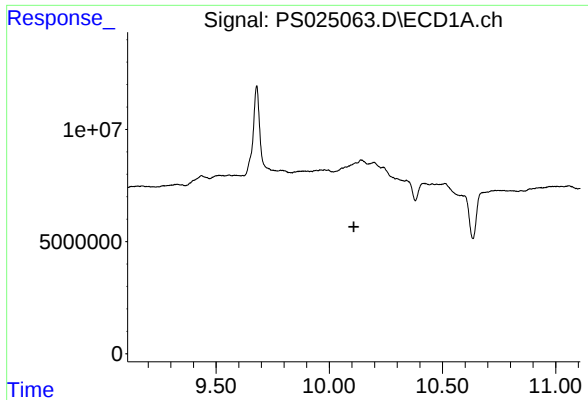

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
HEXANE

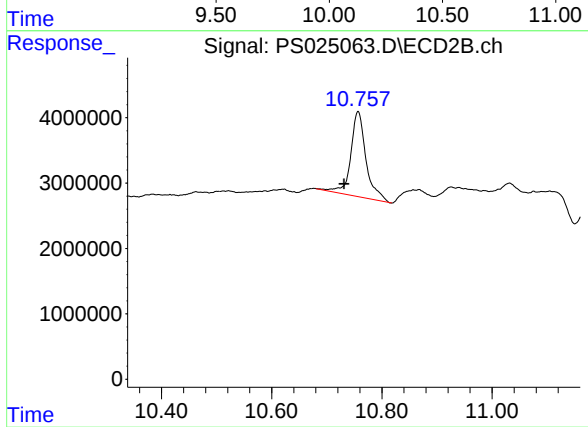

#16 DCPA

R.T.: 10.757 min
Delta R.T.: 0.025 min
Response: 25077157
Conc: 4.63 ng/ml