

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121223\
 Data File : PS025064.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 11:24
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 13:23:30 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.355	6.769	1167.1E6	371.6E6	521.523	512.857
Target Compounds							
1) T	Dalapon	2.508	2.561	8255630	4081509	2.863	3.558
2) T	3,5-DICHL...	5.697	0.000	346805	0	<MDL	N.D. #
5) T	DICAMBA	0.000	6.970	0	979450	N.D.	<MDL
6) T	MCP	0.000	6.970f	0	979450	N.D.	<MDL
8) T	DICHLORPROP	0.000	7.559	0	2035051	N.D.	2.587
11) T	2,4,5-TP ...	0.000	8.606	0	155948	N.D.	<MDL
12) T	2,4,5-T	0.000	8.978	0	543782	N.D.	<MDL
15) T	Picloram	9.683	10.761	44587174	11645877	2.288	1.779
16) T	DCPA	0.000	10.761	0	11645877	N.D.	2.149



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121223\
Data File : PS025064.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 11:24
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 13:23:30 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

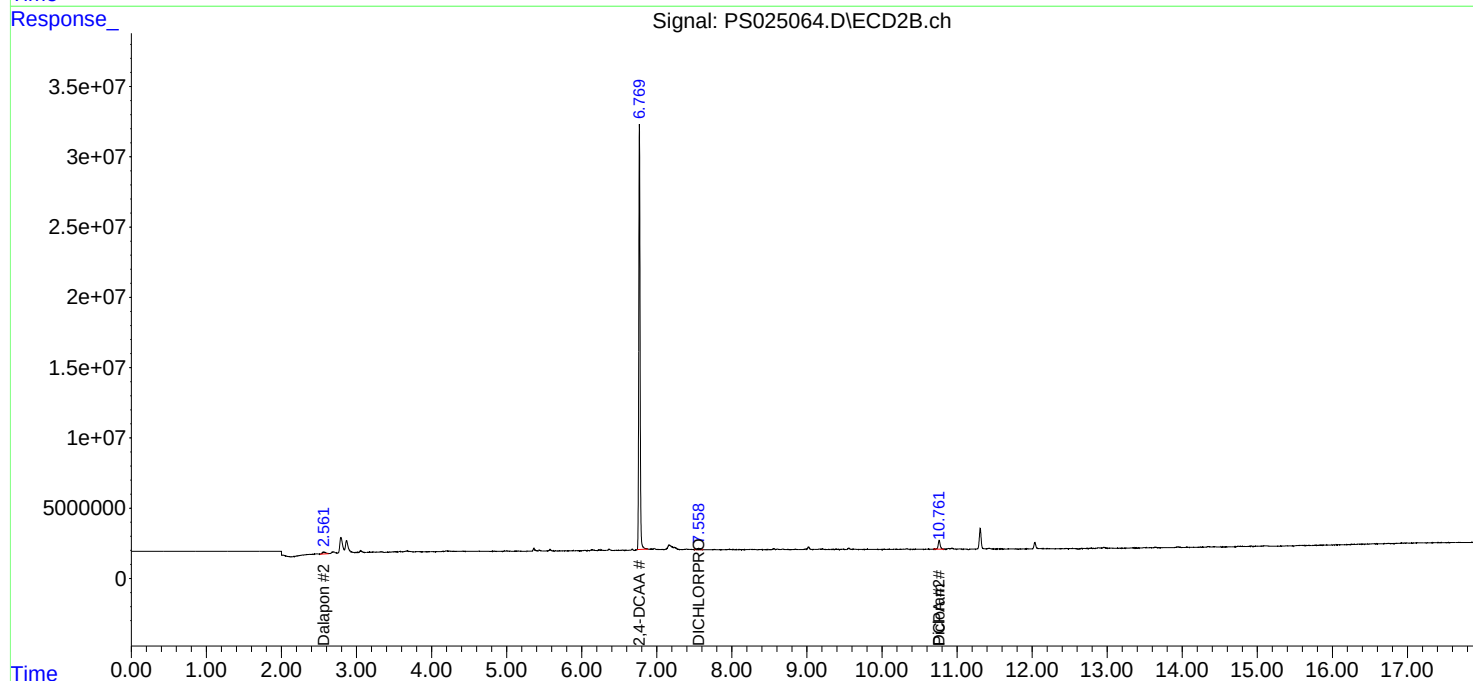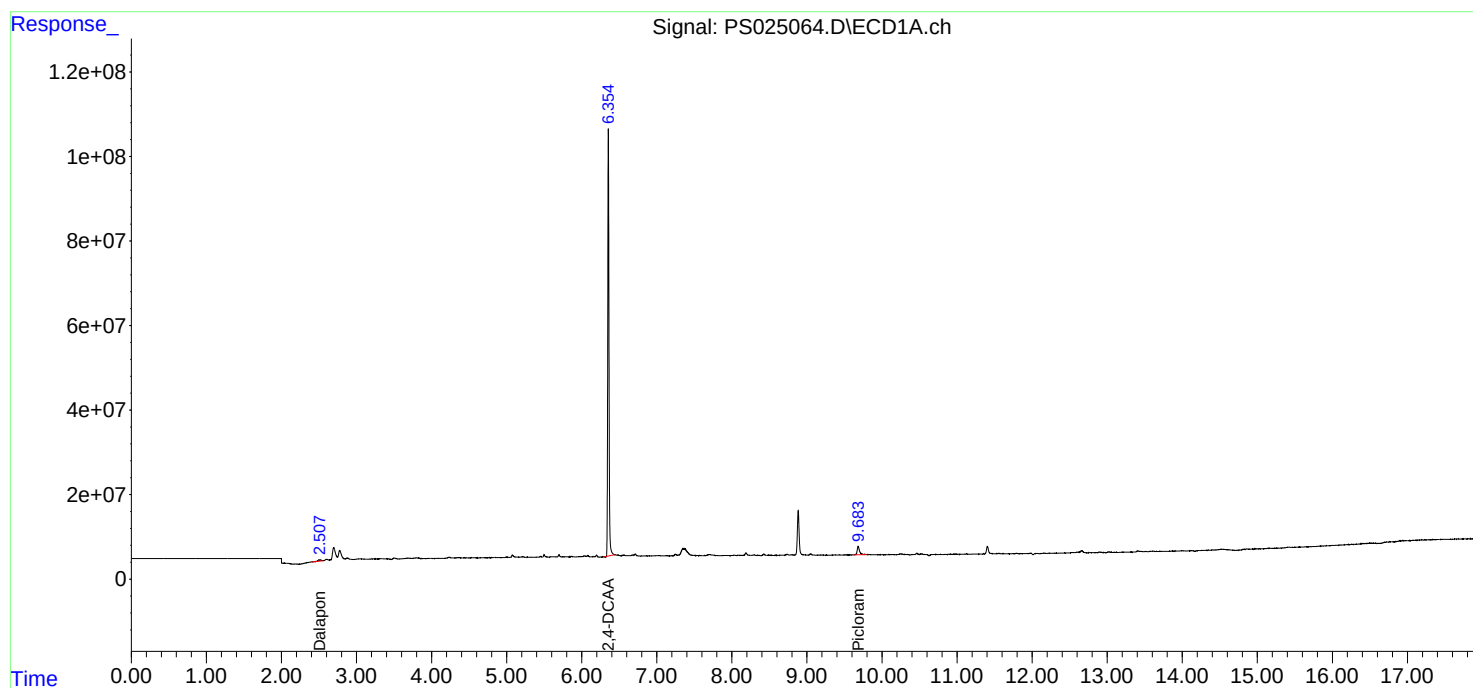


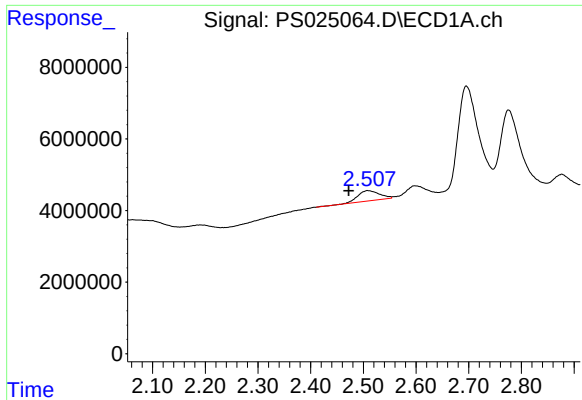

#1 Dalapon


R.T.: 2.508 min
Delta R.T.: 0.036 min
Response: 8255630
Conc: 2.86 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

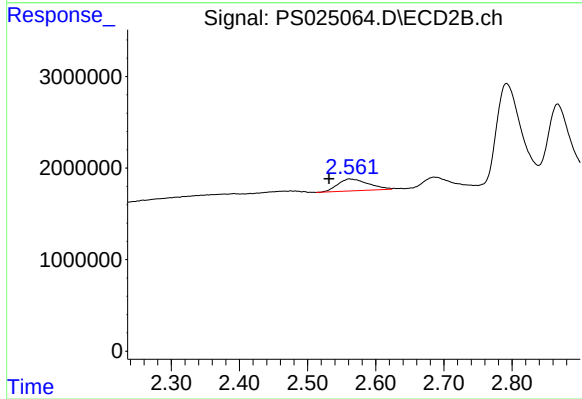


#1 Dalapon

R.T.: 2.561 min
Delta R.T.: 0.030 min
Response: 4081509
Conc: 3.56 ng/ml

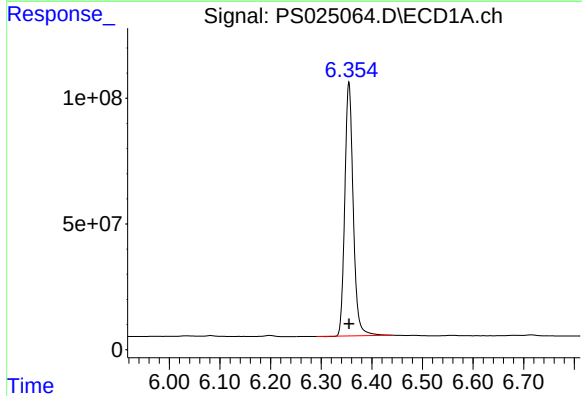


#4 2,4-DCAA

R.T.: 6.355 min
Delta R.T.: 0.000 min
Response: 1167087882
Conc: 521.52 ng/ml

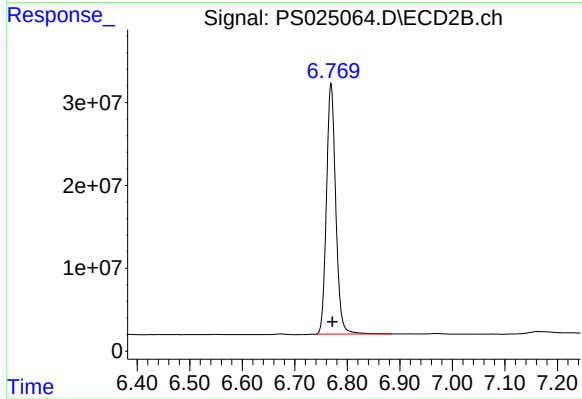

#4 2,4-DCAA


R.T.: 6.769 min
Delta R.T.: -0.002 min
Response: 371592550
Conc: 512.86 ng/ml

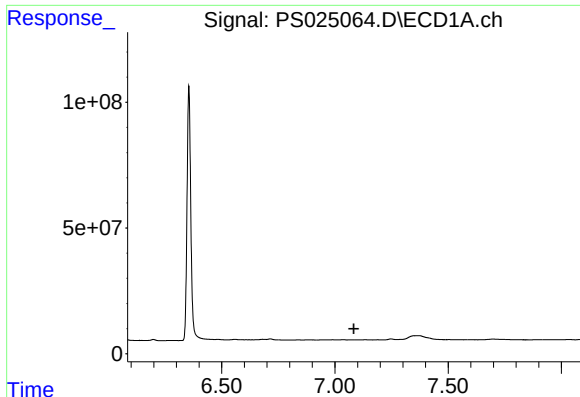

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

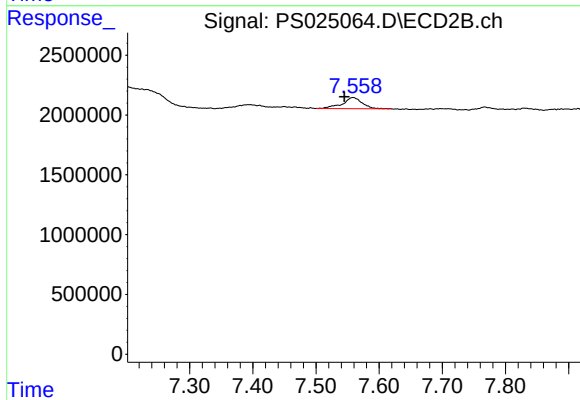


#8 DICHLORPROP

R.T.: 7.559 min
Delta R.T.: 0.014 min
Response: 2035051
Conc: 2.59 ng/ml

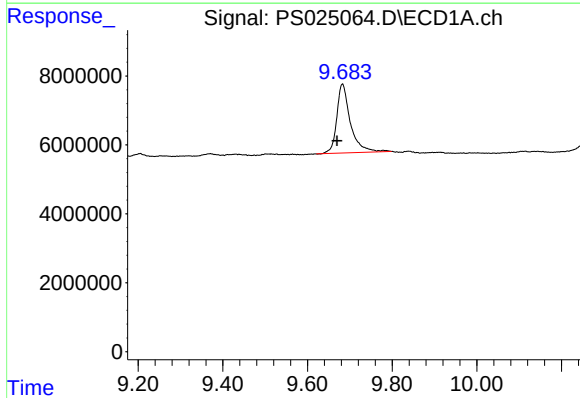


#15 Picloram

R.T.: 9.683 min
Delta R.T.: 0.013 min
Response: 44587174
Conc: 2.29 ng/ml

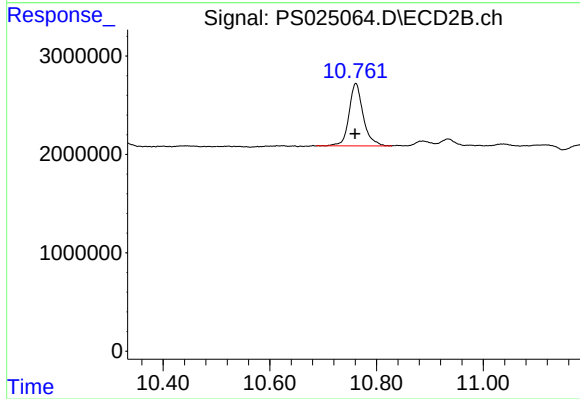

#15 Picloram


R.T.: 10.761 min
Delta R.T.: 0.001 min
Response: 11645877
Conc: 1.78 ng/ml

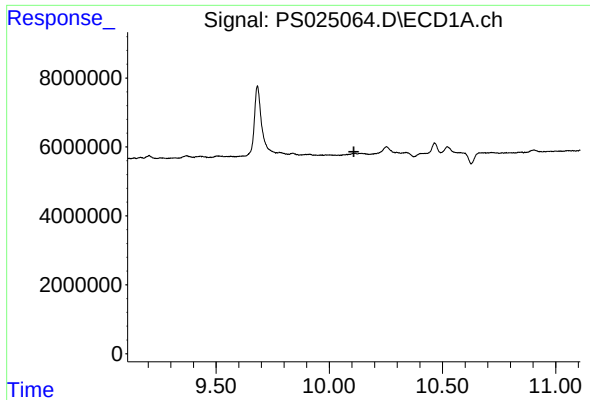

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

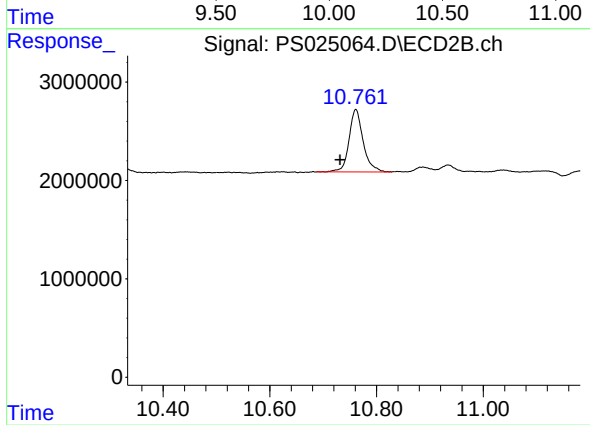

#16 DCPA

R.T.: 10.761 min
Delta R.T.: 0.030 min
Response: 11645877
Conc: 2.15 ng/ml