

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121223\
 Data File : PS025074.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2023 16:37
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 12 22:35:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 28 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	6.354	6.769	1171.0E6	374.6E6	523.264	516.989
Target Compounds							
1) T	Dalapon	2.508	2.564	8561215	4136115	2.969	3.606
2) T	3,5-DICHL...	5.696	0.000	2008077	0	<MDL	N.D. #
3) T	4-Nitroph...	6.197	0.000	7323007	0	4.973	N.D. #
5) T	DICAMBA	0.000	6.969	0	2373022	N.D.	<MDL
6) T	MCP	6.679	7.077f	4685321	591776	<MDL	<MDL #
7) T	MCPA	0.000	7.218	0	5094745	N.D.	1.549
8) T	DICHLORPROP	0.000	7.556	0	5211461	N.D.	6.625
9) T	2,4-D	7.245	7.766f	12417531	678084	4.088	<MDL #
10) T	Pentachlo...	0.000	8.301f	0	837336	N.D.	<MDL
11) T	2,4,5-TP ...	0.000	8.608	0	39083	N.D.	<MDL
12) T	2,4,5-T	0.000	8.979	0	1010257	N.D.	<MDL
13) T	2,4-DB	0.000	9.474	0	1050500	N.D.	1.898
15) T	Picloram	9.677	10.759	85584105	23837730	4.392	3.642
16) T	DCPA	0.000	10.759	0	23837730	N.D.	4.398



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121223\
Data File : PS025074.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2023 16:37
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 12 22:35:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112823.M
Quant Title : 8080.M
QLast Update : Tue Nov 28 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

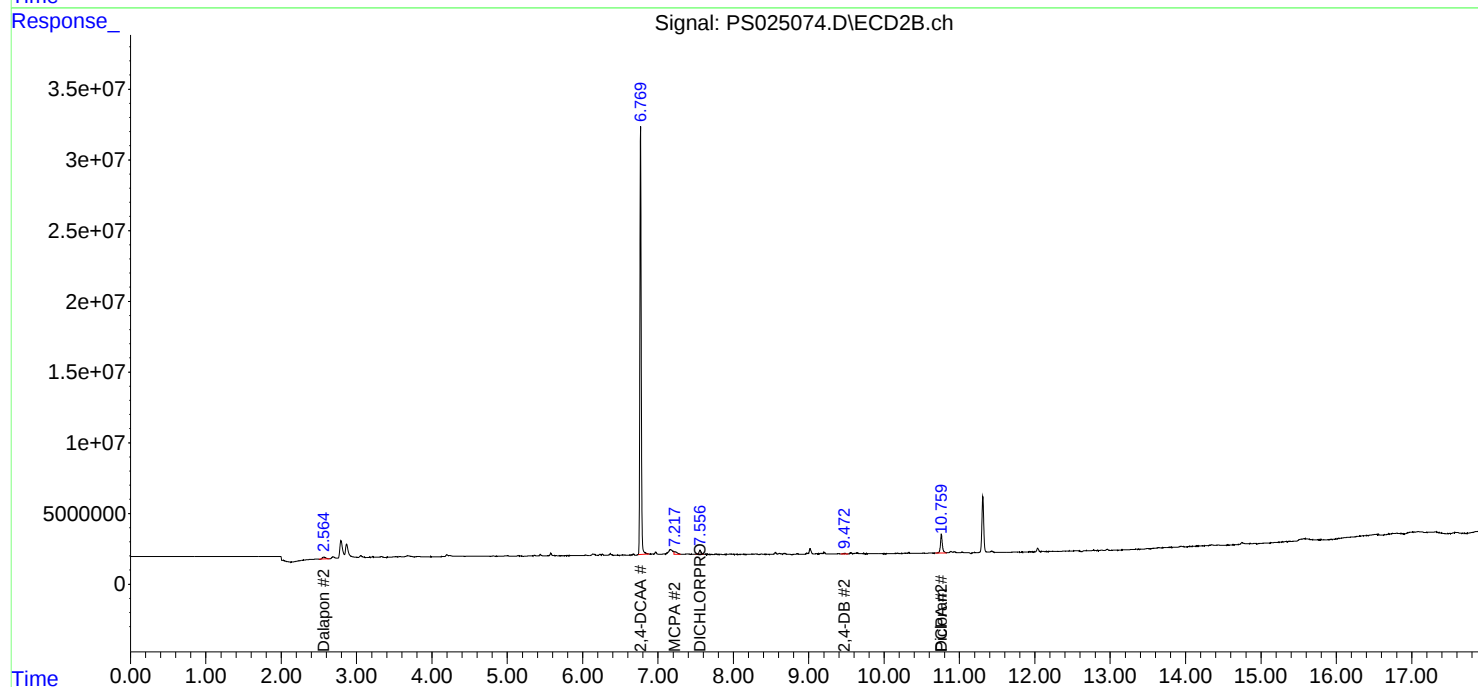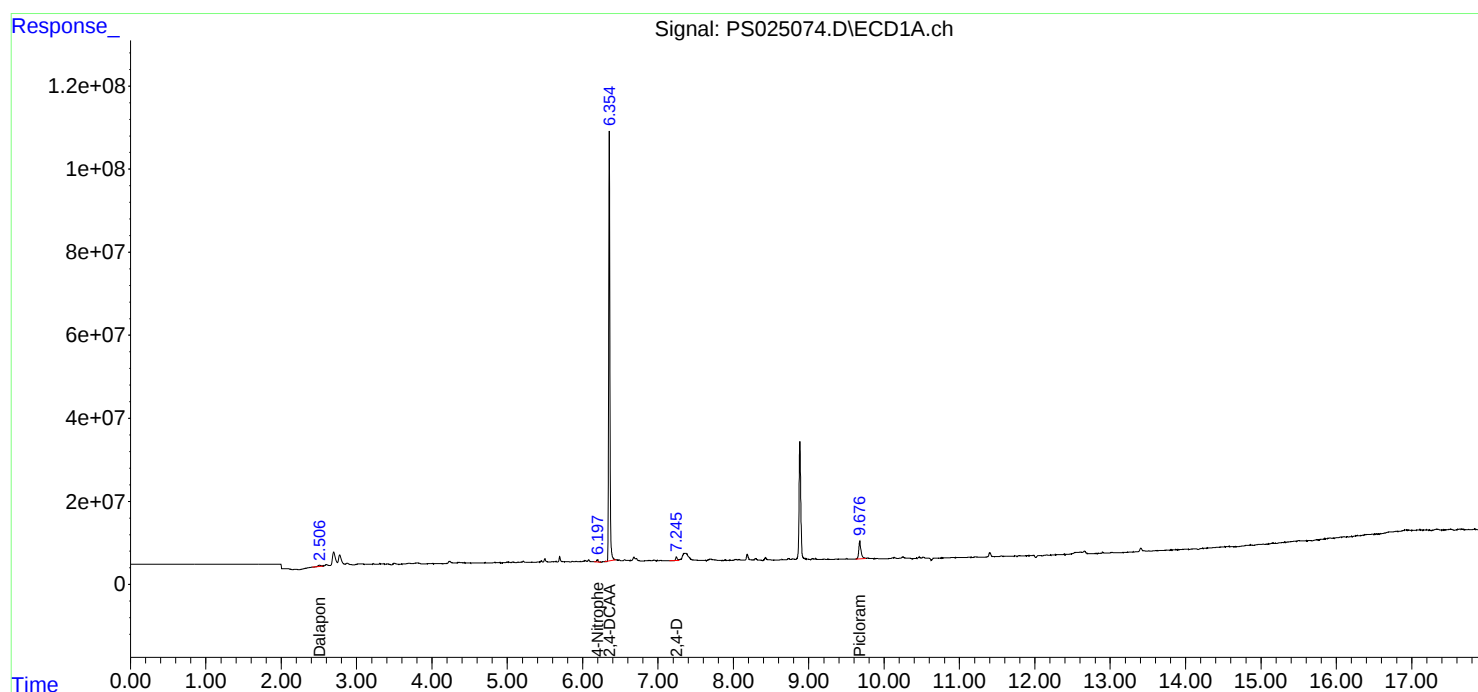


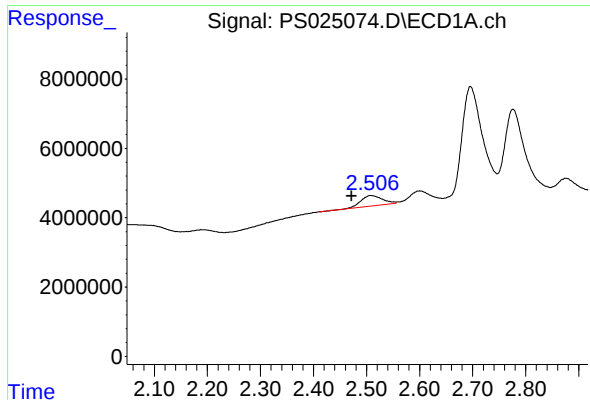

#1 Dalapon


R.T.: 2.508 min
Delta R.T.: 0.036 min
Response: 8561215
Conc: 2.97 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

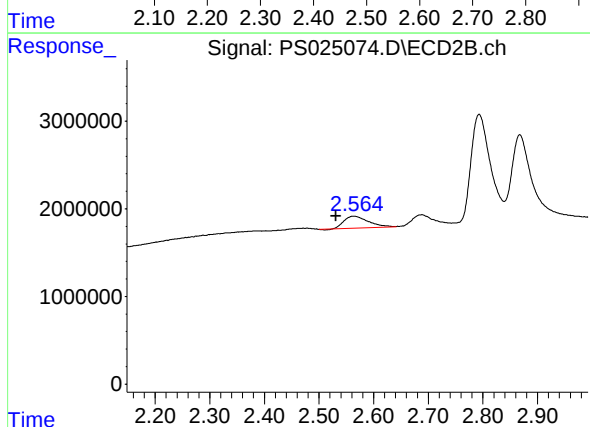


#1 Dalapon

R.T.: 2.564 min
Delta R.T.: 0.033 min
Response: 4136115
Conc: 3.61 ng/ml

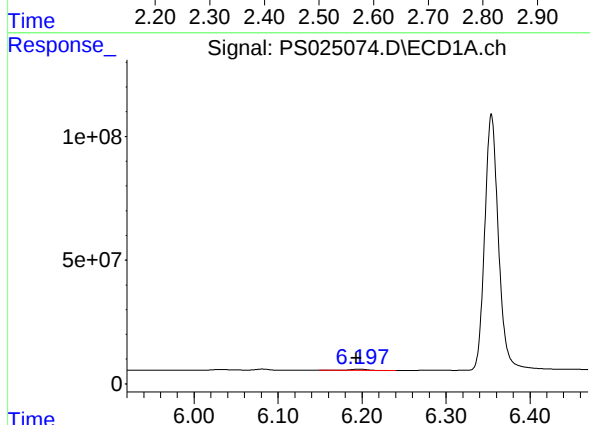


#3 4-Nitrophenol

R.T.: 6.197 min
Delta R.T.: 0.004 min
Response: 7323007
Conc: 4.97 ng/ml

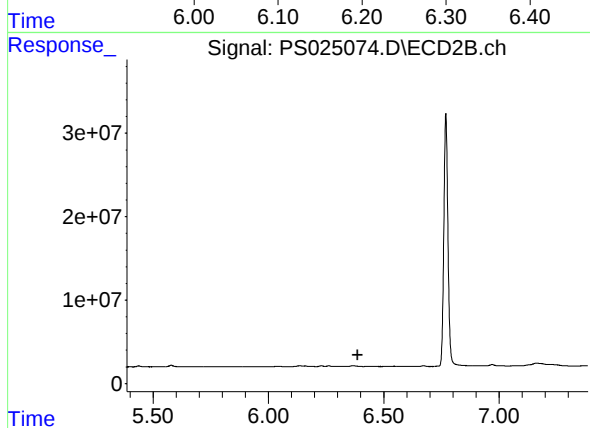

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 6.386 min
Response: 0
Conc: N.D.

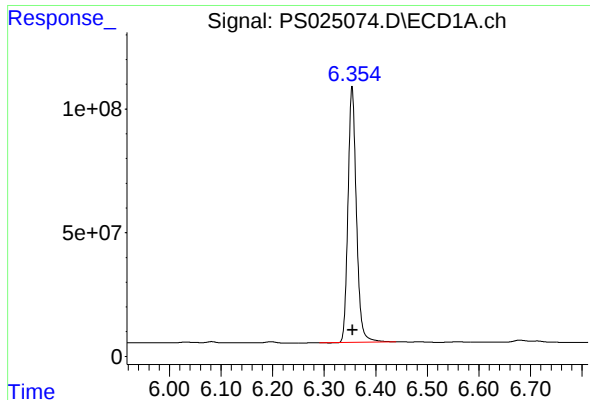

#4 2,4-DCAA


R.T.: 6.354 min
Delta R.T.: 0.000 min
Response: 1170983581
Conc: 523.26 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

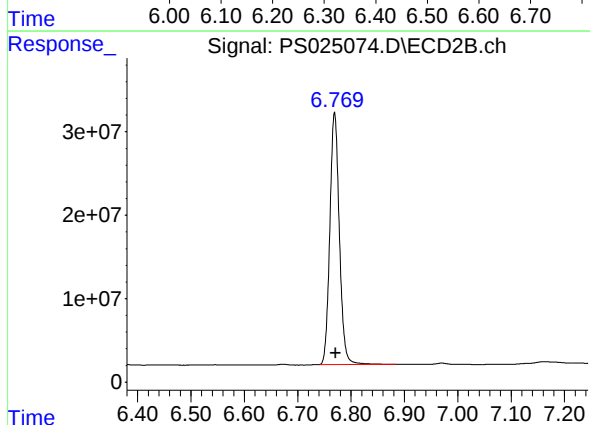


#4 2,4-DCAA

R.T.: 6.769 min
Delta R.T.: -0.002 min
Response: 374587052
Conc: 516.99 ng/ml

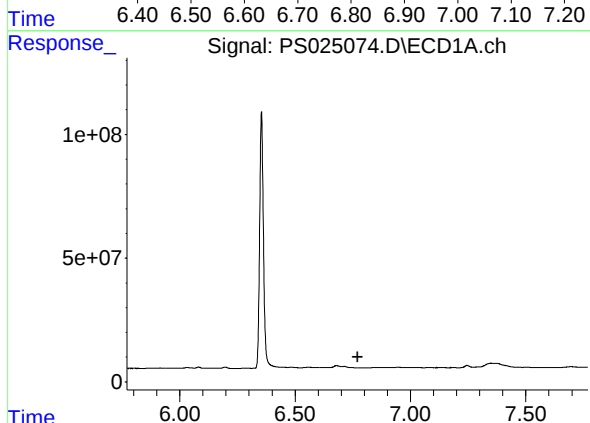


#7 MCPA

R.T.: 0.000 min
Exp R.T.: 6.771 min
Response: 0
Conc: N.D.

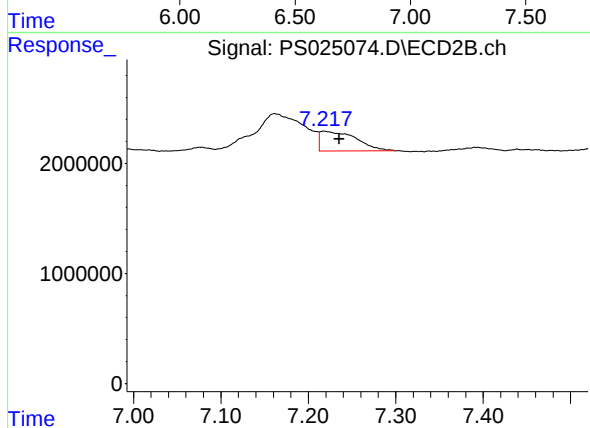

#7 MCPA


R.T.: 7.218 min
Delta R.T.: -0.018 min
Response: 5094745
Conc: 1.55 ug/ml

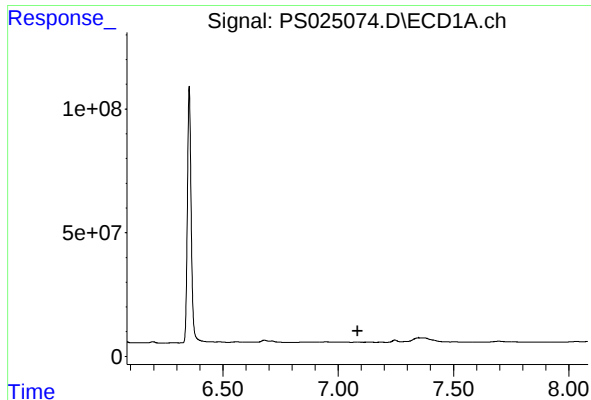

#8 DICHLORPROP


R.T.: 0.000 min
Exp R.T.: 7.083 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

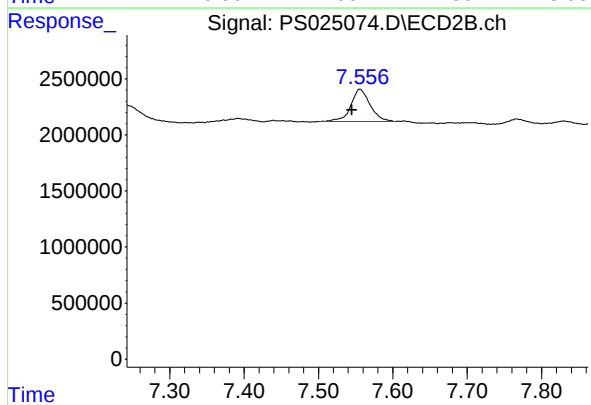


#8 DICHLORPROP

R.T.: 7.556 min
Delta R.T.: 0.011 min
Response: 5211461
Conc: 6.62 ng/ml

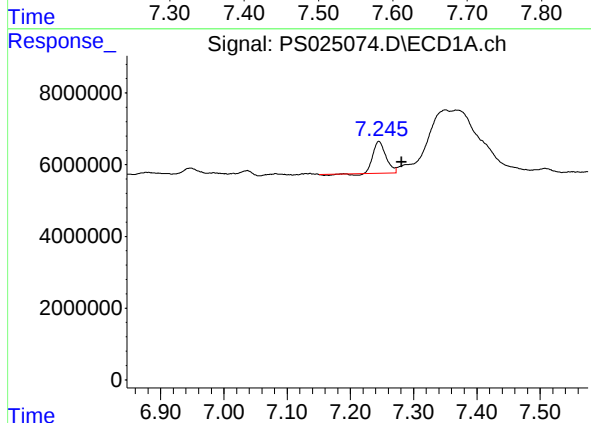


#9 2,4-D

R.T.: 7.245 min
Delta R.T.: -0.036 min
Response: 12417531
Conc: 4.09 ng/ml

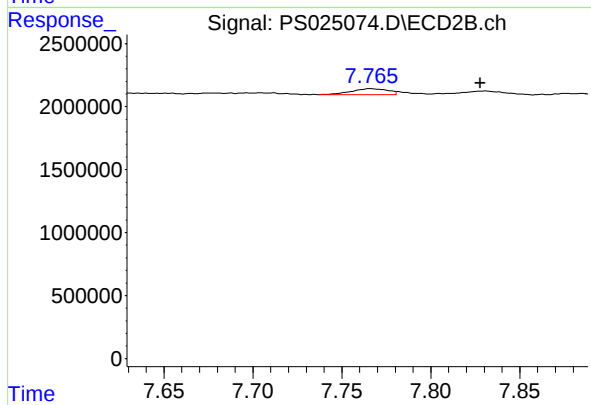

#9 2,4-D


R.T.: 7.766 min
Delta R.T.: -0.062 min
Response: 678084
Conc: N.D.

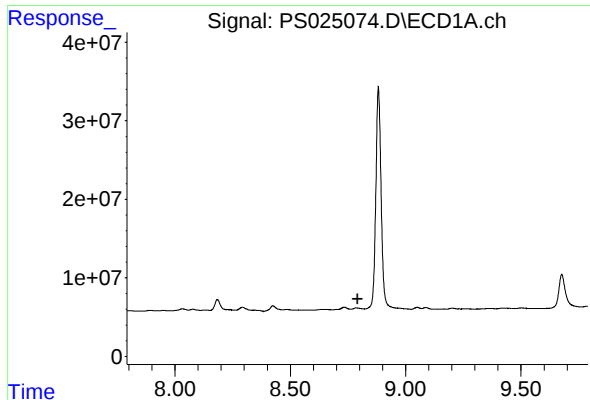

#13 2,4-DB


R.T.: 0.000 min
Exp R.T.: 8.791 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

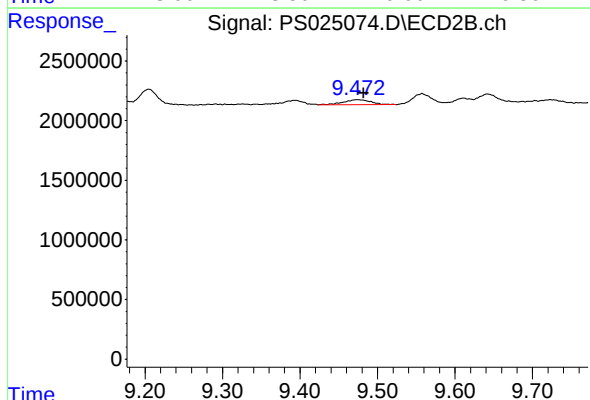


#13 2,4-DB

R.T.: 9.474 min
Delta R.T.: -0.008 min
Response: 1050500
Conc: 1.90 ng/ml

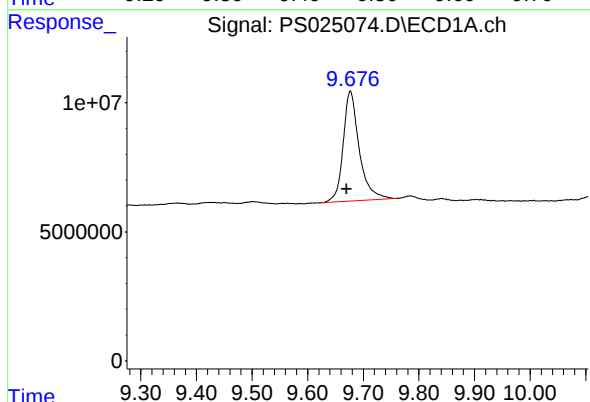


#15 Picloram

R.T.: 9.677 min
Delta R.T.: 0.007 min
Response: 85584105
Conc: 4.39 ng/ml

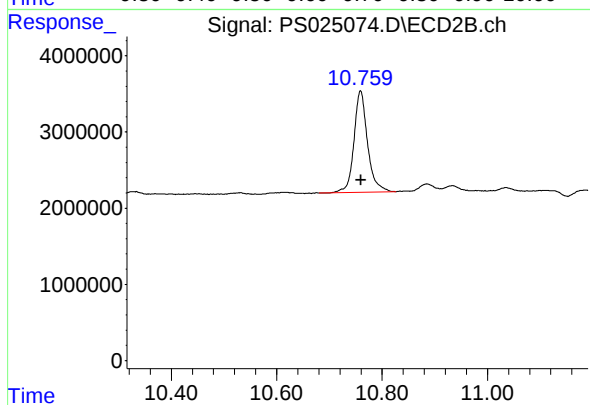

#15 Picloram


R.T.: 10.759 min
Delta R.T.: 0.000 min
Response: 23837730
Conc: 3.64 ng/ml

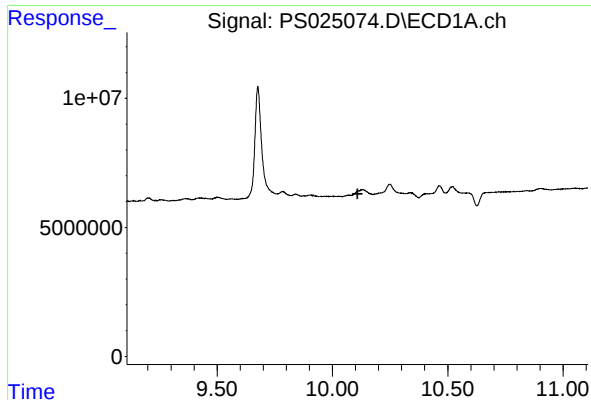

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 10.109 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :
I.BLK

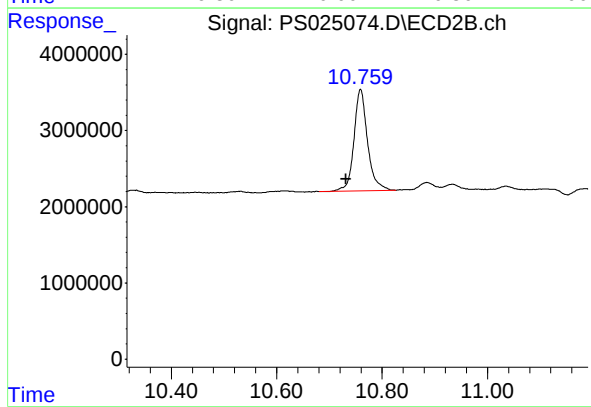

#16 DCPA

R.T.: 10.759 min
Delta R.T.: 0.027 min
Response: 23837730
Conc: 4.40 ng/ml