

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121224\
 Data File : PS028763.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2024 10:16
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:01:39 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.222	7.714	1309.1E6	570.3E6	488.041	423.348
Target Compounds							
1) T	Dalapon	2.671f	0.000	20294798	0	6.994	N.D. #
2) T	3,5-DICHL...	6.402	0.000	360778	0	<MDL	N.D. #
3) T	4-Nitroph...	7.019	0.000	4905644	0	2.854	N.D. #
5) T	DICAMBA	0.000	7.915	0	3501385	N.D.	<MDL
7) T	MCPA	7.762	8.239f	308731	10490200	<MDL	1.690 #
8) T	DICHLORPROP	8.090f	0.000	855842	0	<MDL	N.D. #
10) T	Pentachlo...	8.645	0.000	1393160	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.220	0.000	682039	0	<MDL	N.D. #
12) T	2,4,5-T	9.526	0.000	1685435	0	<MDL	N.D. #
14) T	DINOSEB	11.292	0.000	1805995	0	<MDL	N.D. #
15) T	Picloram	11.137f	12.331	11964250	4822159	<MDL	<MDL #
16) T	DCPA	11.591	0.000	1562953	0	<MDL	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121224\
Data File : PS028763.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2024 10:16
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:01:39 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

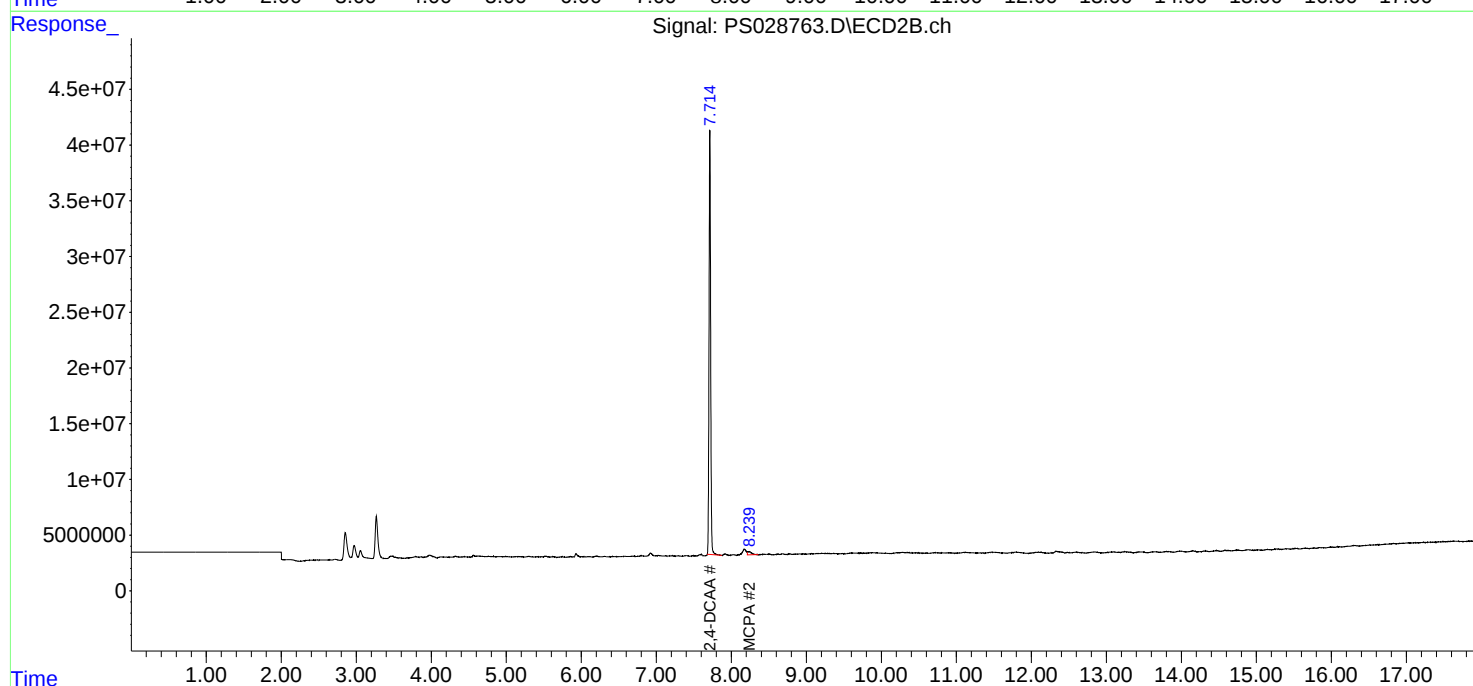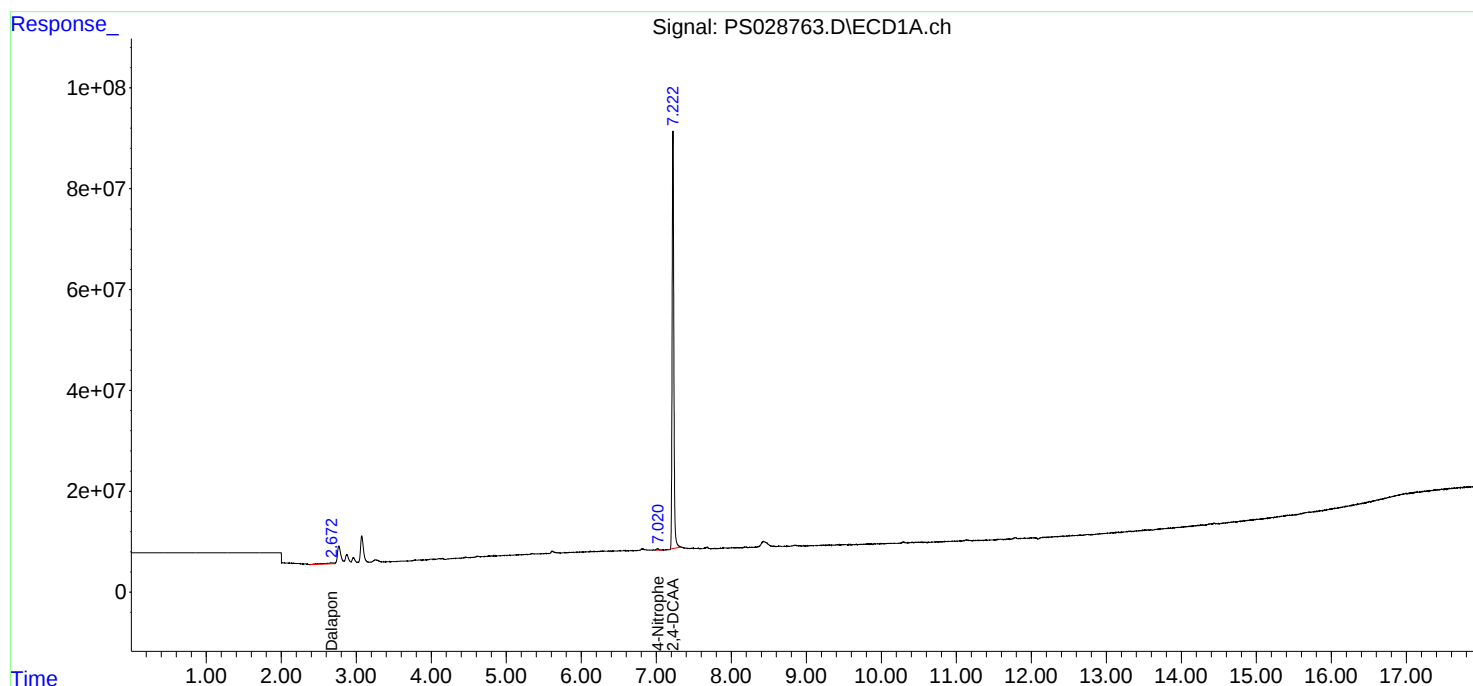


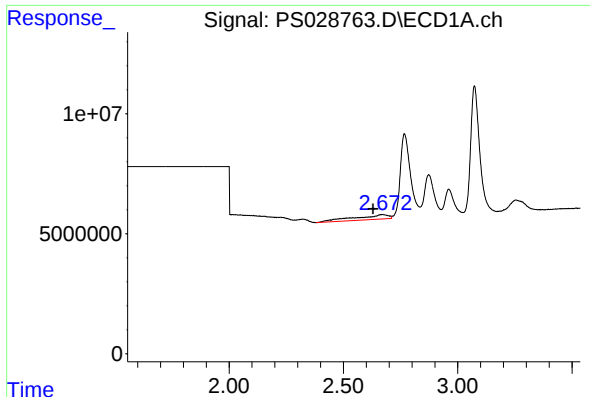

#1 Dalapon


R.T.: 2.671 min
Delta R.T.: 0.041 min
Response: 20294798
Conc: 6.99 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

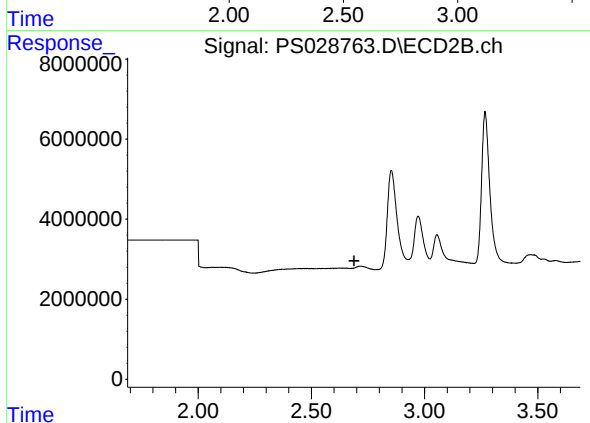


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

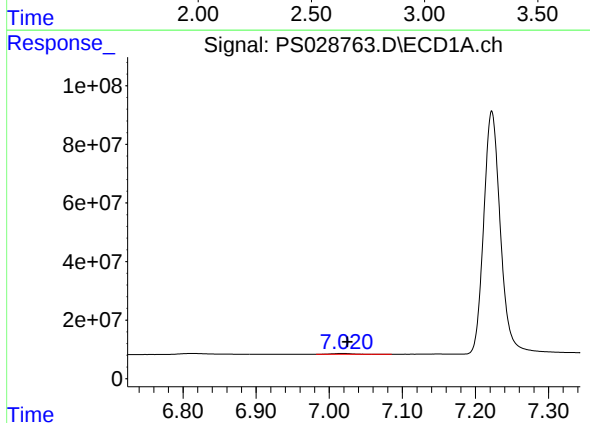


#3 4-Nitrophenol

R.T.: 7.019 min
Delta R.T.: -0.006 min
Response: 4905644
Conc: 2.85 ng/ml

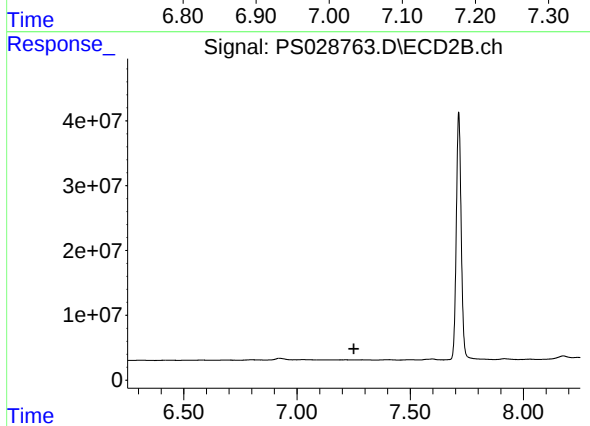

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

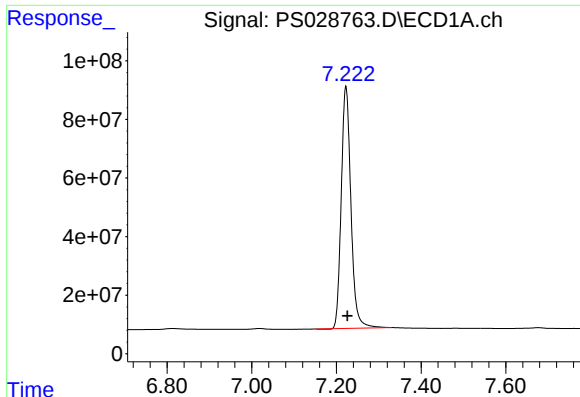

#4 2,4-DCAA


R.T.: 7.222 min
Delta R.T.: -0.004 min
Response: 1309092697
Conc: 488.04 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

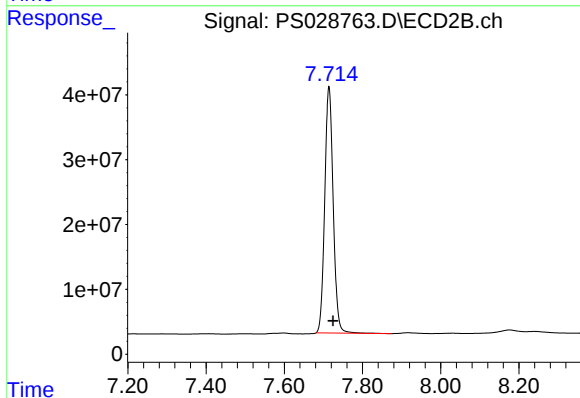


#4 2,4-DCAA

R.T.: 7.714 min
Delta R.T.: -0.010 min
Response: 570262171
Conc: 423.35 ng/ml

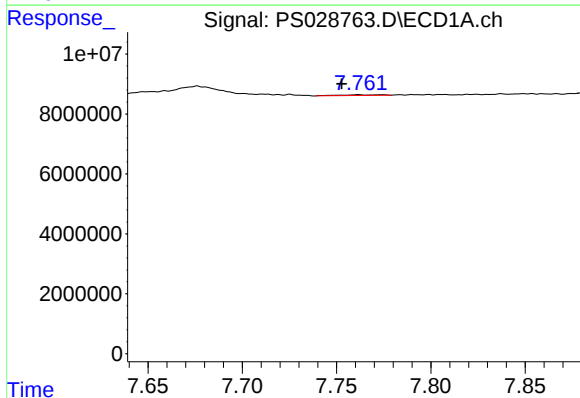

#7 MCPA

R.T.: 7.762 min
Delta R.T.: 0.009 min
Response: 308731
Conc: N.D.

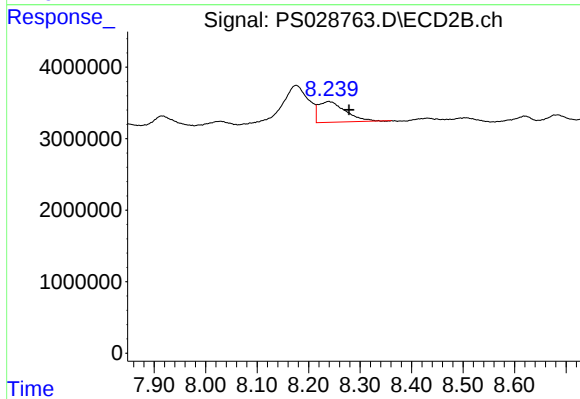

#7 MCPA

R.T.: 8.239 min
Delta R.T.: -0.039 min
Response: 10490200
Conc: 1.69 ug/ml