

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121224\
 Data File : PS028774.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 12 Dec 2024 20:17
 Operator : AR\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 13 03:05:13 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
 Quant Title : 8080.M
 QLast Update : Tue Nov 26 14:44:30 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	7.220	7.713	1310.3E6	581.8E6	488.476	431.932
Target Compounds							
1) T	Dalapon	2.669f	0.000	20182599	0	6.955	N.D. #
2) T	3,5-DICHL...	6.418	0.000	205010	0	<MDL	N.D. #
3) T	4-Nitroph...	7.016	0.000	5130385	0	2.985	N.D. #
5) T	DICAMBA	0.000	7.911	0	4886107	N.D.	<MDL
7) T	MCPA	7.767	0.000	348098	0	<MDL	N.D. #
8) T	DICHLORPROP	8.121	8.677f	213890	6988457	<MDL	4.372 #
10) T	Pentachlo...	8.639	0.000	1310685	0	<MDL	N.D. #
11) T	2,4,5-TP ...	9.216	0.000	305228	0	<MDL	N.D. #
12) T	2,4,5-T	9.516	10.279	2903899	6354760	<MDL	<MDL #
14) T	DINOSEB	11.308	0.000	1176566	0	<MDL	N.D. #
15) T	Picloram	11.114	12.320	14649254	3569605	<MDL	<MDL #
16) T	DCPA	11.583	12.320f	2530626	3569605	<MDL	<MDL #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121224\
Data File : PS028774.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 12 Dec 2024 20:17
Operator : AR\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 13 03:05:13 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS112624.M
Quant Title : 8080.M
QLast Update : Tue Nov 26 14:44:30 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

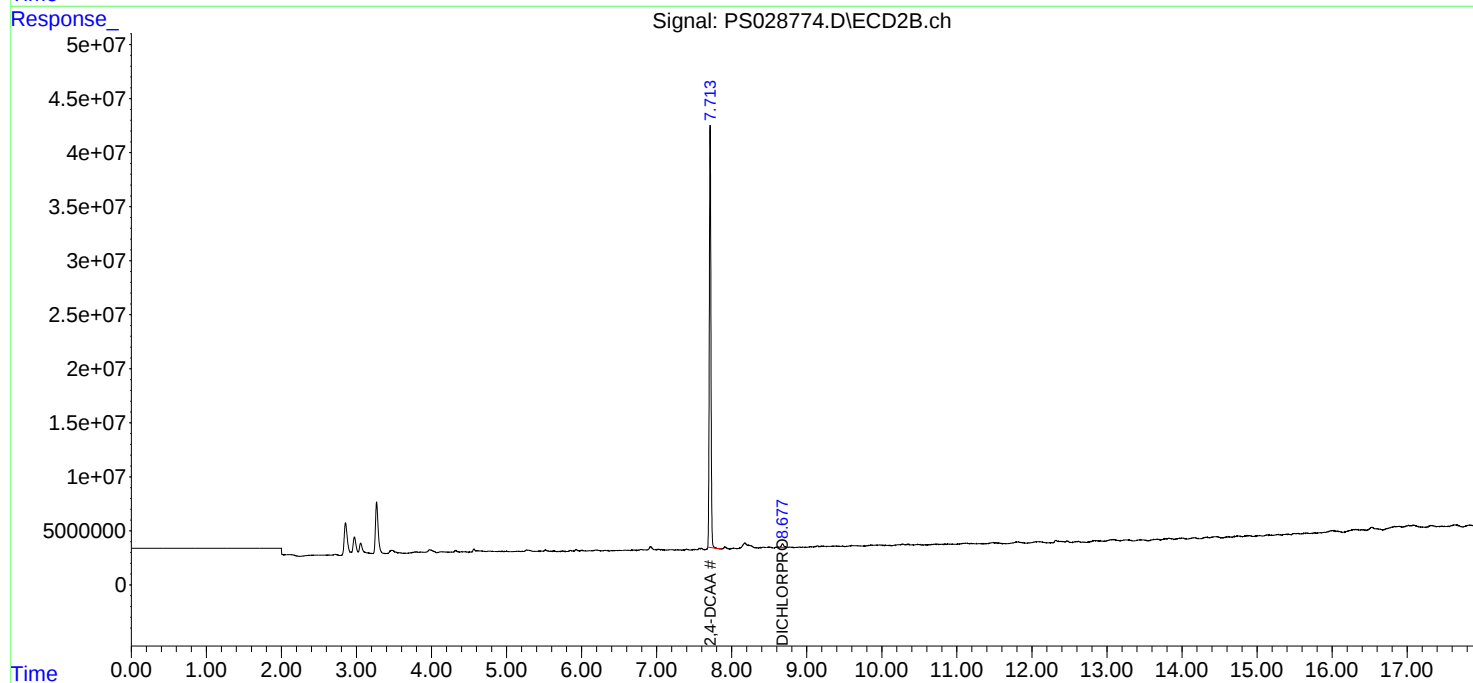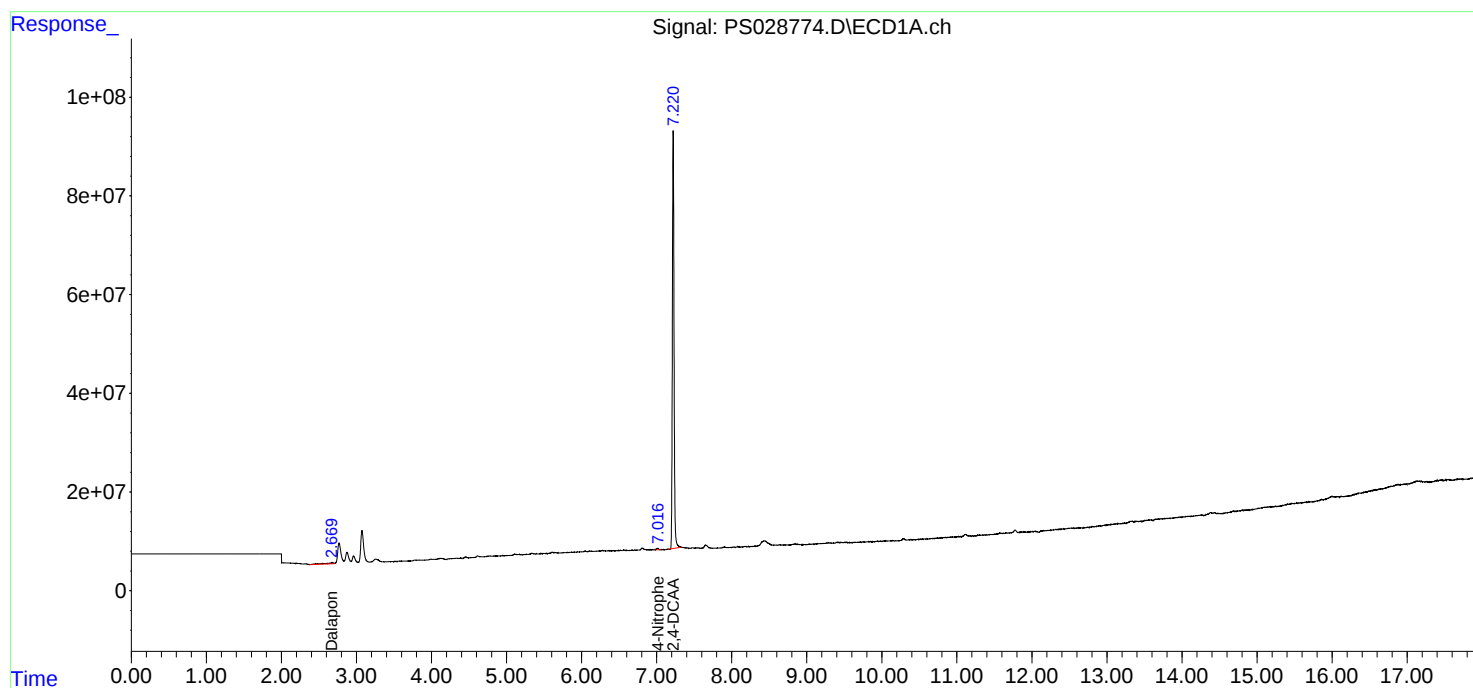


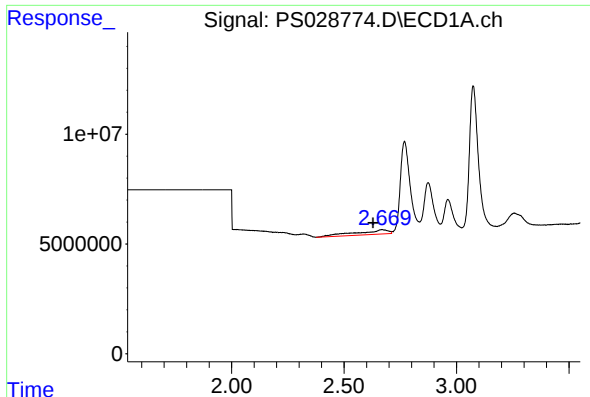

#1 Dalapon


R.T.: 2.669 min
Delta R.T.: 0.039 min
Response: 20182599
Conc: 6.96 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

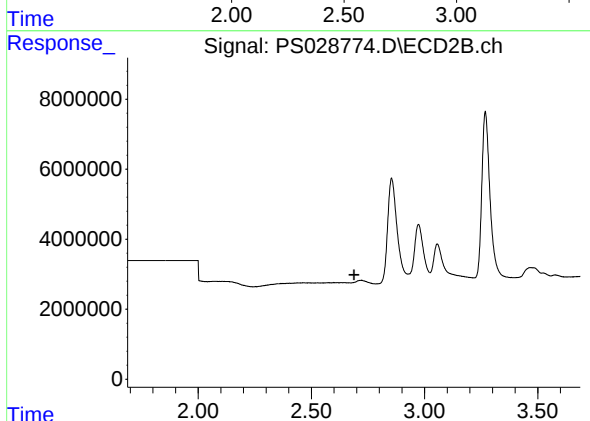


#1 Dalapon

R.T.: 0.000 min
Exp R.T. : 2.688 min
Response: 0
Conc: N.D.

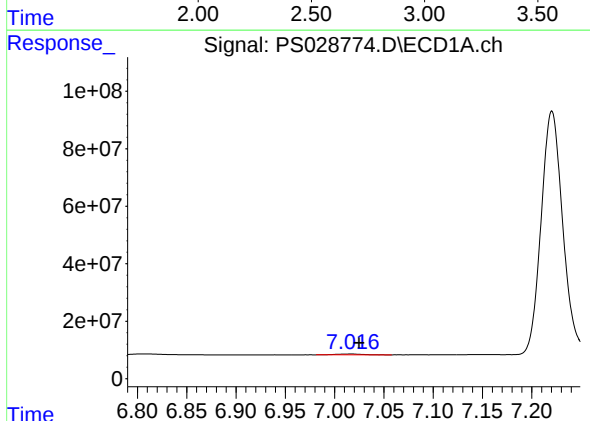


#3 4-Nitrophenol

R.T.: 7.016 min
Delta R.T.: -0.009 min
Response: 5130385
Conc: 2.98 ng/ml

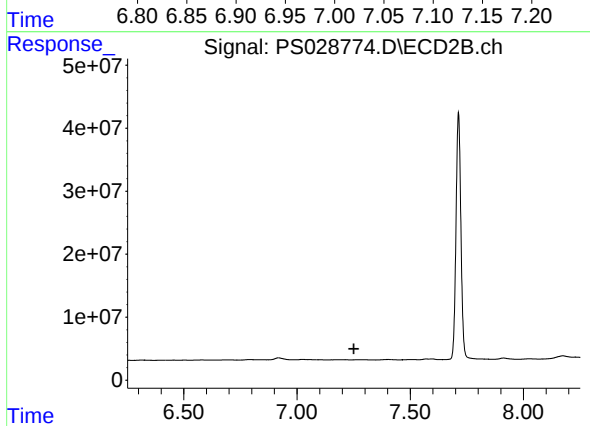

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T. : 7.251 min
Response: 0
Conc: N.D.

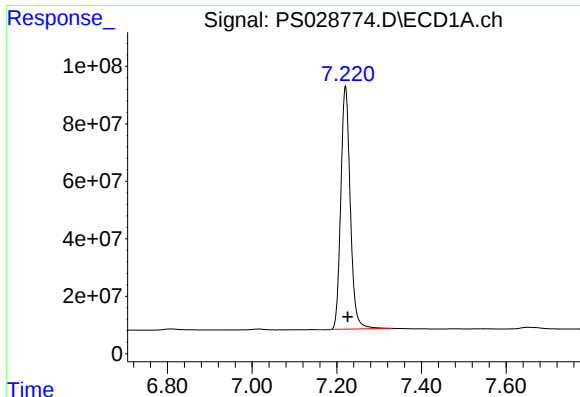

#4 2,4-DCAA


R.T.: 7.220 min
Delta R.T.: -0.006 min
Response: 1310260675
Conc: 488.48 ng/ml

Instrument :
ECD_S
ClientSampleId :
I.BLK

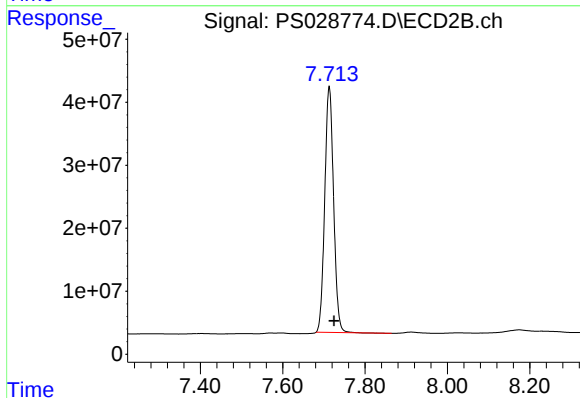


#4 2,4-DCAA

R.T.: 7.713 min
Delta R.T.: -0.012 min
Response: 581825031
Conc: 431.93 ng/ml

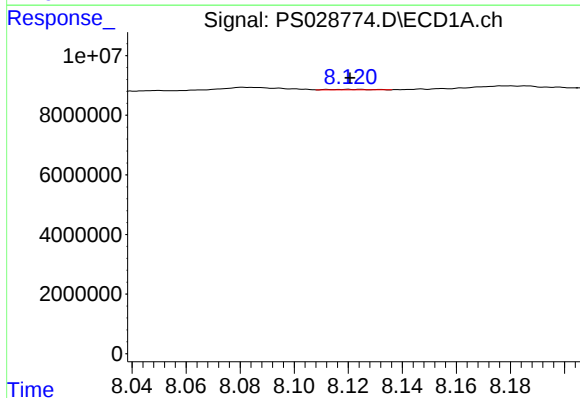

#8 DICHLORPROP

R.T.: 8.121 min
Delta R.T.: 0.000 min
Response: 213890
Conc: N.D.

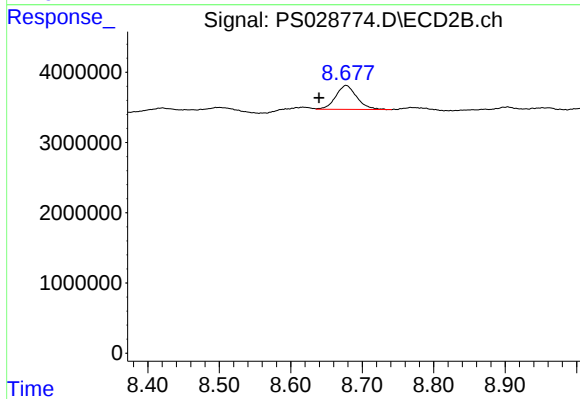

#8 DICHLORPROP

R.T.: 8.677 min
Delta R.T.: 0.038 min
Response: 6988457
Conc: 4.37 ng/ml