

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
 Data File : PS002593.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2018 19:42
 Operator : EI\SJ
 Sample : PB115583BL
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 05:01:19 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.397	10.895	174.5E6	174.9E6	549.801	452.091
Target Compounds							
1) T	Dalapon	2.881	2.338	8105225	6379414	17.608	14.017
3) T	4-Nitroph...	0.000	10.054	0	1096141	N.D.	6.133 #
5) T	DICAMBA	0.000	11.138	0	78431550	N.D.	55.016 #
6) T	MCP	12.080	0.000	66090286	0	66.239	N.D. #
7) T	MCPA	12.353	11.794	1128356	4377091	0.749	3.045 #
9) T	2,4-D	0.000	12.731	0	926022	N.D.	2.186 #
11) T	2,4,5-TP ...	0.000	13.909	0	8137586	N.D.	3.876 #
14) T	DINOSEB	0.000	15.644	0	1072681	N.D.	0.703 #
15) T	Picloram	16.876	16.778	4821291	6877445	1.900	2.500 #
16) T	DCPA	0.000	16.843	0	8187891	N.D.	2.818 #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
Data File : PS002593.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2018 19:42
Operator : EI\SJ
Sample : PB115583BL
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 05:01:19 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

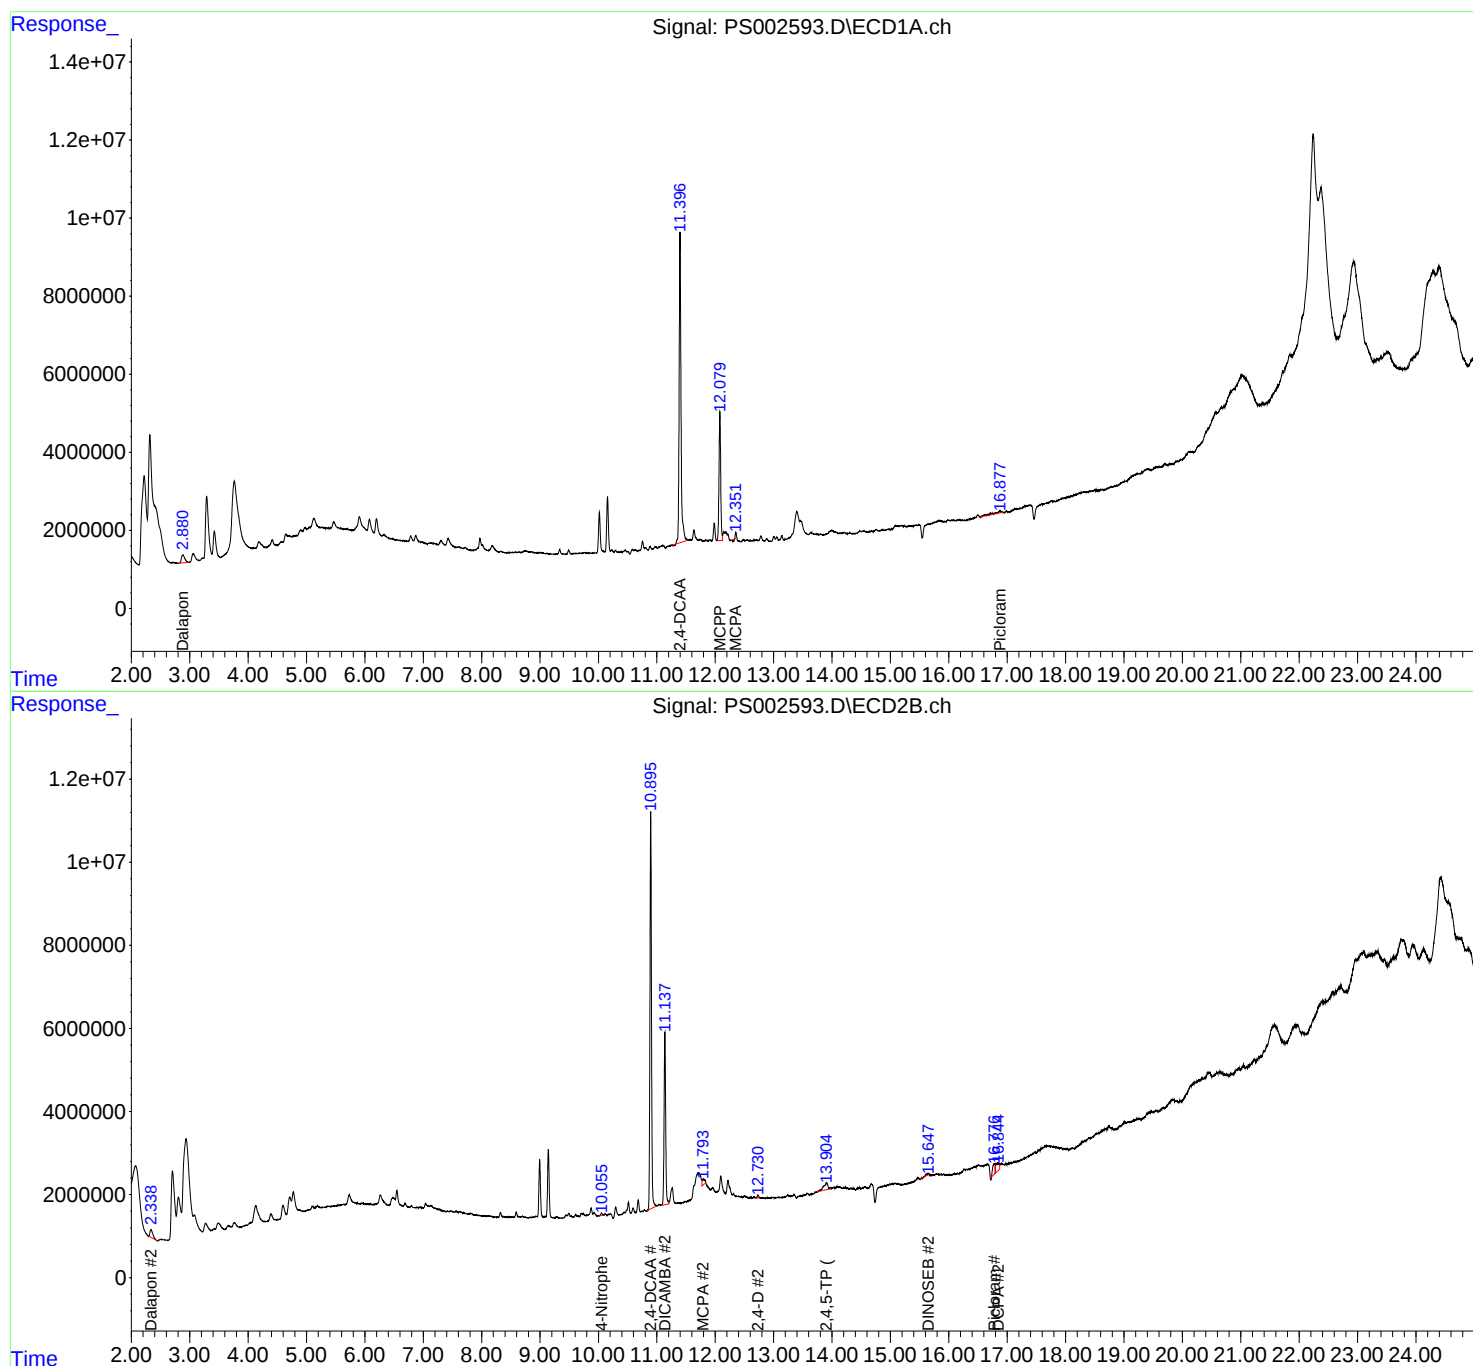


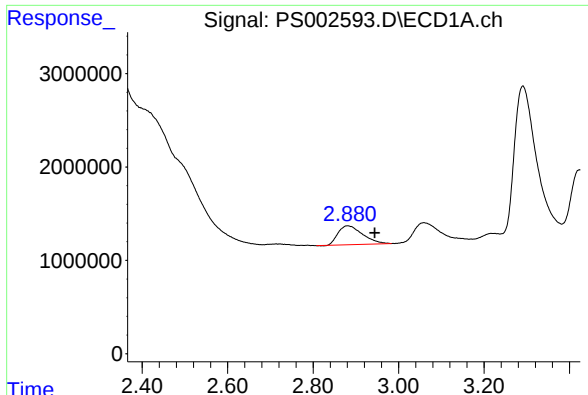

#1 Dalapon


R.T.: 2.881 min
Delta R.T.: -0.063 min
Response: 8105225
Conc: 17.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

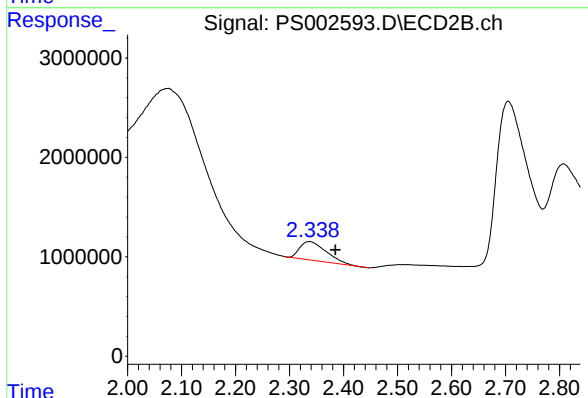


#1 Dalapon

R.T.: 2.338 min
Delta R.T.: -0.047 min
Response: 6379414
Conc: 14.02 ng/ml

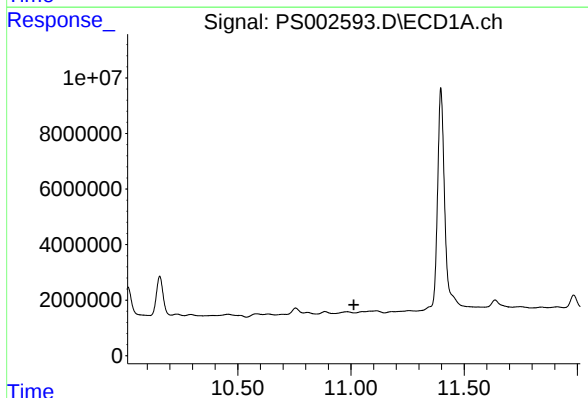


#3 4-Nitrophenol

R.T.: 0.000 min
Exp R.T. : 11.013 min
Response: 0
Conc: N.D.

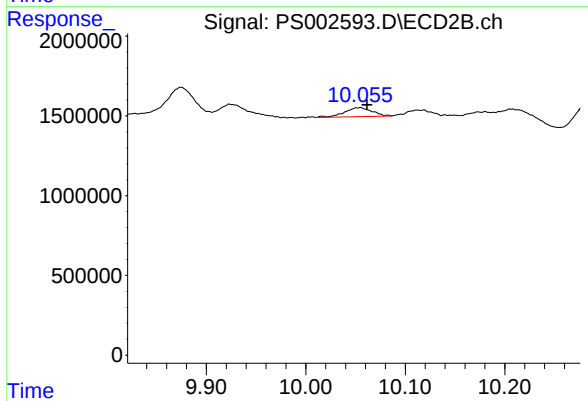

#3 4-Nitrophenol


R.T.: 10.054 min
Delta R.T.: -0.008 min
Response: 1096141
Conc: 6.13 ng/ml

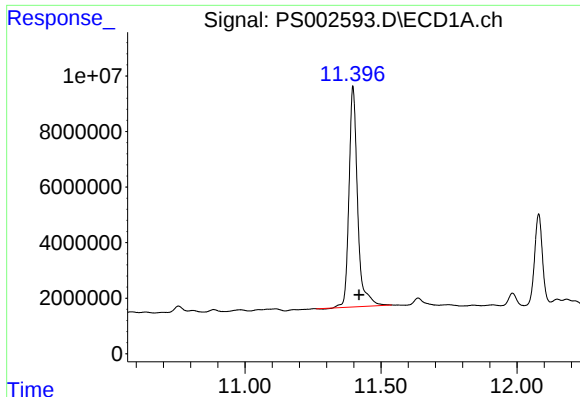

#4 2,4-DCAA


R.T.: 11.397 min
Delta R.T.: -0.023 min
Response: 174517855
Conc: 549.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

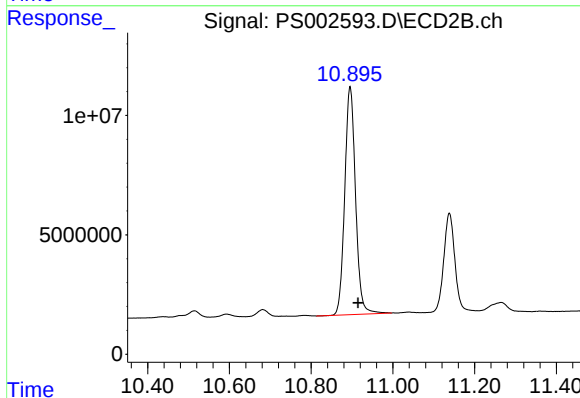


#4 2,4-DCAA

R.T.: 10.895 min
Delta R.T.: -0.019 min
Response: 174855282
Conc: 452.09 ng/ml

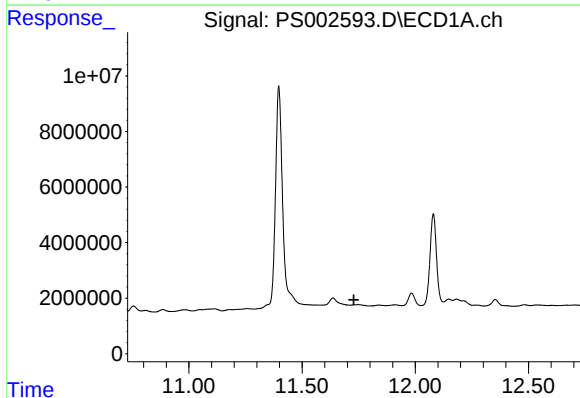


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.729 min
Response: 0
Conc: N.D.

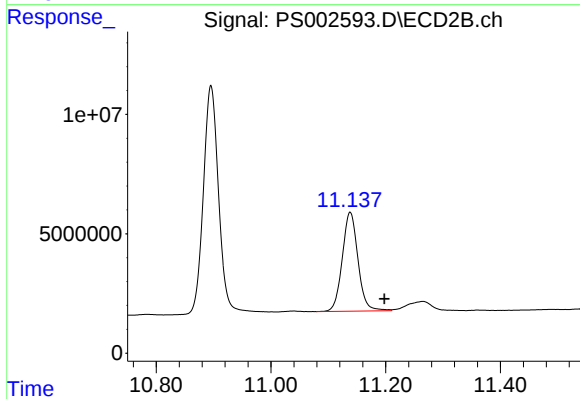

#5 DICAMBA


R.T.: 11.138 min
Delta R.T.: -0.059 min
Response: 78431550
Conc: 55.02 ng/ml

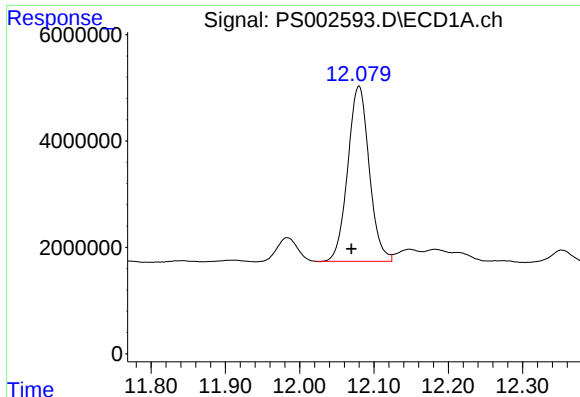

#6 MCPP


R.T.: 12.080 min
Delta R.T.: 0.010 min
Response: 66090286
Conc: 66.24 ug/ml

Instrument :
ECD_S
ClientSampleId :

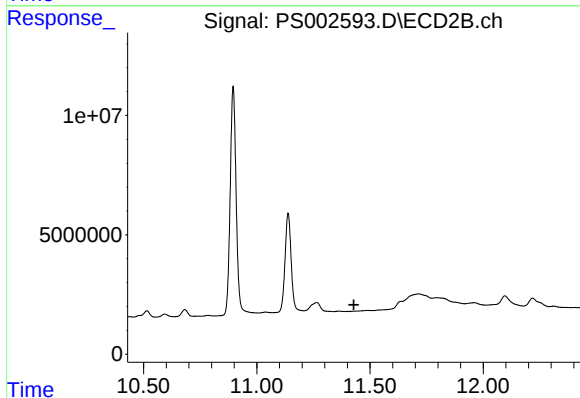


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.429 min
Response: 0
Conc: N.D.

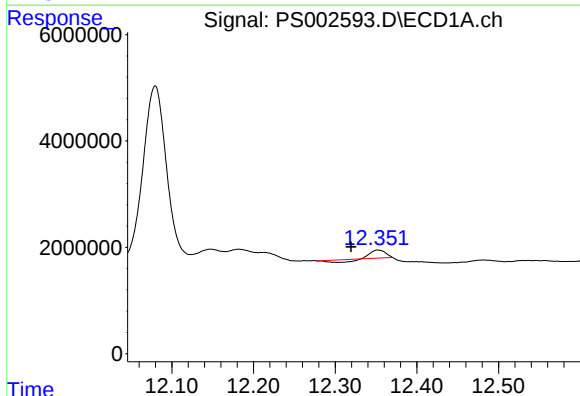


#7 MCPA

R.T.: 12.353 min
Delta R.T.: 0.034 min
Response: 1128356
Conc: 0.75 ug/ml

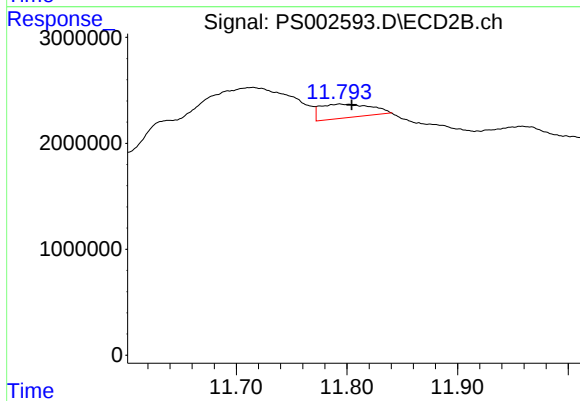

#7 MCPA


R.T.: 11.794 min
Delta R.T.: -0.010 min
Response: 4377091
Conc: 3.05 ug/ml

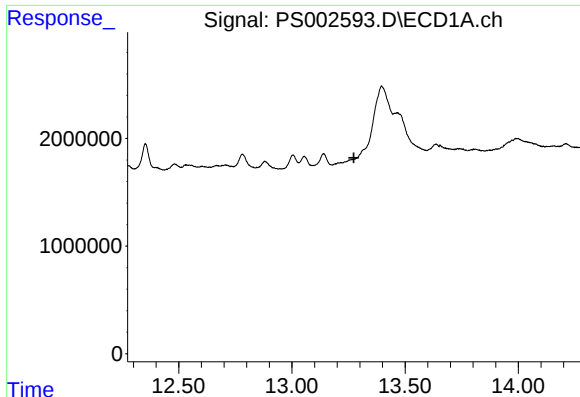

#9 2,4-D


R.T.: 0.000 min
Exp R.T.: 13.274 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

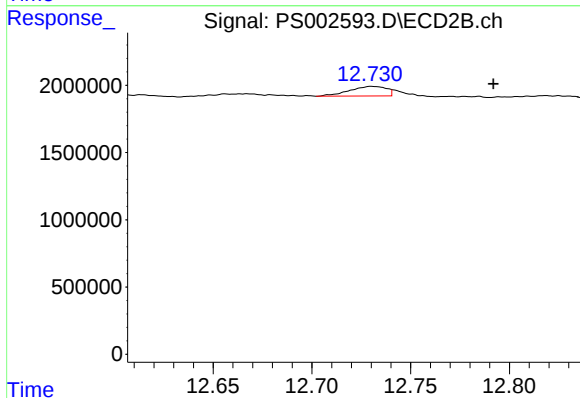


#9 2,4-D

R.T.: 12.731 min
Delta R.T.: -0.061 min
Response: 926022
Conc: 2.19 ng/ml

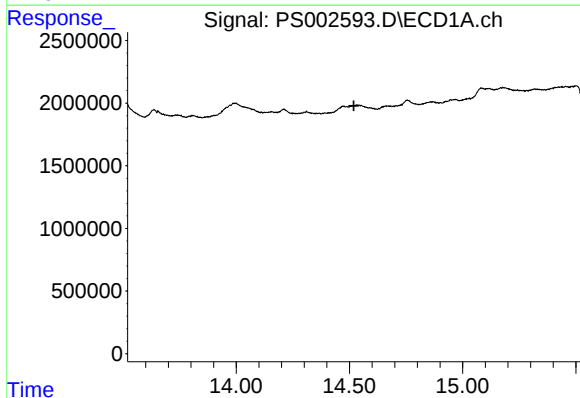


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.519 min
Response: 0
Conc: N.D.

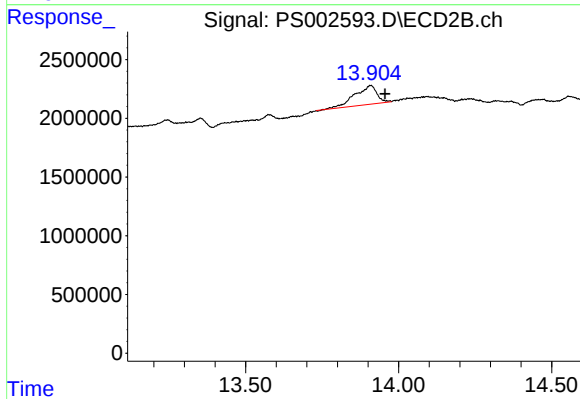

#11 2,4,5-TP (SILVEX)


R.T.: 13.909 min
Delta R.T.: -0.047 min
Response: 8137586
Conc: 3.88 ng/ml

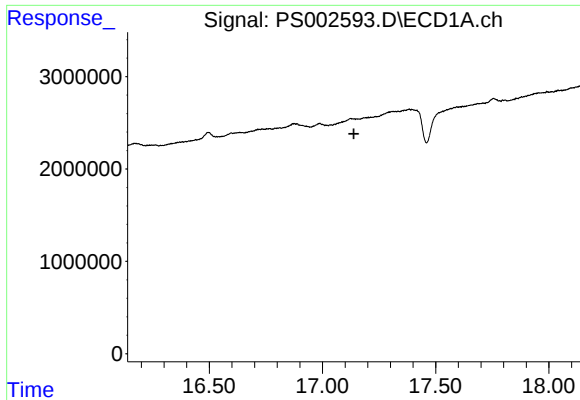

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

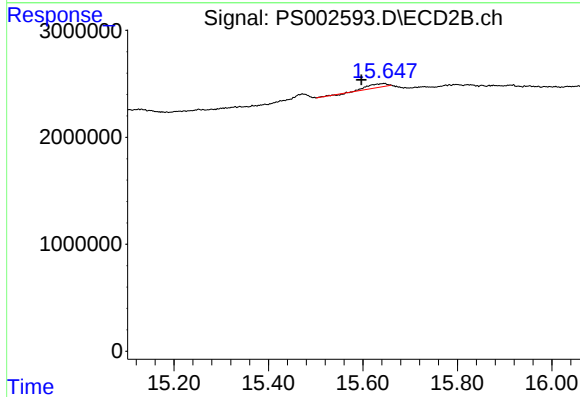


#14 DINOSEB

R.T.: 15.644 min
Delta R.T.: 0.048 min
Response: 1072681
Conc: 0.70 ng/ml

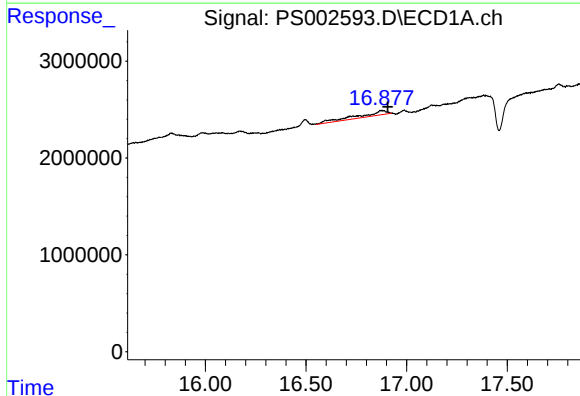


#15 Picloram

R.T.: 16.876 min
Delta R.T.: -0.030 min
Response: 4821291
Conc: 1.90 ng/ml

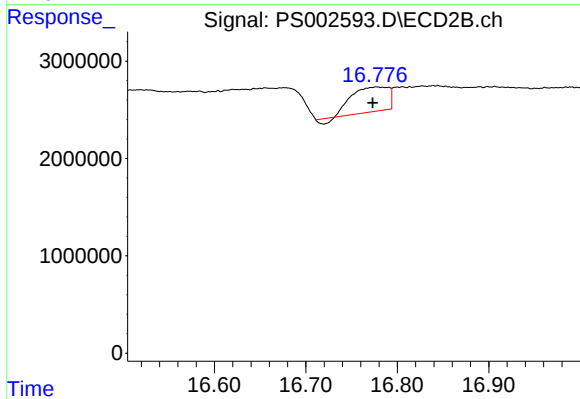

#15 Picloram


R.T.: 16.778 min
Delta R.T.: 0.005 min
Response: 6877445
Conc: 2.50 ng/ml

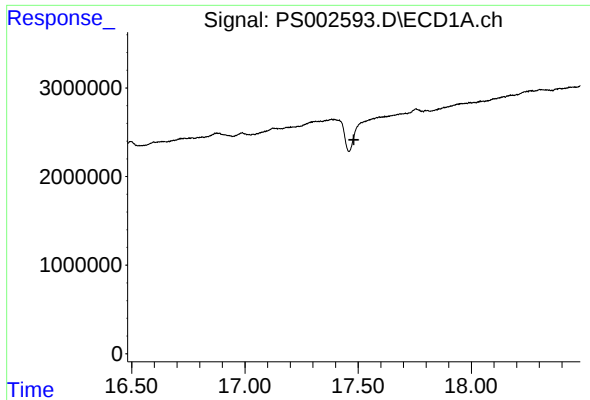

#16 DCPA

R.T.: 0.000 min
Exp R.T.: 17.481 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

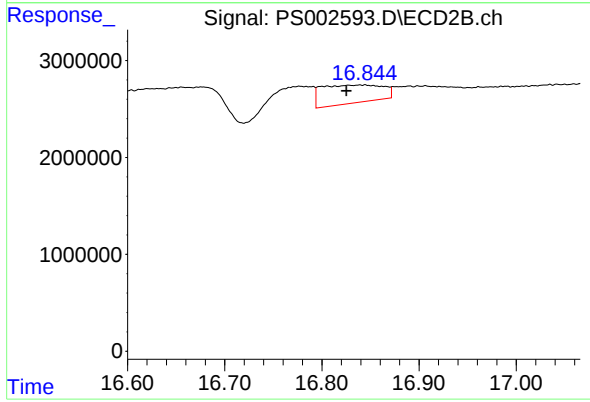

#16 DCPA

R.T.: 16.843 min
Delta R.T.: 0.018 min
Response: 8187891
Conc: 2.82 ng/ml