

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
 Data File : PS002598.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 13 Dec 2018 22:17
 Operator : EI\SJ
 Sample : J6340-02
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 05:02:28 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.413	10.911	134.1E6	123.5E6	422.420	319.260
Target Compounds							
3) T	4-Nitroph...	11.062	0.000	8960310	0	56.554	N.D. #
5) T	DICAMBA	0.000	11.154	0	79480019	N.D.	55.752 #
6) T	MCP	12.095	0.000	65110536	0	65.257	N.D. #
7) T	MCPA	0.000	11.816	0	1561745	N.D.	1.086 #
10) T	Pentachlo...	0.000	13.360	0	2155049	N.D.	0.410 #
11) T	2,4,5-TP ...	0.000	13.980	0	902600	N.D.	0.430 #
12) T	2,4,5-T	0.000	14.567	0	1487438	N.D.	0.869 #
13) T	2,4-DB	15.682	15.156	4370978	1995831	19.327	8.239 #
14) T	DINOSEB	0.000	15.588	0	1775576	N.D.	1.164 #
15) T	Picloram	16.896	0.000	5220684	0	2.057	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
Data File : PS002598.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 13 Dec 2018 22:17
Operator : EI\SJ
Sample : J6340-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 05:02:28 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

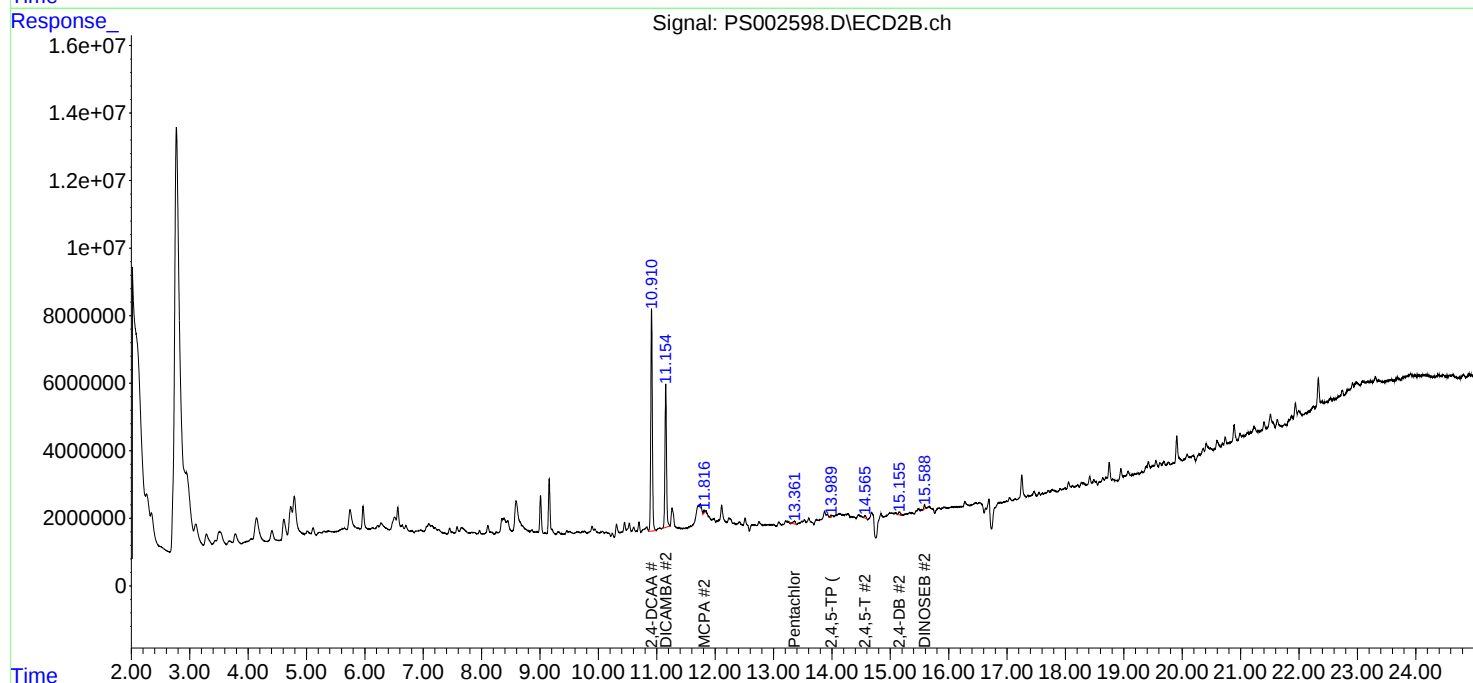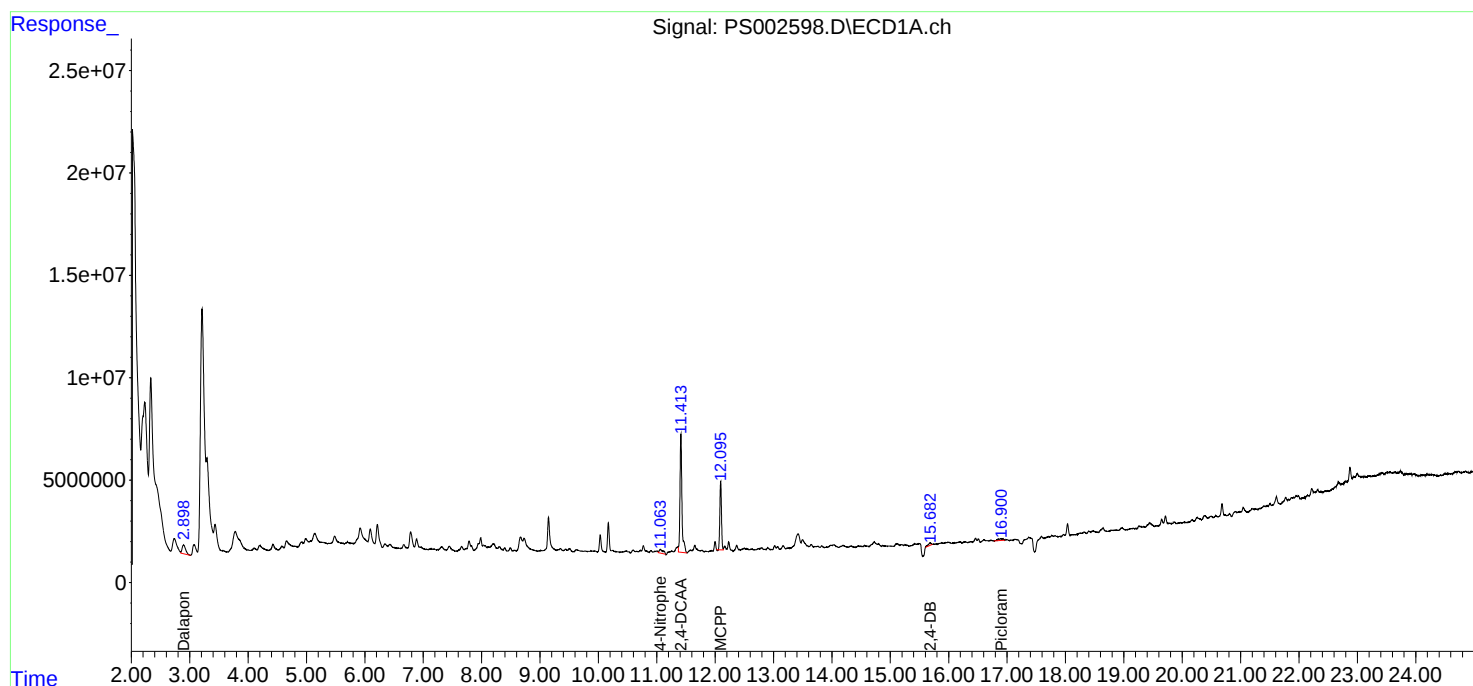


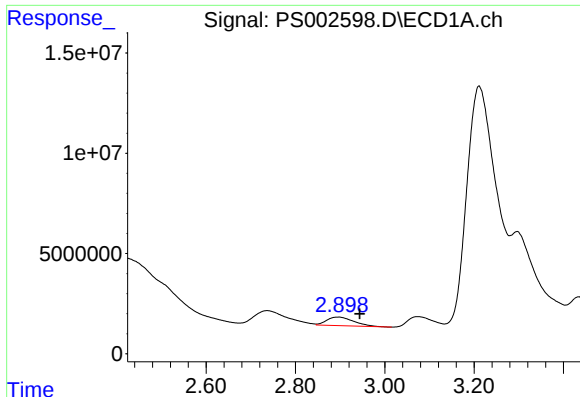

#1 Dalapon


R.T.: 2.898 min
Delta R.T.: -0.046 min
Response: 18042526
Conc: 39.20 ng/ml

Instrument :
ECD_S
ClientSampleId :

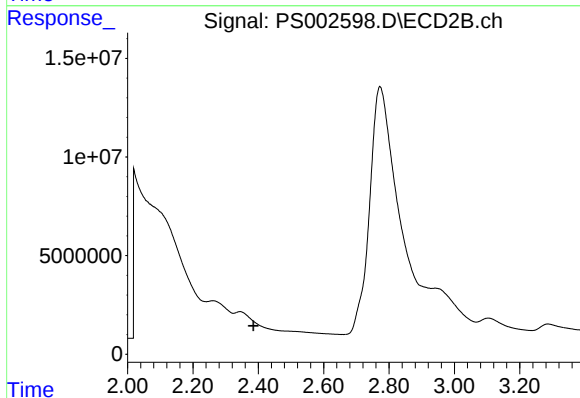


#1 Dalapon

R.T.: 2.344 min
Delta R.T.: -0.041 min
Response: -42653584
Conc: N.D.

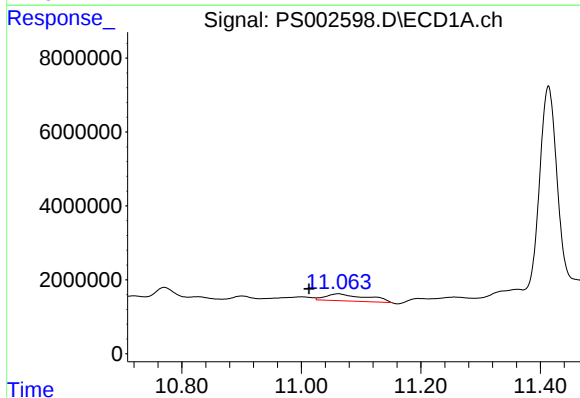


#3 4-Nitrophenol

R.T.: 11.062 min
Delta R.T.: 0.048 min
Response: 8960310
Conc: 56.55 ng/ml

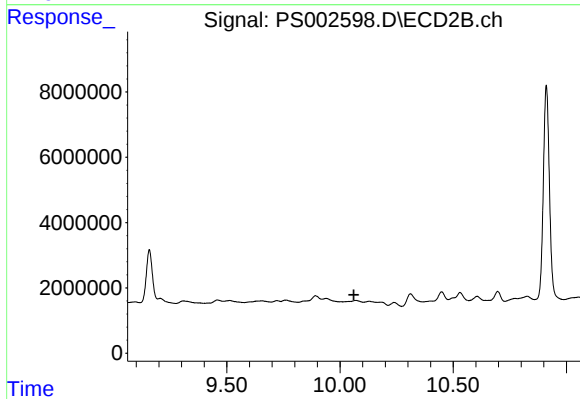

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 10.061 min
Response: 0
Conc: N.D.

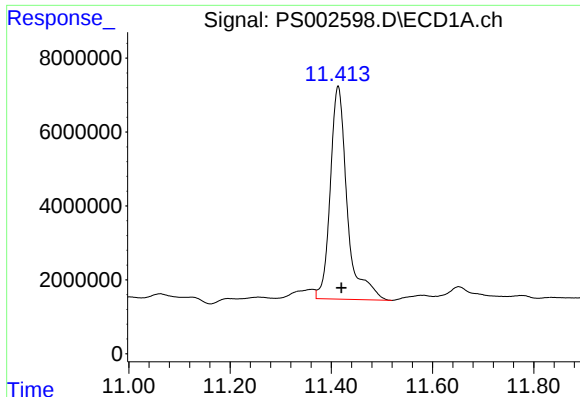

#4 2,4-DCAA


R.T.: 11.413 min
Delta R.T.: -0.006 min
Response: 134084467
Conc: 422.42 ng/ml

Instrument :
ECD_S
ClientSampleId :

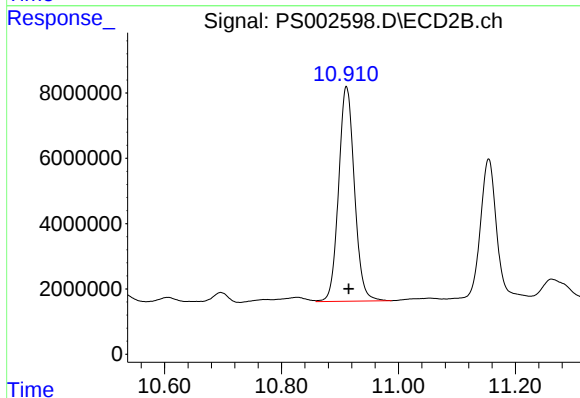


#4 2,4-DCAA

R.T.: 10.911 min
Delta R.T.: -0.004 min
Response: 123480088
Conc: 319.26 ng/ml

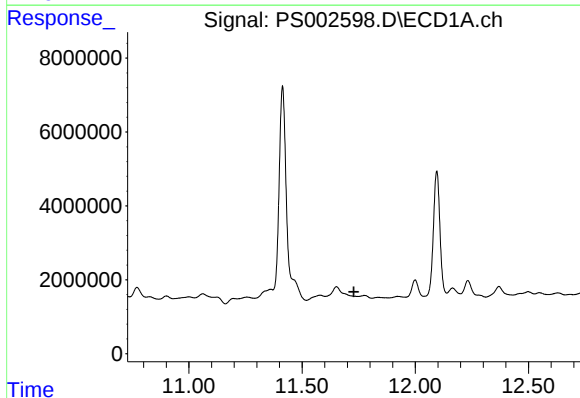


#5 DICAMBA

R.T.: 0.000 min
Exp R.T. : 11.729 min
Response: 0
Conc: N.D.

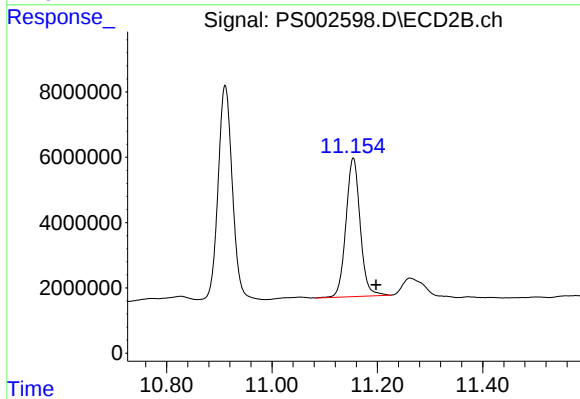

#5 DICAMBA


R.T.: 11.154 min
Delta R.T.: -0.043 min
Response: 79480019
Conc: 55.75 ng/ml

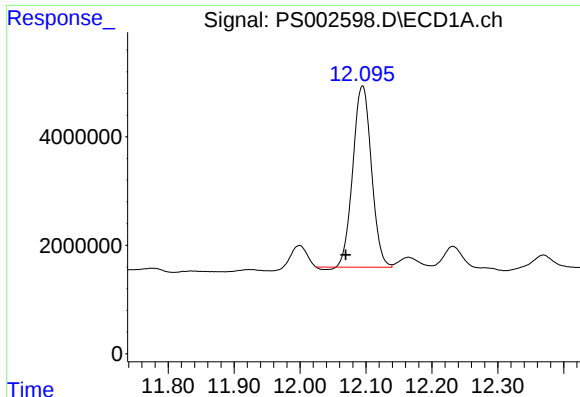

#6 MCPP


R.T.: 12.095 min
Delta R.T.: 0.025 min
Response: 65110536
Conc: 65.26 ug/ml

Instrument :
ECD_S
ClientSampleId :

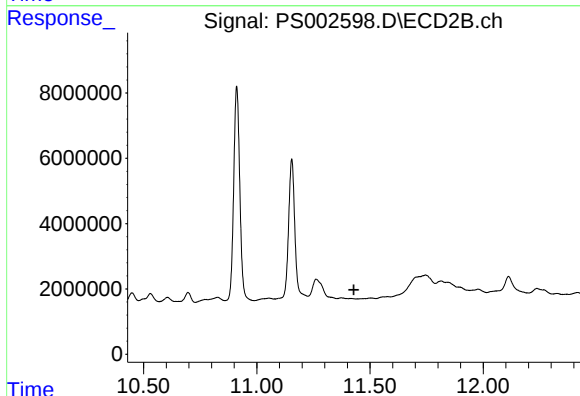


#6 MCPP

R.T.: 0.000 min
Exp R.T. : 11.429 min
Response: 0
Conc: N.D.

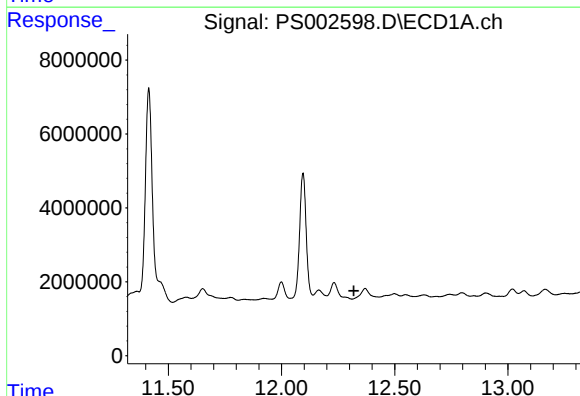


#7 MCPA

R.T.: 0.000 min
Exp R.T. : 12.319 min
Response: 0
Conc: N.D.

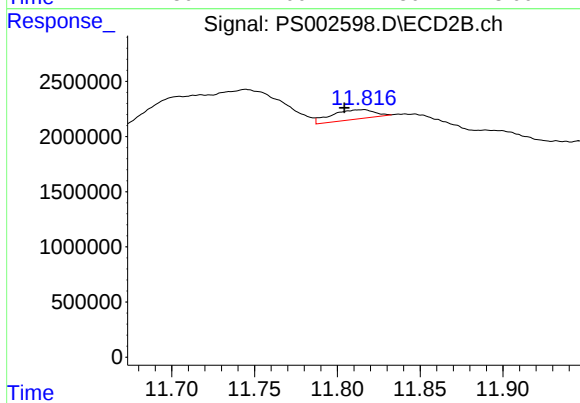

#7 MCPA


R.T.: 11.816 min
Delta R.T.: 0.011 min
Response: 1561745
Conc: 1.09 ug/ml

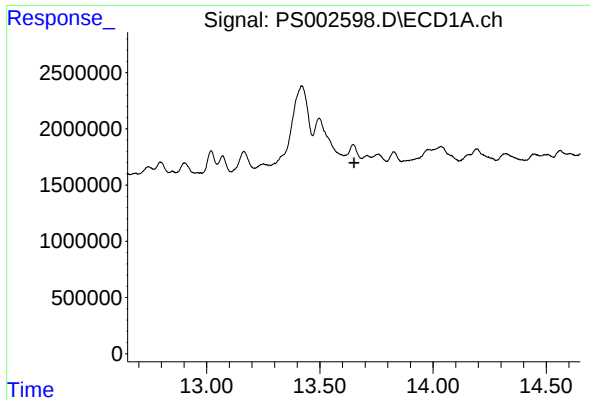

#10 Pentachlorophenol


R.T.: 0.000 min
Exp R.T.: 13.651 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

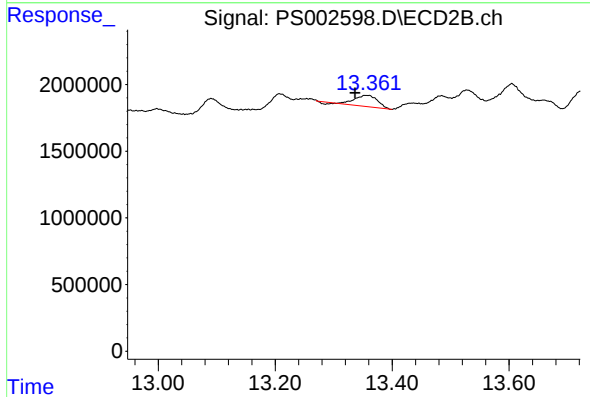


#10 Pentachlorophenol

R.T.: 13.360 min
Delta R.T.: 0.023 min
Response: 2155049
Conc: 0.41 ng/ml

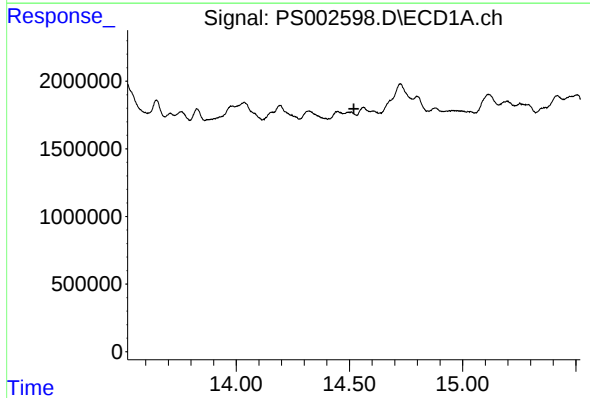


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T.: 14.519 min
Response: 0
Conc: N.D.

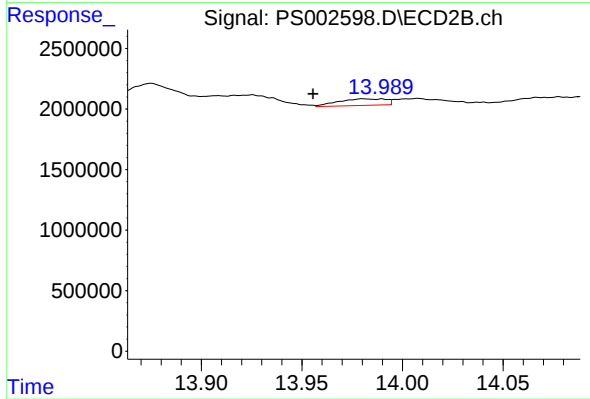

#11 2,4,5-TP (SILVEX)


R.T.: 13.980 min
Delta R.T.: 0.025 min
Response: 902600
Conc: 0.43 ng/ml

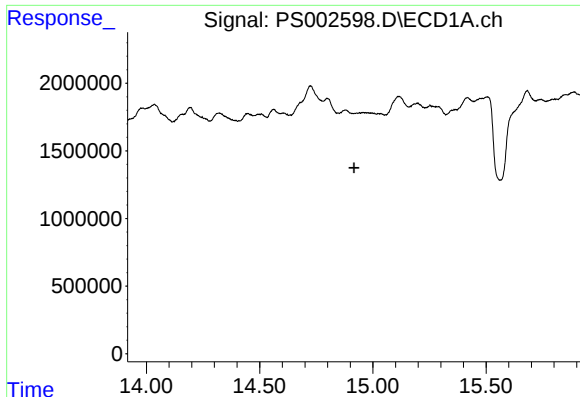

#12 2,4,5-T


R.T.: 0.000 min
Exp R.T.: 14.917 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

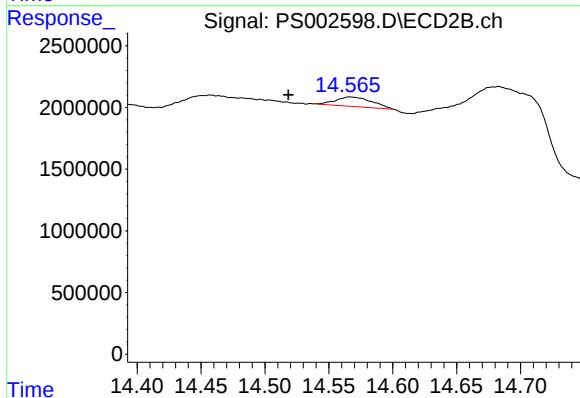


#12 2,4,5-T

R.T.: 14.567 min
Delta R.T.: 0.048 min
Response: 1487438
Conc: 0.87 ng/ml

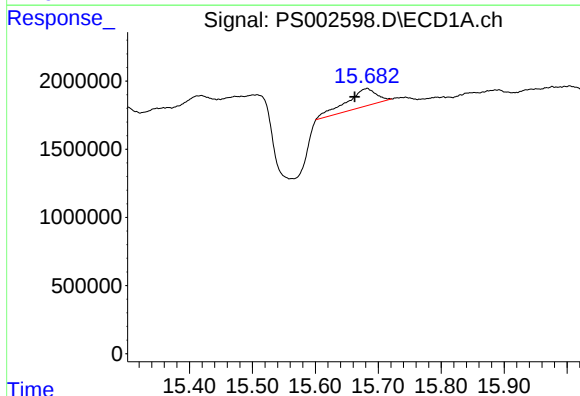


#13 2,4-DB

R.T.: 15.682 min
Delta R.T.: 0.019 min
Response: 4370978
Conc: 19.33 ng/ml

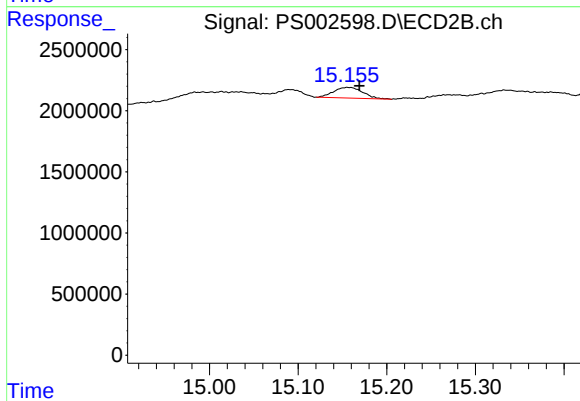

#13 2,4-DB


R.T.: 15.156 min
Delta R.T.: -0.013 min
Response: 1995831
Conc: 8.24 ng/ml

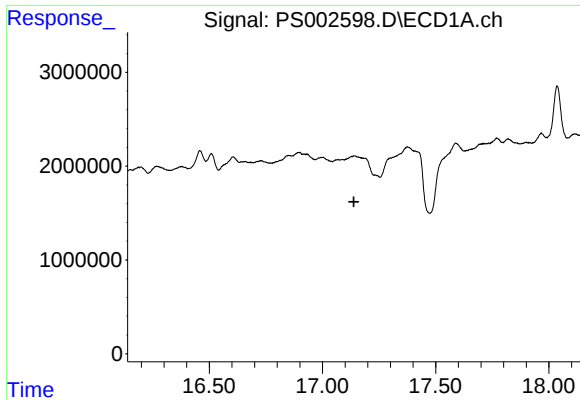

#14 DINOSEB


R.T.: 0.000 min
Exp R.T.: 17.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

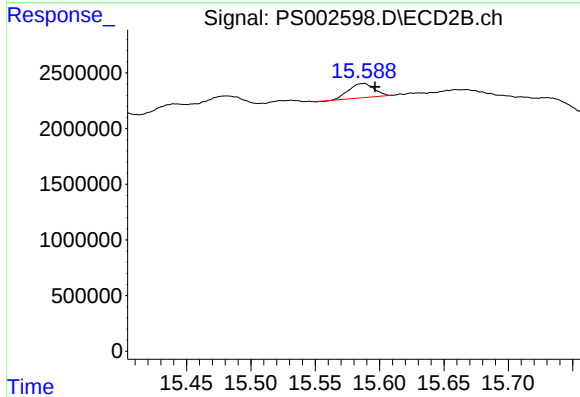


#14 DINOSEB

R.T.: 15.588 min
Delta R.T.: -0.009 min
Response: 1775576
Conc: 1.16 ng/ml

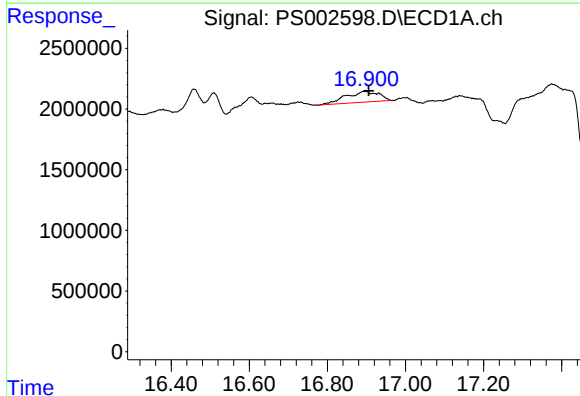

#15 Picloram

R.T.: 16.896 min
Delta R.T.: -0.010 min
Response: 5220684
Conc: 2.06 ng/ml

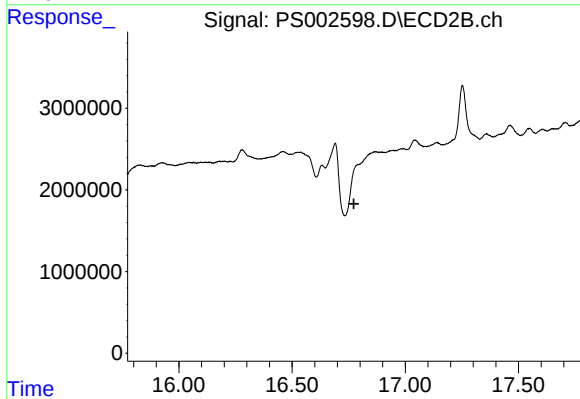

#15 Picloram

R.T.: 0.000 min
Exp R.T.: 16.773 min
Response: 0
Conc: N.D.