

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
 Data File : PS002604.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2018 01:24
 Operator : EI\SJ
 Sample : J6340-09
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 05:03:40 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.411	10.911	152.0E6	151.6E6	478.900	391.889
Target Compounds							
3) T	4-Nitroph...	11.051	10.069	3227135	2391122	20.368	13.378 #
5) T	DICAMBA	0.000	11.153	0	84420885	N.D.	59.217 #
6) T	MCP	12.093	11.416	72586139	8283093	72.750	8.860 #
7) T	MCPA	0.000	11.816	0	8199580	N.D.	5.704 #
8) T	DICHLORPROP	12.911	12.368	2895085	679028	8.142	1.899 #
10) T	Pentachlo...	13.644	13.352	9041575	1800613	1.803	0.342 #
11) T	2,4,5-TP ...	0.000	13.925	0	1465878	N.D.	0.698 #
13) T	2,4-DB	15.676	15.161	7828019	14843132	34.612	61.272 #
14) T	DINOSEB	17.133	15.623	6375287	25397726	4.381	16.643 #
15) T	Picloram	16.935	0.000	4964344	0	1.956	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
Data File : PS002604.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2018 01:24
Operator : EI\SJ
Sample : J6340-09
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 05:03:40 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

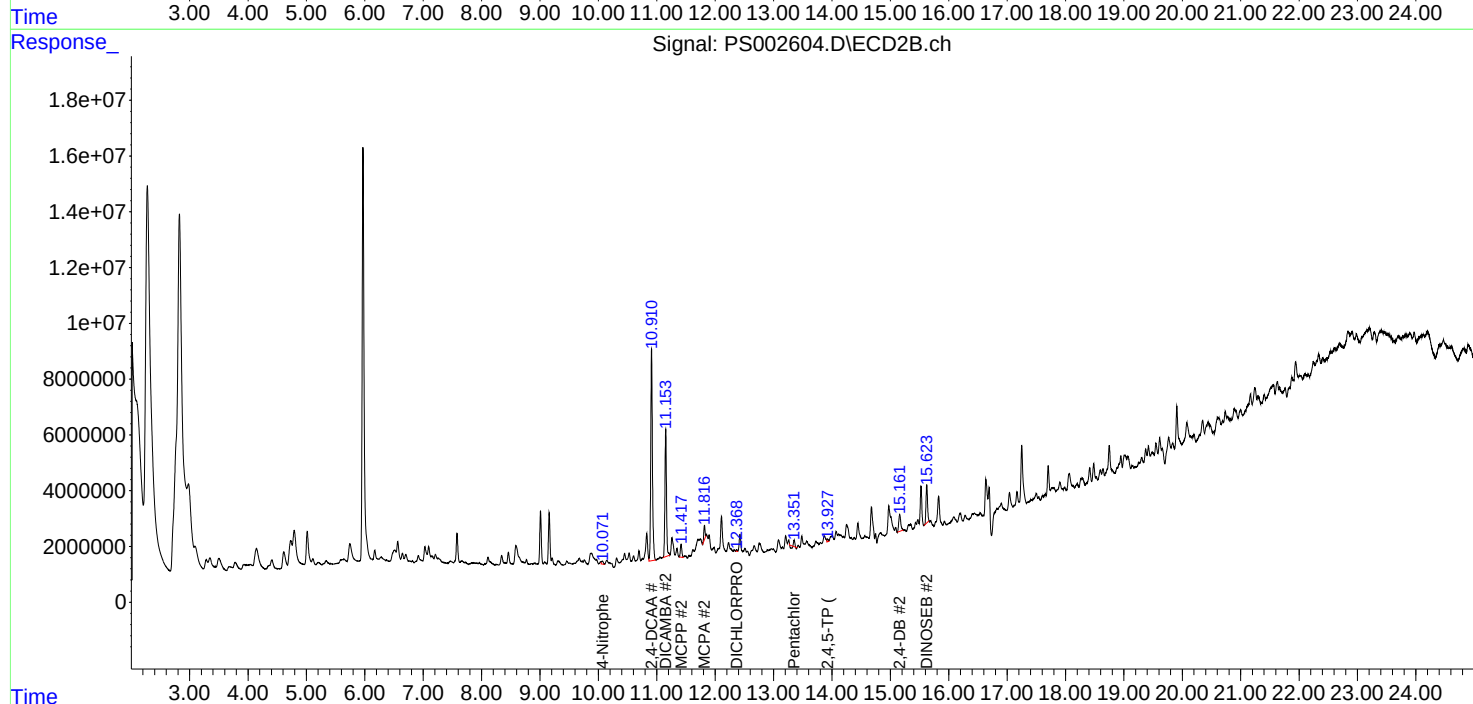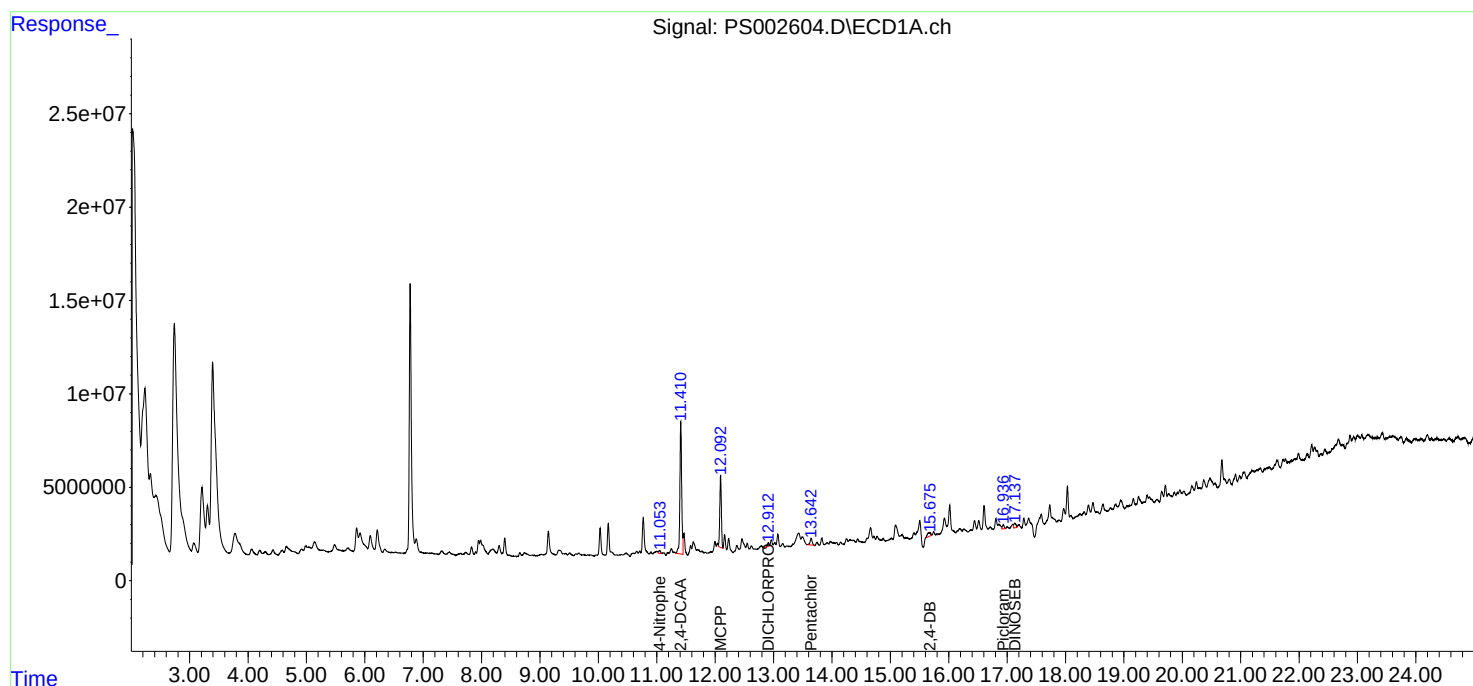


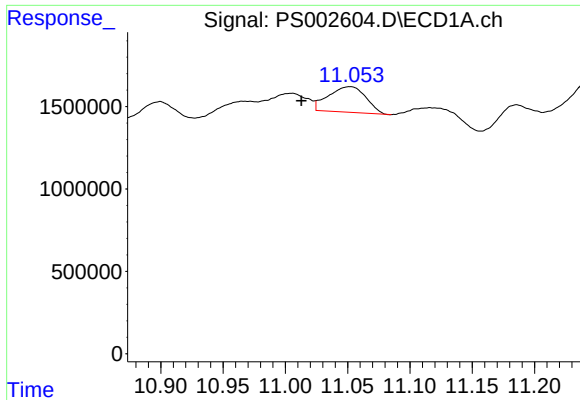

#3 4-Nitrophenol


R.T.: 11.051 min
Delta R.T.: 0.038 min
Response: 3227135
Conc: 20.37 ng/ml

Instrument :
ECD_S
ClientSampleId :

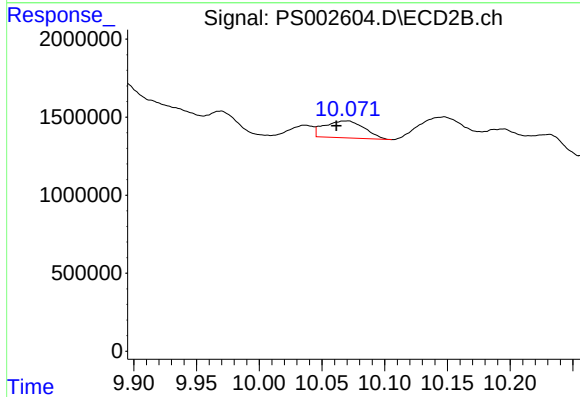


#3 4-Nitrophenol

R.T.: 10.069 min
Delta R.T.: 0.007 min
Response: 2391122
Conc: 13.38 ng/ml

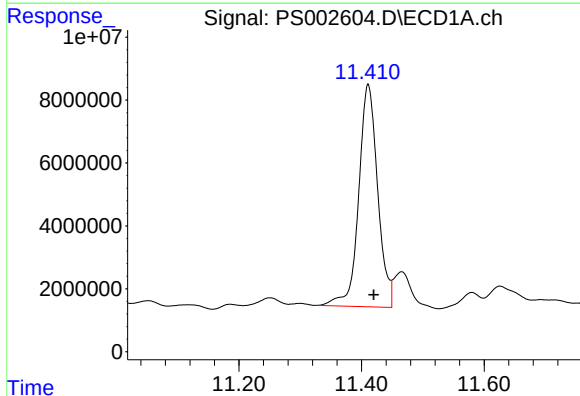


#4 2,4-DCAA

R.T.: 11.411 min
Delta R.T.: -0.009 min
Response: 152012308
Conc: 478.90 ng/ml

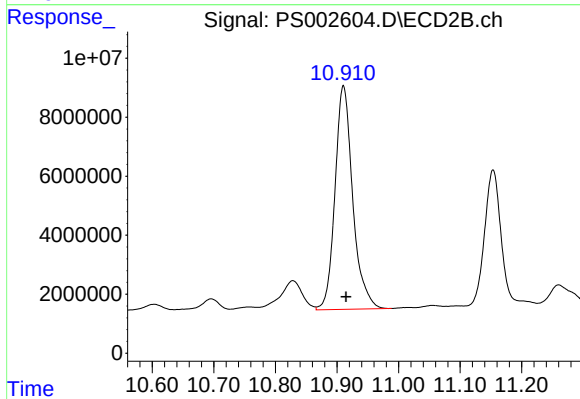

#4 2,4-DCAA


R.T.: 10.911 min
Delta R.T.: -0.004 min
Response: 151570600
Conc: 391.89 ng/ml

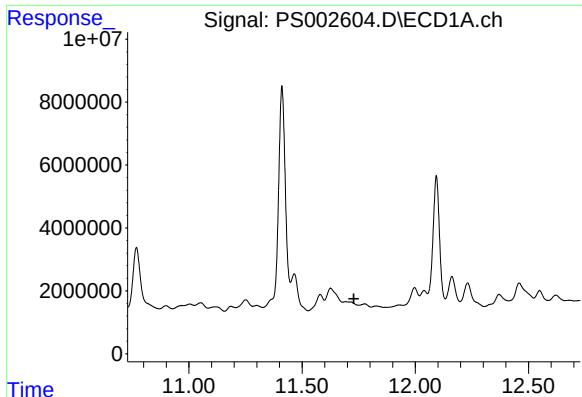

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

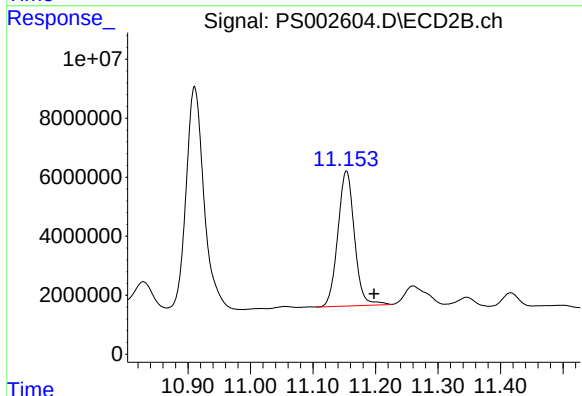


#5 DICAMBA

R.T.: 11.153 min
Delta R.T.: -0.044 min
Response: 84420885
Conc: 59.22 ng/ml

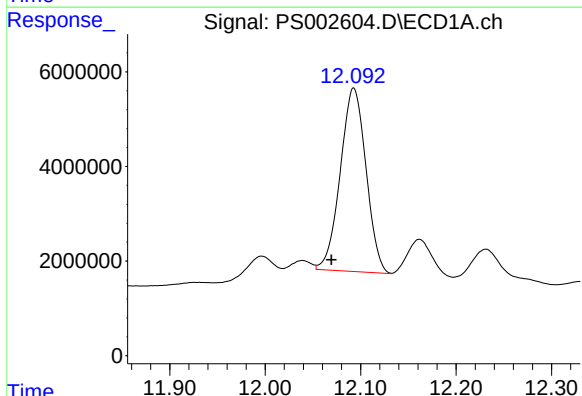


#6 MCP

R.T.: 12.093 min
Delta R.T.: 0.023 min
Response: 72586139
Conc: 72.75 ug/ml

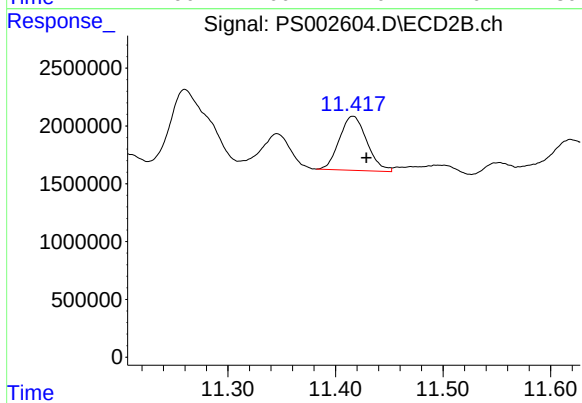

#6 MCP


R.T.: 11.416 min
Delta R.T.: -0.013 min
Response: 8283093
Conc: 8.86 ug/ml

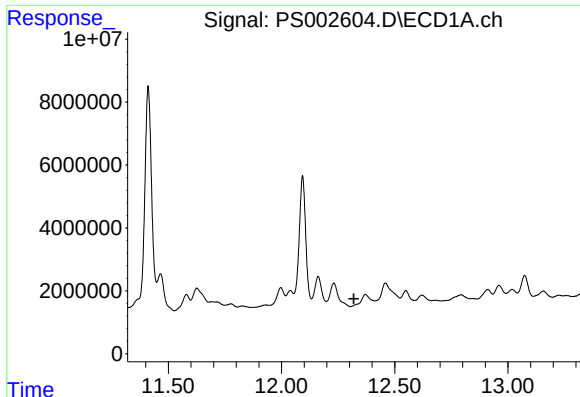

#7 MCPA


R.T.: 0.000 min
Exp R.T.: 12.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

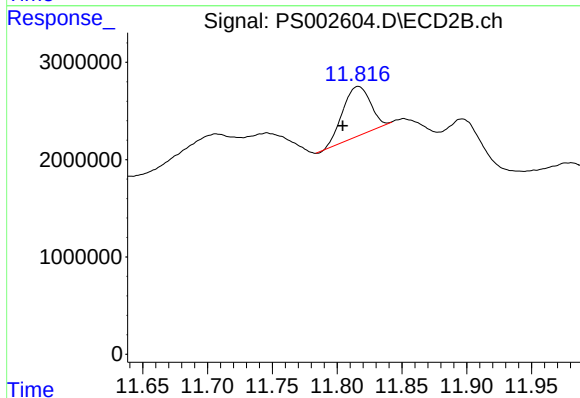


#7 MCPA

R.T.: 11.816 min
Delta R.T.: 0.012 min
Response: 8199580
Conc: 5.70 ug/ml

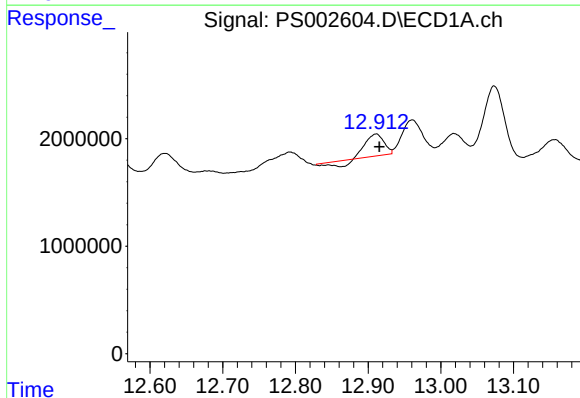


#8 DICHLORPROP

R.T.: 12.911 min
Delta R.T.: -0.005 min
Response: 2895085
Conc: 8.14 ng/ml

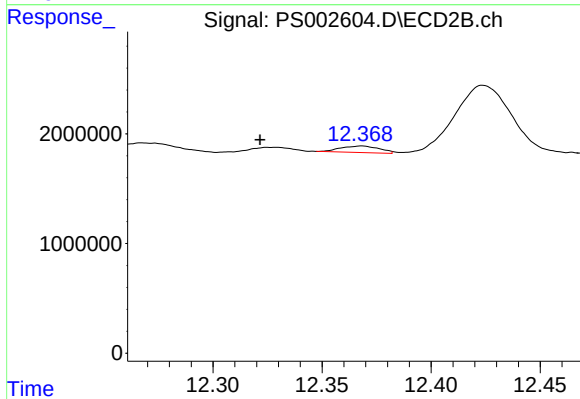

#8 DICHLORPROP


R.T.: 12.368 min
Delta R.T.: 0.046 min
Response: 679028
Conc: 1.90 ng/ml

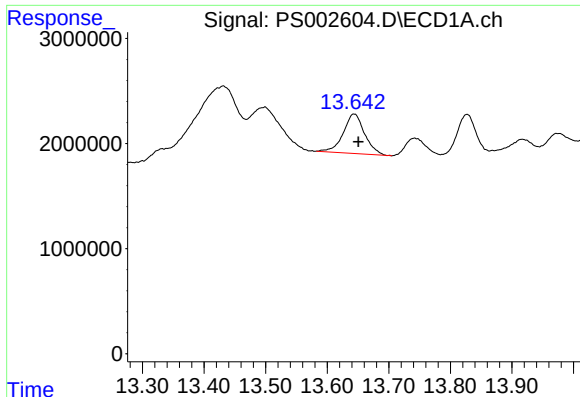

#10 Pentachlorophenol


R.T.: 13.644 min
Delta R.T.: -0.007 min
Response: 9041575
Conc: 1.80 ng/ml

Instrument :
ECD_S
ClientSampleId :

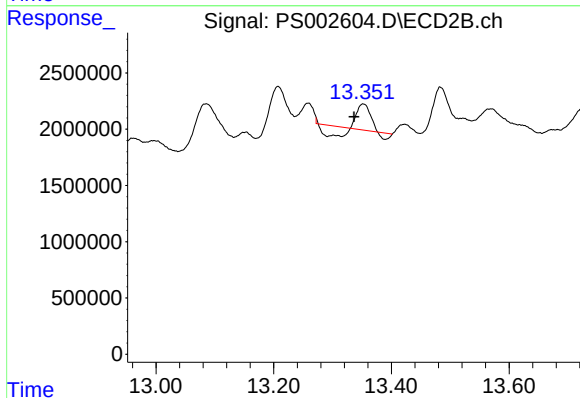


#10 Pentachlorophenol

R.T.: 13.352 min
Delta R.T.: 0.016 min
Response: 1800613
Conc: 0.34 ng/ml

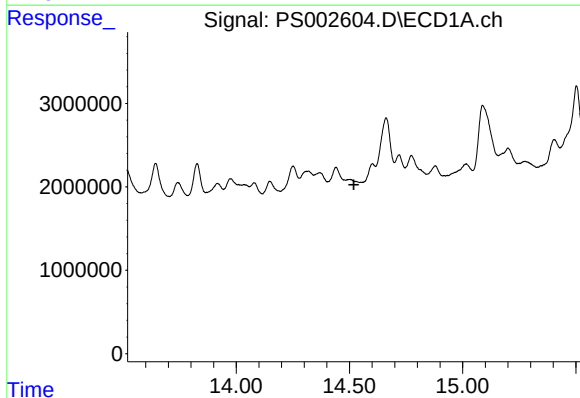


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.519 min
Response: 0
Conc: N.D.

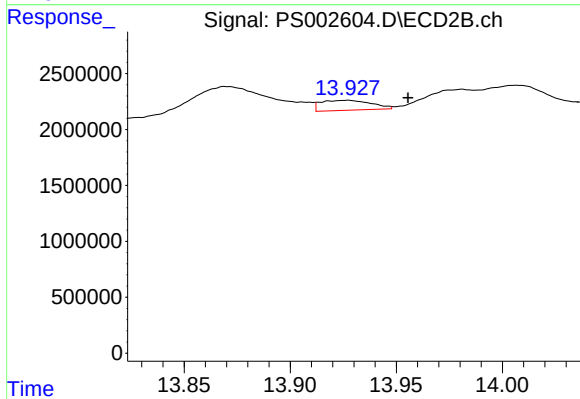

#11 2,4,5-TP (SILVEX)


R.T.: 13.925 min
Delta R.T.: -0.031 min
Response: 1465878
Conc: 0.70 ng/ml

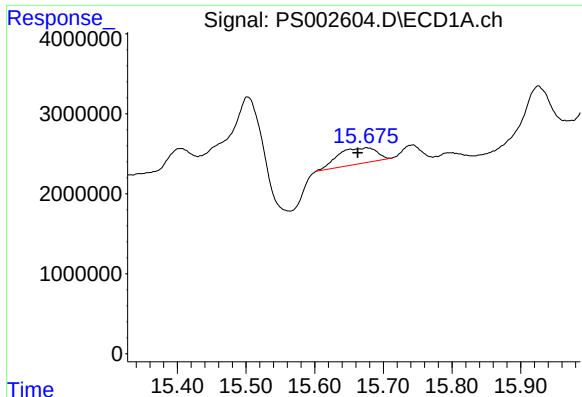

#13 2,4-DB


R.T.: 15.676 min
Delta R.T.: 0.013 min
Response: 7828019
Conc: 34.61 ng/ml

Instrument :
ECD_S
ClientSampleId :

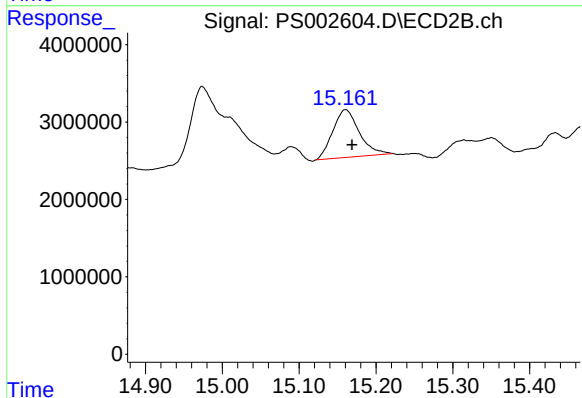


#13 2,4-DB

R.T.: 15.161 min
Delta R.T.: -0.008 min
Response: 14843132
Conc: 61.27 ng/ml

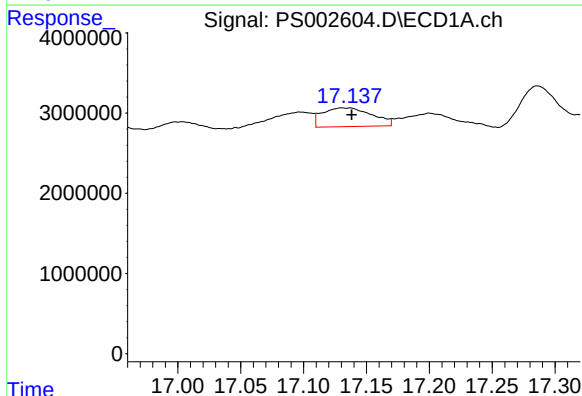


#14 DINOSEB

R.T.: 17.133 min
Delta R.T.: -0.005 min
Response: 6375287
Conc: 4.38 ng/ml

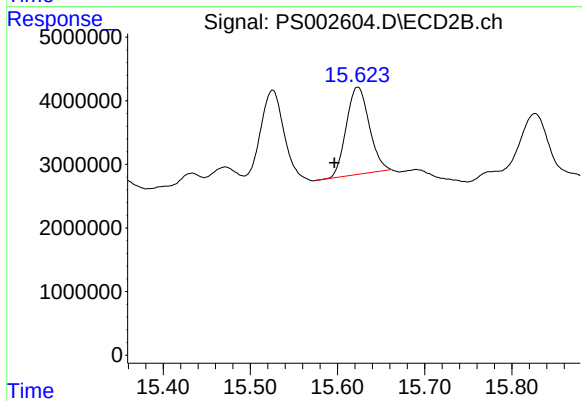

#14 DINOSEB


R.T.: 15.623 min
Delta R.T.: 0.027 min
Response: 25397726
Conc: 16.64 ng/ml

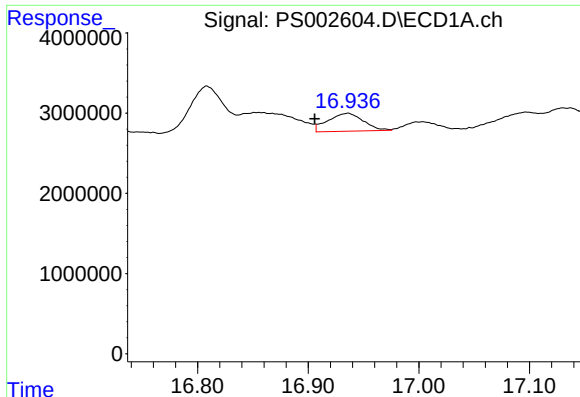

#15 Picloram

R.T.: 16.935 min
Delta R.T.: 0.029 min
Response: 4964344
Conc: 1.96 ng/ml

Instrument :
ECD_S
ClientSampleId :

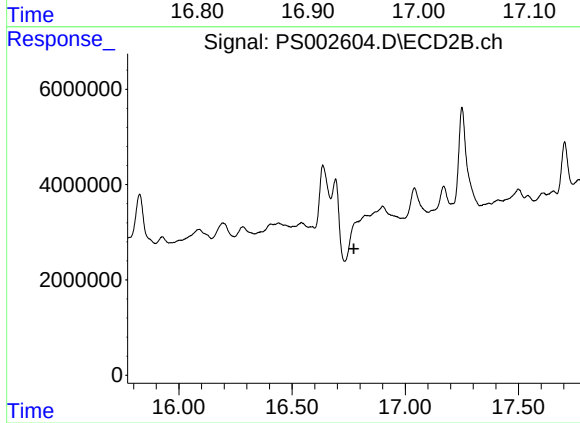

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.773 min
Response: 0
Conc: N.D.