

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
 Data File : PS002615.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2018 07:05
 Operator : EI\SJ
 Sample : J6357-07
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 07:48:36 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.406	10.908	101.0E6	90912965	318.205	235.057 #
Target Compounds							
5) T	DICAMBA	0.000	11.150	0	88925381	N.D.	62.377 #
6) T	MCPD	12.086	11.370	74140140	121486	74.307	0.130 #
7) T	MCPA	12.358	11.808	4033829	792092	2.678	0.551 #
8) T	DICHLORPROP	12.894	12.264	2441492	80283	6.866	0.224 #
10) T	Pentachlo...	13.656	13.360	5124047	2354372	1.022	0.448 #
11) T	2,4,5-TP ...	0.000	13.924	0	2402631	N.D.	1.144 #
12) T	2,4,5-T	14.912	14.565	5056988	1353643	2.692	0.791 #
13) T	2,4-DB	15.674	15.157	8404470	5048885	37.161	20.842 #
14) T	DINOSEB	0.000	15.548	0	1300954	N.D.	0.852 #
16) T	DCPA	0.000	16.882	0	10339247	N.D.	3.559 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
Data File : PS002615.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2018 07:05
Operator : EI\SJ
Sample : J6357-07
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 07:48:36 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

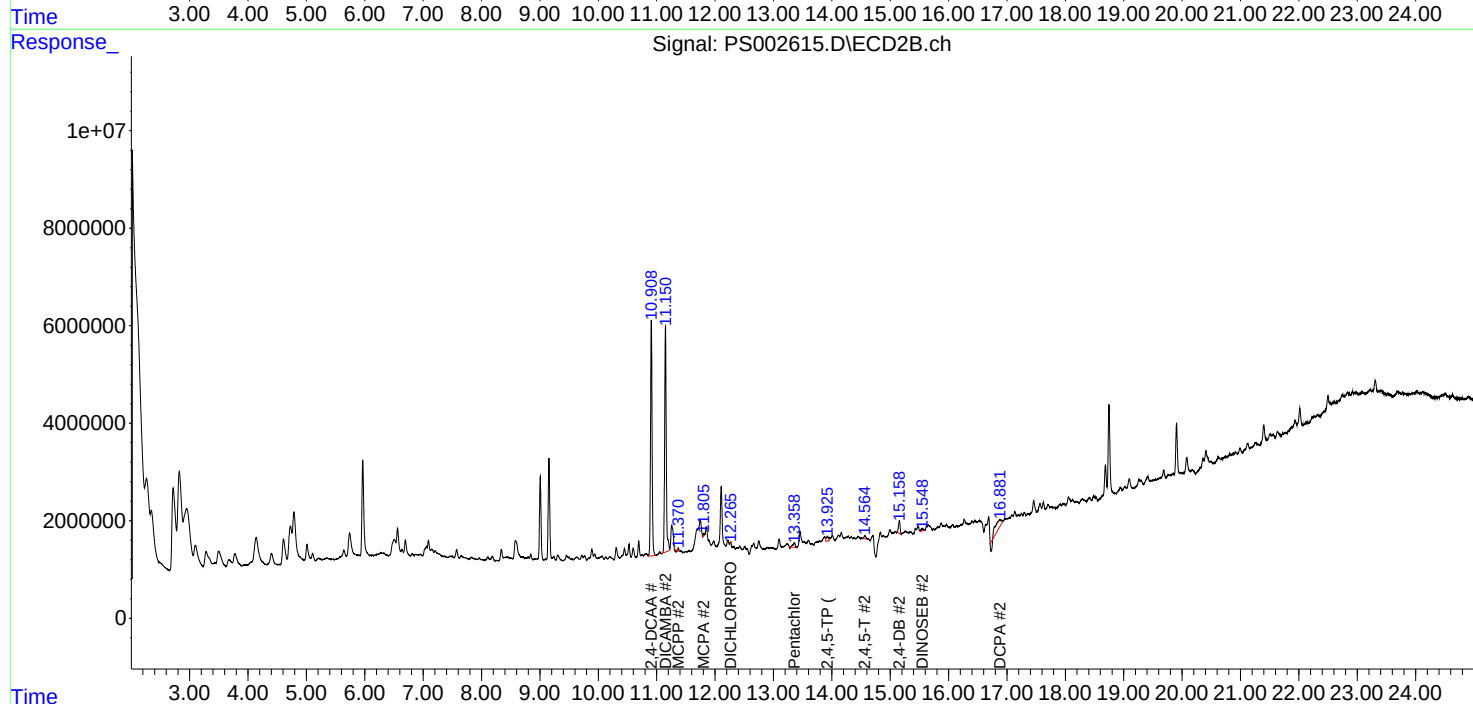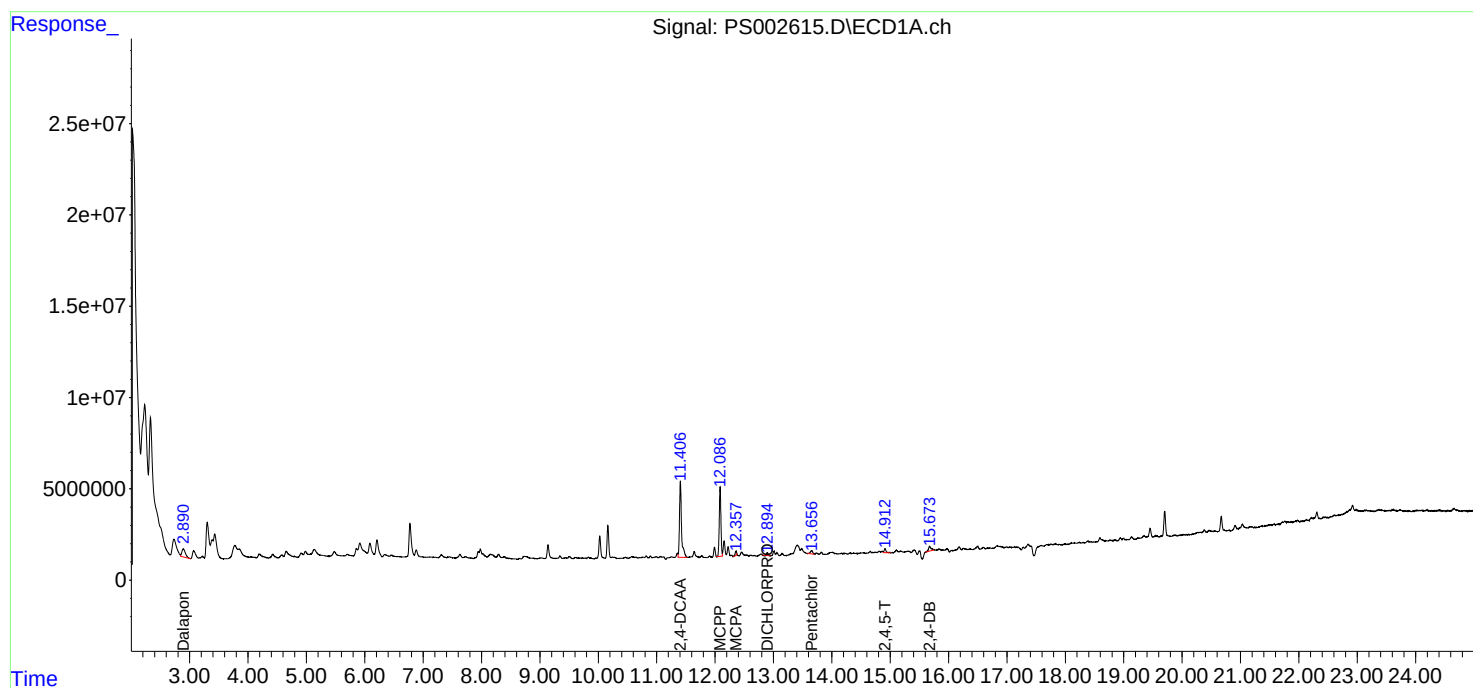


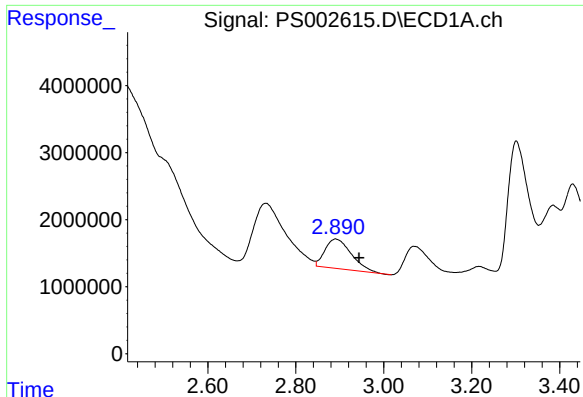

#1 Dalapon


R.T.: 2.890 min
Delta R.T.: -0.054 min
Response: 18169647
Conc: 39.47 ng/ml

Instrument :
ECD_S
ClientSampleId :

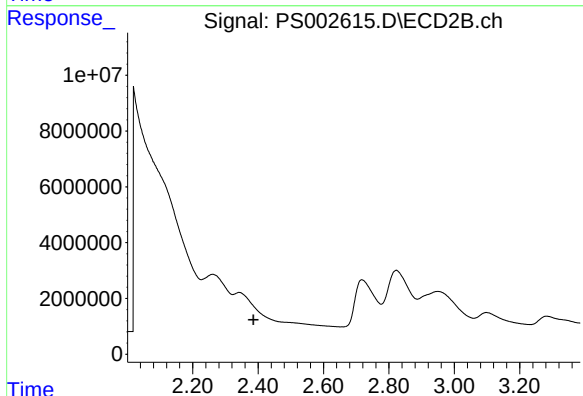


#1 Dalapon

R.T.: 2.342 min
Delta R.T.: -0.043 min
Response: -44529330
Conc: N.D.

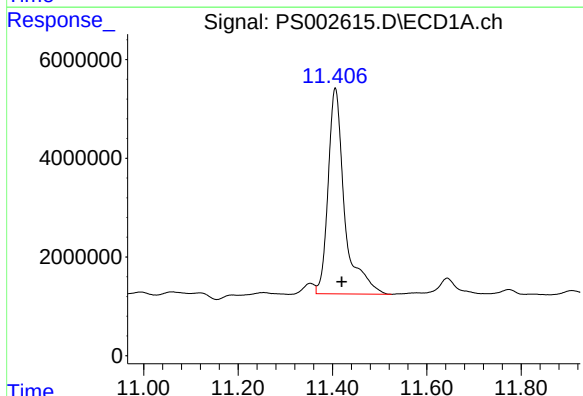


#4 2,4-DCAA

R.T.: 11.406 min
Delta R.T.: -0.014 min
Response: 101004546
Conc: 318.20 ng/ml

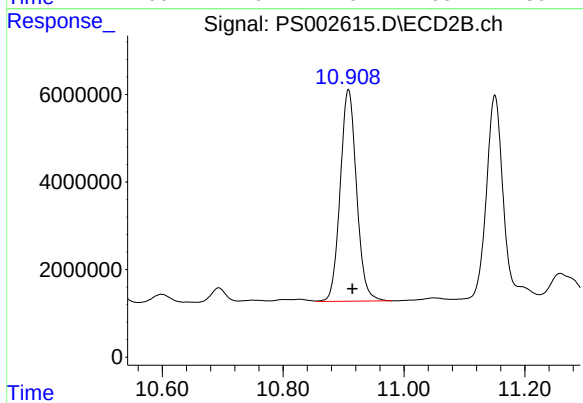

#4 2,4-DCAA


R.T.: 10.908 min
Delta R.T.: -0.007 min
Response: 90912965
Conc: 235.06 ng/ml

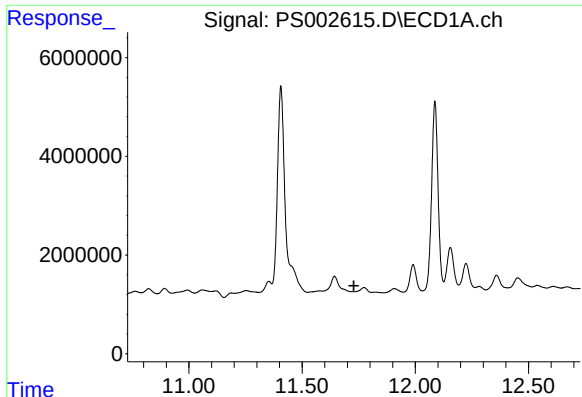

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

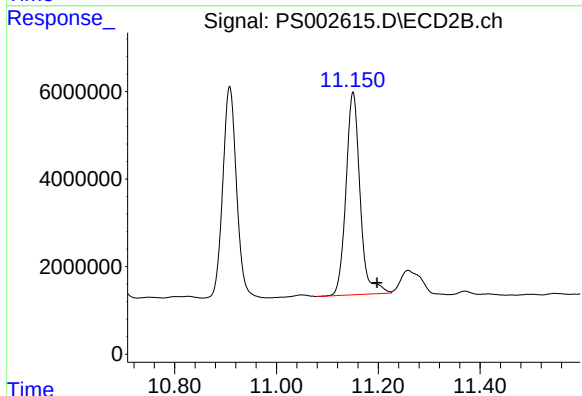


#5 DICAMBA

R.T.: 11.150 min
Delta R.T.: -0.047 min
Response: 88925381
Conc: 62.38 ng/ml

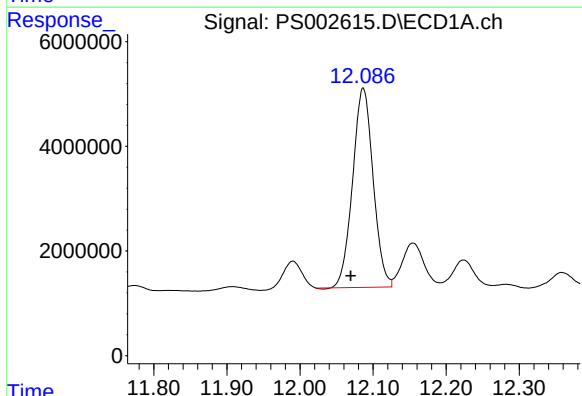


#6 MCP

R.T.: 12.086 min
Delta R.T.: 0.017 min
Response: 74140140
Conc: 74.31 ug/ml

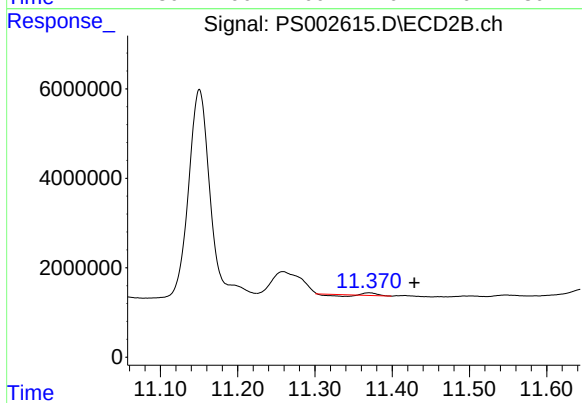

#6 MCP


R.T.: 11.370 min
Delta R.T.: -0.059 min
Response: 121486
Conc: 0.13 ug/ml

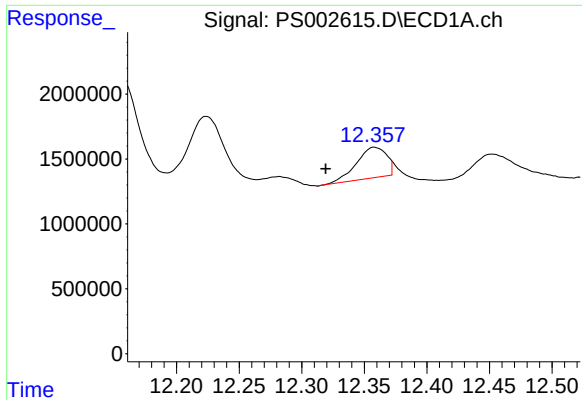

#7 MCPA


R.T.: 12.358 min
Delta R.T.: 0.039 min
Response: 4033829
Conc: 2.68 ug/ml

Instrument :
ECD_S
ClientSampleId :

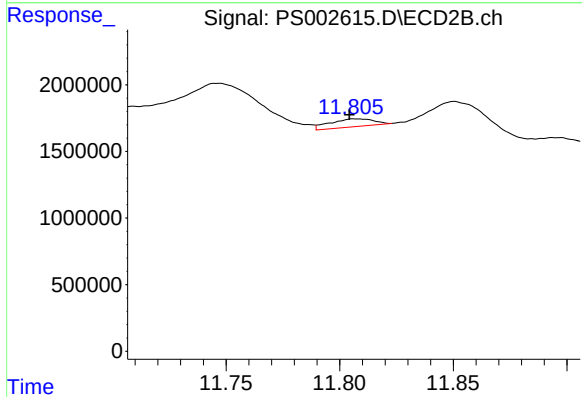


#7 MCPA

R.T.: 11.808 min
Delta R.T.: 0.004 min
Response: 792092
Conc: 0.55 ug/ml

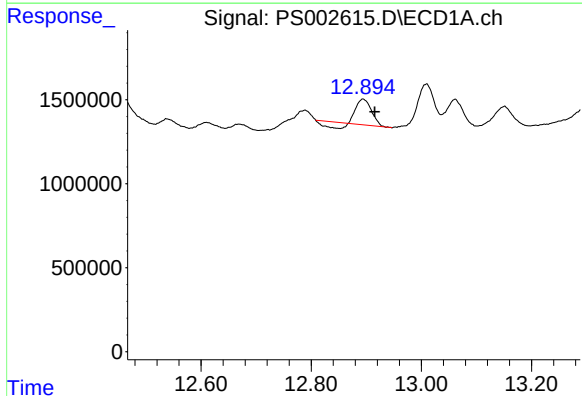


#8 DICHLORPROP

R.T.: 12.894 min
Delta R.T.: -0.021 min
Response: 2441492
Conc: 6.87 ng/ml

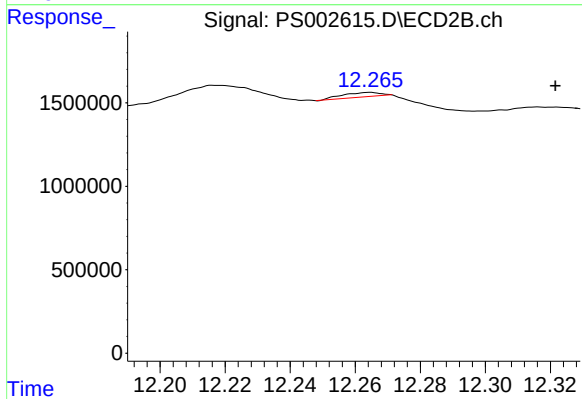

#8 DICHLORPROP


R.T.: 12.264 min
Delta R.T.: -0.057 min
Response: 80283
Conc: 0.22 ng/ml

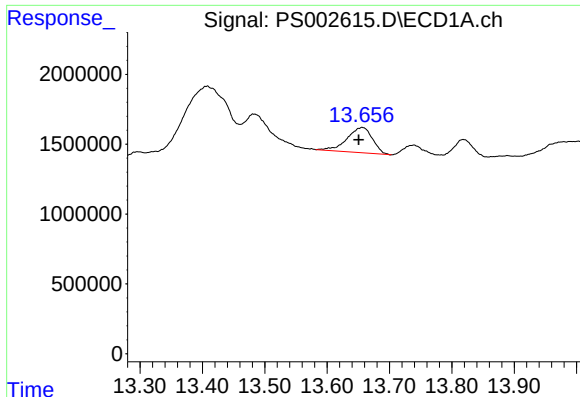

#10 Pentachlorophenol


R.T.: 13.656 min
Delta R.T.: 0.005 min
Response: 5124047
Conc: 1.02 ng/ml

Instrument :
ECD_S
ClientSampleId :

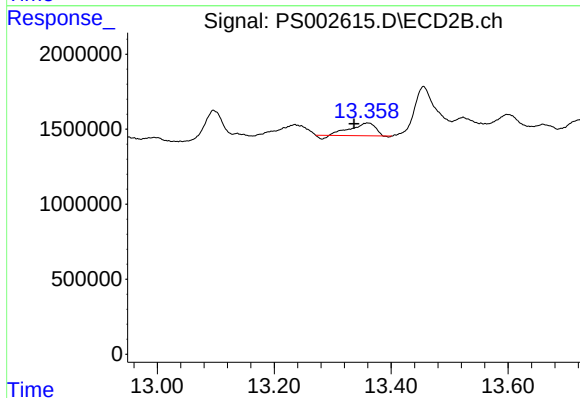


#10 Pentachlorophenol

R.T.: 13.360 min
Delta R.T.: 0.023 min
Response: 2354372
Conc: 0.45 ng/ml

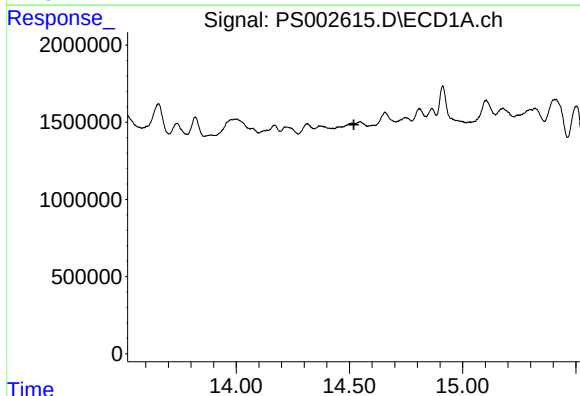


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.519 min
Response: 0
Conc: N.D.

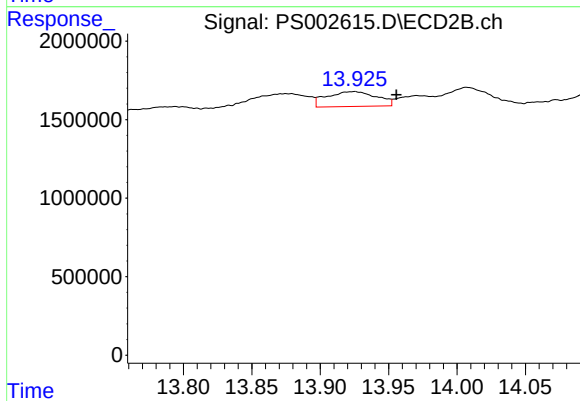

#11 2,4,5-TP (SILVEX)


R.T.: 13.924 min
Delta R.T.: -0.031 min
Response: 2402631
Conc: 1.14 ng/ml

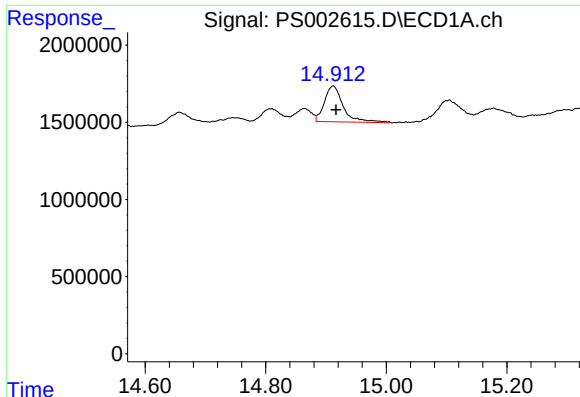

#12 2,4,5-T


R.T.: 14.912 min
Delta R.T.: -0.005 min
Response: 5056988
Conc: 2.69 ng/ml

Instrument :
ECD_S
ClientSampleId :

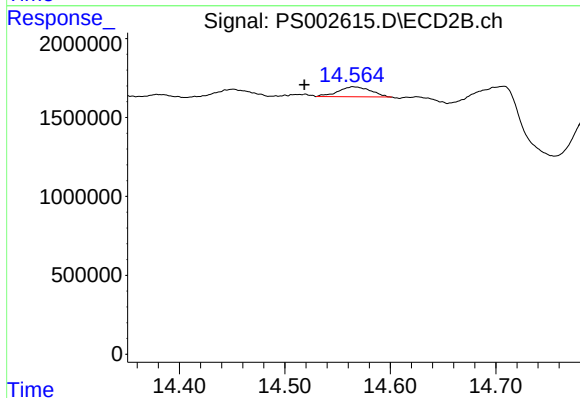


#12 2,4,5-T

R.T.: 14.565 min
Delta R.T.: 0.047 min
Response: 1353643
Conc: 0.79 ng/ml

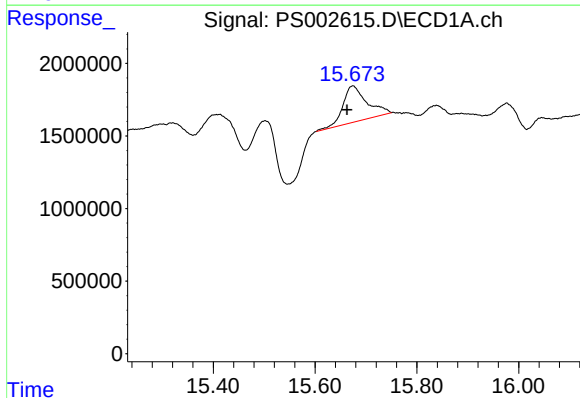


#13 2,4-DB

R.T.: 15.674 min
Delta R.T.: 0.011 min
Response: 8404470
Conc: 37.16 ng/ml

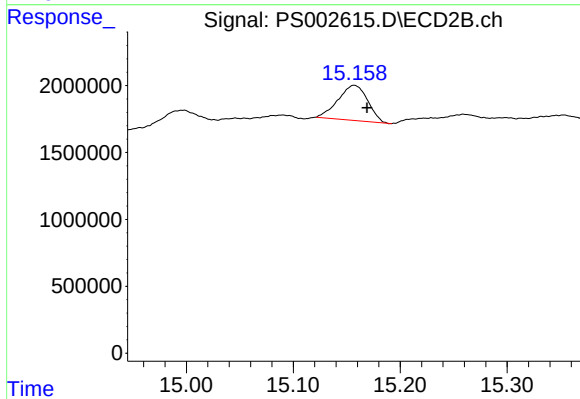

#13 2,4-DB


R.T.: 15.157 min
Delta R.T.: -0.012 min
Response: 5048885
Conc: 20.84 ng/ml

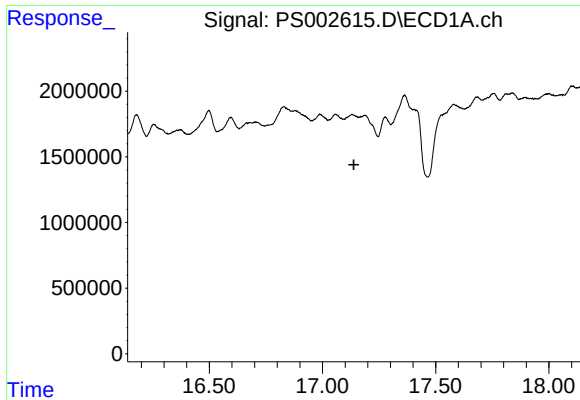

#14 DINOSEB


R.T.: 0.000 min
Exp R.T. : 17.138 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

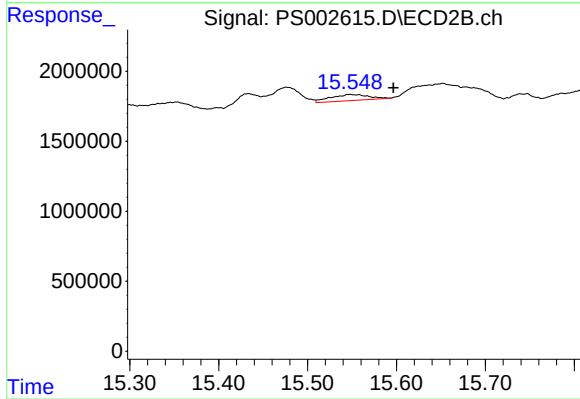


#14 DINOSEB

R.T.: 15.548 min
Delta R.T.: -0.048 min
Response: 1300954
Conc: 0.85 ng/ml

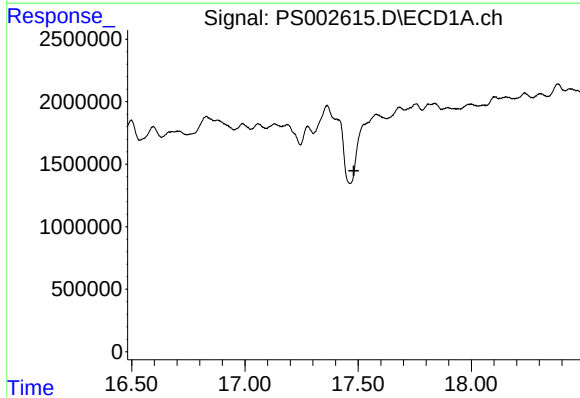

#16 DCPA

R.T.: 0.000 min
Exp R.T. : 17.481 min
Response: 0
Conc: N.D.

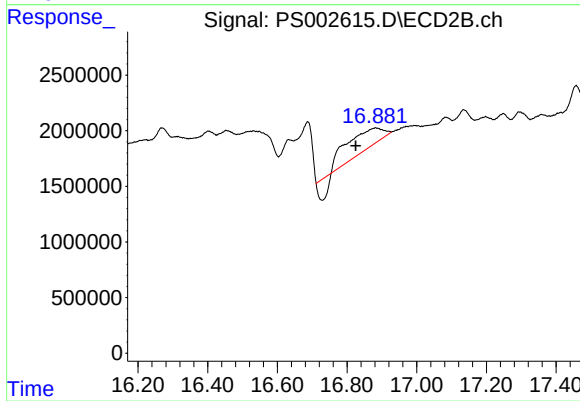

#16 DCPA

R.T.: 16.882 min
Delta R.T.: 0.056 min
Response: 10339247
Conc: 3.56 ng/ml