

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
 Data File : PS002616.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2018 07:36
 Operator : EI\SJ
 Sample : J6357-08
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 12:47:29 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.395	10.895	150.0E6	138.9E6	472.409	359.039
Target Compounds							
3) T	4-Nitroph...	0.000	10.120	0	862816	N.D.	4.827 #
5) T	DICAMBA	0.000	11.183	0	5220454	N.D.	3.662 #
6) T	MCP	12.077	11.421	78185657	1771085	78.362	1.894 #
7) T	MCPA	12.353	11.800	298093	1087087	0.198	0.756 #
8) T	DICHLORPROP	12.891	12.308	5242144	2807286	14.742	7.849 #
10) T	Pentachlo...	13.629	13.343	3836612	4308113	0.765	0.819
11) T	2,4,5-TP ...	0.000	13.952	0	4336229	N.D.	2.065 #
12) T	2,4,5-T	14.904	14.502	3644043	3541135	1.940	2.070
13) T	2,4-DB	15.669	15.141	24488165	15966589	108.276	65.909 #
14) T	DINOSEB	17.113	15.617	3118782	884936	2.143	0.580 #
15) T	Picloram	16.896	16.756	12323520	12003037	4.856	4.363
16) T	DCPA	17.513	16.818	-3722895	22514733	N.D.	7.750



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
Data File : PS002616.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2018 07:36
Operator : EI\SJ
Sample : J6357-08
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 12:47:29 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

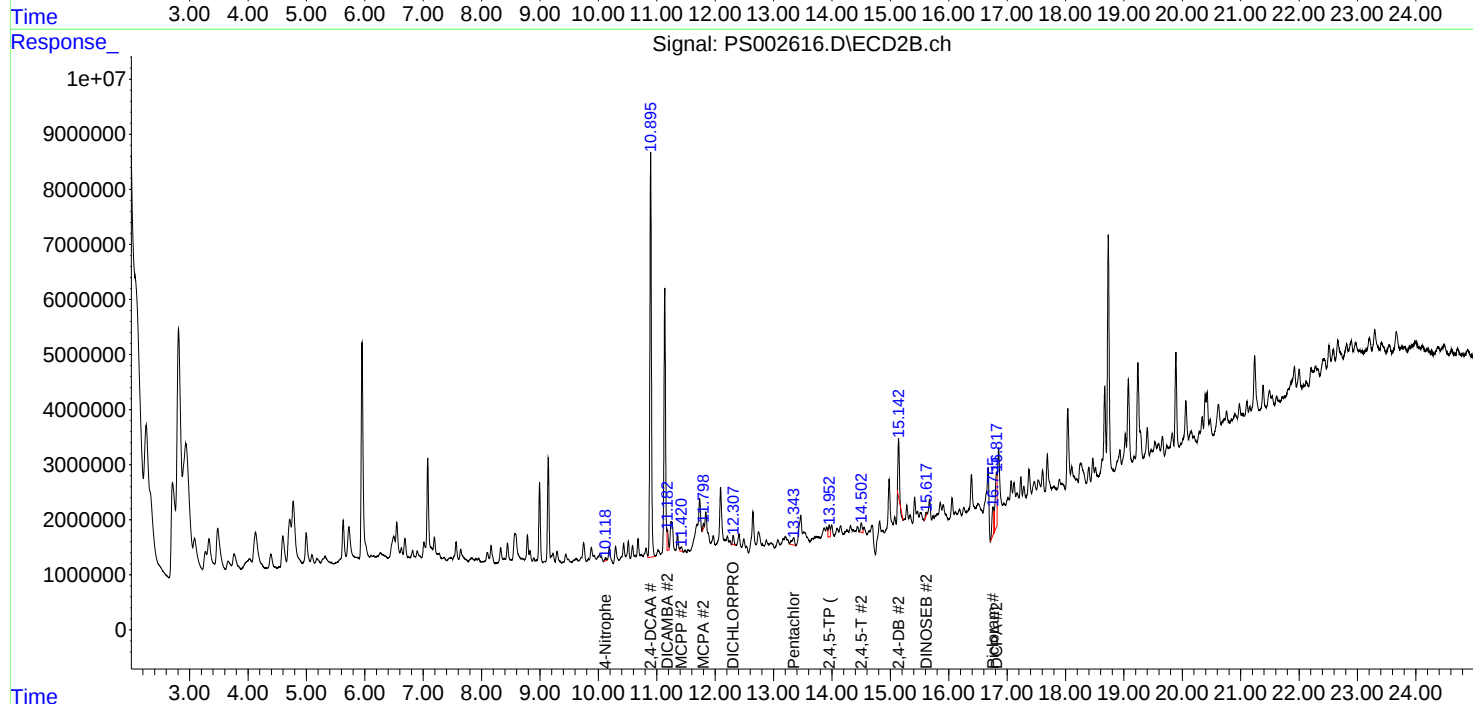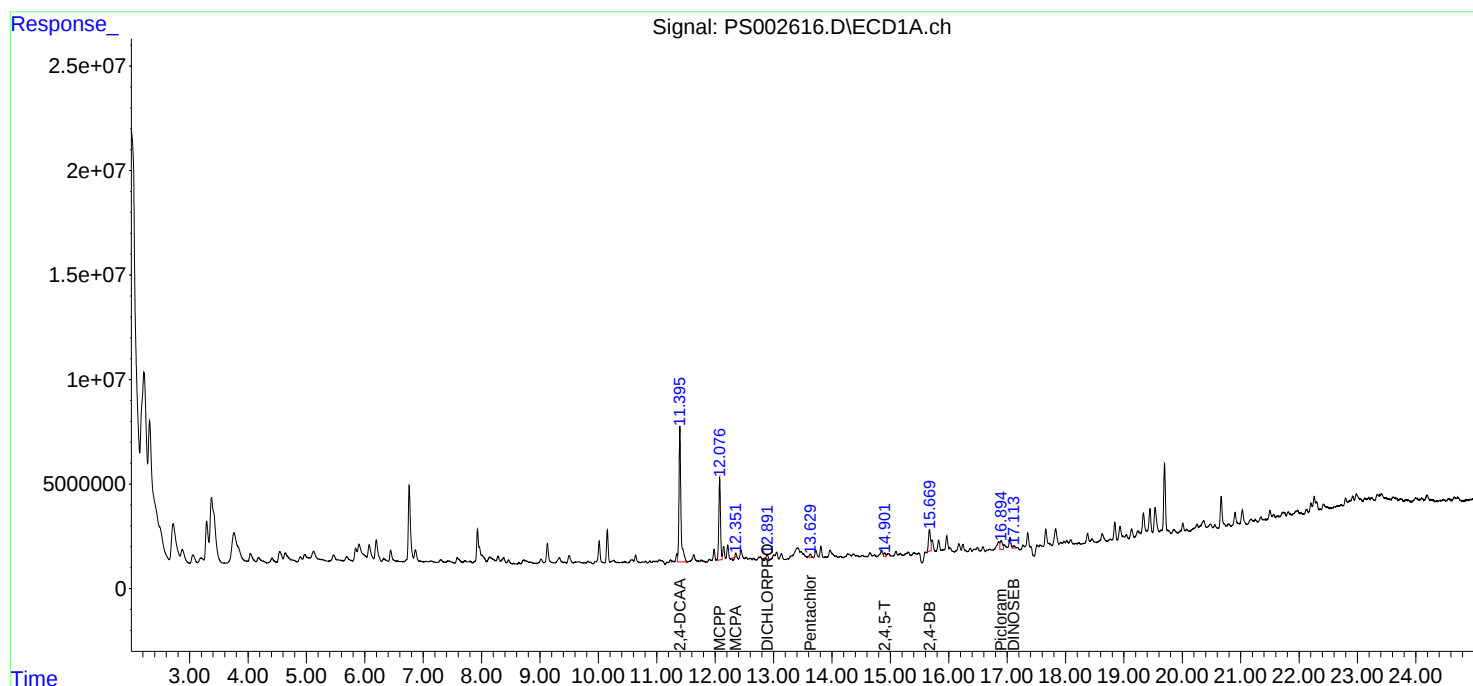


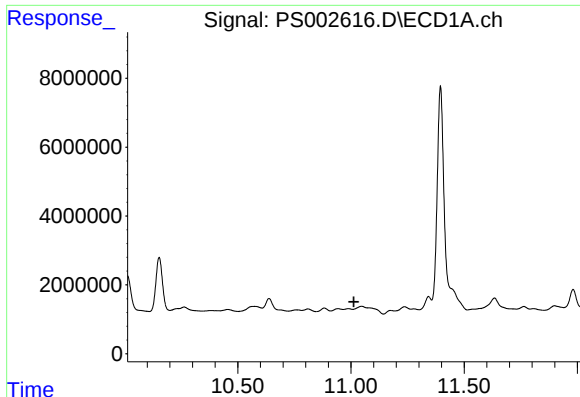

#3 4-Nitrophenol


R.T.: 0.000 min
Exp R.T.: 11.013 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

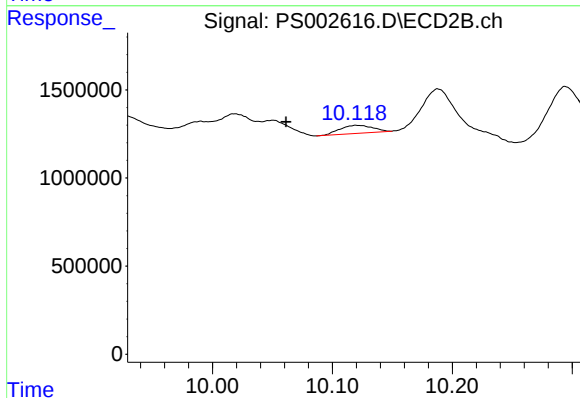


#3 4-Nitrophenol

R.T.: 10.120 min
Delta R.T.: 0.058 min
Response: 862816
Conc: 4.83 ng/ml

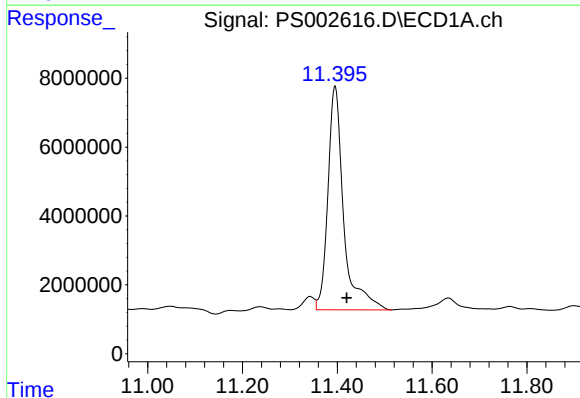


#4 2,4-DCAA

R.T.: 11.395 min
Delta R.T.: -0.025 min
Response: 149951881
Conc: 472.41 ng/ml

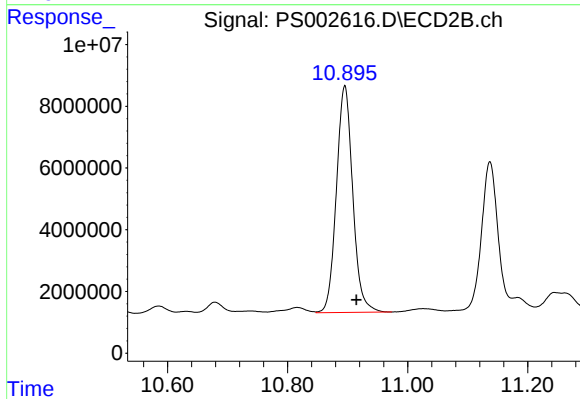

#4 2,4-DCAA


R.T.: 10.895 min
Delta R.T.: -0.019 min
Response: 138865491
Conc: 359.04 ng/ml

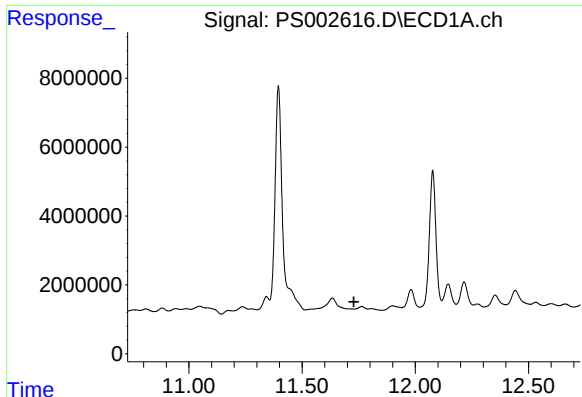

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

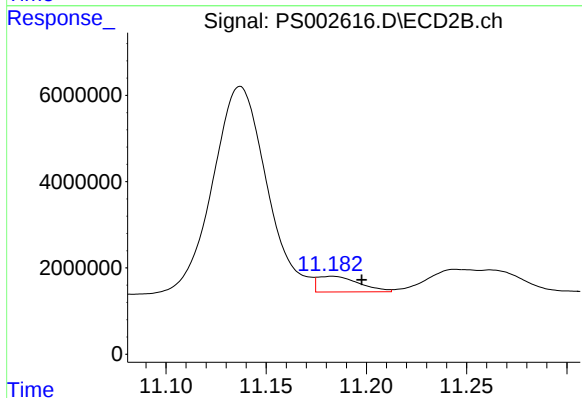


#5 DICAMBA

R.T.: 11.183 min
Delta R.T.: -0.014 min
Response: 5220454
Conc: 3.66 ng/ml

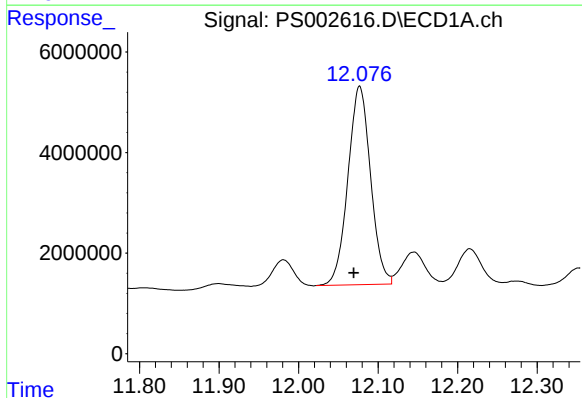


#6 MCP

R.T.: 12.077 min
Delta R.T.: 0.007 min
Response: 78185657
Conc: 78.36 ug/ml

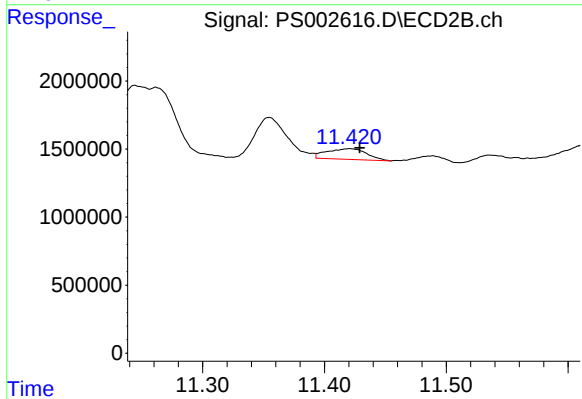

#6 MCP


R.T.: 11.421 min
Delta R.T.: -0.008 min
Response: 1771085
Conc: 1.89 ug/ml

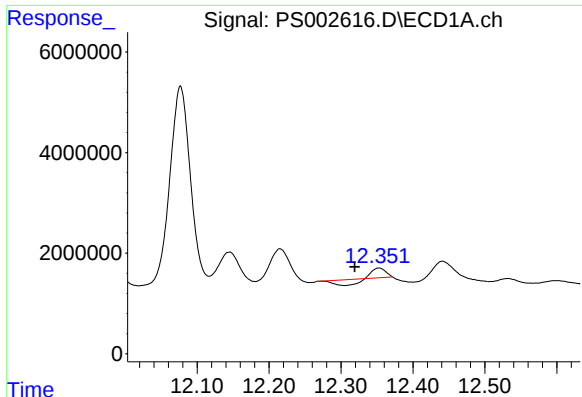

#7 MCPA


R.T.: 12.353 min
Delta R.T.: 0.033 min
Response: 298093
Conc: 0.20 ug/ml

Instrument :
ECD_S
ClientSampleId :

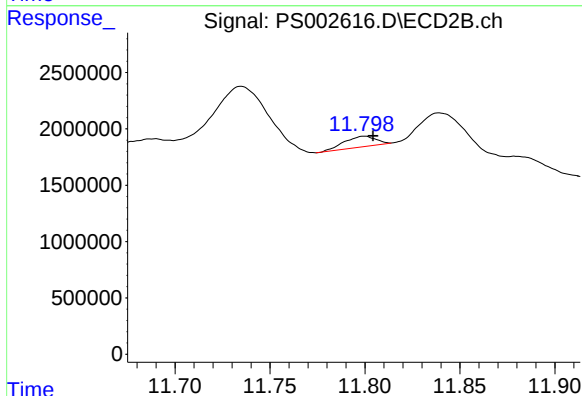


#7 MCPA

R.T.: 11.800 min
Delta R.T.: -0.005 min
Response: 1087087
Conc: 0.76 ug/ml

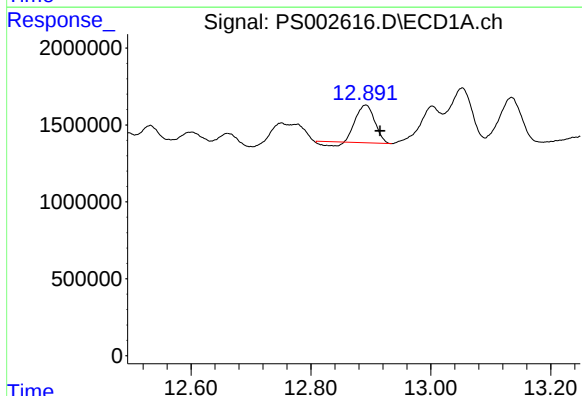


#8 DICHLORPROP

R.T.: 12.891 min
Delta R.T.: -0.024 min
Response: 5242144
Conc: 14.74 ng/ml

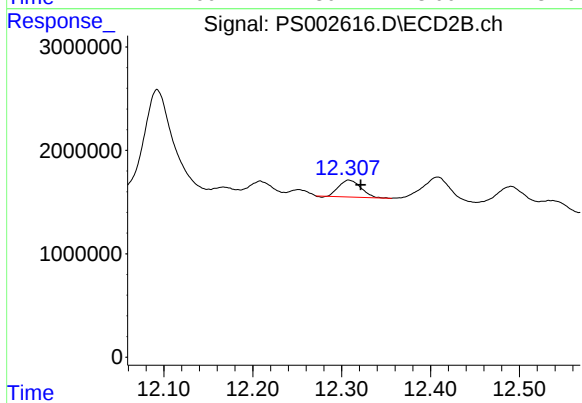

#8 DICHLORPROP


R.T.: 12.308 min
Delta R.T.: -0.014 min
Response: 2807286
Conc: 7.85 ng/ml

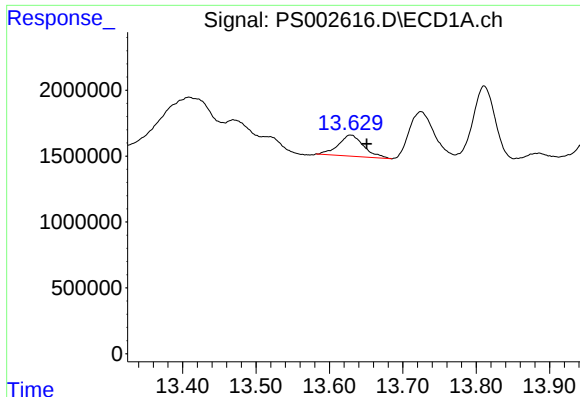

#10 Pentachlorophenol


R.T.: 13.629 min
Delta R.T.: -0.022 min
Response: 3836612
Conc: 0.77 ng/ml

Instrument :
ECD_S
ClientSampleId :

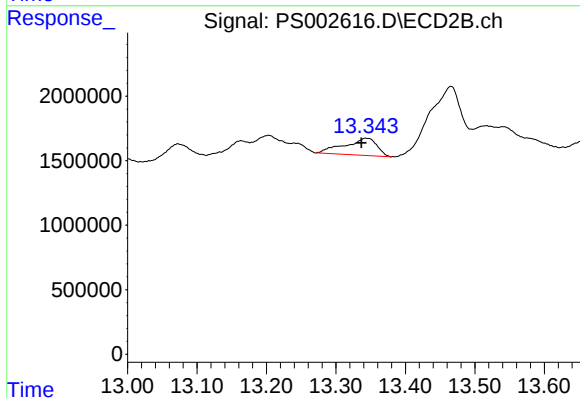


#10 Pentachlorophenol

R.T.: 13.343 min
Delta R.T.: 0.006 min
Response: 4308113
Conc: 0.82 ng/ml

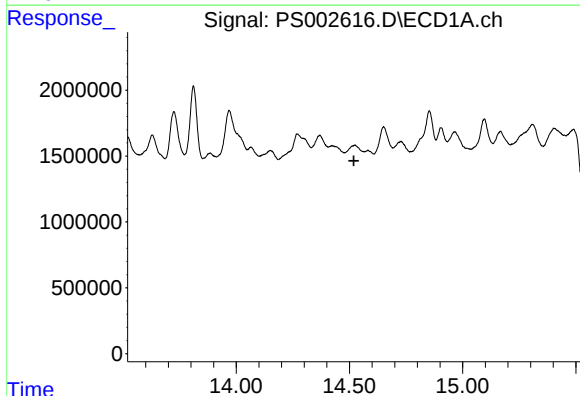


#11 2,4,5-TP (SILVEX)

R.T.: 0.000 min
Exp R.T. : 14.519 min
Response: 0
Conc: N.D.

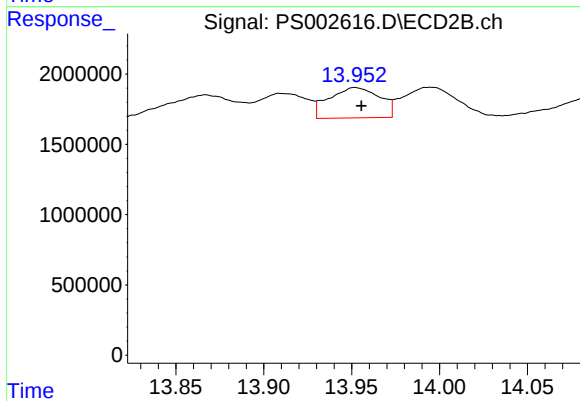

#11 2,4,5-TP (SILVEX)


R.T.: 13.952 min
Delta R.T.: -0.004 min
Response: 4336229
Conc: 2.07 ng/ml

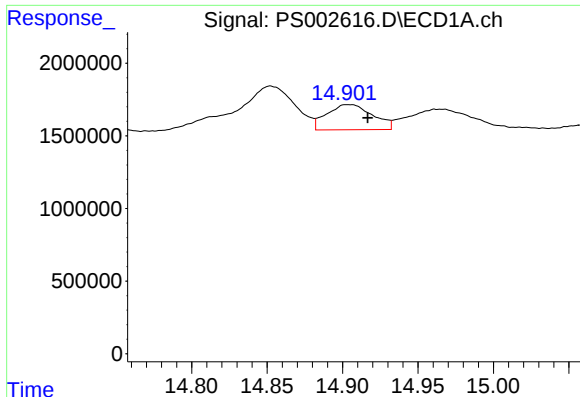

#12 2,4,5-T


R.T.: 14.904 min
Delta R.T.: -0.012 min
Response: 3644043
Conc: 1.94 ng/ml

Instrument :
ECD_S
ClientSampleId :

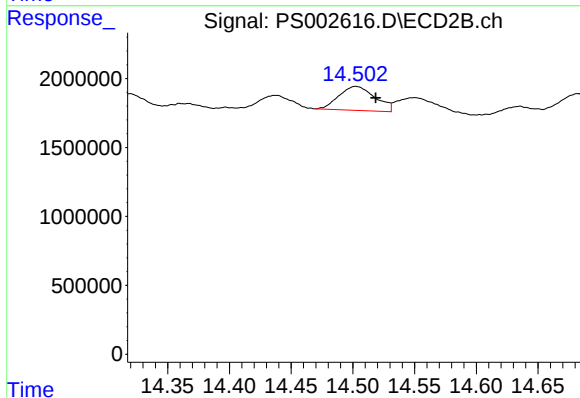


#12 2,4,5-T

R.T.: 14.502 min
Delta R.T.: -0.016 min
Response: 3541135
Conc: 2.07 ng/ml

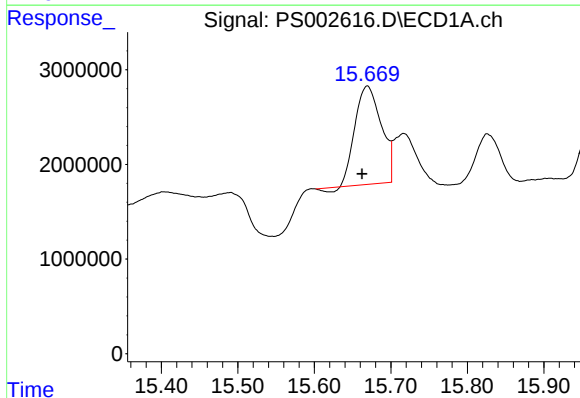


#13 2,4-DB

R.T.: 15.669 min
Delta R.T.: 0.007 min
Response: 24488165
Conc: 108.28 ng/ml

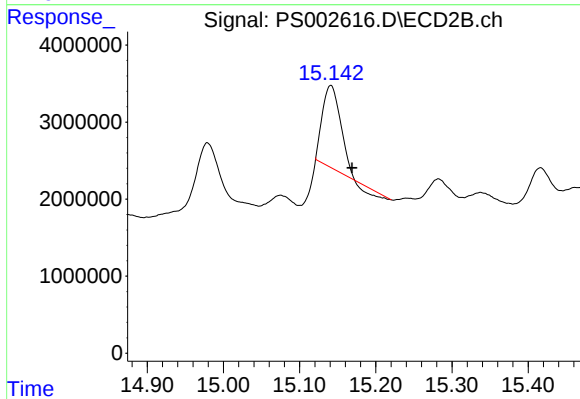

#13 2,4-DB


R.T.: 15.141 min
Delta R.T.: -0.028 min
Response: 15966589
Conc: 65.91 ng/ml

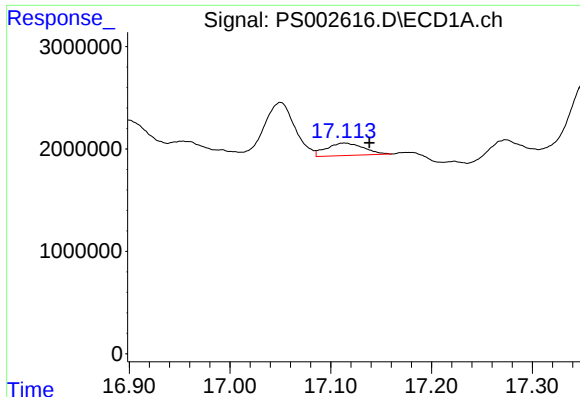

#14 DINOSEB


R.T.: 17.113 min
Delta R.T.: -0.025 min
Response: 3118782
Conc: 2.14 ng/ml

Instrument :
ECD_S
ClientSampleId :

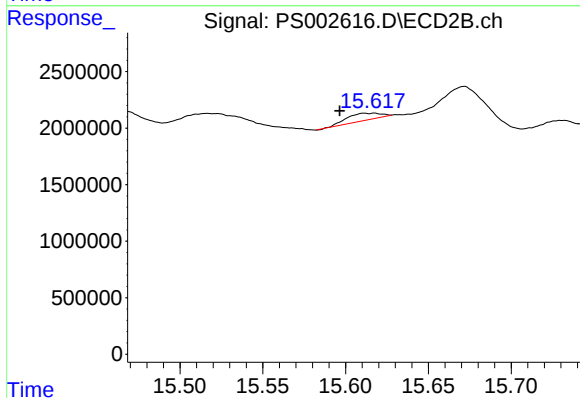


#14 DINOSEB

R.T.: 15.617 min
Delta R.T.: 0.021 min
Response: 884936
Conc: 0.58 ng/ml

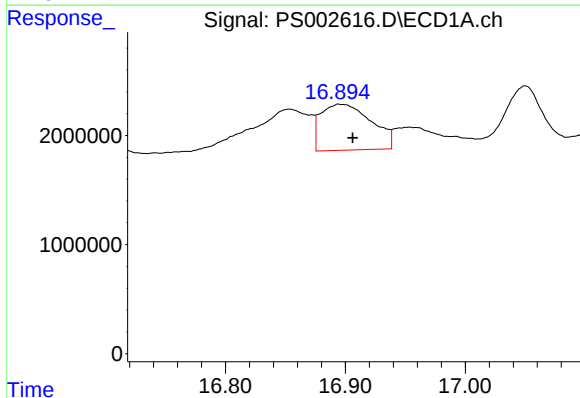


#15 Picloram

R.T.: 16.896 min
Delta R.T.: -0.010 min
Response: 12323520
Conc: 4.86 ng/ml

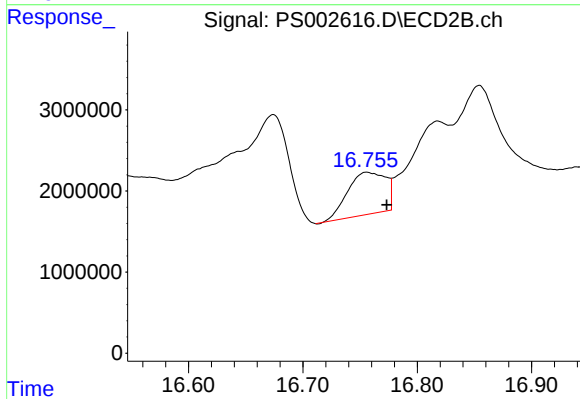

#15 Picloram


R.T.: 16.756 min
Delta R.T.: -0.017 min
Response: 12003037
Conc: 4.36 ng/ml

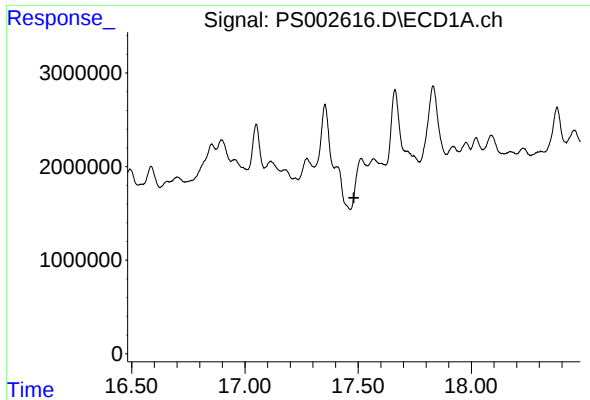

#16 DCPA

R.T.: 17.513 min
Delta R.T.: 0.032 min
Response: -3722895
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

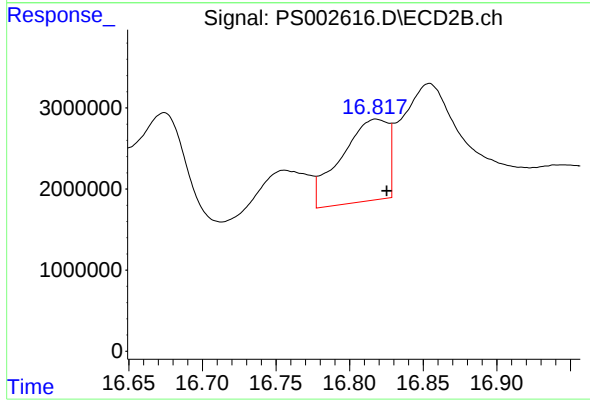

#16 DCPA

R.T.: 16.818 min
Delta R.T.: -0.007 min
Response: 22514733
Conc: 7.75 ng/ml