

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
 Data File : PS002618.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 14 Dec 2018 08:39
 Operator : EI\SJ
 Sample : J6357-10
 Misc :
 ALS Vial : 33 Sample Multiplier: 1

Instrument :
 ECD_S
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Dec 14 12:48:47 2018
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
 Quant Title : 8080.M
 QLast Update : Mon Dec 10 06:14:54 2018
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
4) S	2,4-DCAA	11.413	10.911	83223856	75333297	262.189	194.776 #
Target Compounds							
1) T	Dalapon	2.895	2.355	22782099	25715953	49.492	56.502
5) T	DICAMBA	0.000	11.153	0	82654297	N.D.	57.978 #
6) T	MCPD	12.093	0.000	64407629	0	64.553	N.D. #
7) T	MCPA	0.000	11.807	0	1099955	N.D.	0.765 #
10) T	Pentachlo...	0.000	13.363	0	1686541	N.D.	0.321 #
11) T	2,4,5-TP ...	0.000	14.016	0	945605	N.D.	0.450 #
12) T	2,4,5-T	0.000	14.570	0	1441225	N.D.	0.842 #
13) T	2,4-DB	15.678	0.000	3300829	0	14.595	N.D. #
15) T	Picloram	16.895	0.000	3840676	0	1.513	N.D. #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_S\Data\PS121318\
Data File : PS002618.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 14 Dec 2018 08:39
Operator : EI\SJ
Sample : J6357-10
Misc :
ALS Vial : 33 Sample Multiplier: 1

Instrument :
ECD_S
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Dec 14 12:48:47 2018
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_S\Method\PS120618.M
Quant Title : 8080.M
QLast Update : Mon Dec 10 06:14:54 2018
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : Rtx-CLPesticides Signal #2 Phase: Rtx-CLPesticides2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

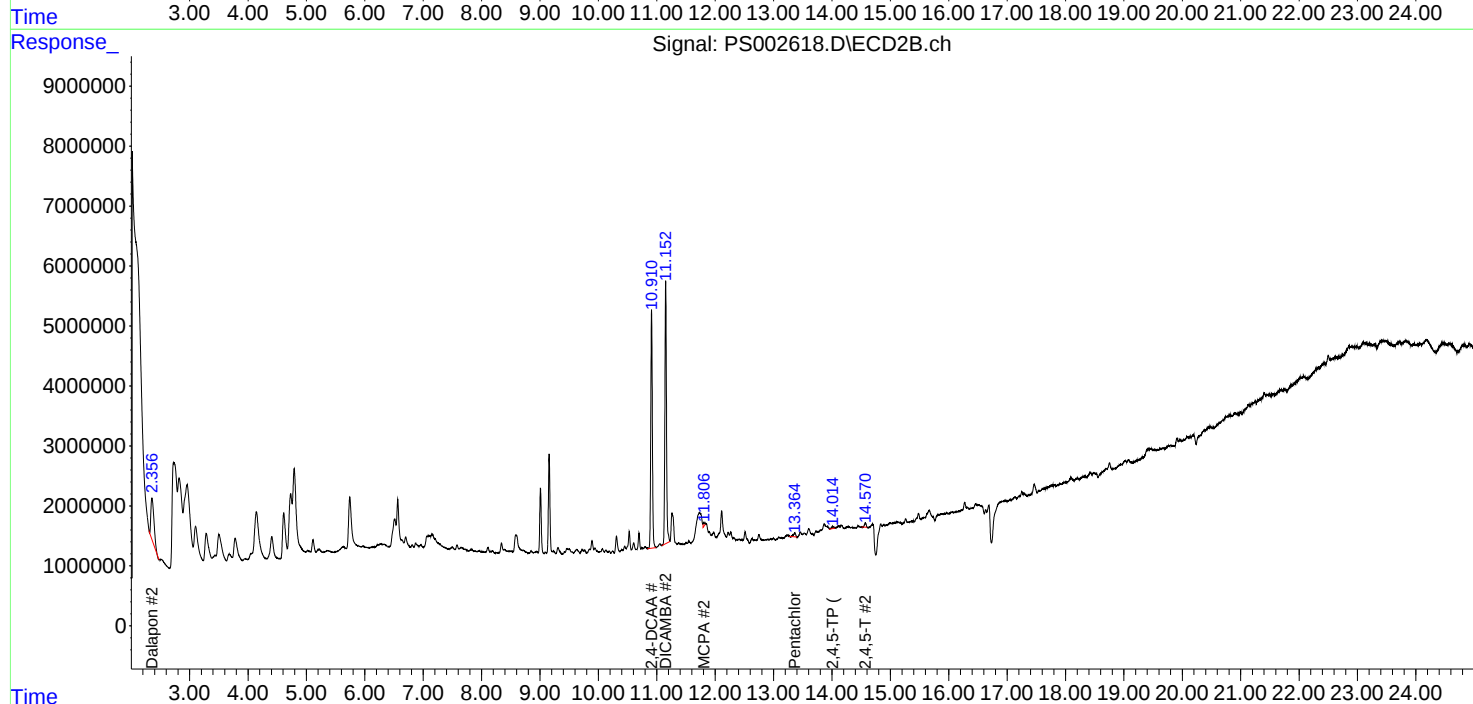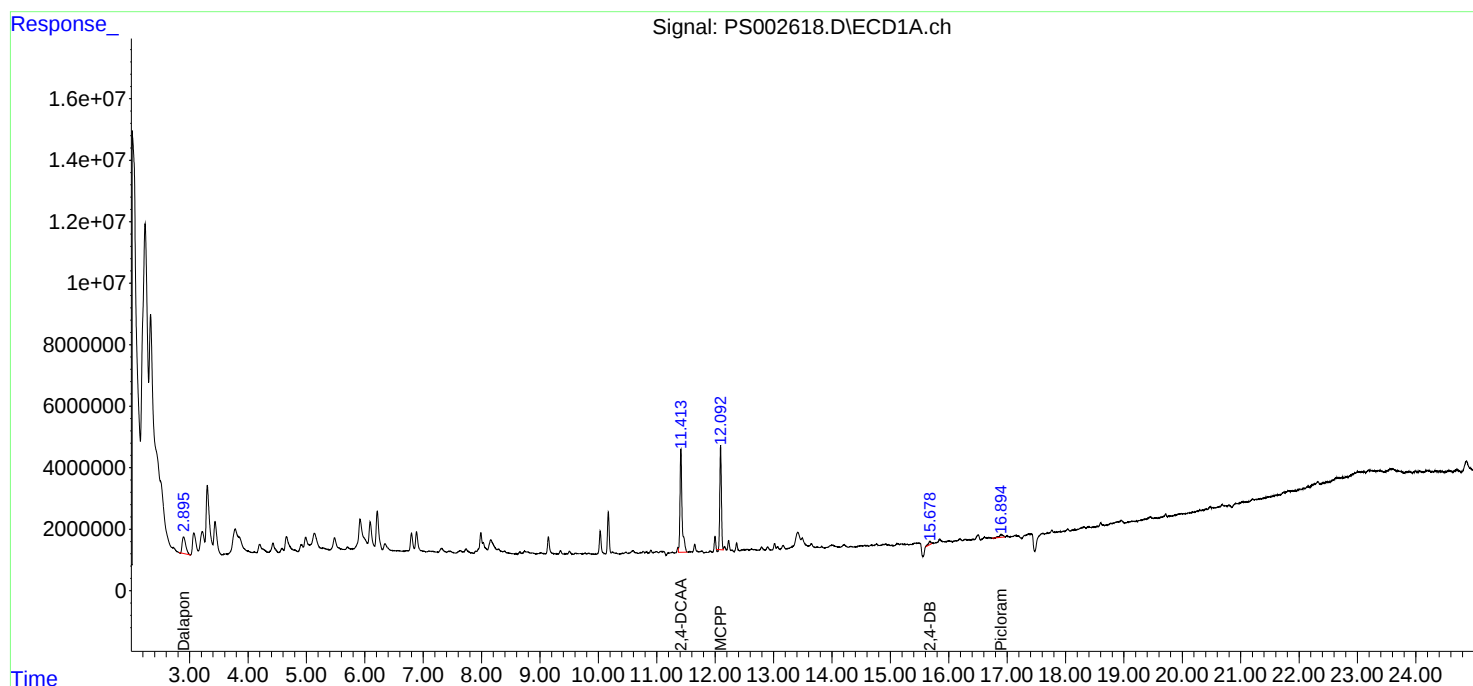


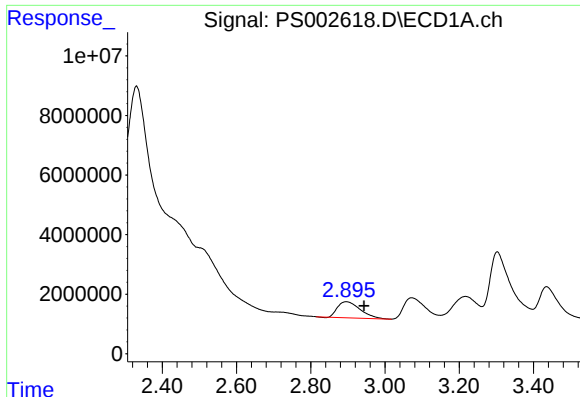

#1 Dalapon


R.T.: 2.895 min
Delta R.T.: -0.049 min
Response: 22782099
Conc: 49.49 ng/ml

Instrument :
ECD_S
ClientSampleId :

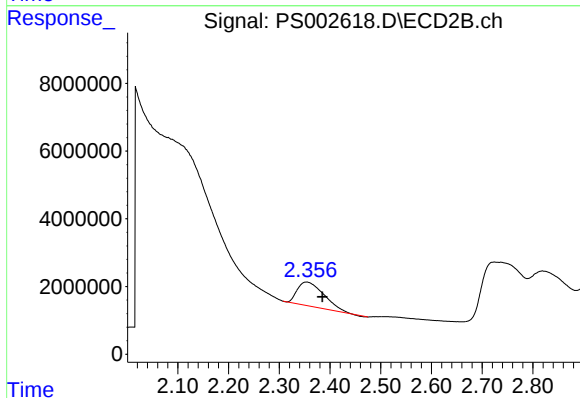


#1 Dalapon

R.T.: 2.355 min
Delta R.T.: -0.031 min
Response: 25715953
Conc: 56.50 ng/ml

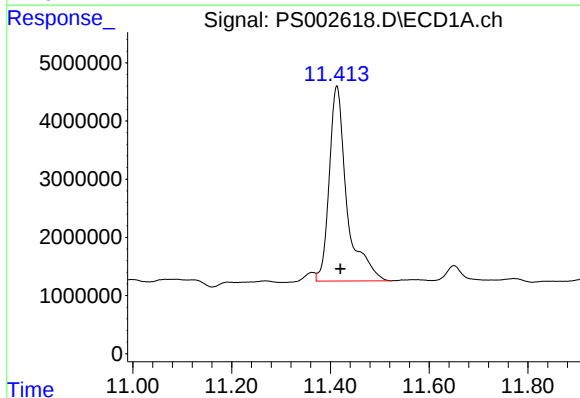


#4 2,4-DCAA

R.T.: 11.413 min
Delta R.T.: -0.007 min
Response: 83223856
Conc: 262.19 ng/ml

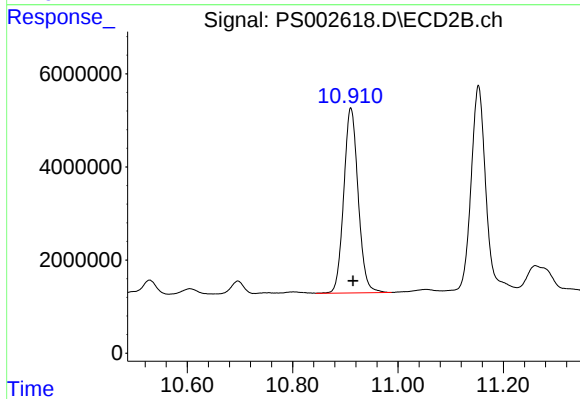

#4 2,4-DCAA


R.T.: 10.911 min
Delta R.T.: -0.004 min
Response: 75333297
Conc: 194.78 ng/ml

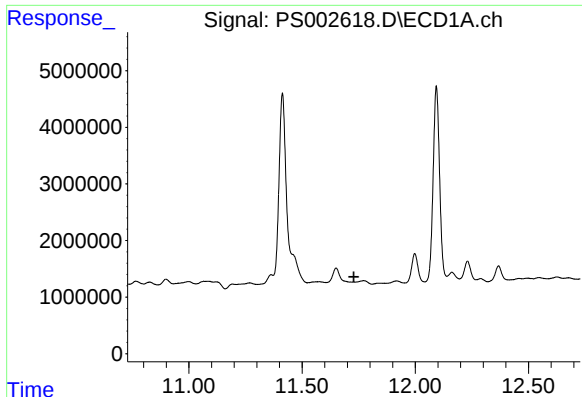

#5 DICAMBA


R.T.: 0.000 min
Exp R.T.: 11.729 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

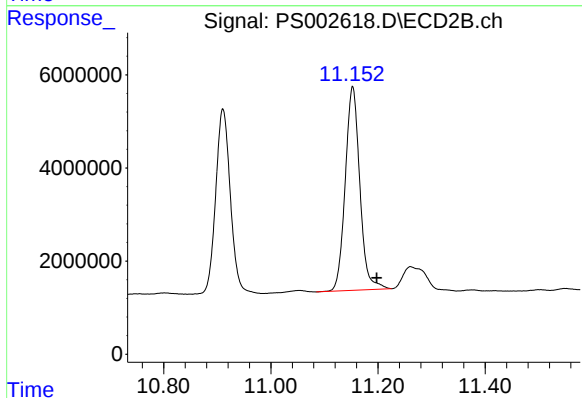


#5 DICAMBA

R.T.: 11.153 min
Delta R.T.: -0.045 min
Response: 82654297
Conc: 57.98 ng/ml

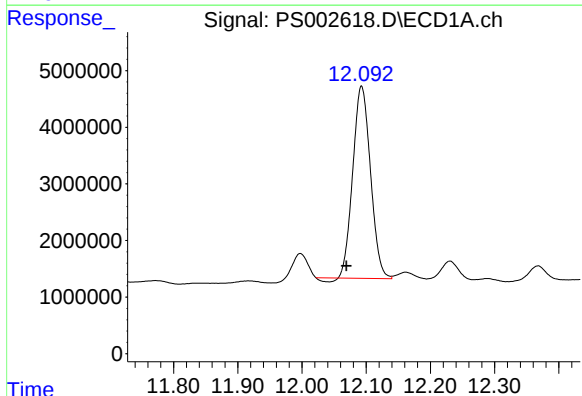


#6 MCP

R.T.: 12.093 min
Delta R.T.: 0.023 min
Response: 64407629
Conc: 64.55 ug/ml

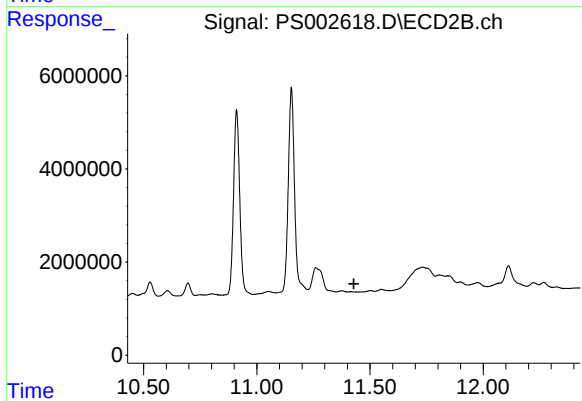

#6 MCP


R.T.: 0.000 min
Exp R.T.: 11.429 min
Response: 0
Conc: N.D.

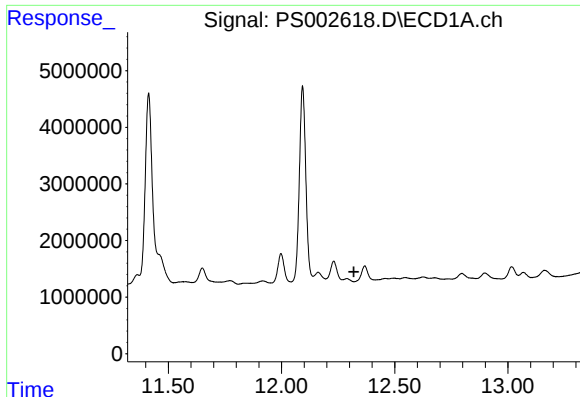

#7 MCPA


R.T.: 0.000 min
Exp R.T. : 12.319 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

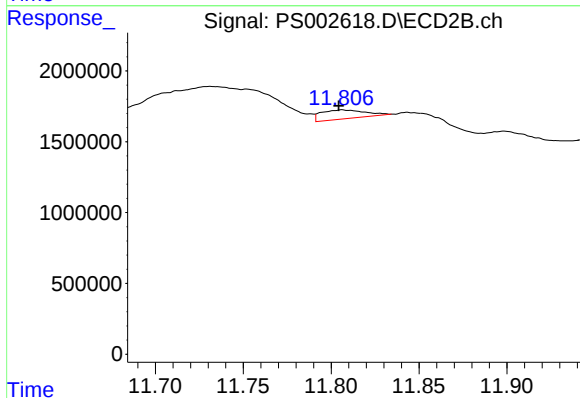


#7 MCPA

R.T.: 11.807 min
Delta R.T.: 0.002 min
Response: 1099955
Conc: 0.77 ug/ml

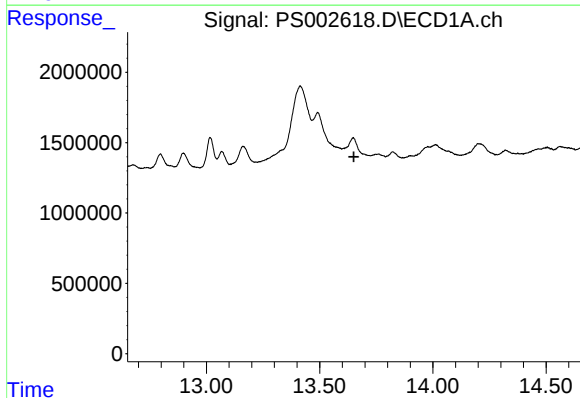


#10 Pentachlorophenol

R.T.: 0.000 min
Exp R.T. : 13.651 min
Response: 0
Conc: N.D.

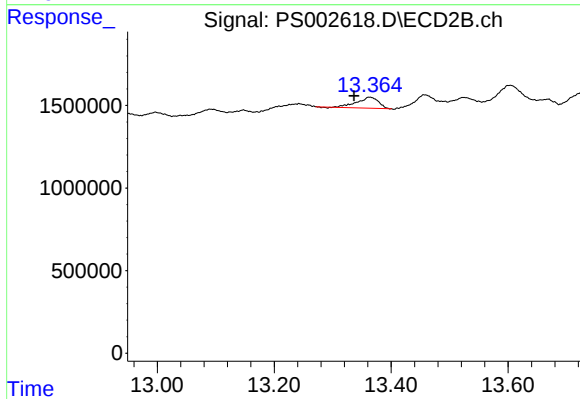

#10 Pentachlorophenol


R.T.: 13.363 min
Delta R.T.: 0.027 min
Response: 1686541
Conc: 0.32 ng/ml

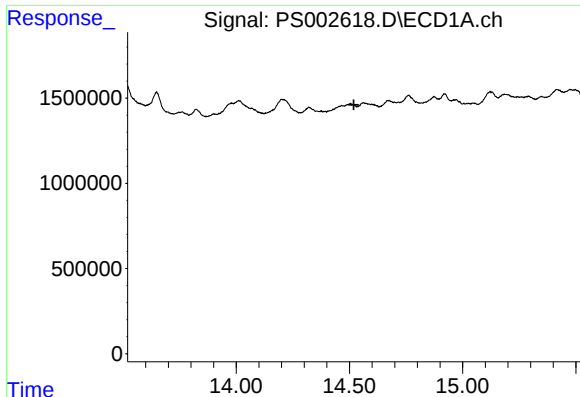

#11 2,4,5-TP (SILVEX)


R.T.: 0.000 min
Exp R.T.: 14.519 min
Response: 0
Conc: N.D.

Instrument :
ECD_S
ClientSampleId :

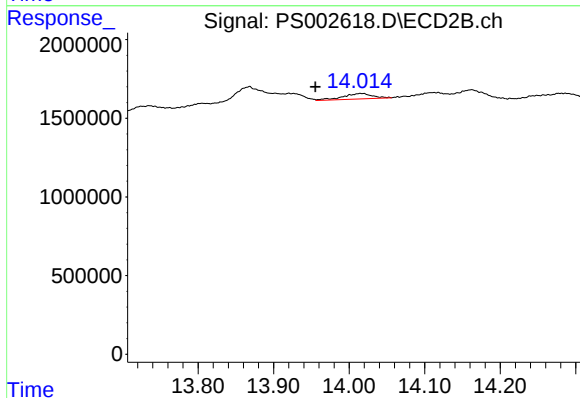


#11 2,4,5-TP (SILVEX)

R.T.: 14.016 min
Delta R.T.: 0.060 min
Response: 945605
Conc: 0.45 ng/ml

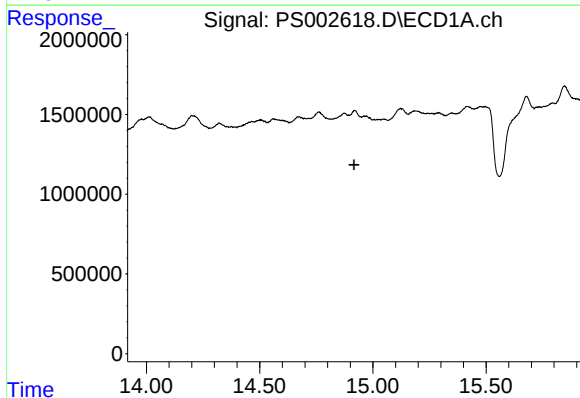


#12 2,4,5-T

R.T.: 0.000 min
Exp R.T.: 14.917 min
Response: 0
Conc: N.D.

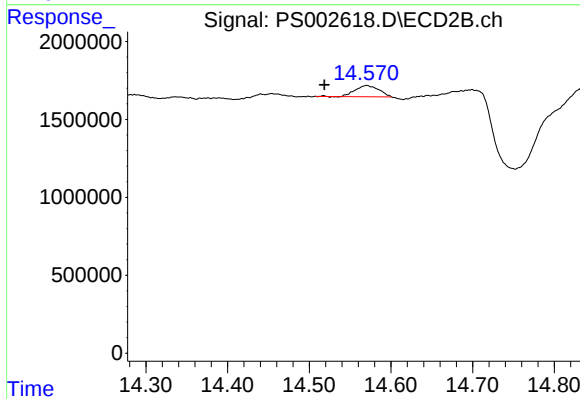

#12 2,4,5-T


R.T.: 14.570 min
Delta R.T.: 0.052 min
Response: 1441225
Conc: 0.84 ng/ml

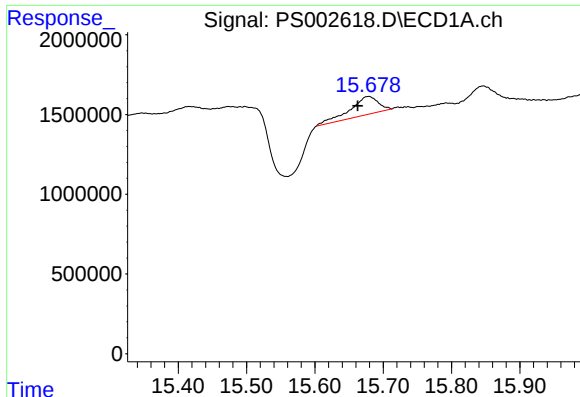

#13 2,4-DB


R.T.: 15.678 min
Delta R.T.: 0.015 min
Response: 3300829
Conc: 14.59 ng/ml

Instrument :
ECD_S
ClientSampleId :

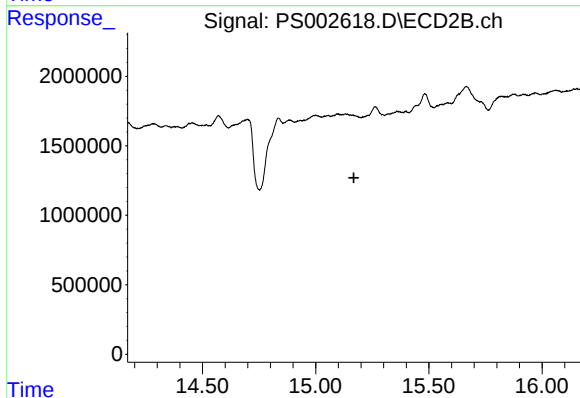


#13 2,4-DB

R.T.: 0.000 min
Exp R.T. : 15.169 min
Response: 0
Conc: N.D.

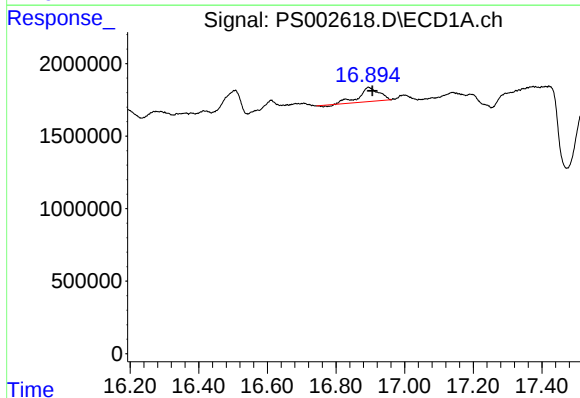

#15 Picloram

R.T.: 16.895 min
Delta R.T.: -0.011 min
Response: 3840676
Conc: 1.51 ng/ml

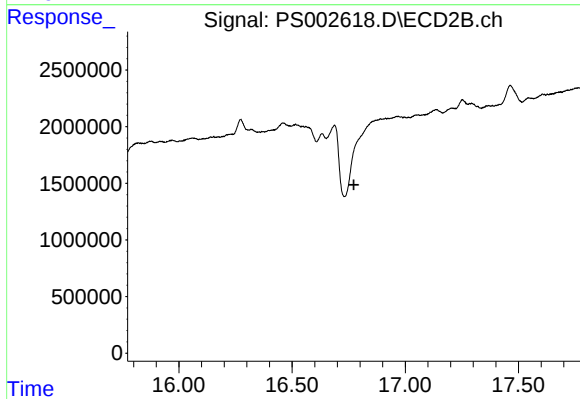

#15 Picloram

R.T.: 0.000 min
Exp R.T. : 16.773 min
Response: 0
Conc: N.D.